

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 10:37
 Operator : DD\AJ
 Sample : L3611-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFL0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:30:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	10966452	16543417	11.340	11.423
27)	SA Decachlor...	7.843	8.863	15750435	12717703	14.953	9.273 #
Target Compounds							
8)	B Heptachlo...	0.000	5.776f	0	9490196	N.D.	5.699
9)	A Endosulfan I	0.000	6.004f	0	1857778	N.D.	1.198
10)	B trans-Chl...	0.000	5.934	0	872452	N.D.	0.524
11)	B cis-Chlor...	0.000	6.004	0	1857778	N.D.	1.103
16)	A 4,4'-DDD	0.000	6.626f	0	846629	N.D.	0.646
19)	B Endosulfa...	6.346	0.000	1873796	0	1.831	N.D. #
23)	Toxaphene-2	5.503	0.000	32451120	0	4484.939	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 10:37
Operator : DD\AJ
Sample : L3611-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFL0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:30:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

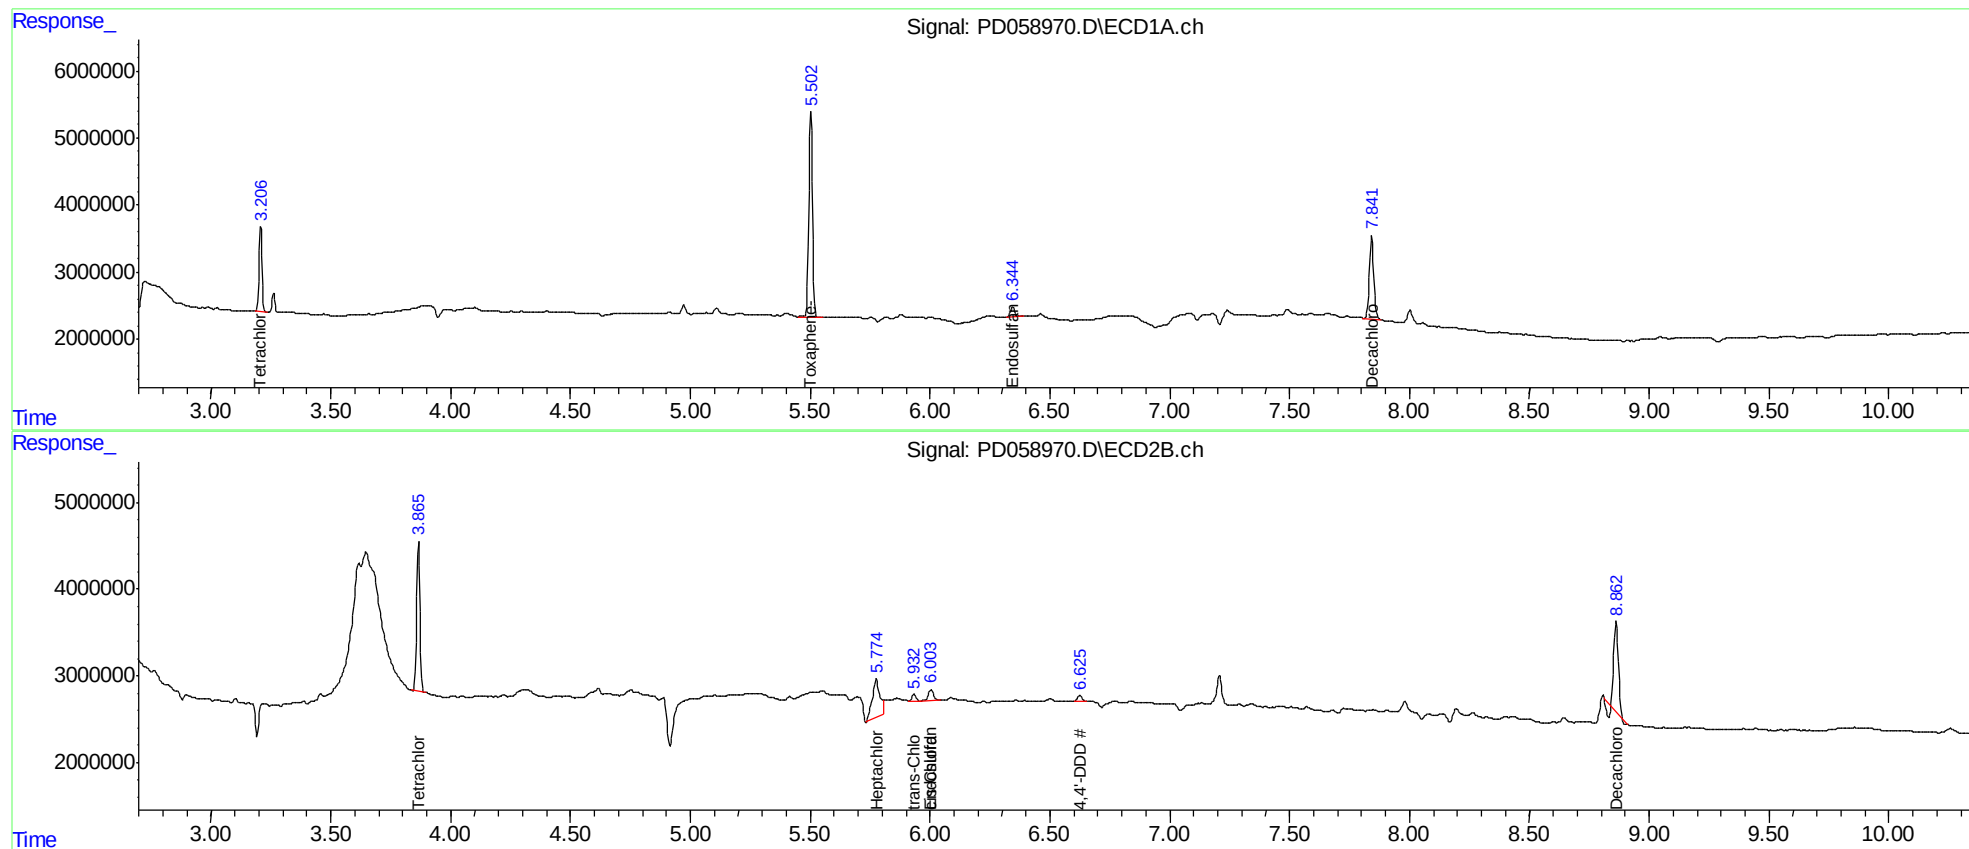


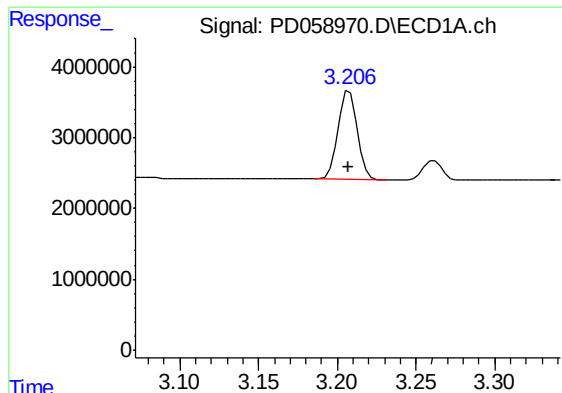

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 10966452
Conc: 11.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

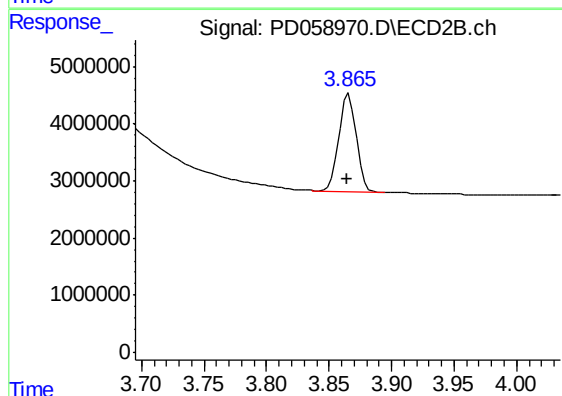


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.001 min
Response: 16543417
Conc: 11.42 ng/ml

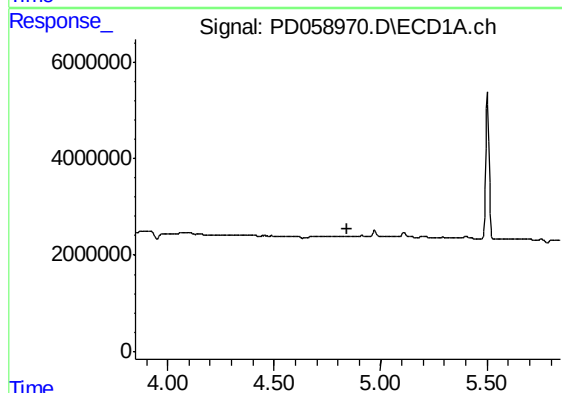


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

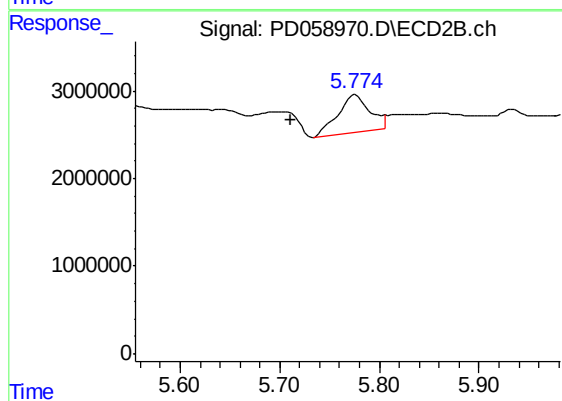

#8 Heptachlor epoxide


R.T.: 5.776 min
Delta R.T.: 0.065 min
Response: 9490196
Conc: 5.70 ng/ml

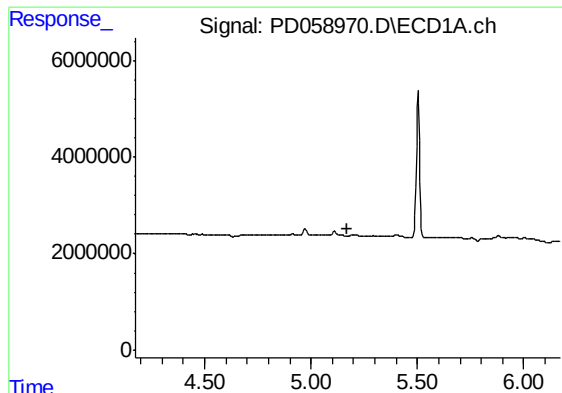

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL0

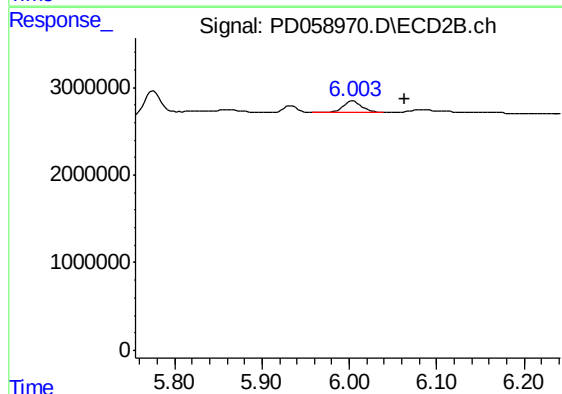


#9 Endosulfan I

R.T.: 6.004 min
Delta R.T.: -0.060 min
Response: 1857778
Conc: 1.20 ng/ml

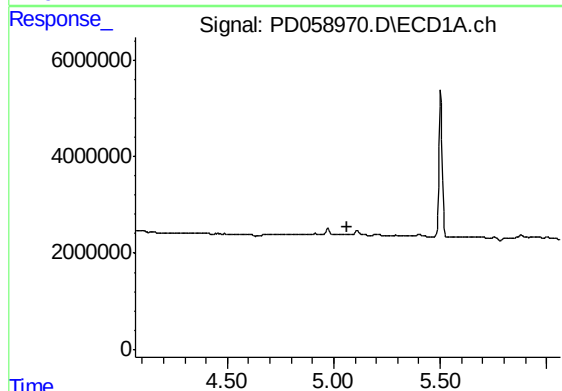


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

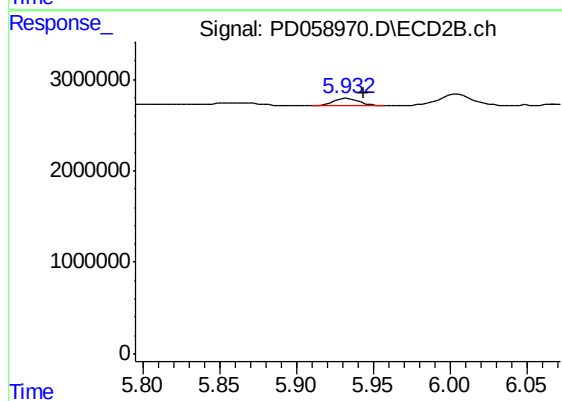

#10 trans-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.010 min
Response: 872452
Conc: 0.52 ng/ml

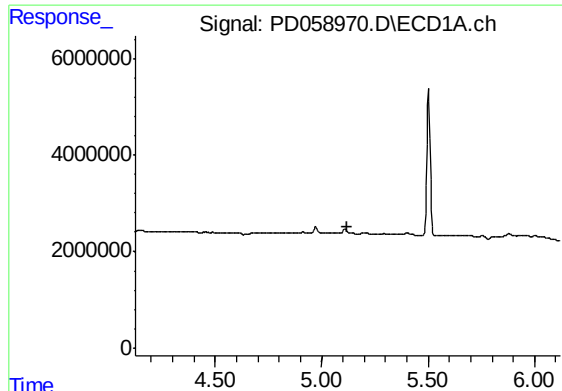

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL0

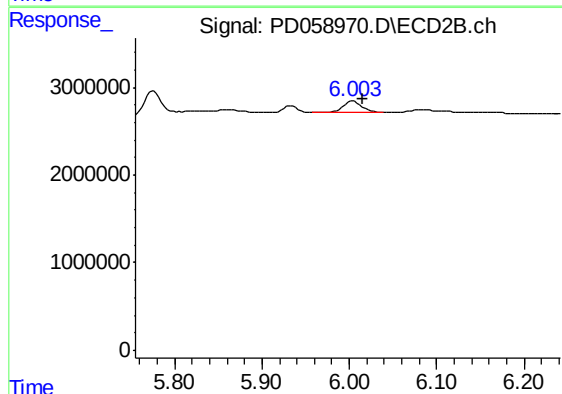


#11 cis-Chlordane

R.T.: 6.004 min
Delta R.T.: -0.012 min
Response: 1857778
Conc: 1.10 ng/ml

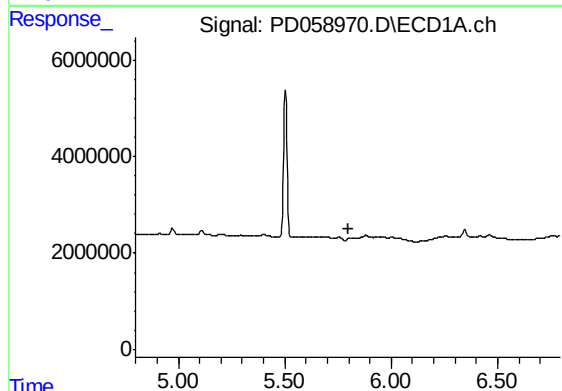


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.798 min
Response: 0
Conc: N.D.

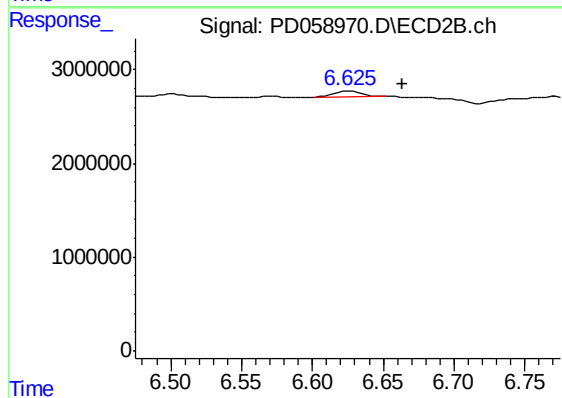

#16 4,4'-DDD


R.T.: 6.626 min
Delta R.T.: -0.037 min
Response: 846629
Conc: 0.65 ng/ml

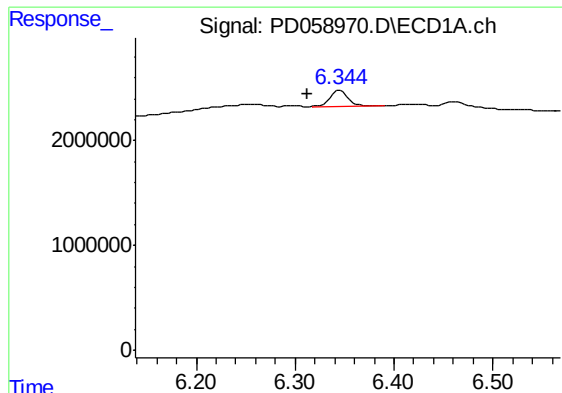

#19 Endosulfan Sulfate


R.T.: 6.346 min
Delta R.T.: 0.033 min
Response: 1873796
Conc: 1.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

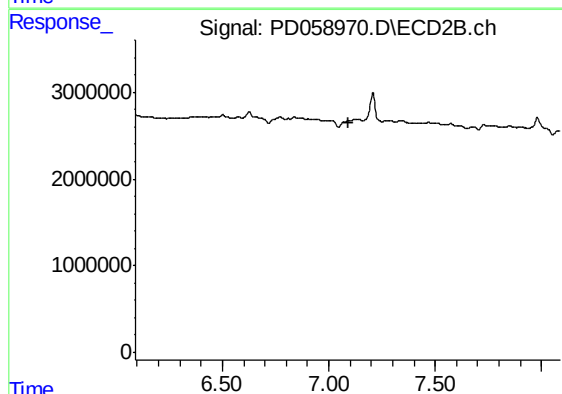


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

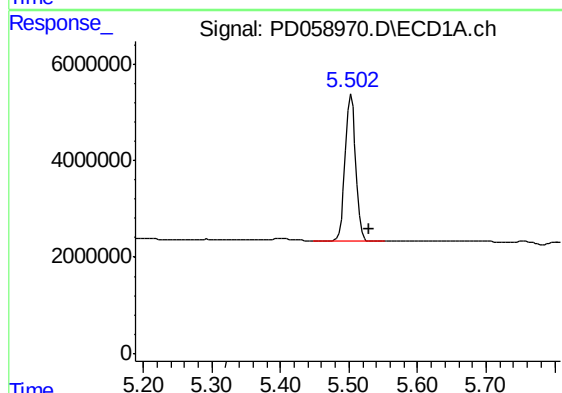


#23 Toxaphene-2

R.T.: 5.503 min
Delta R.T.: -0.026 min
Response: 32451120
Conc: 4484.94 ng/ml

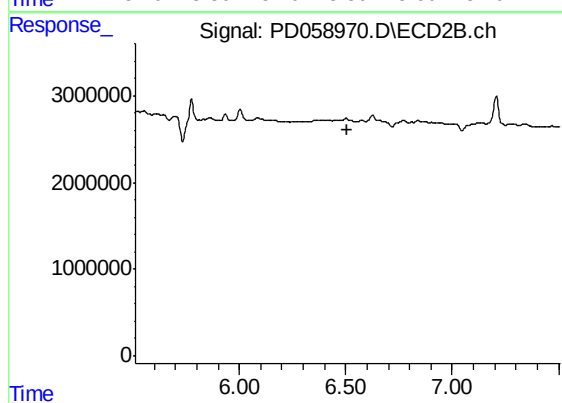

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

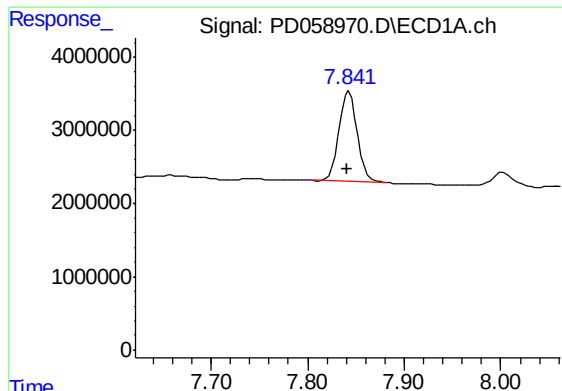

#27 Decachlorobiphenyl

R.T.: 7.843 min
Delta R.T.: 0.002 min
Response: 15750435
Conc: 14.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

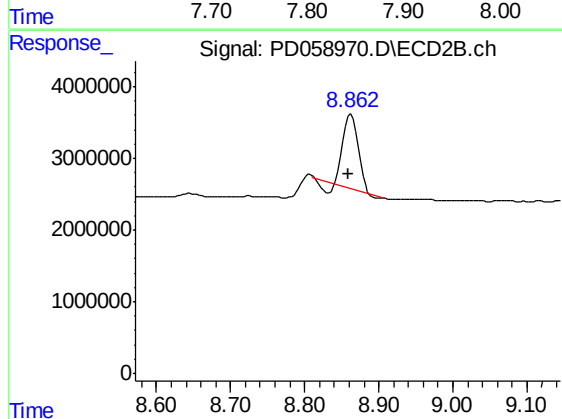

#27 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.004 min
Response: 12717703
Conc: 9.27 ng/ml