

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 11:33
 Operator : DD\AJ
 Sample : L3611-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFL6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:31:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	18496189	27803325	19.126	19.198
27)	SA Decachlor...	7.841	8.861	28014770	29992940	26.597	21.870
Target Compounds							
10)	B trans-Chl...	0.000	5.934	0	2410038	N.D.	1.447
13)	MA Dieldrin	0.000	6.353	0	605393	N.D.	0.362
16)	A 4,4'-DDD	0.000	6.625f	0	723068	N.D.	0.552
21)	B Endrin ke...	0.000	7.616f	0	852214	N.D.	0.586


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 11:33
Operator : DD\AJ
Sample : L3611-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFL6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:31:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

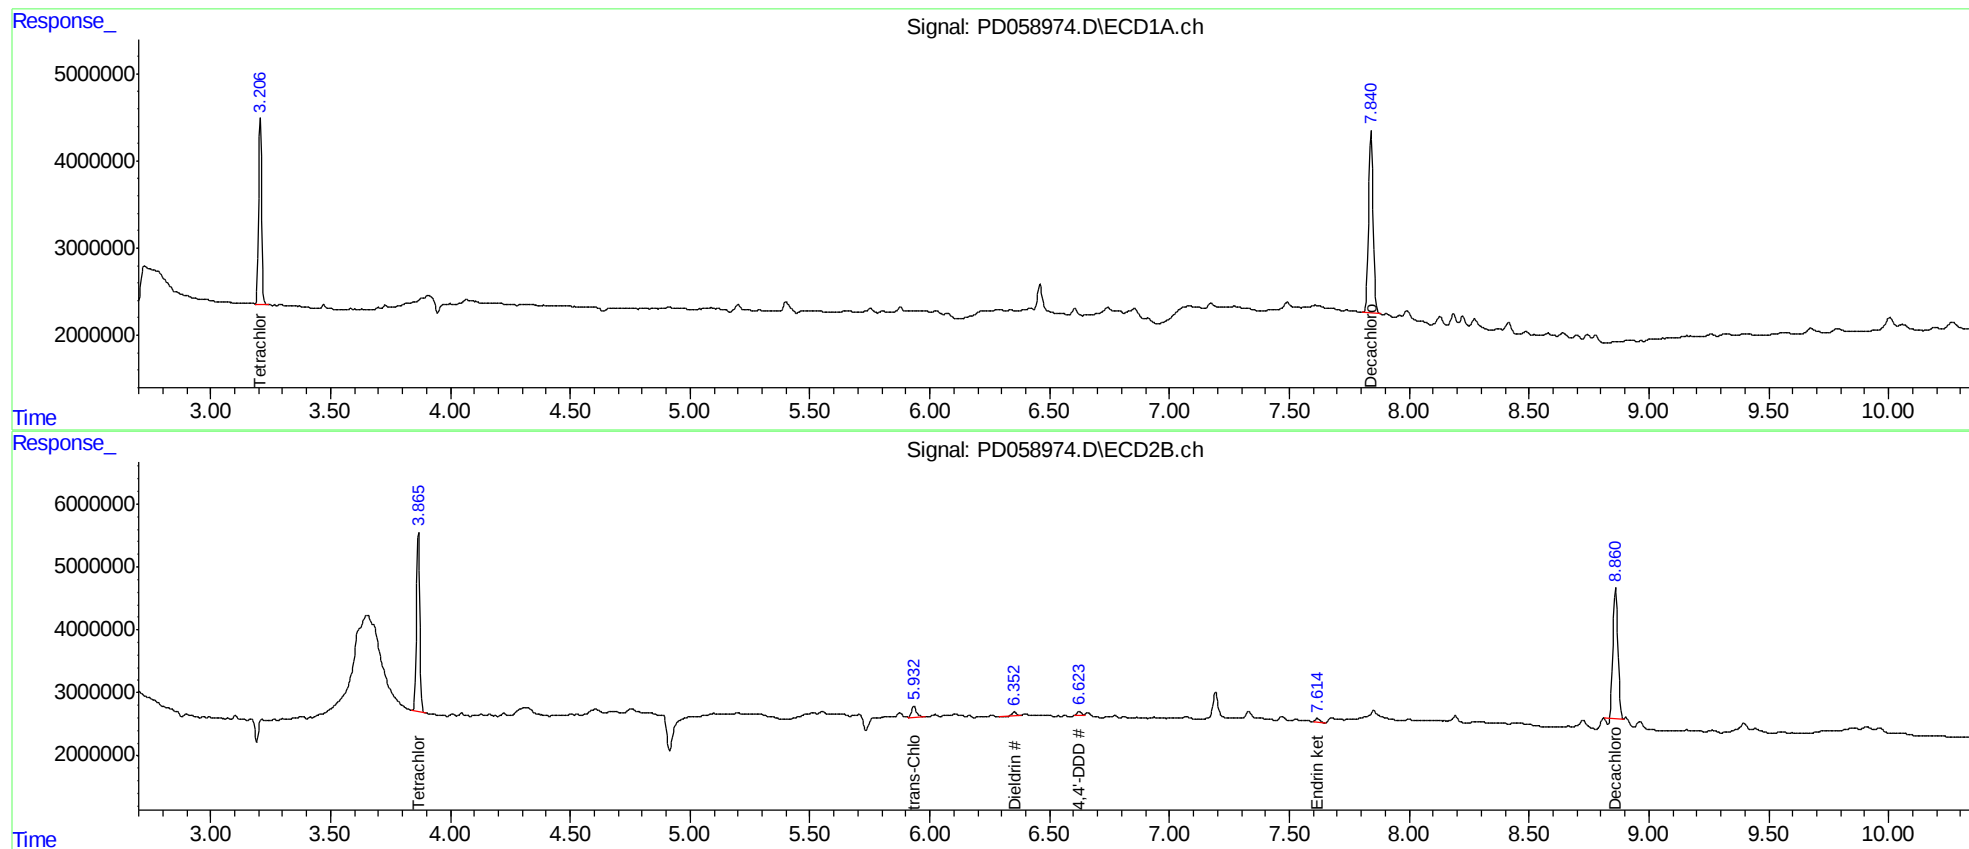


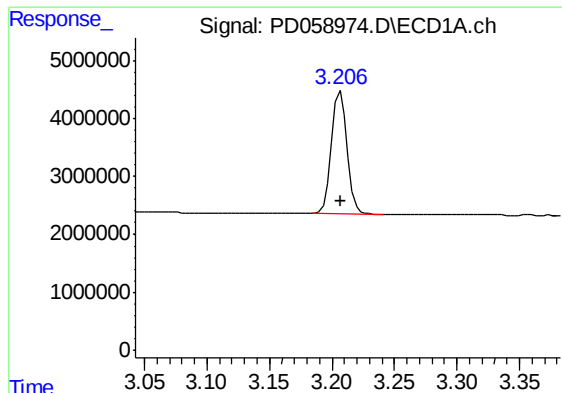

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 18496189
Conc: 19.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL6

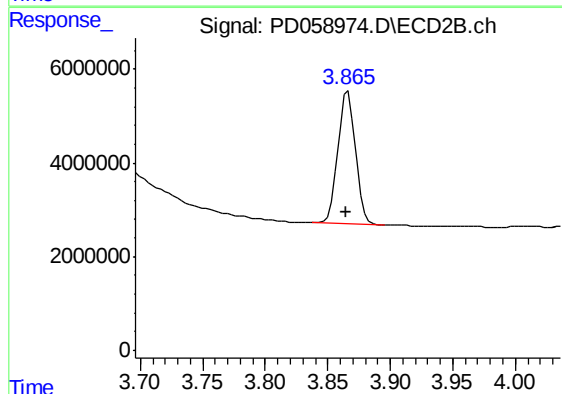


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.001 min
Response: 27803325
Conc: 19.20 ng/ml

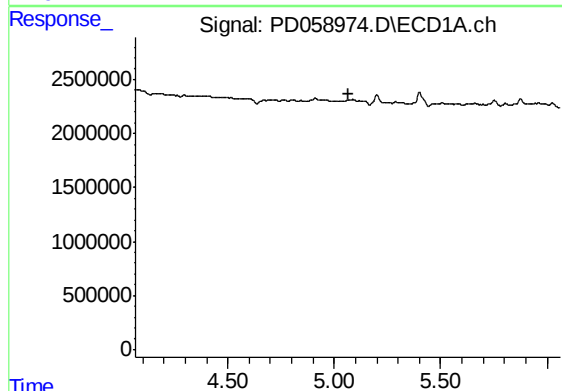


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

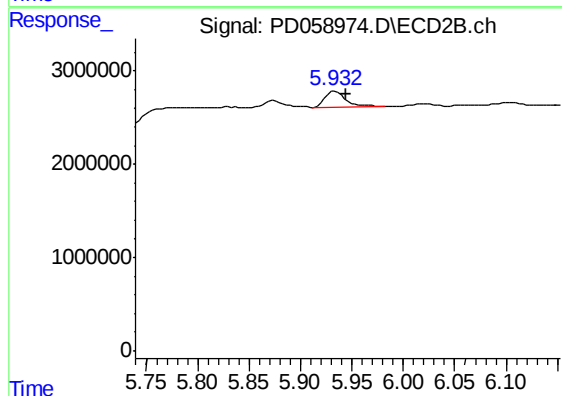

#10 trans-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.010 min
Response: 2410038
Conc: 1.45 ng/ml

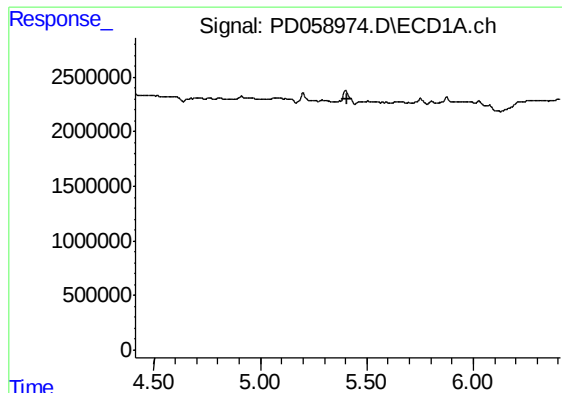

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL6

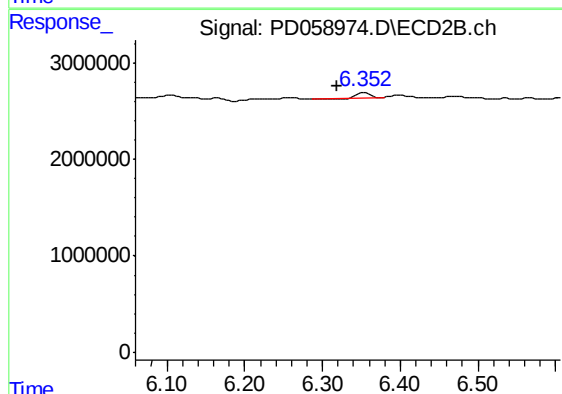


#13 Dieldrin

R.T.: 6.353 min
Delta R.T.: 0.034 min
Response: 605393
Conc: 0.36 ng/ml

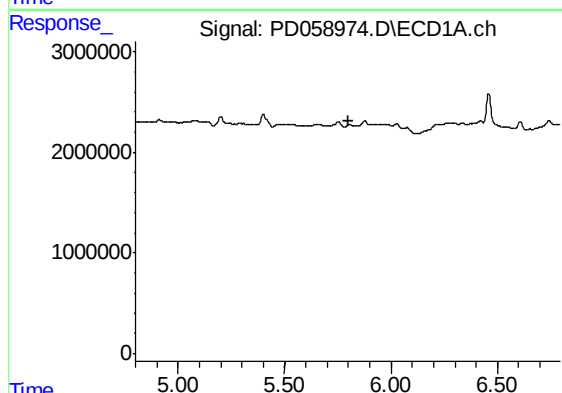


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

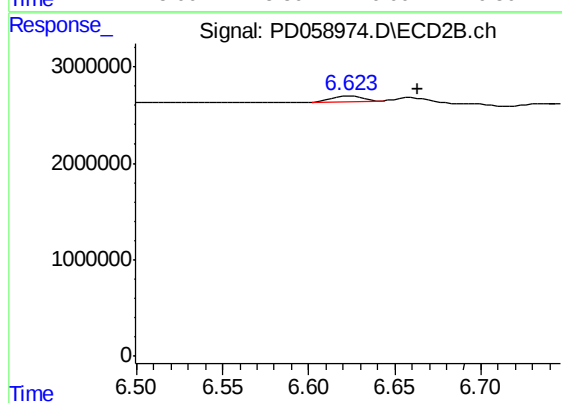

#16 4,4'-DDD


R.T.: 6.625 min
Delta R.T.: -0.039 min
Response: 723068
Conc: 0.55 ng/ml

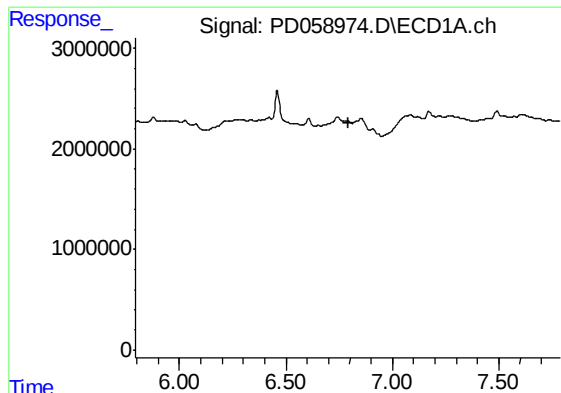

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL6

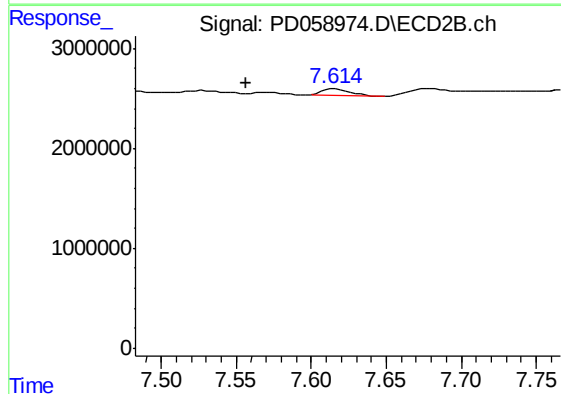


#21 Endrin ketone

R.T.: 7.616 min
Delta R.T.: 0.060 min
Response: 852214
Conc: 0.59 ng/ml

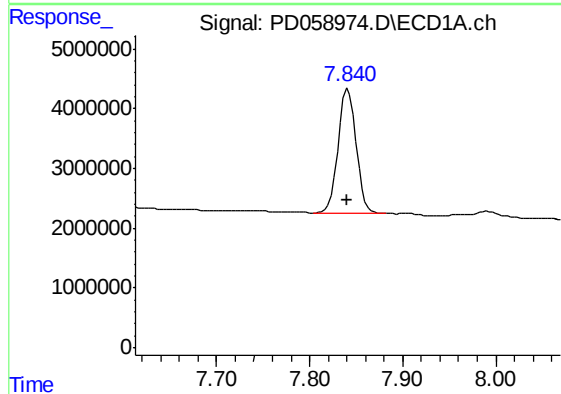

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 28014770
Conc: 26.60 ng/ml

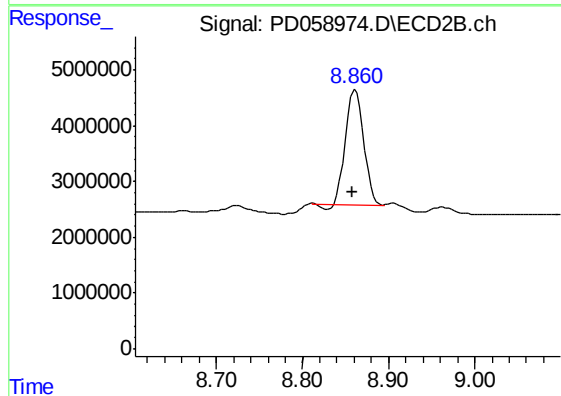

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.003 min
Response: 29992940
Conc: 21.87 ng/ml