

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 12:02
 Operator : DD\AJ
 Sample : L3611-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:31:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	11993241	17434204	12.401	12.038
27)	SA Decachlor...	7.842	8.861	17843751	19553131	16.941	14.258
Target Compounds							
9)	A Endosulfan I	0.000	6.019f	0	790942	N.D.	0.510
10)	B trans-Chl...	0.000	5.934	0	1544004	N.D.	0.927
11)	B cis-Chlor...	0.000	6.019	0	790942	N.D.	0.470
16)	A 4,4'-DDD	0.000	6.625f	0	2465423	N.D.	1.881


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 12:02
Operator : DD\AJ
Sample : L3611-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFM1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:31:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

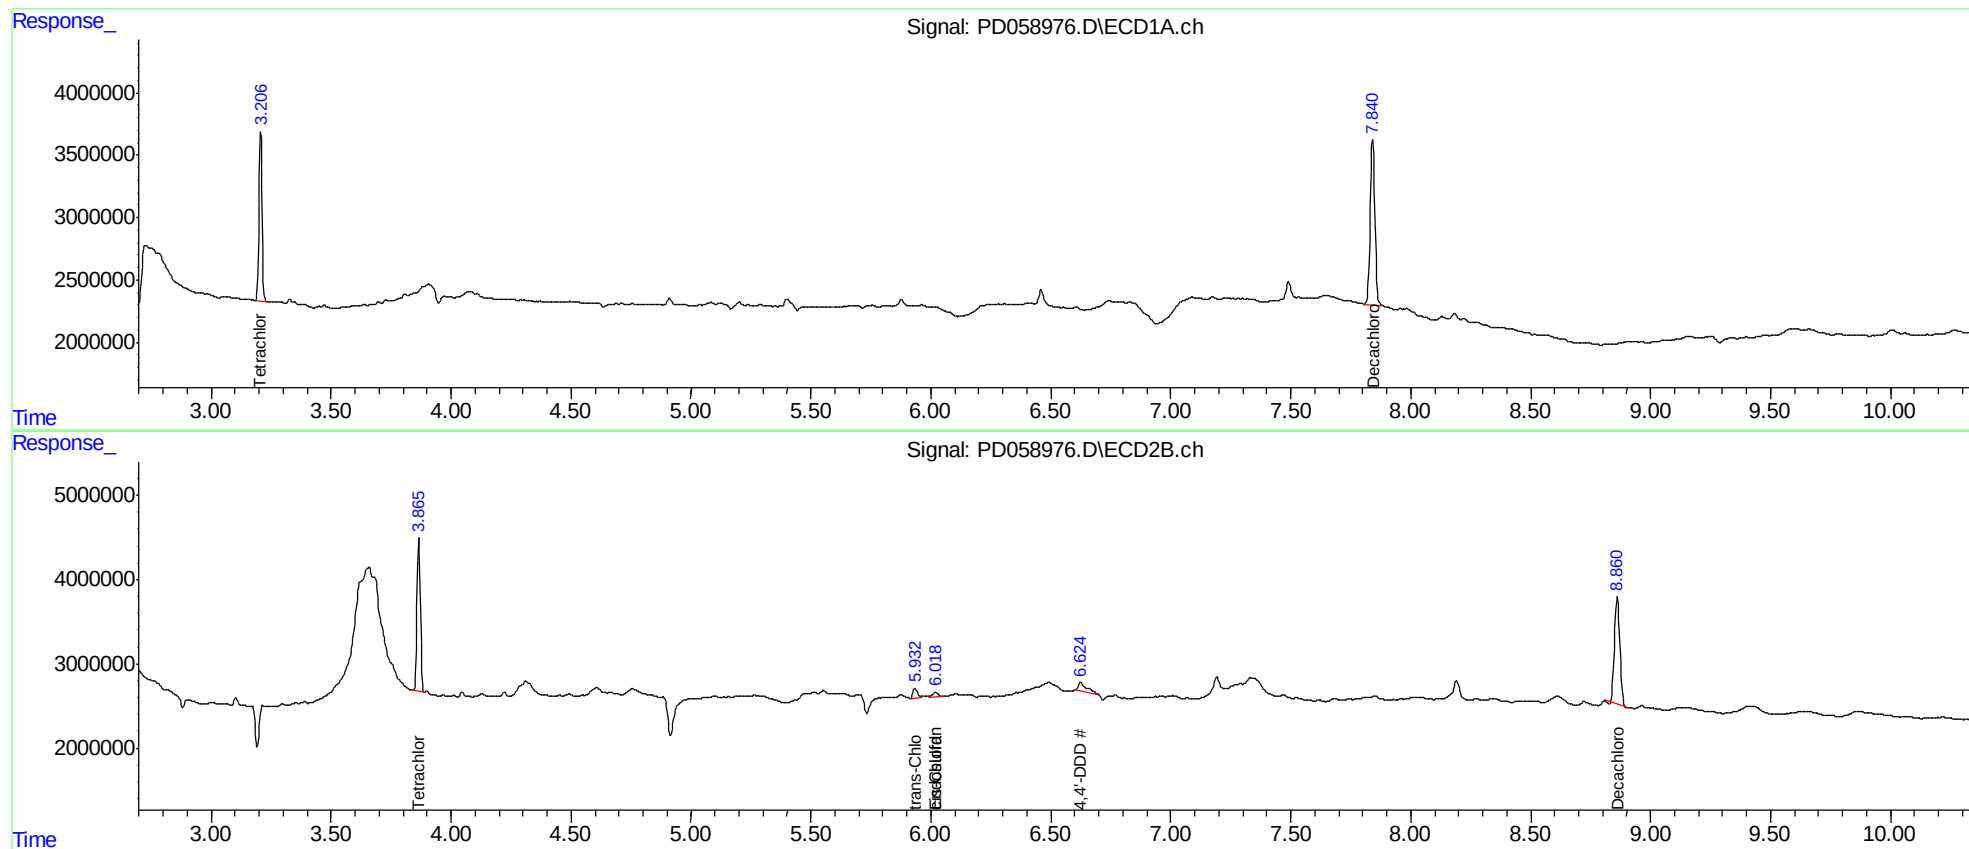


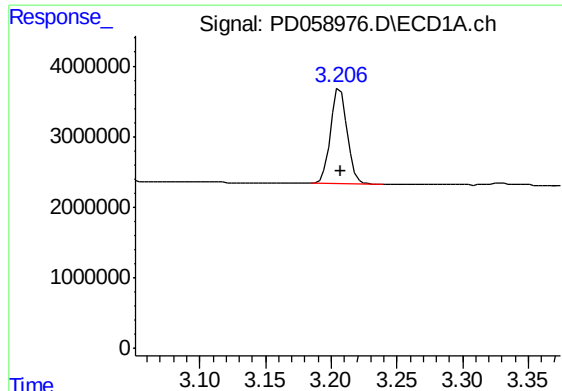

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 11993241
Conc: 12.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFM1

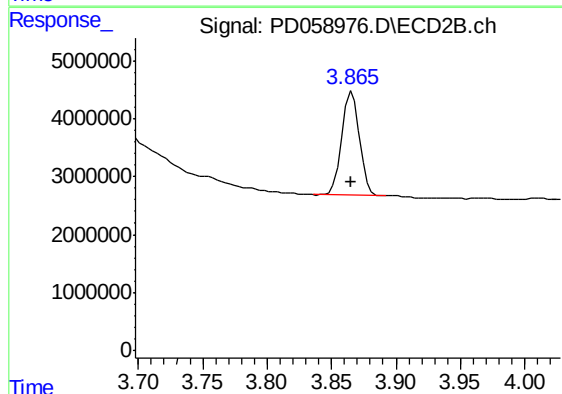


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.001 min
Response: 17434204
Conc: 12.04 ng/ml

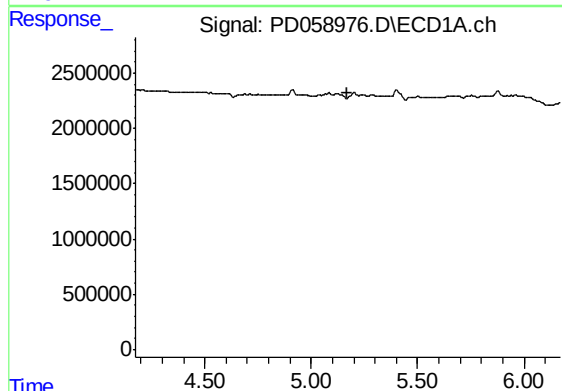


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

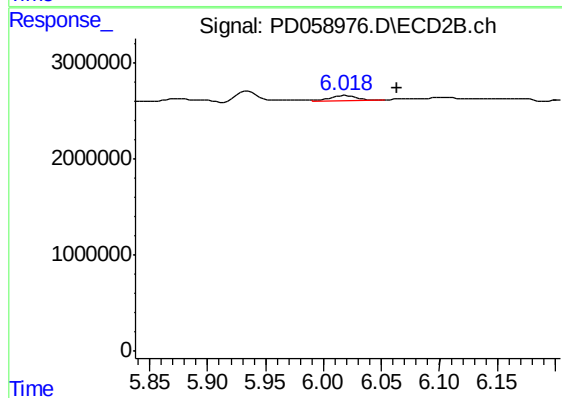

#9 Endosulfan I


R.T.: 6.019 min
Delta R.T.: -0.044 min
Response: 790942
Conc: 0.51 ng/ml

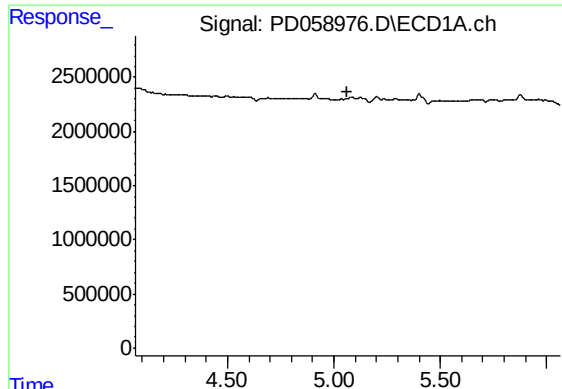

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFM1

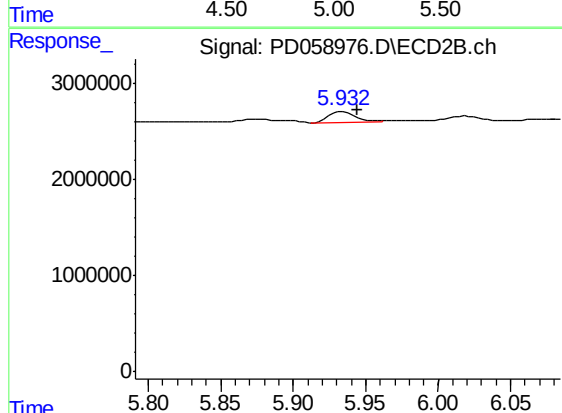


#10 trans-Chlordane

R.T.: 5.934 min
Delta R.T.: -0.010 min
Response: 1544004
Conc: 0.93 ng/ml

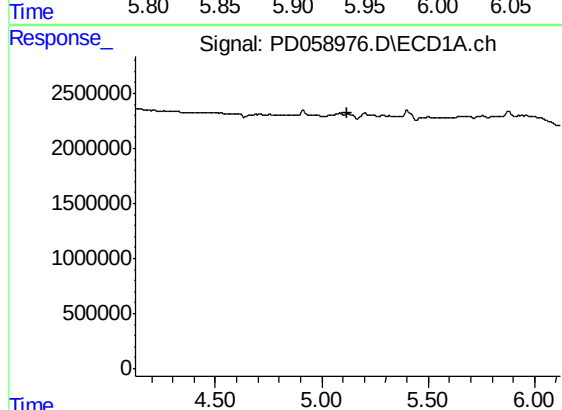


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

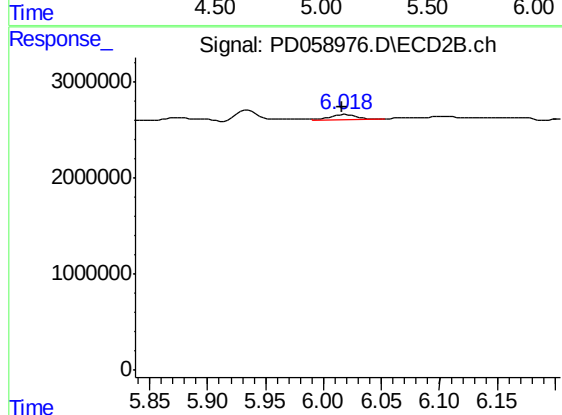

#11 cis-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.004 min
Response: 790942
Conc: 0.47 ng/ml

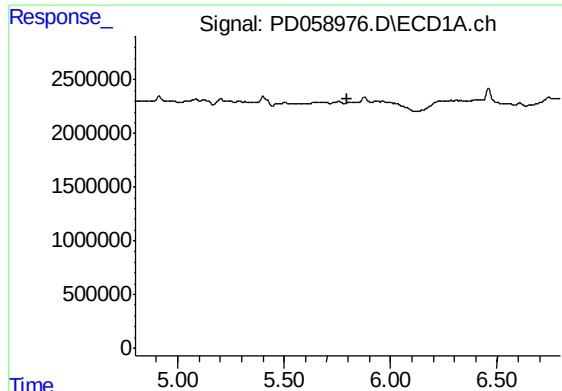

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFM1

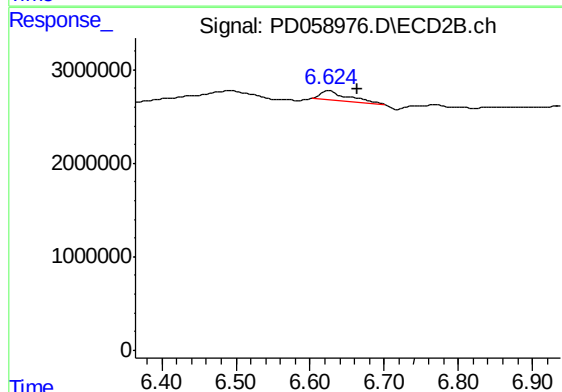


#16 4,4'-DDD

R.T.: 6.625 min
Delta R.T.: -0.038 min
Response: 2465423
Conc: 1.88 ng/ml

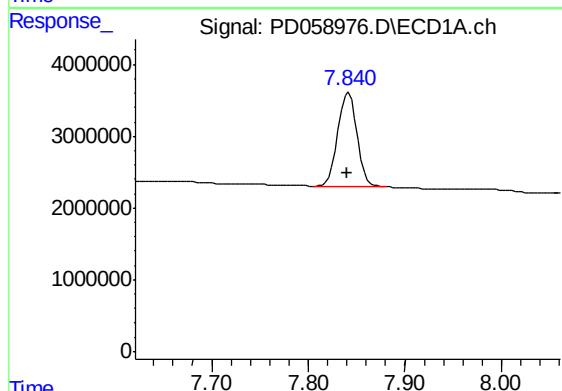

#27 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.001 min
Response: 17843751
Conc: 16.94 ng/ml

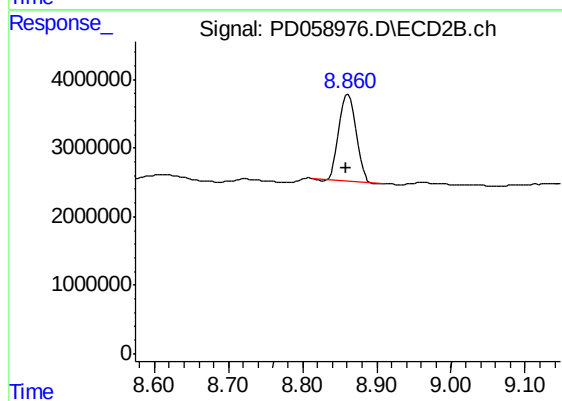

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.003 min
Response: 19553131
Conc: 14.26 ng/ml