

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 15:07
 Operator : DD\AJ
 Sample : L3611-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM0

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:38:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 06:40:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	17876908	26859893	18.485	18.547
27)	SA Decachlor...	7.841	8.861	36397003	48526400	34.555	35.384
Target Compounds							
8)	B Heptachlo...	4.843	5.712	664452	2511174	0.588m	1.508m#
10)	B trans-Chl...	5.067	5.932	4750360	50215539	4.108	30.145 #
11)	B cis-Chlor...	5.121	6.017	4235095	10375749	3.639m	6.163m#
12)	B 4,4'-DDE	5.292	6.174	13291271	15202548	11.551	9.593m
13)	MA Dieldrin	5.407	6.322	79835822	39350330	65.722	23.509 #
16)	A 4,4'-DDD	5.802	6.660	4308810	32731932	4.569m	24.970 #
17)	MA 4,4'-DDT	6.030	6.961	37417122	54938666	41.606m	41.632m
19)	B Endosulfa...	6.304	7.097	4207259	4884626	4.111	3.399

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 15:07
Operator : DD\AJ
Sample : L3611-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 06:40:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

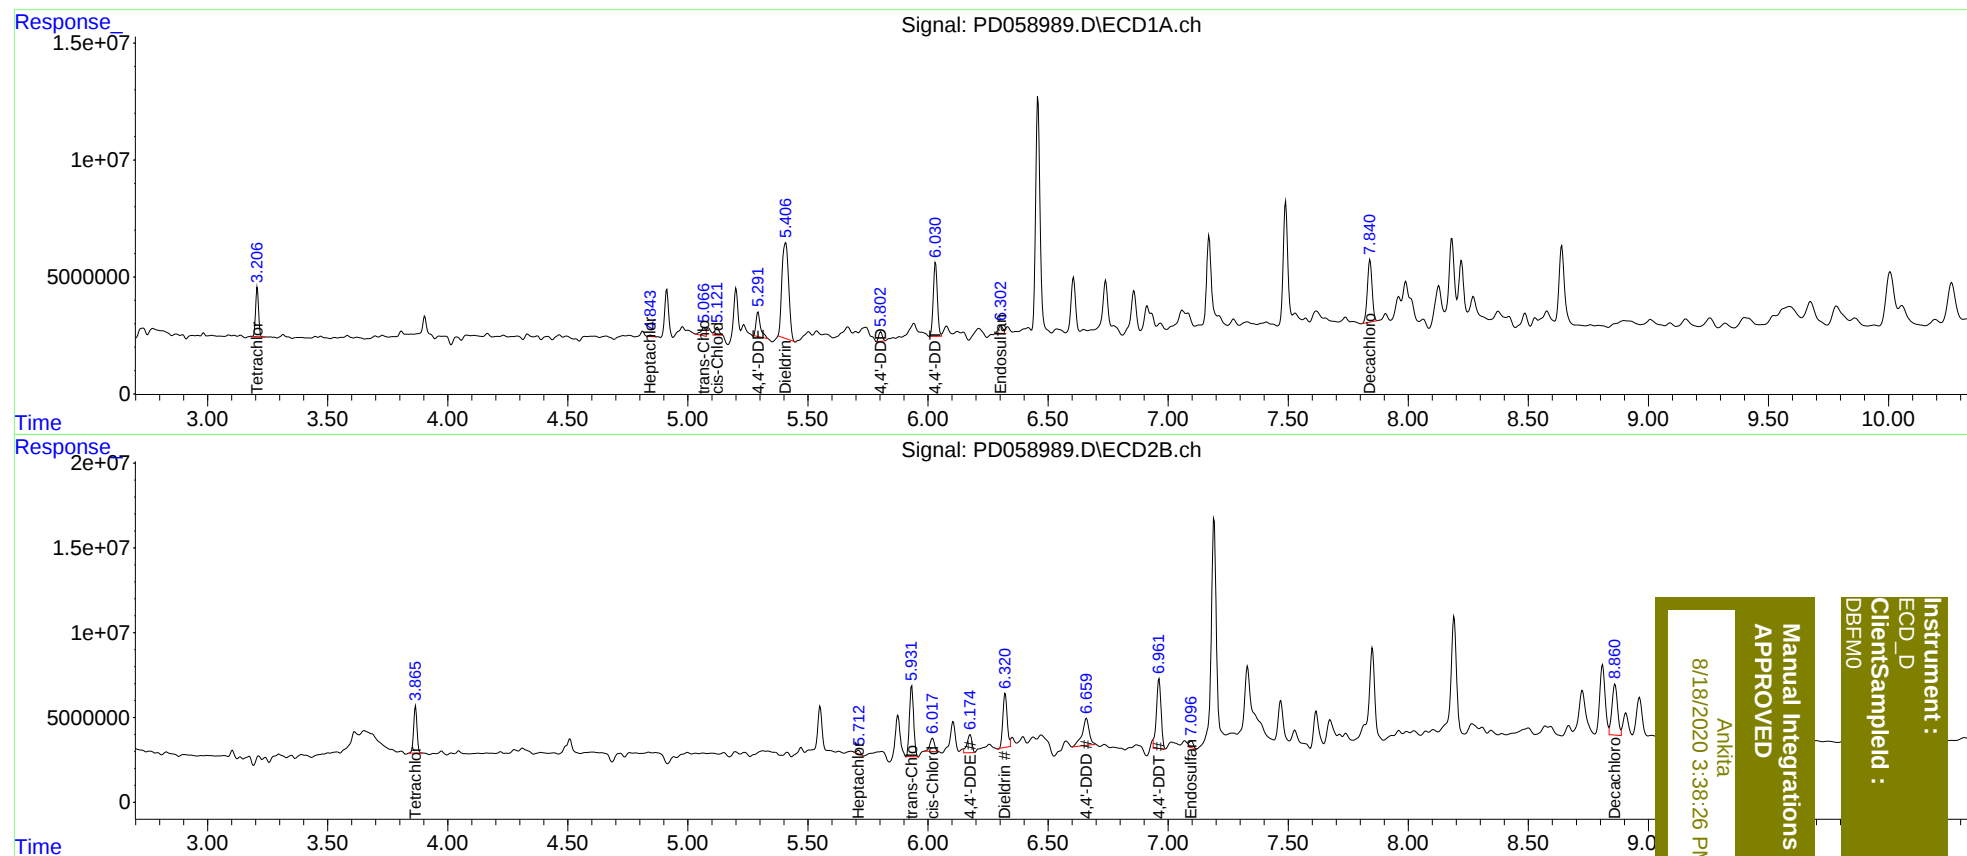

8/18/2020 3:38:26 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
DBFMO