

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 15:22
 Operator : DD\AJ
 Sample : L3611-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM3

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:38:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 06:59:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	12129267	16805424	12.542	11.604
27)	SA Decachlor...	7.840	8.860	22648989	29596391	21.503	21.581
Target Compounds							
8)	B Heptachlo...	4.845	5.708	732466	3683111	0.648m	2.212 #
10)	B trans-Chl...	5.071	5.932	1364598	71165992	1.180m	42.722 #
11)	B cis-Chlor...	5.111	6.021	3266705	11043829	2.807m	6.560 #
12)	B 4,4'-DDE	5.291	6.167	2679680	2581482	2.329m	1.629 #
14)	MA Endrin	5.664	6.534	1488557	1071249	1.498m	0.790m#
16)	A 4,4'-DDD	5.802	6.658	3757915	16647786	3.985m	12.700 #
17)	MA 4,4'-DDT	6.029	6.964	4210223	2441675	4.682m	1.850 #
19)	B Endosulfa...	6.305	7.099	4019492	4450486	3.928	3.097

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 15:22
Operator : DD\AJ
Sample : L3611-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 06:59:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

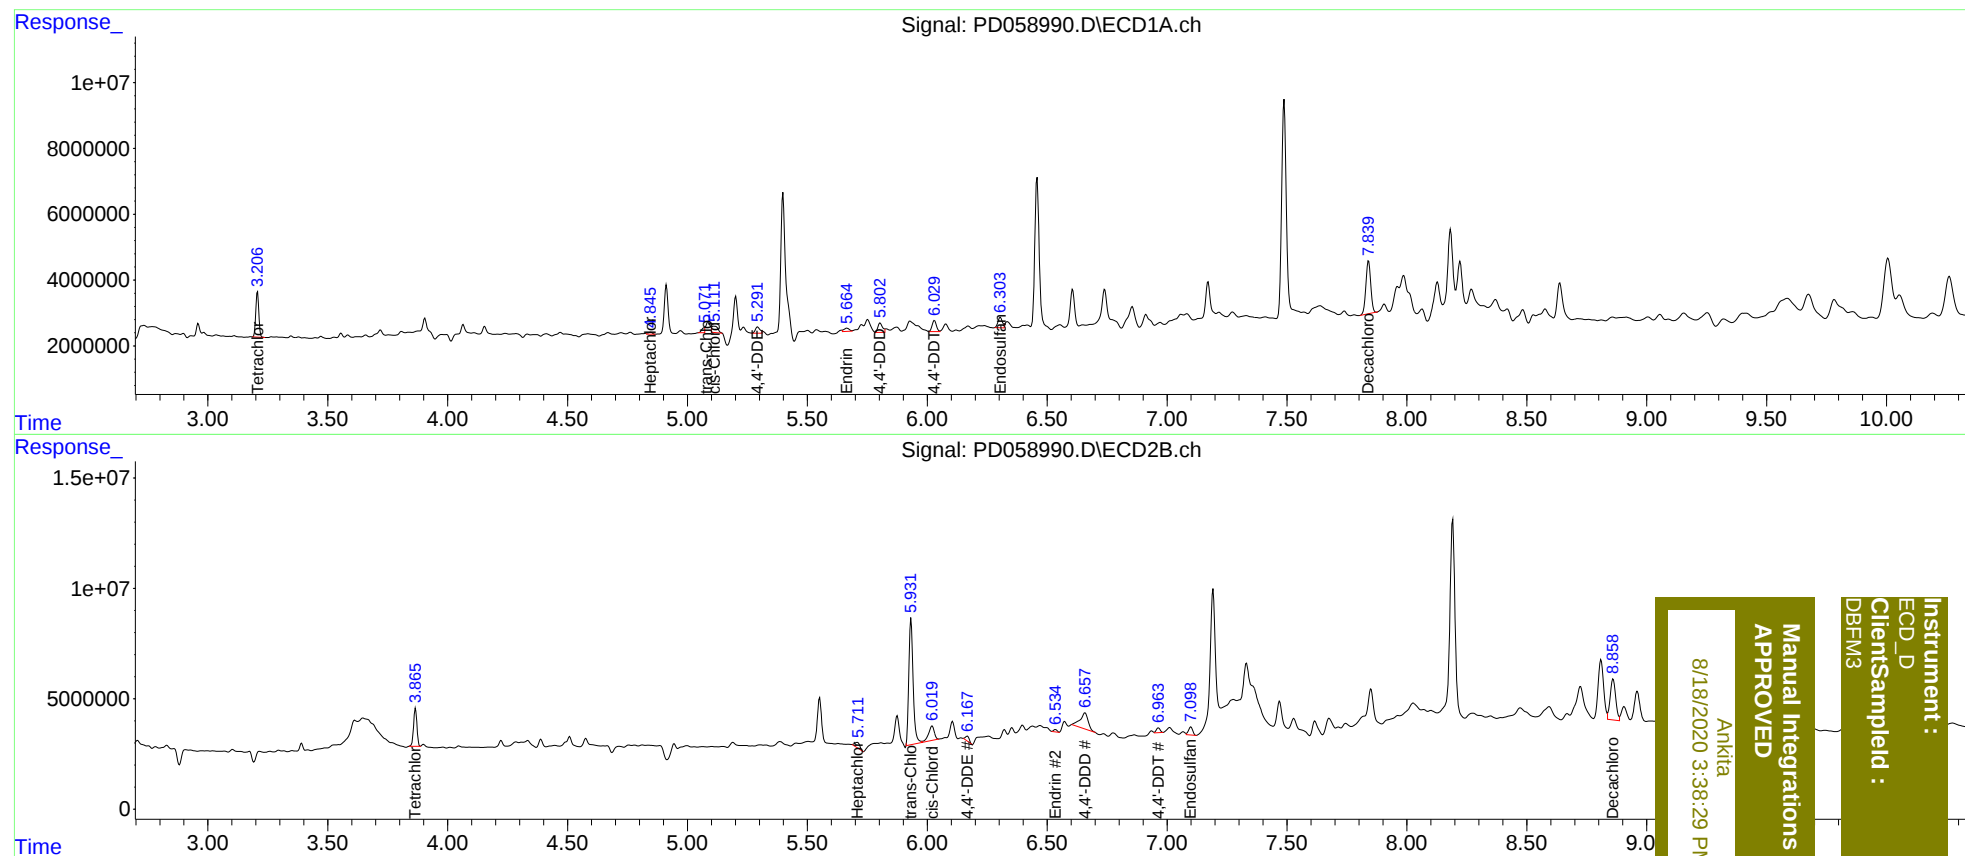

8/18/2020 3:38:29 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
DBFM3