

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
 Data File : PD058977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 12:16
 Operator : DD\AJ
 Sample : L3611-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM2

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:38:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:31:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	15529214	22662272	16.058	15.648
27)	SA Decachlor...	7.842	8.862	23922947	32368998	22.712	23.603
Target Compounds							
10)	B trans-Chl...	5.066	5.942	2071039	4974710	1.791m	2.986 #
11)	B cis-Chlor...	5.120	6.019	1503919	3435070	1.292m	2.040 #
12)	B 4,4'-DDE	5.290	6.175	1676797	1697741	1.457m	1.071m#
16)	A 4,4'-DDD	5.800	6.666	584844	1584965	0.620m	1.209 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081720\
Data File : PD058977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 12:16
Operator : DD\AJ
Sample : L3611-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:31:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

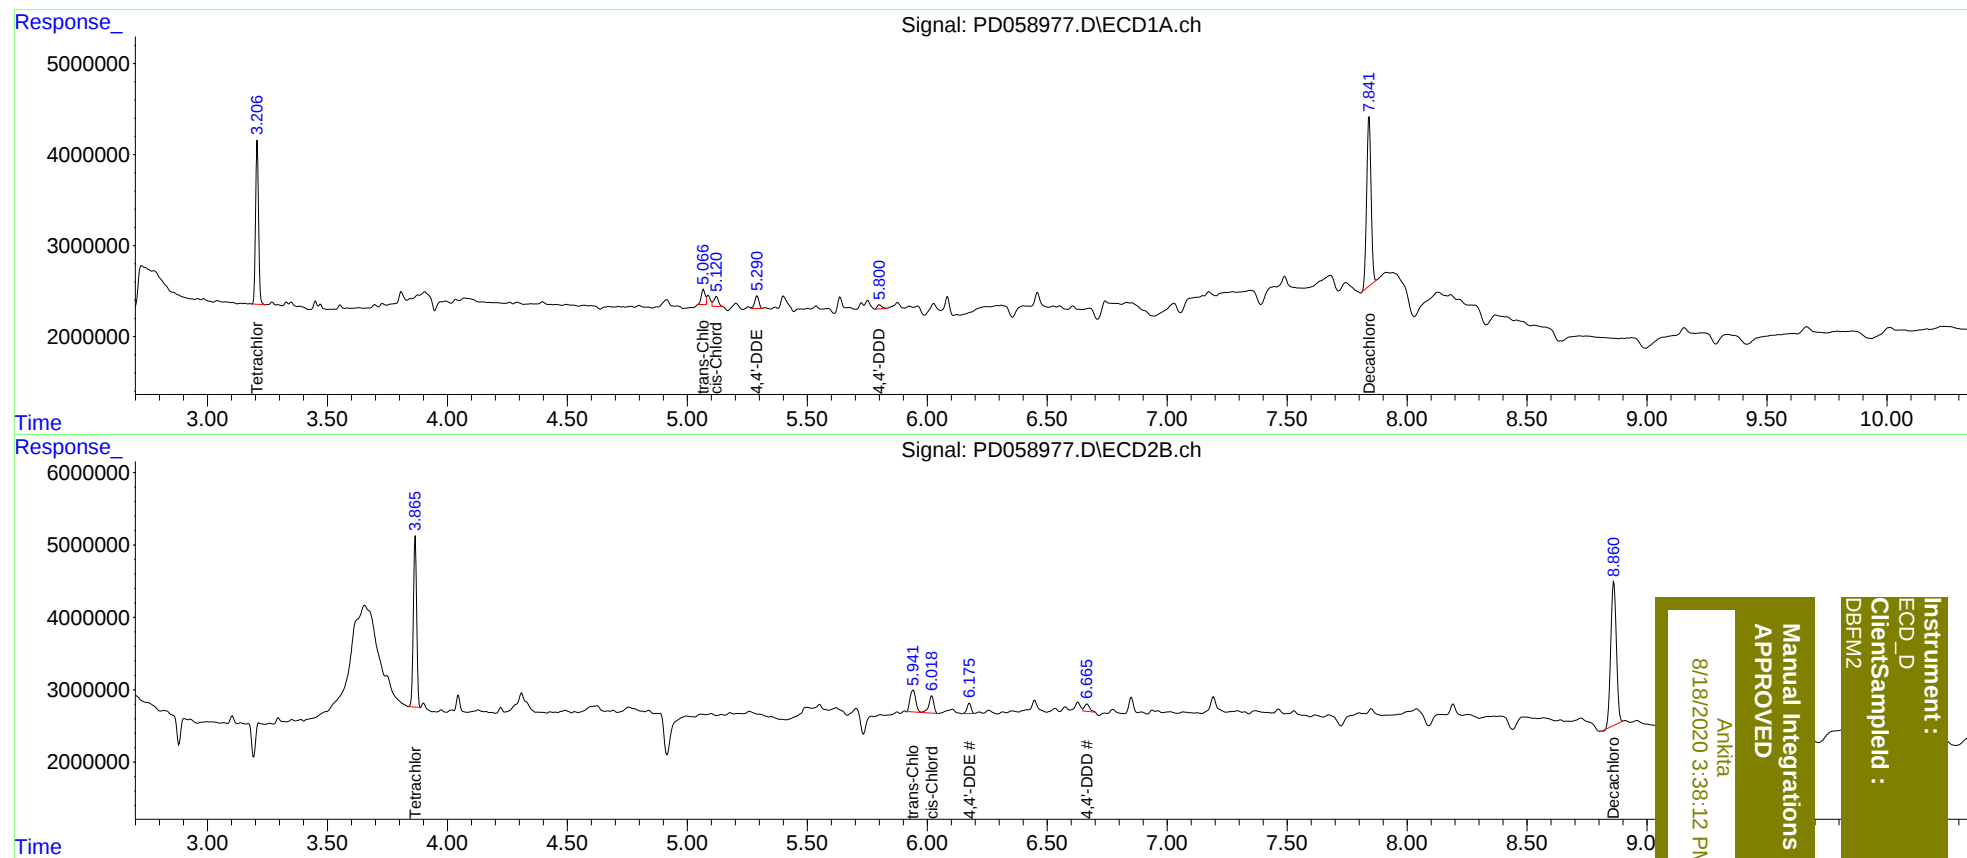

Instrument :
ECD_D
ClientSampled :
DBFM2

8/18/2020 3:38:12 PM
Ankita

Manual Integrations
APPROVED