

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 16:26
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 02:03:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:03:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	5144194	42044218	5.333	5.438
27)	SA Decachlor...	8.243	9.084	11022060	49969198	11.052	10.706
Target Compounds							
2)	A alpha-BHC	3.937	4.408	6677995	54879837	5.089	5.085
3)	MA gamma-BHC...	4.220	4.695	7409408	53222220	5.750	5.282
4)	MA Heptachlor	4.519	5.199	6262543	49512123	5.267	5.350
9)	A Endosulfan I	5.547	6.251	5307878	36180723	5.202	5.320
13)	MA Dieldrin	5.790	6.509	10834046	72437508	10.167	10.330
14)	MA Endrin	6.048	6.729	9554135	56464711	10.341	10.132
16)	A 4,4'-DDD	6.170	6.851	8437593	52619878	9.980	9.714
17)	MA 4,4'-DDT	6.411	7.149	8726963	53431229	9.827	9.766
20)	A Methoxychlor	6.957	7.608	23324162	132.9E6	50.734	52.998


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 16:26
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:03:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:03:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

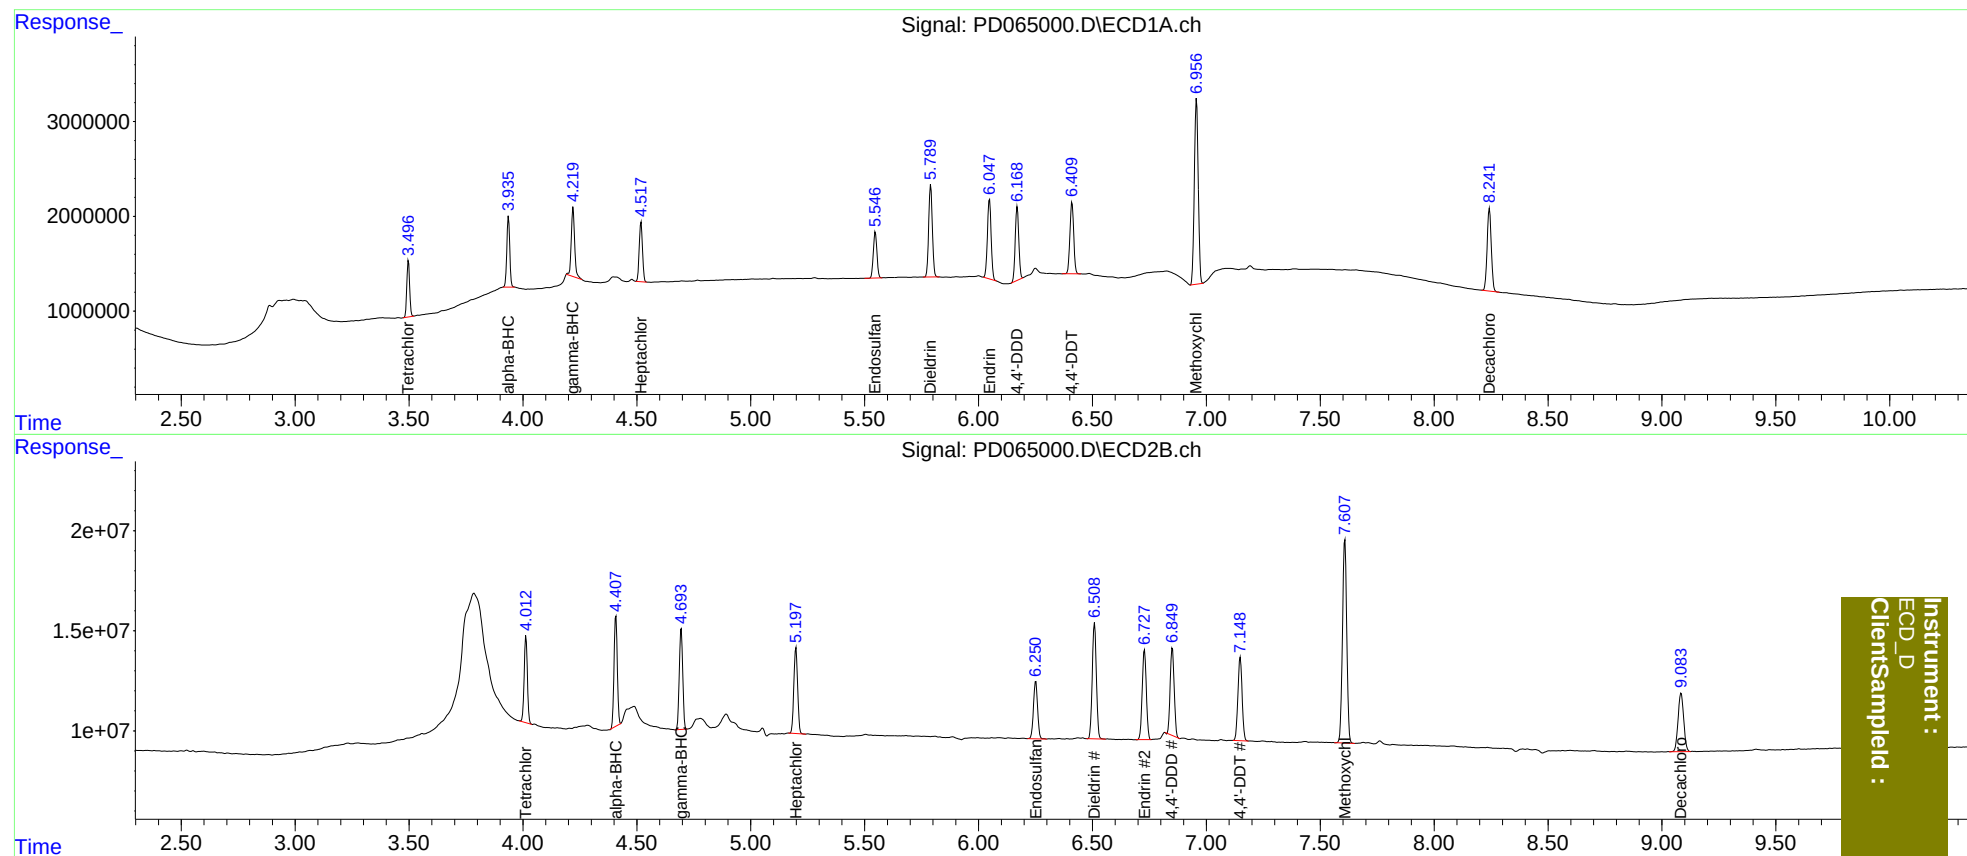


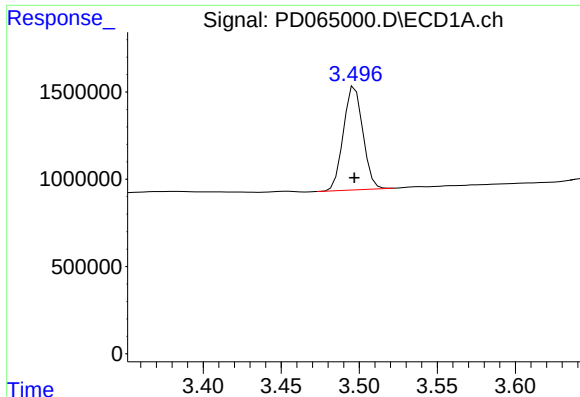

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 5144194
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

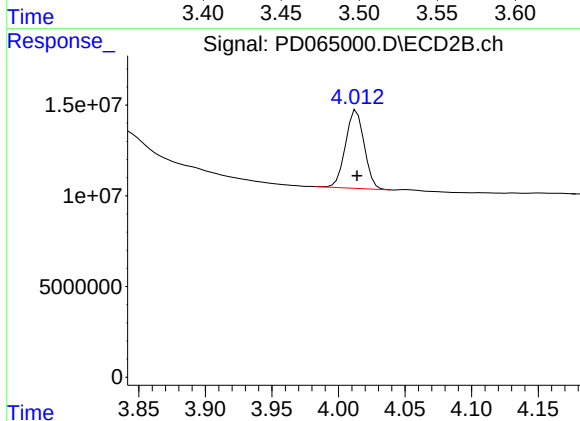


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 42044218
Conc: 5.44 ng/ml

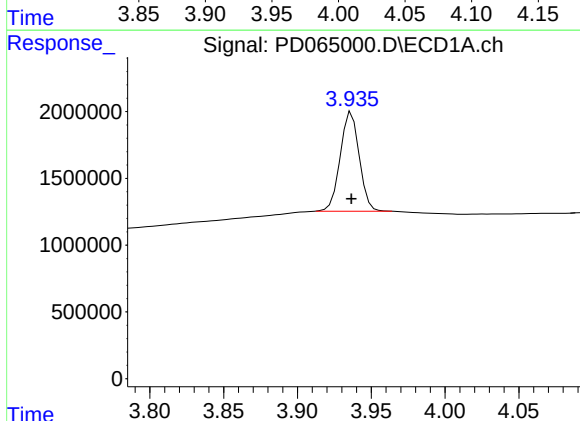


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 6677995
Conc: 5.09 ng/ml

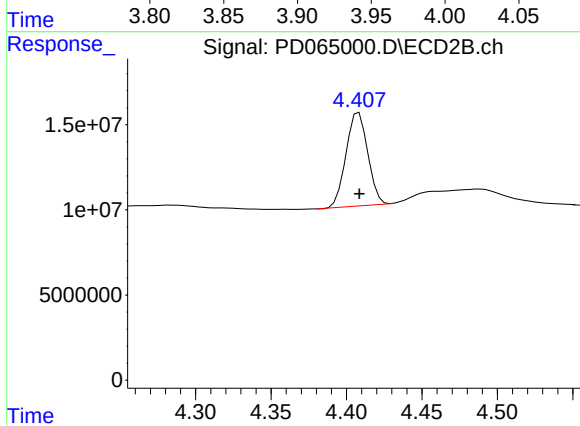

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 54879837
Conc: 5.08 ng/ml

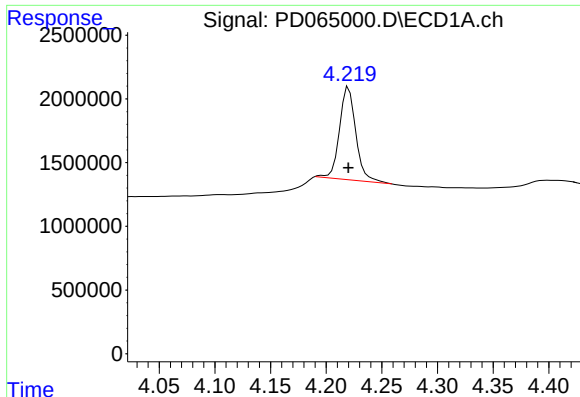

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 7409408
Conc: 5.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

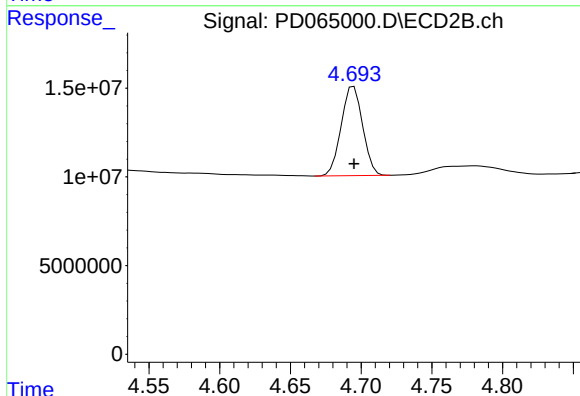


#3 gamma-BHC (Lindane)

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 53222220
Conc: 5.28 ng/ml

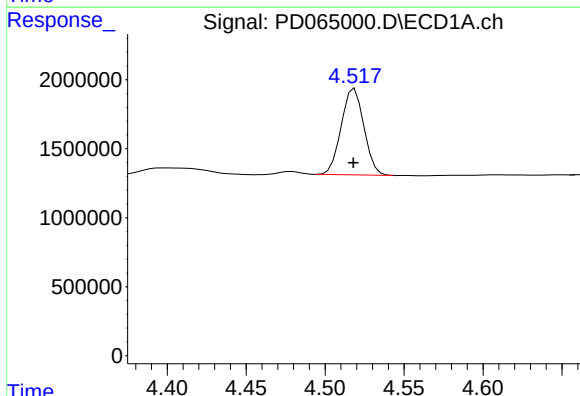


#4 Heptachlor

R.T.: 4.519 min
Delta R.T.: 0.000 min
Response: 6262543
Conc: 5.27 ng/ml

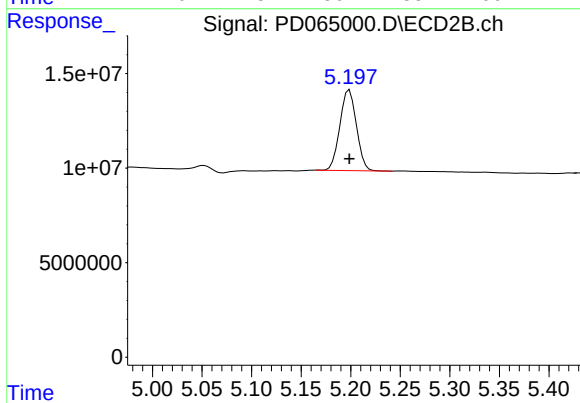

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 49512123
Conc: 5.35 ng/ml

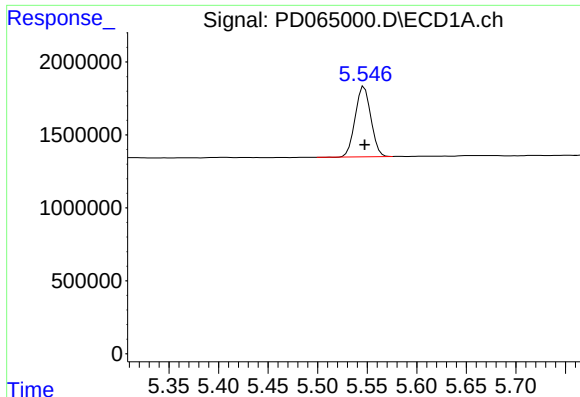

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 5307878
Conc: 5.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

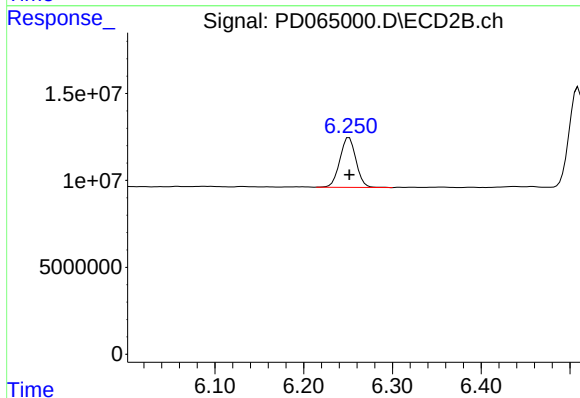


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 36180723
Conc: 5.32 ng/ml

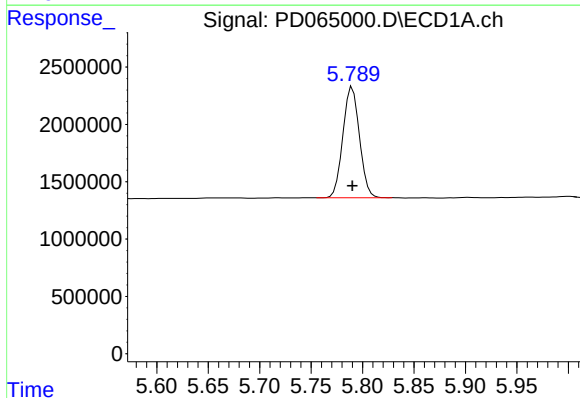


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 10834046
Conc: 10.17 ng/ml

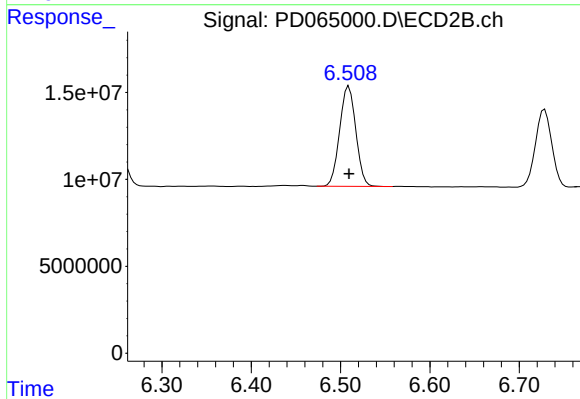

#13 Dieldrin


R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 72437508
Conc: 10.33 ng/ml

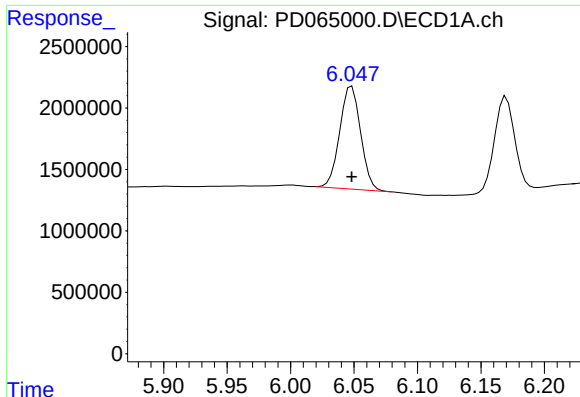

#14 Endrin


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 9554135
Conc: 10.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

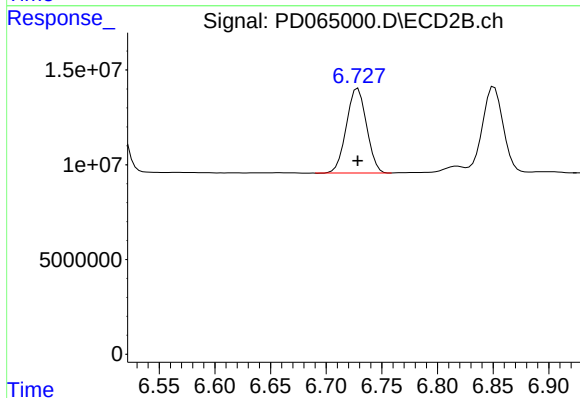


#14 Endrin

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 56464711
Conc: 10.13 ng/ml

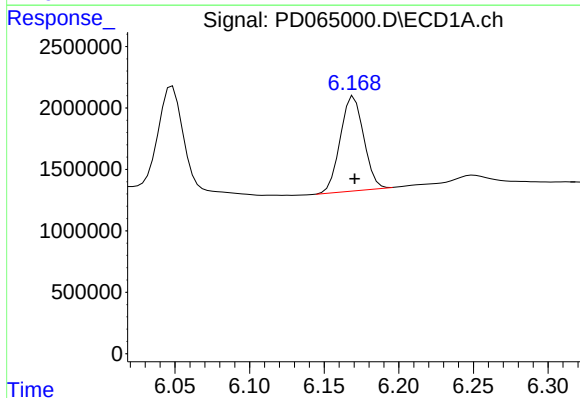


#16 4,4'-DDD

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 8437593
Conc: 9.98 ng/ml

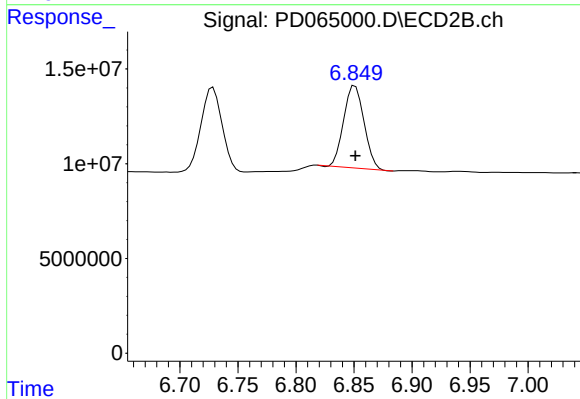

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 52619878
Conc: 9.71 ng/ml

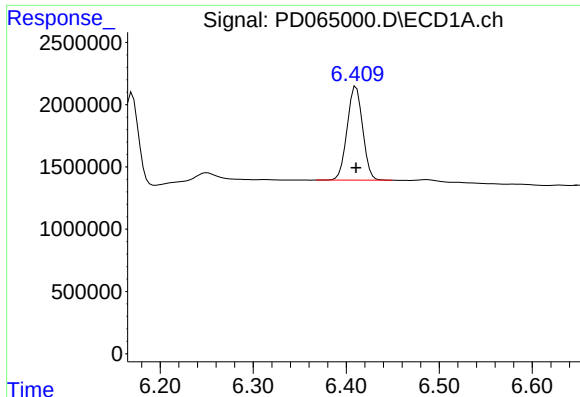

#17 4,4'-DDT


R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 8726963
Conc: 9.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

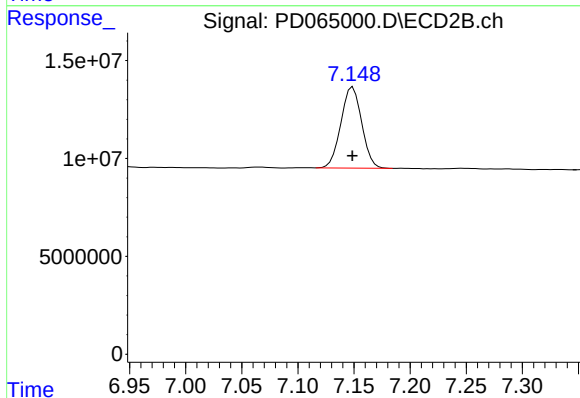


#17 4,4'-DDT

R.T.: 7.149 min
Delta R.T.: 0.000 min
Response: 53431229
Conc: 9.77 ng/ml

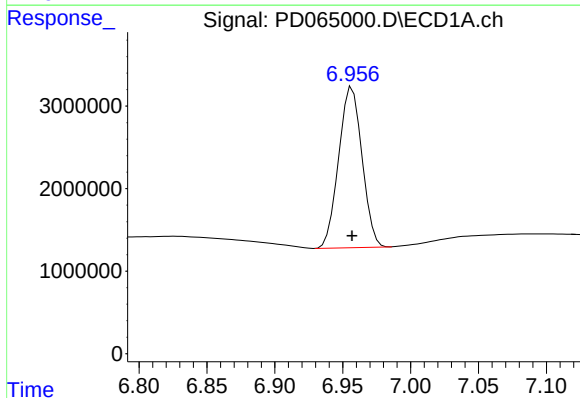


#20 Methoxychlor

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 23324162
Conc: 50.73 ng/ml

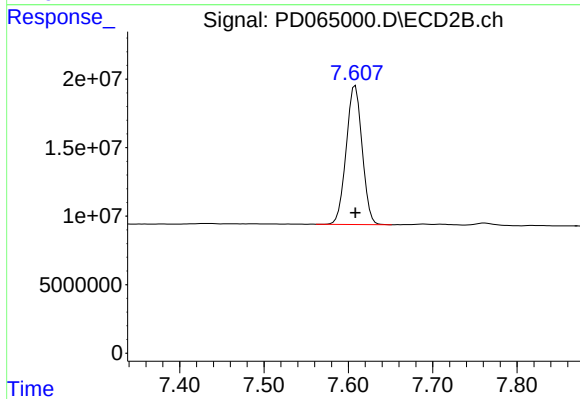

#20 Methoxychlor


R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 132946014
Conc: 53.00 ng/ml

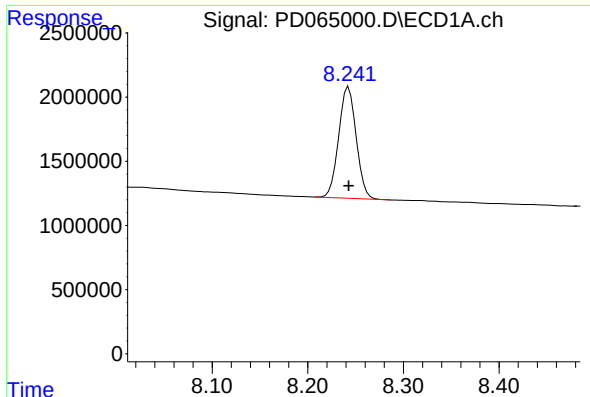

#27 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 11022060
Conc: 11.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

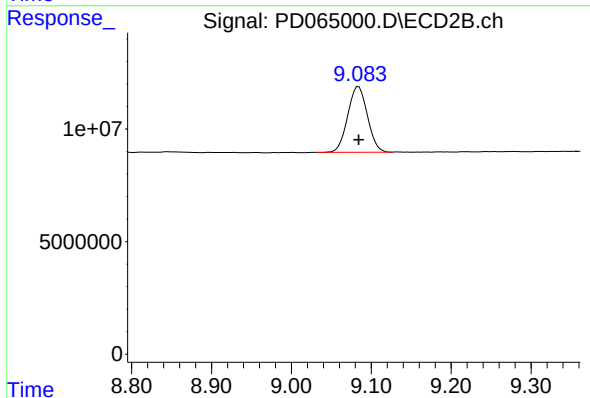

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 49969198
Conc: 10.71 ng/ml