

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 16:54
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 02:03:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:03:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.013	10092075	82036149	10.463	10.611
27)	SA Decachlor...	8.242	9.084	21344624	98443867	21.402	21.092
Target Compounds							
2)	A alpha-BHC	3.937	4.408	13175854	110.8E6	10.040	10.267
3)	MA gamma-BHC...	4.220	4.695	13376615	105.6E6	10.380	10.484
4)	MA Heptachlor	4.518	5.198	12394578	98063088	10.424	10.596
9)	A Endosulfan I	5.547	6.251	10637289	71205084	10.425	10.470
13)	MA Dieldrin	5.790	6.509	21642322	145.6E6	20.310	20.764
14)	MA Endrin	6.048	6.728	19016463	112.7E6	20.583	20.223
16)	A 4,4'-DDD	6.170	6.850	17017346	109.7E6	20.128	20.261
17)	MA 4,4'-DDT	6.410	7.148	17873076	110.9E6	20.127	20.262
20)	A Methoxychlor	6.957	7.607	47378064	263.9E6	103.055	105.202

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 16:54
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:03:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:03:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

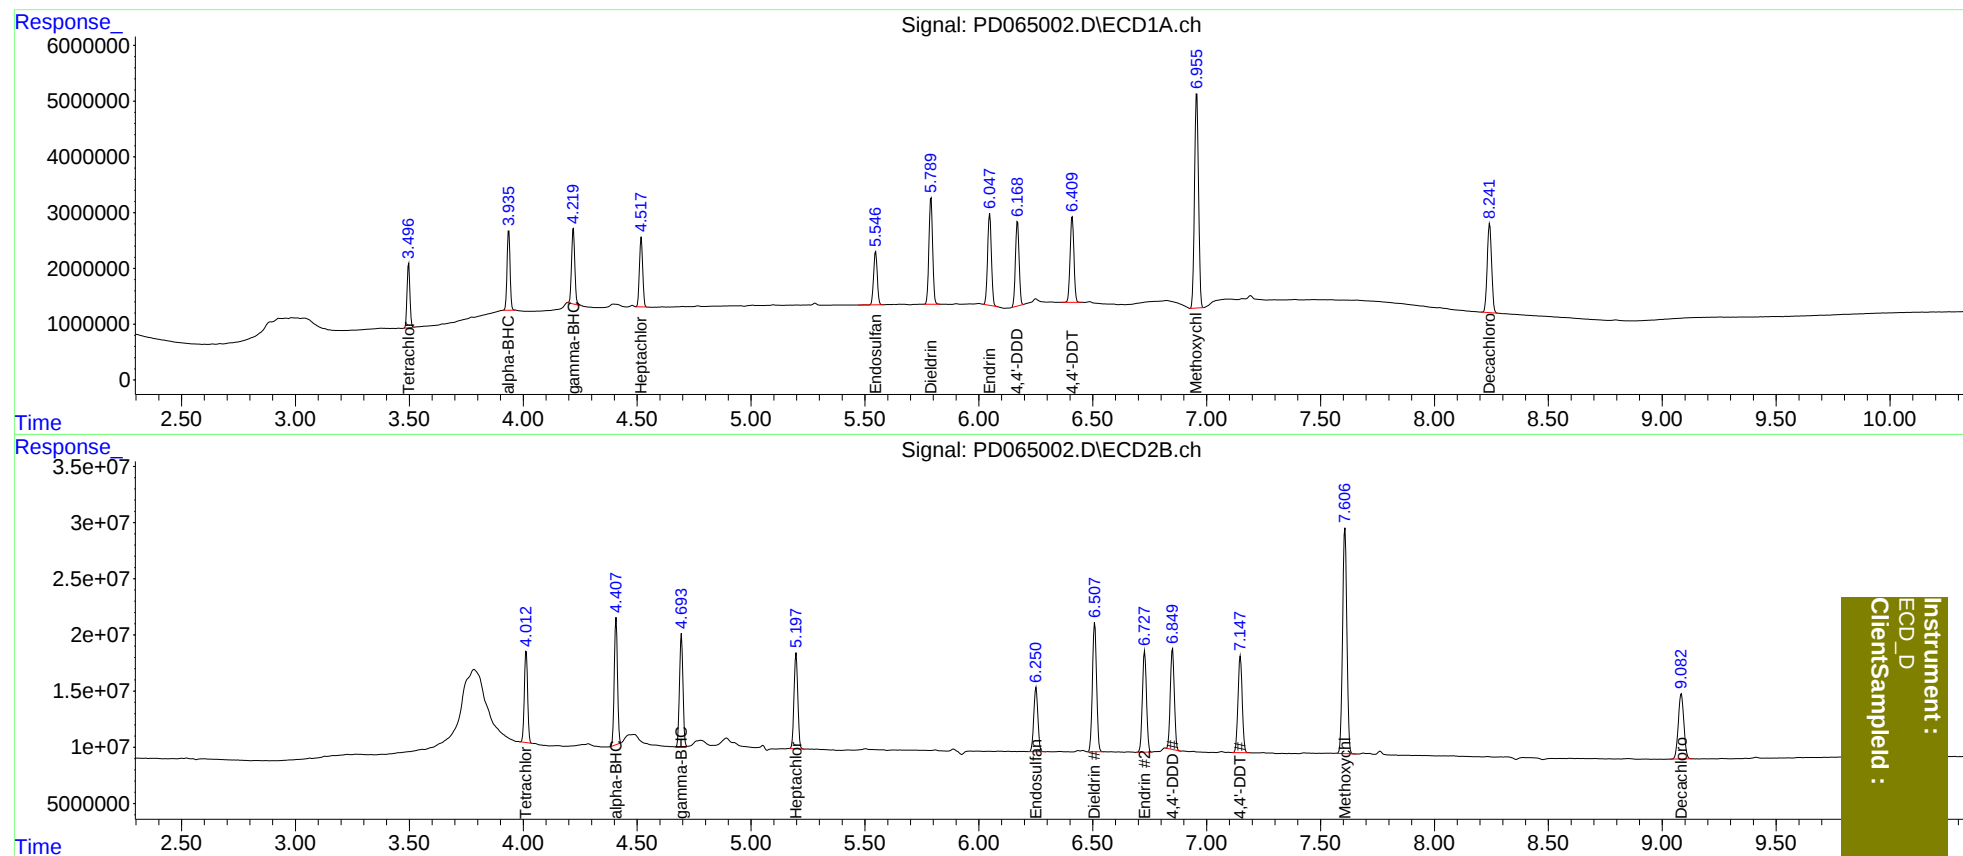


Instrument :
ECD_D
ClientSample : INDA201

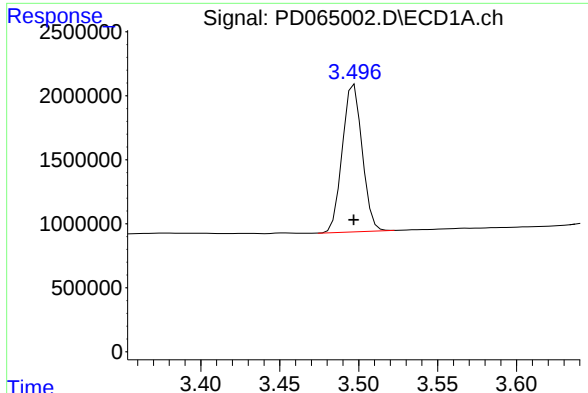

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 10092075
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

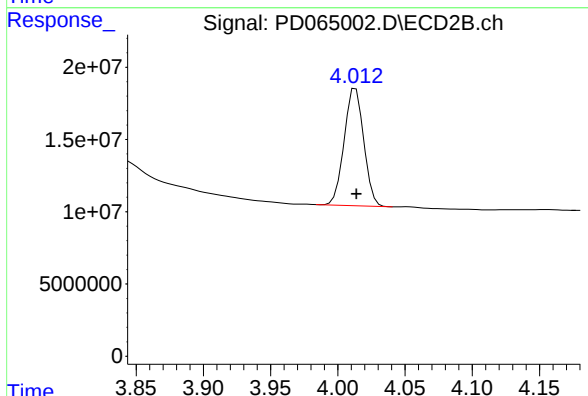


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 82036149
Conc: 10.61 ng/ml

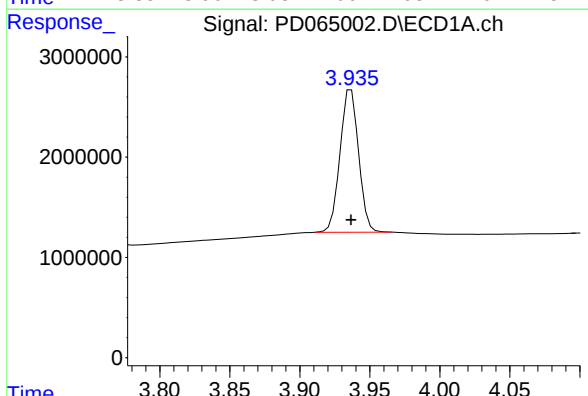


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 13175854
Conc: 10.04 ng/ml

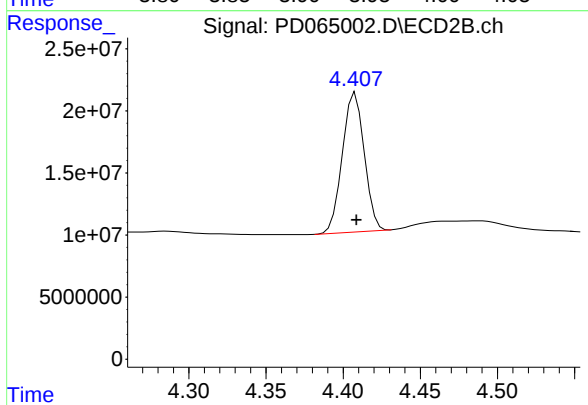

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 110816056
Conc: 10.27 ng/ml

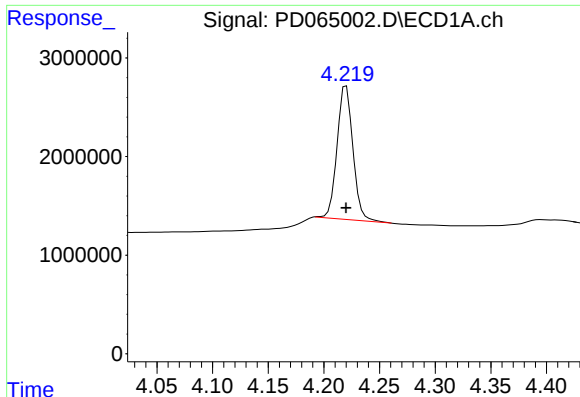

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 13376615
Conc: 10.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

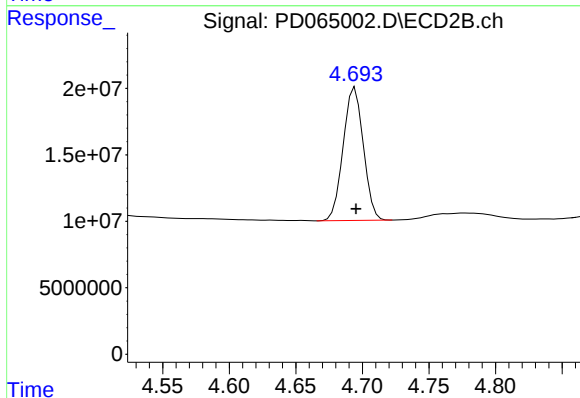


#3 gamma-BHC (Lindane)

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 105649251
Conc: 10.48 ng/ml

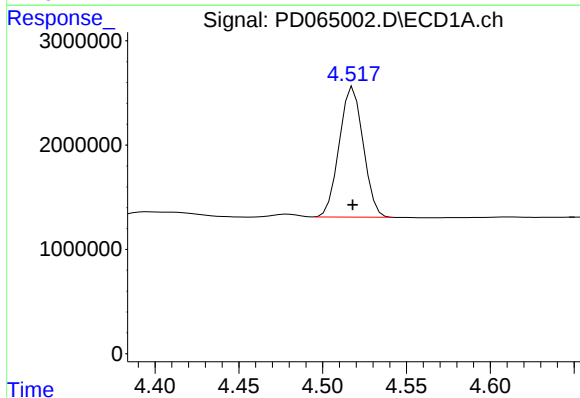


#4 Heptachlor

R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 12394578
Conc: 10.42 ng/ml

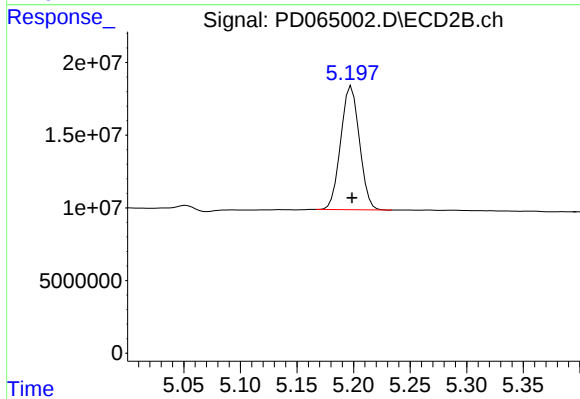

#4 Heptachlor


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 98063088
Conc: 10.60 ng/ml

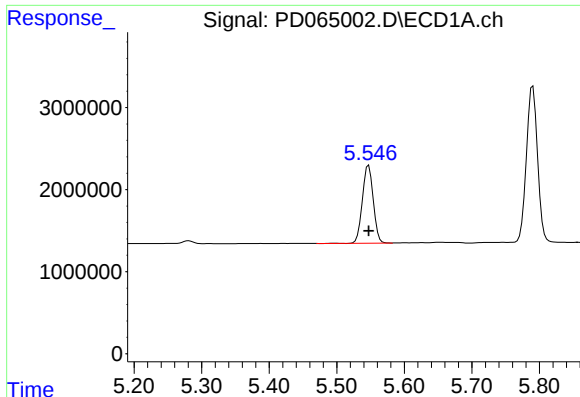

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 10637289
Conc: 10.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

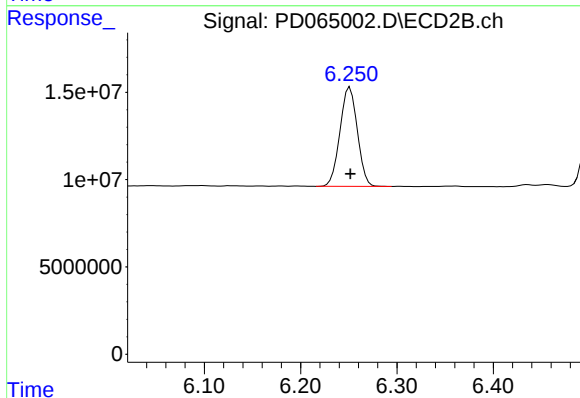


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 71205084
Conc: 10.47 ng/ml

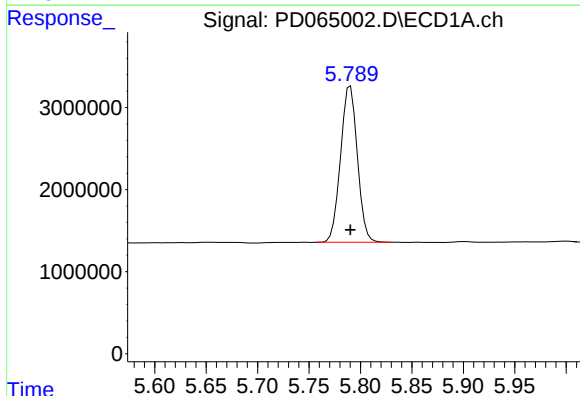


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 21642322
Conc: 20.31 ng/ml

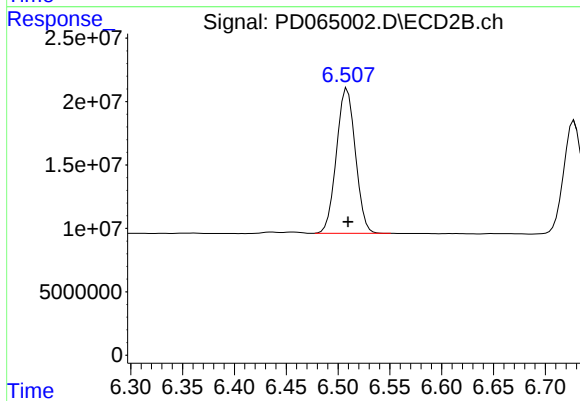

#13 Dieldrin


R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 145600875
Conc: 20.76 ng/ml

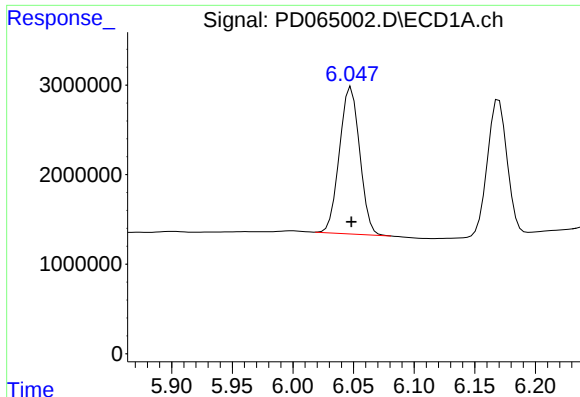

#14 Endrin


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 19016463
Conc: 20.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

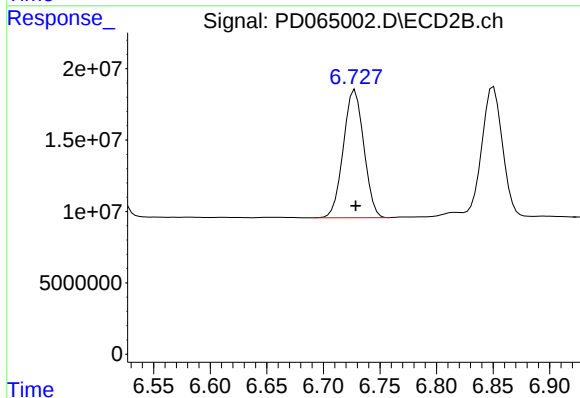


#14 Endrin

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 112705183
Conc: 20.22 ng/ml

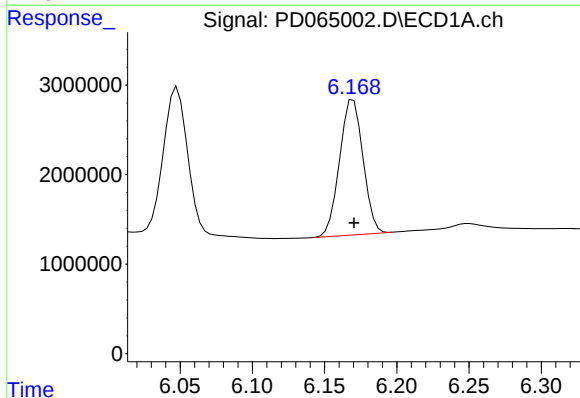


#16 4,4'-DDD

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 17017346
Conc: 20.13 ng/ml

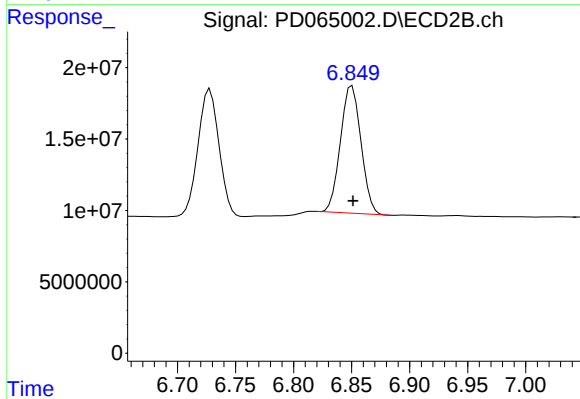

#16 4,4'-DDD


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 109746312
Conc: 20.26 ng/ml

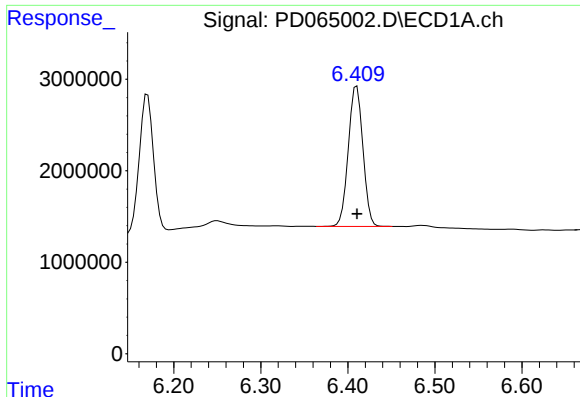

#17 4,4'-DDT


R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 17873076
Conc: 20.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

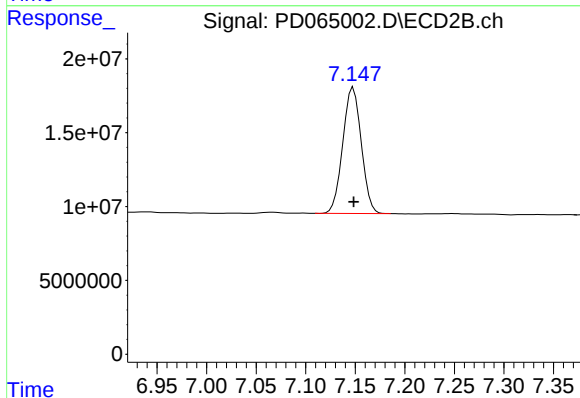


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 110850726
Conc: 20.26 ng/ml

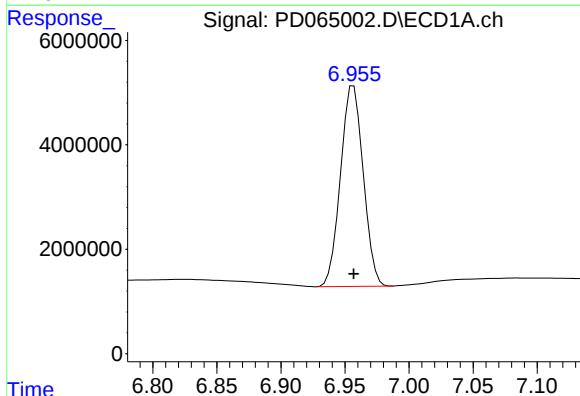


#20 Methoxychlor

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 47378064
Conc: 103.06 ng/ml

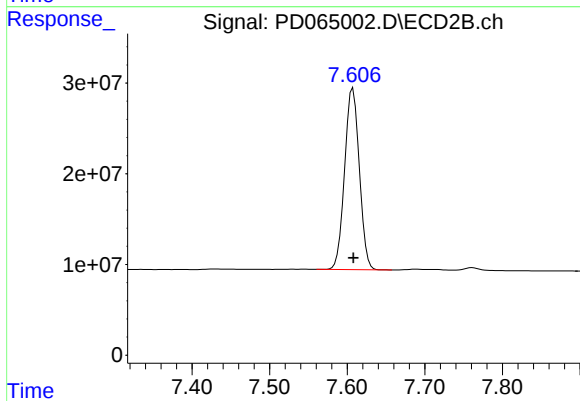

#20 Methoxychlor


R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 263901024
Conc: 105.20 ng/ml

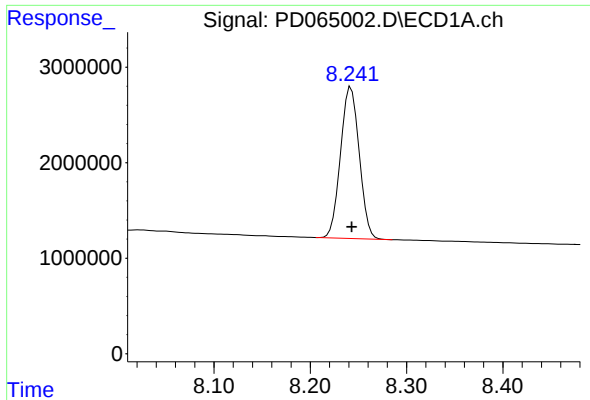

#27 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: 0.000 min
Response: 21344624
Conc: 21.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

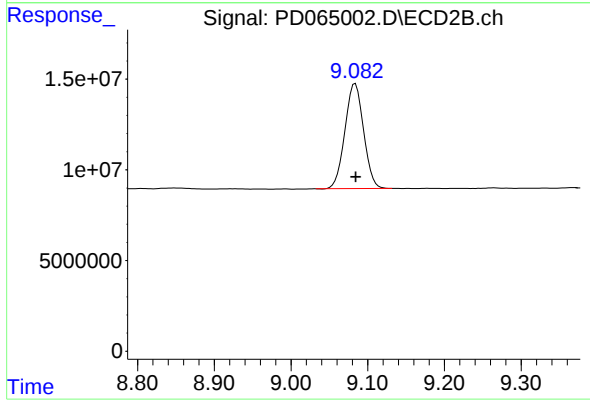

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 98443867
Conc: 21.09 ng/ml