

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 17:22
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 02:04:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:03:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	19291485	154.6E6	20.000	20.000
27)	SA Decachlor...	8.243	9.084	39893339	186.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.937	4.409	26245664	215.9E6	20.000	20.000
3)	MA gamma-BHC...	4.220	4.695	25772771	201.5E6	20.000	20.000
4)	MA Heptachlor	4.518	5.199	23781585	185.1E6	20.000	20.000
9)	A Endosulfan I	5.547	6.252	20408070	136.0E6	20.000	20.000
13)	MA Dieldrin	5.790	6.510	42624605	280.5E6	40.000	40.000
14)	MA Endrin	6.048	6.729	36955244	222.9E6	40.000	40.000
16)	A 4,4'-DDD	6.170	6.851	33818326	216.7E6	40.000	40.000
17)	MA 4,4'-DDT	6.411	7.148	35520687	218.8E6	40.000	40.000
20)	A Methoxychlor	6.957	7.608	91946999	501.7E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 17:22
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:04:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:03:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

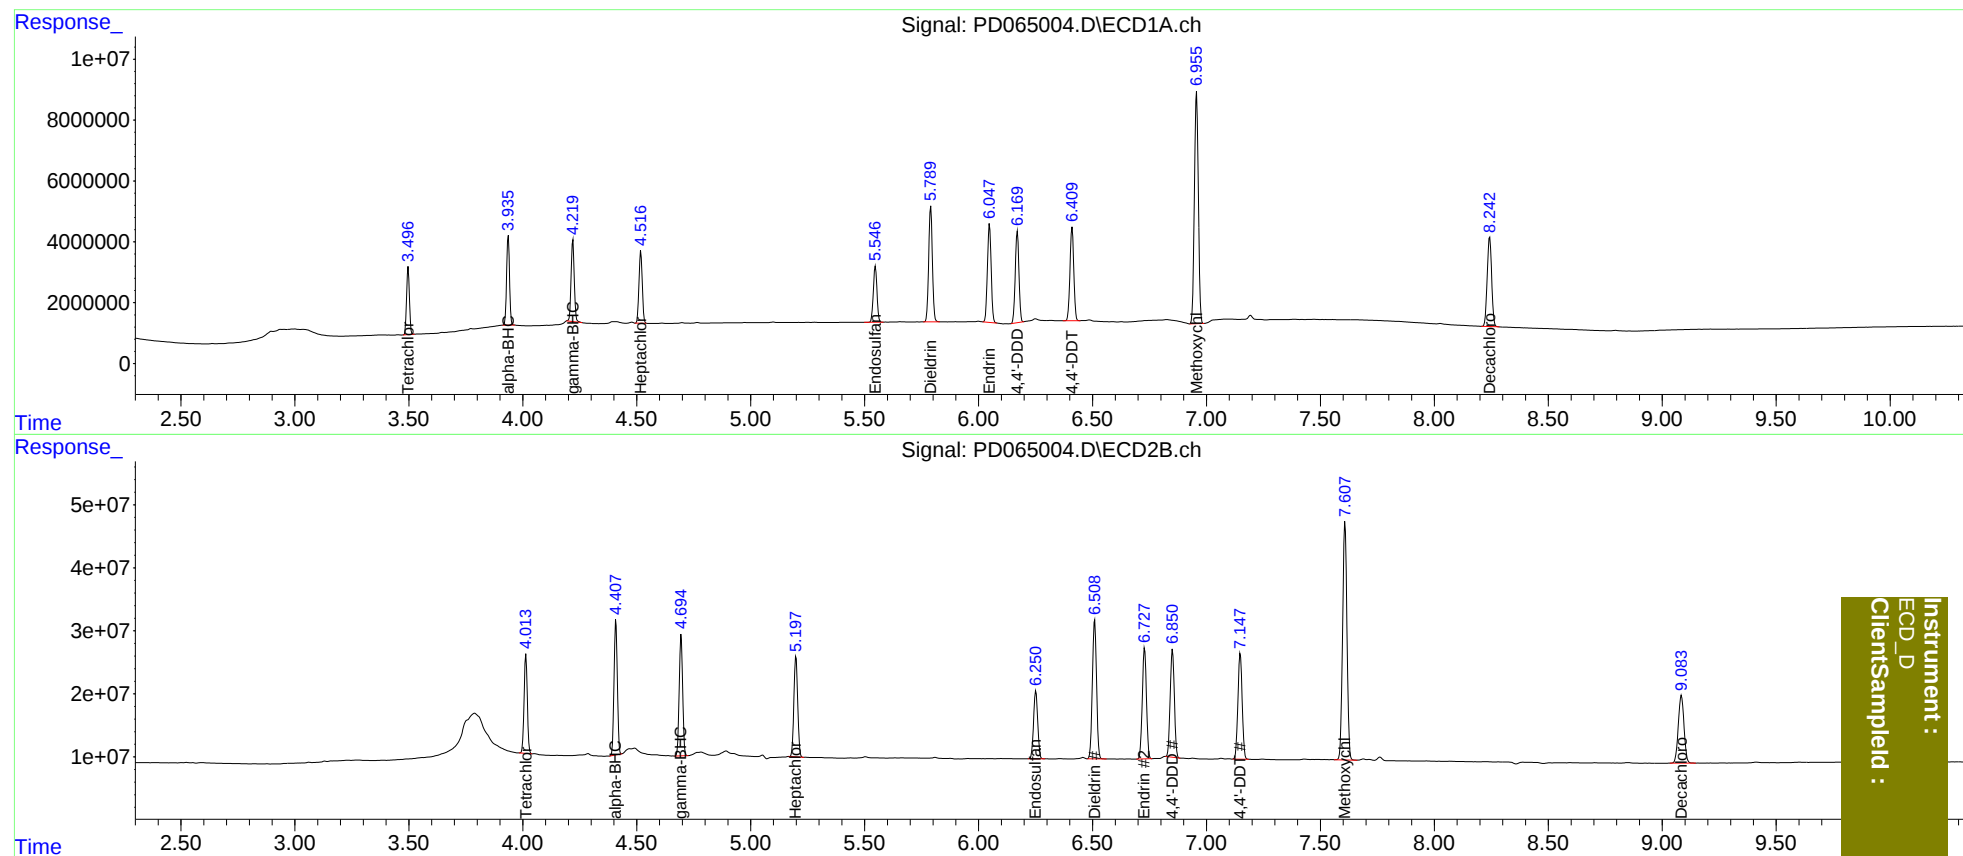


Instrument :
ECD_D
ClientSample :
Sample

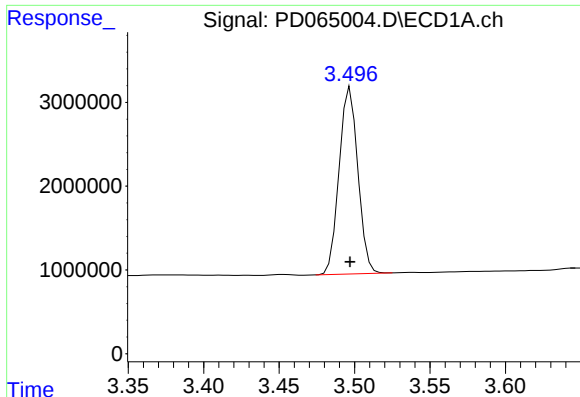

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 19291485
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

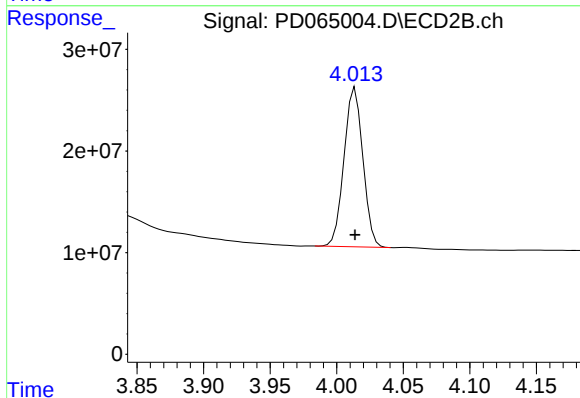


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 154631868
Conc: 20.00 ng/ml

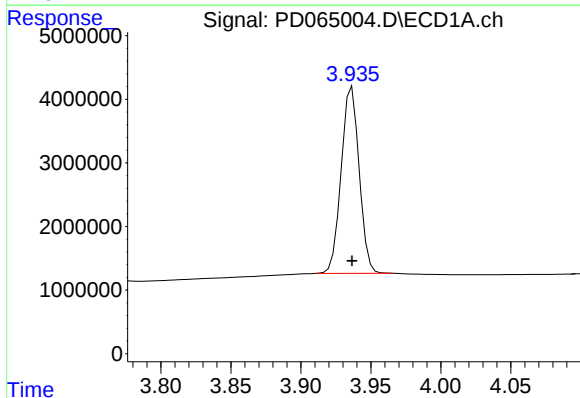


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 26245664
Conc: 20.00 ng/ml

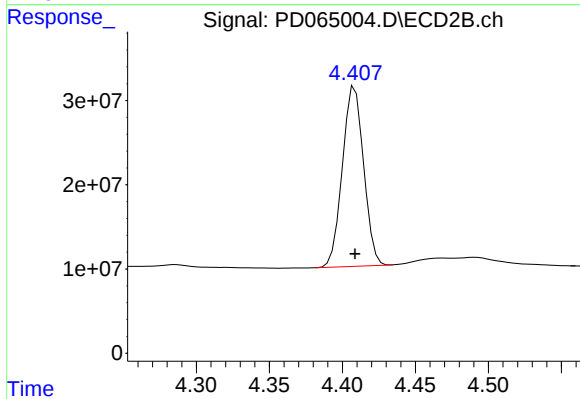

#2 alpha-BHC


R.T.: 4.409 min
Delta R.T.: 0.000 min
Response: 215865687
Conc: 20.00 ng/ml

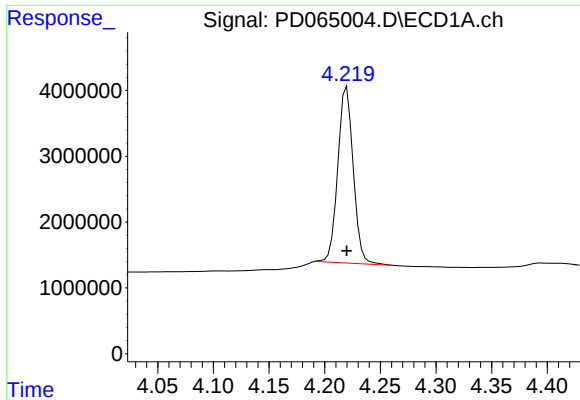

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 25772771
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

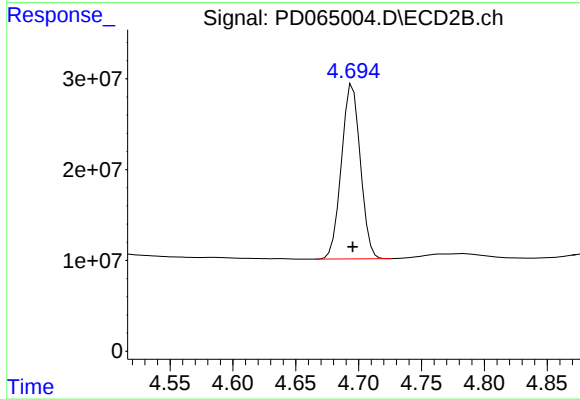


#3 gamma-BHC (Lindane)

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 201541417
Conc: 20.00 ng/ml

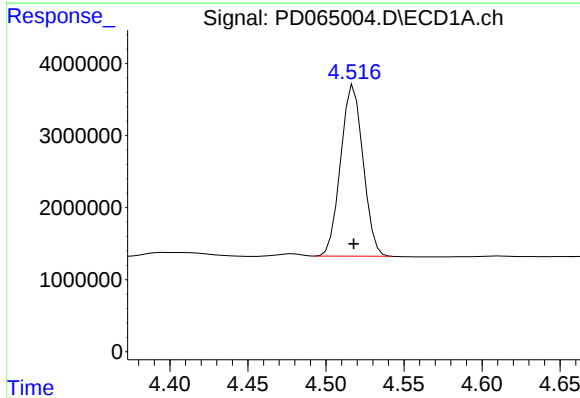


#4 Heptachlor

R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 23781585
Conc: 20.00 ng/ml

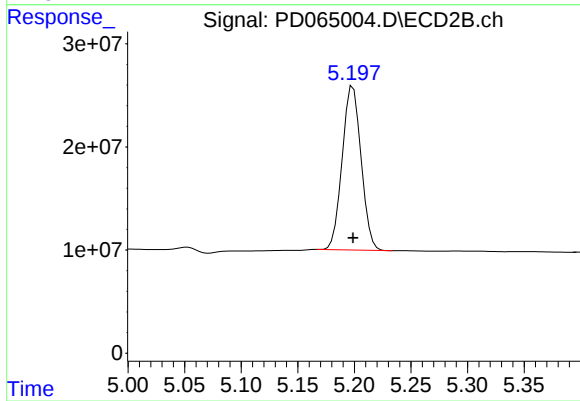

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 185102566
Conc: 20.00 ng/ml

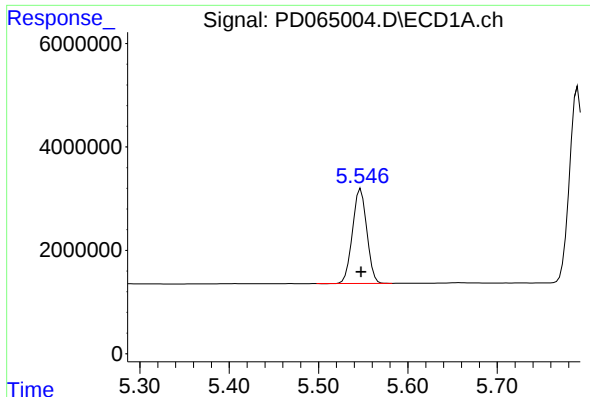

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 20408070
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

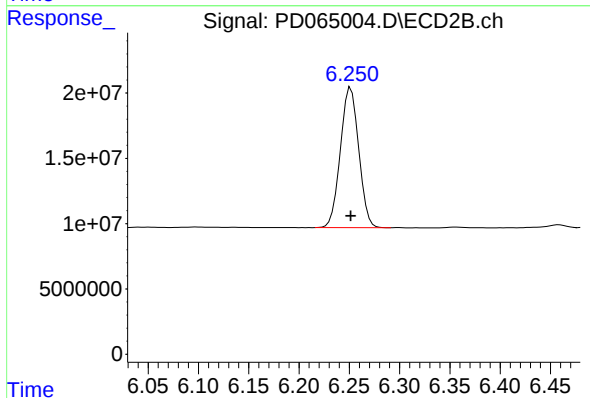


#9 Endosulfan I

R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 136019152
Conc: 20.00 ng/ml

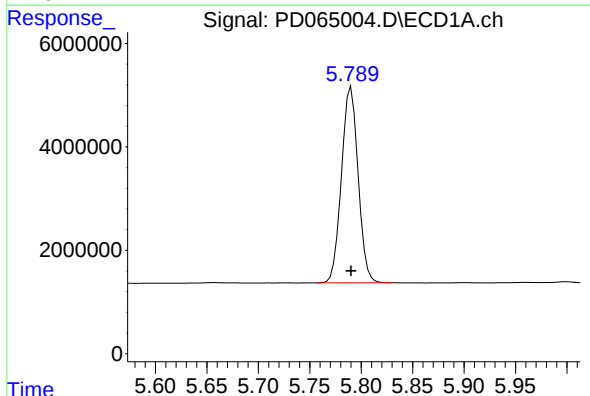


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 42624605
Conc: 40.00 ng/ml

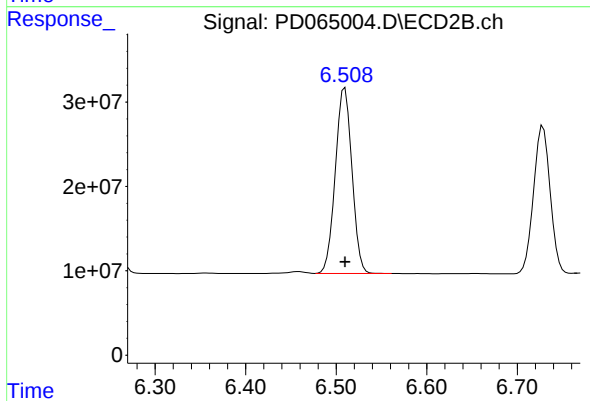

#13 Dieldrin


R.T.: 6.510 min
Delta R.T.: 0.000 min
Response: 280484921
Conc: 40.00 ng/ml

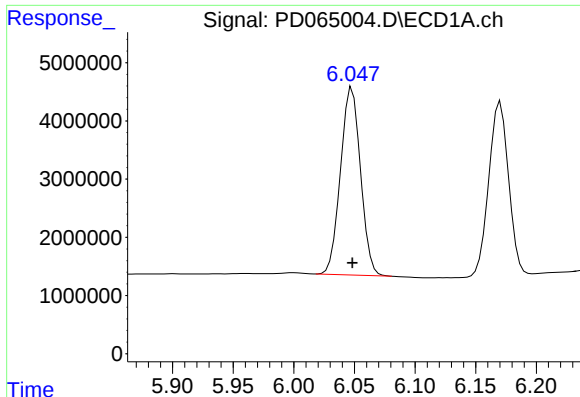

#14 Endrin


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 36955244
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

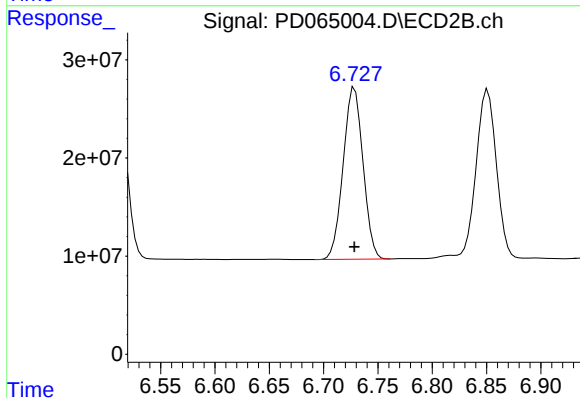


#14 Endrin

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 222923242
Conc: 40.00 ng/ml

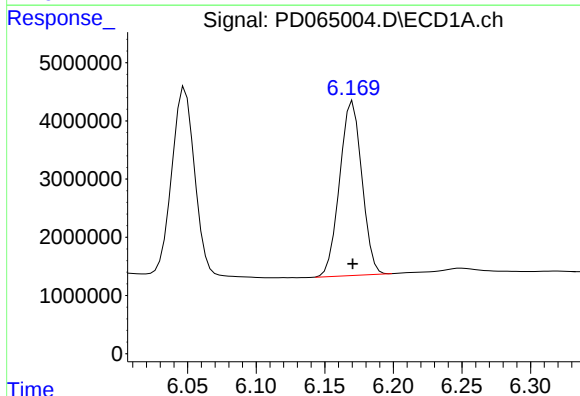


#16 4,4'-DDD

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 33818326
Conc: 40.00 ng/ml

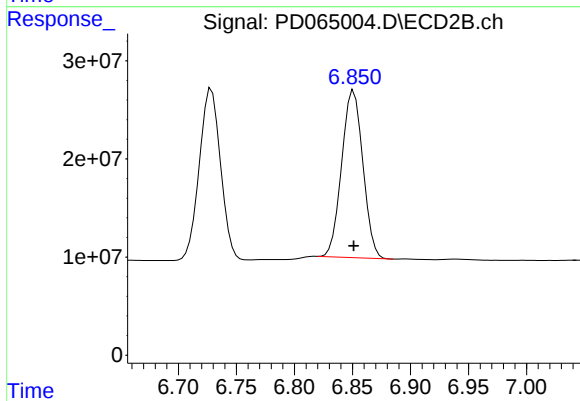

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 216666021
Conc: 40.00 ng/ml

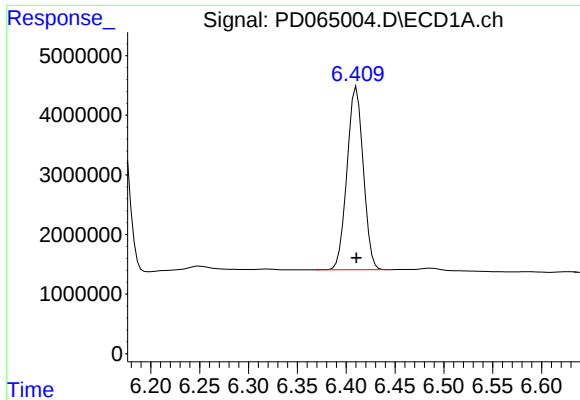

#17 4,4'-DDT


R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 35520687
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

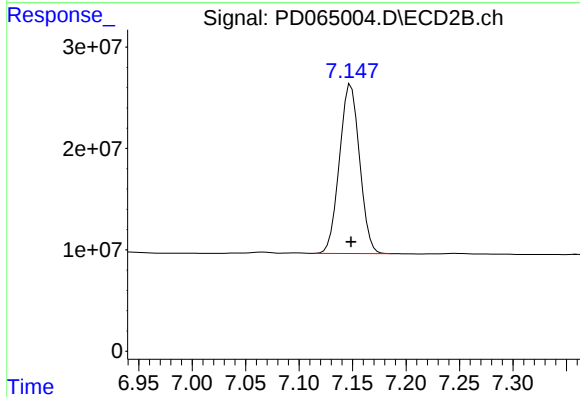


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 218837262
Conc: 40.00 ng/ml

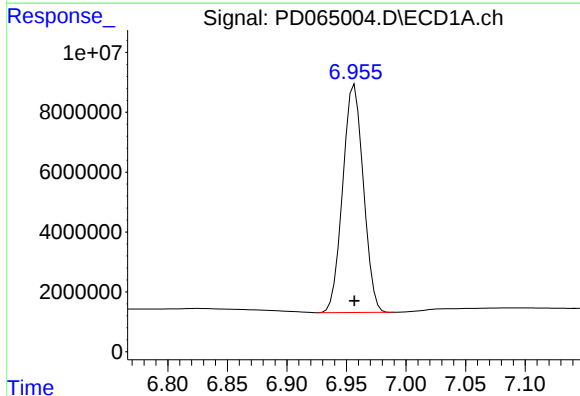


#20 Methoxychlor

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 91946999
Conc: 200.00 ng/ml

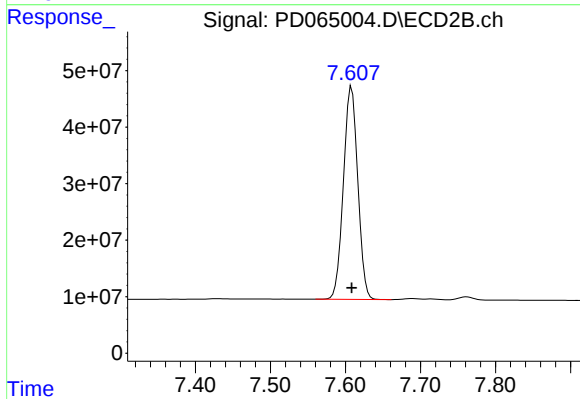

#20 Methoxychlor


R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 501702678
Conc: 200.00 ng/ml

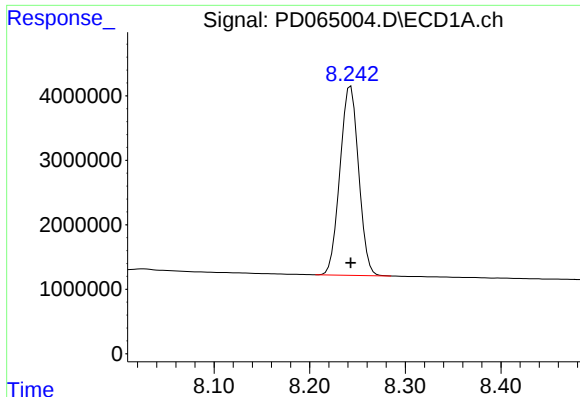

#27 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 39893339
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

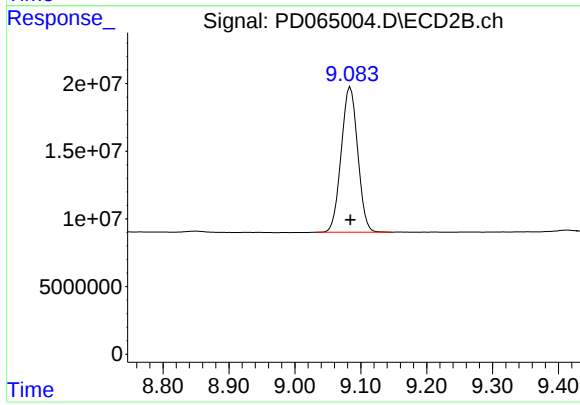

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 186690830
Conc: 40.00 ng/ml