

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 17:49
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 02:04:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:03:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	36686669	288.2E6	38.034	37.270
27)	SA Decachlor...	8.242	9.083	73532235	341.3E6	73.729	73.126
Target Compounds							
2)	A alpha-BHC	3.937	4.409	51708149	414.1E6	39.403	38.370
3)	MA gamma-BHC...	4.220	4.695	49732736	381.8E6	38.593	37.890
4)	MA Heptachlor	4.518	5.199	45581618	348.9E6	38.334	37.695
9)	A Endosulfan I	5.547	6.251	38574089	260.4E6	37.803	38.286
13)	MA Dieldrin	5.791	6.509	83591371	541.6E6	78.444	77.238
14)	MA Endrin	6.049	6.729	72119462	427.1E6	78.061	76.635
16)	A 4,4'-DDD	6.171	6.851	66353836	421.5E6	78.483	77.815
17)	MA 4,4'-DDT	6.410	7.148	69873311	423.0E6	78.685	77.322
20)	A Methoxychlor	6.957	7.607	177.2E6	932.5E6	385.504	371.749


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 17:49
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:04:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:03:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

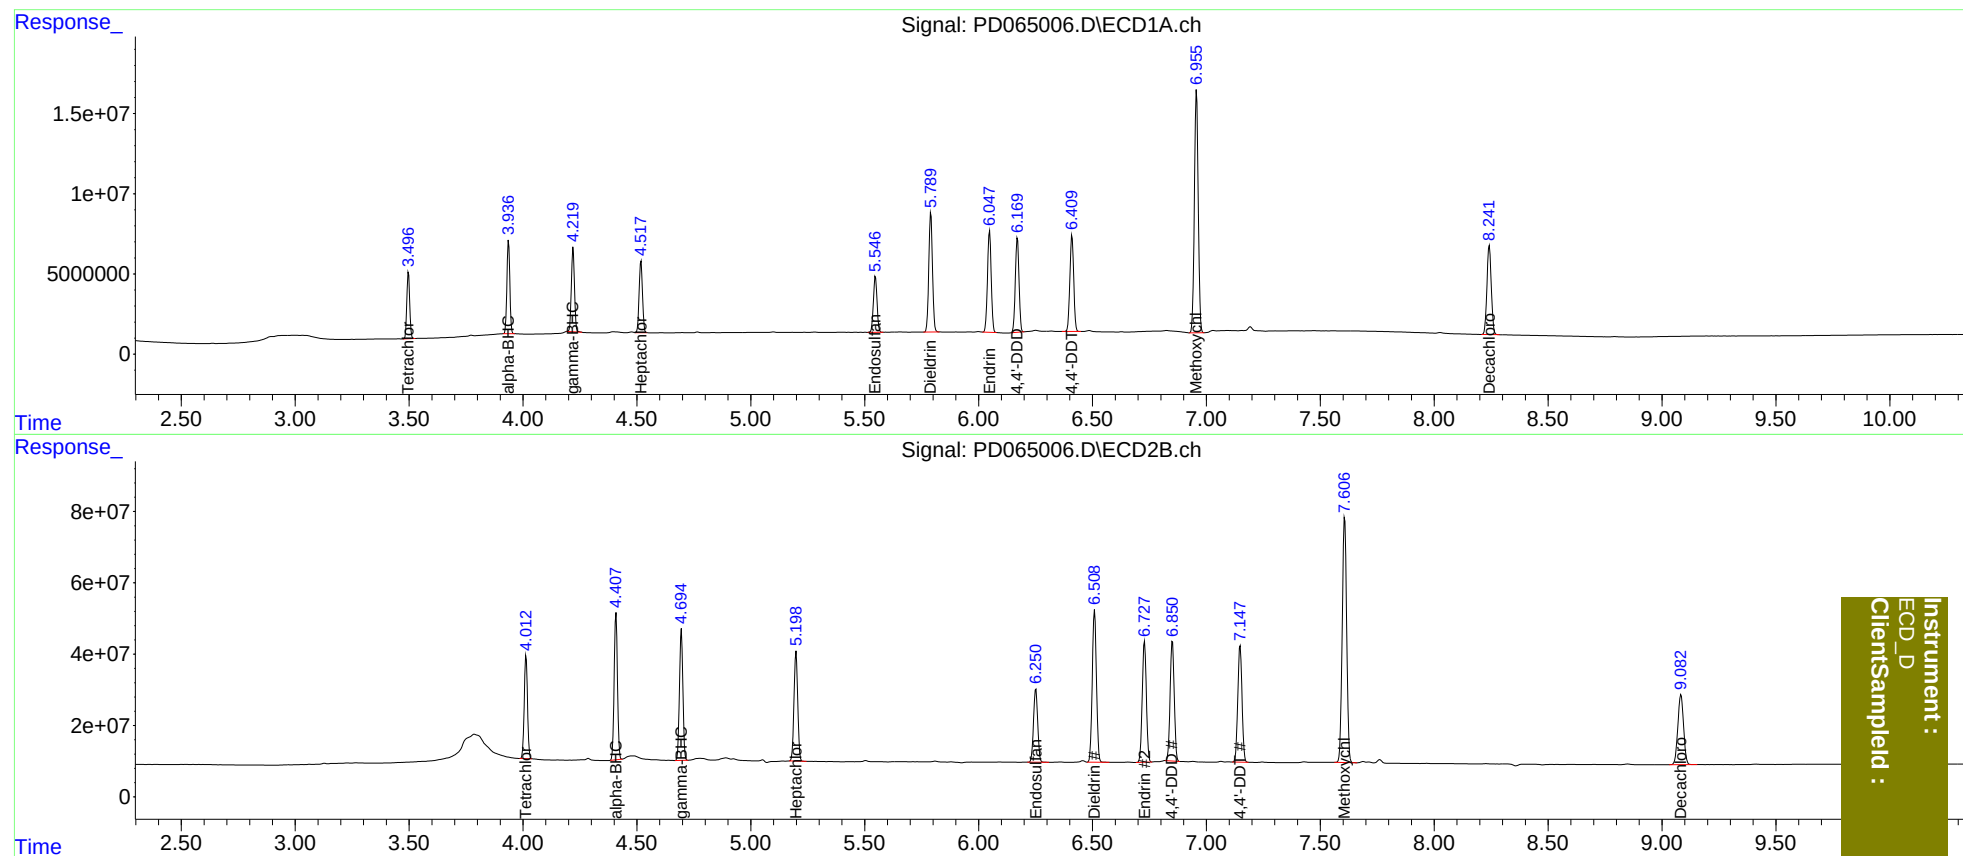


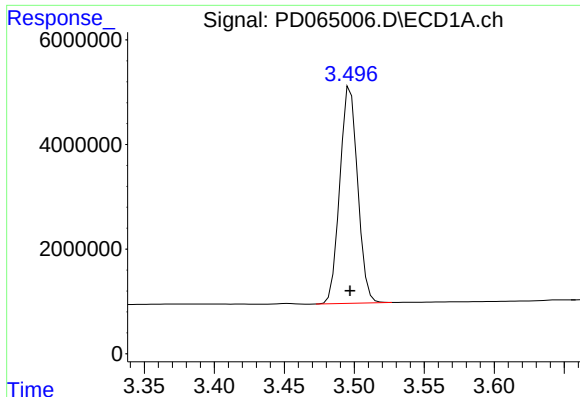

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 36686669
Conc: 38.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

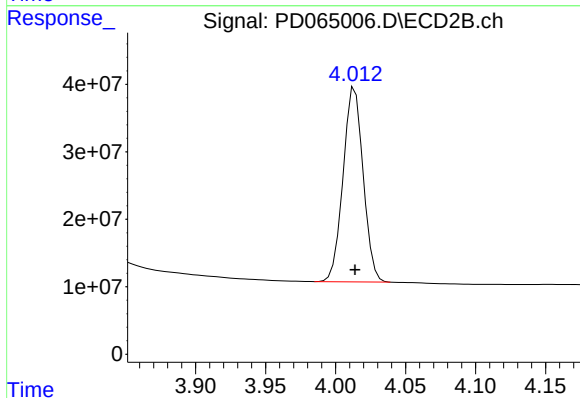


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 288158537
Conc: 37.27 ng/ml

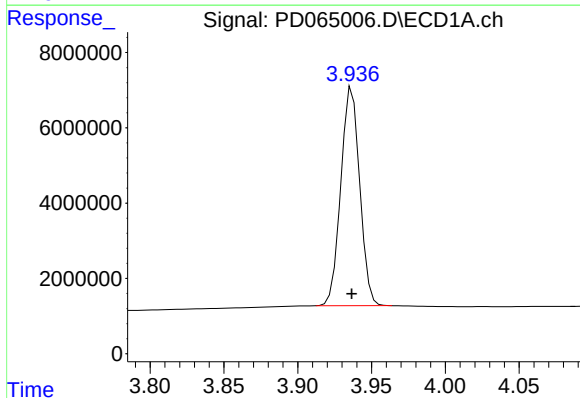


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 51708149
Conc: 39.40 ng/ml

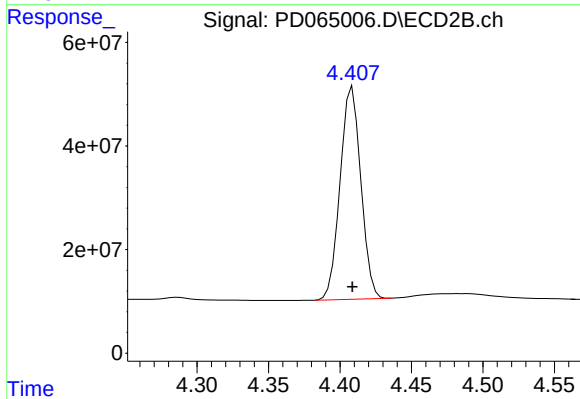

#2 alpha-BHC


R.T.: 4.409 min
Delta R.T.: 0.000 min
Response: 414133777
Conc: 38.37 ng/ml

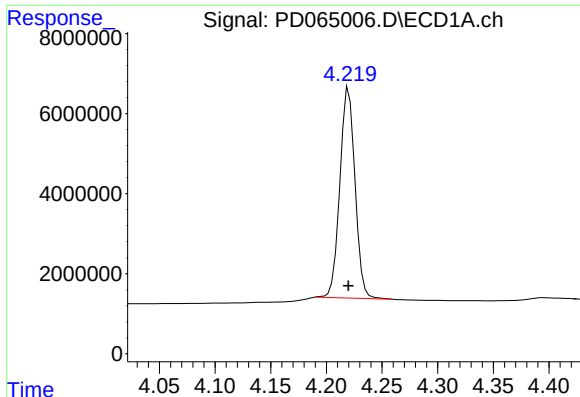

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 49732736
Conc: 38.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

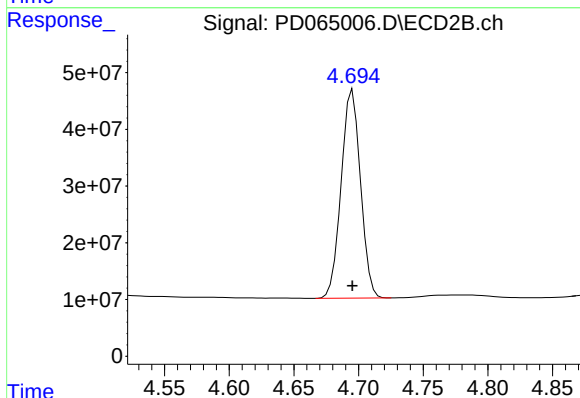


#3 gamma-BHC (Lindane)

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 381816167
Conc: 37.89 ng/ml

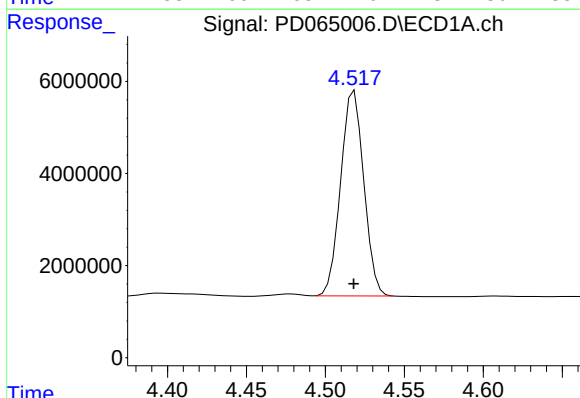


#4 Heptachlor

R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 45581618
Conc: 38.33 ng/ml

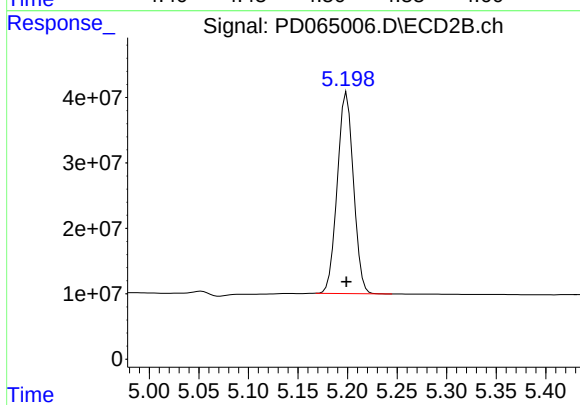

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 348873535
Conc: 37.70 ng/ml

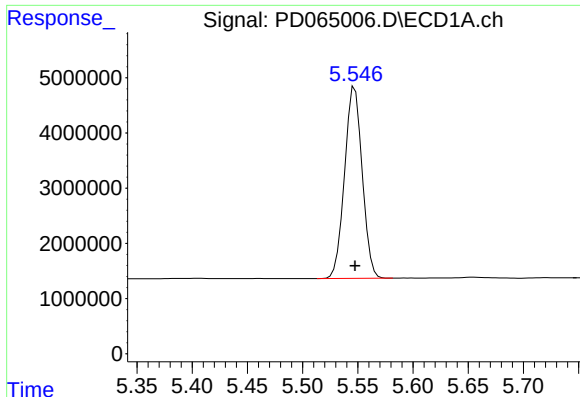

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 38574089
Conc: 37.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

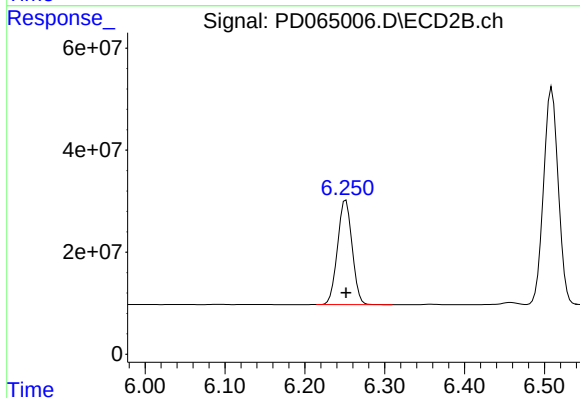


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 260380508
Conc: 38.29 ng/ml

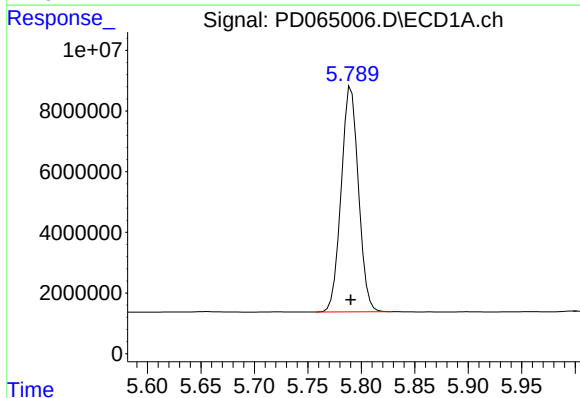


#13 Dieldrin

R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 83591371
Conc: 78.44 ng/ml

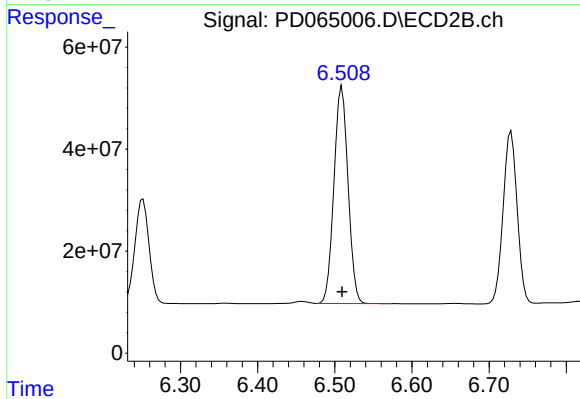

#13 Dieldrin


R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 541599853
Conc: 77.24 ng/ml

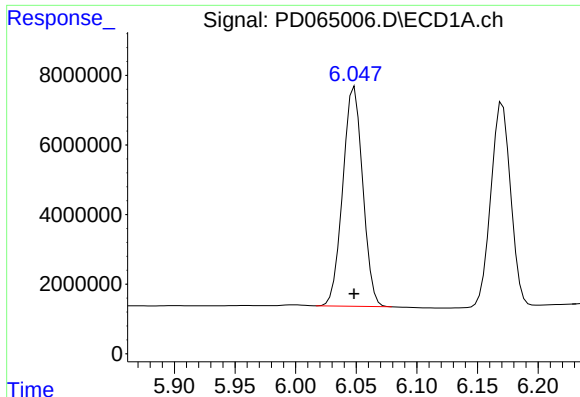

#14 Endrin


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 72119462
Conc: 78.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

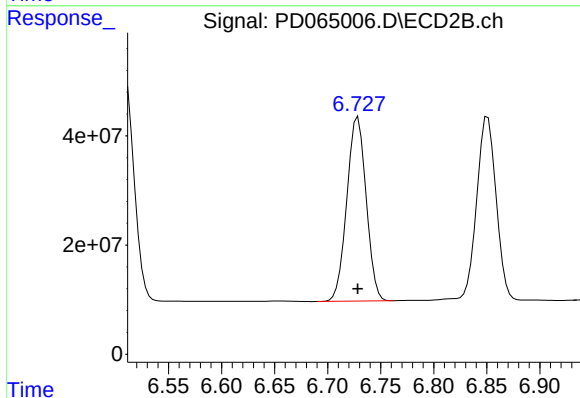


#14 Endrin

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 427095591
Conc: 76.64 ng/ml

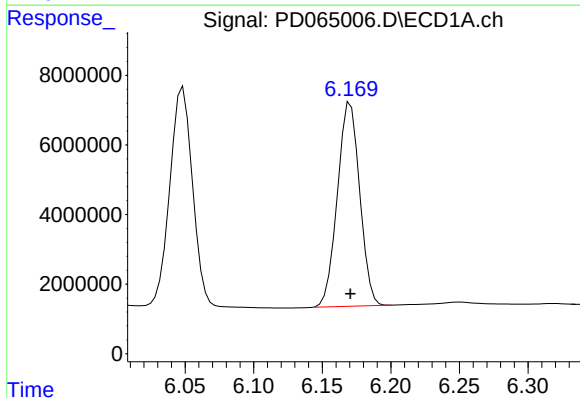


#16 4,4'-DDD

R.T.: 6.171 min
Delta R.T.: 0.000 min
Response: 66353836
Conc: 78.48 ng/ml

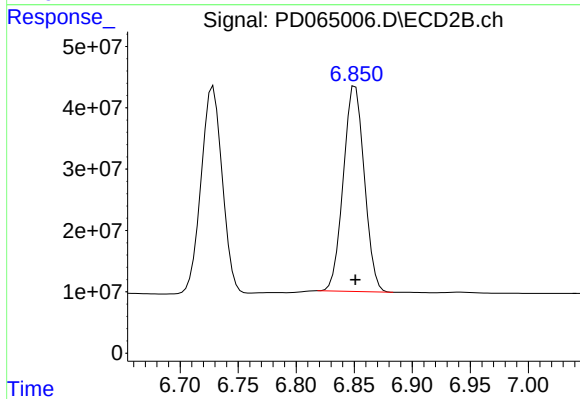

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 421495338
Conc: 77.81 ng/ml

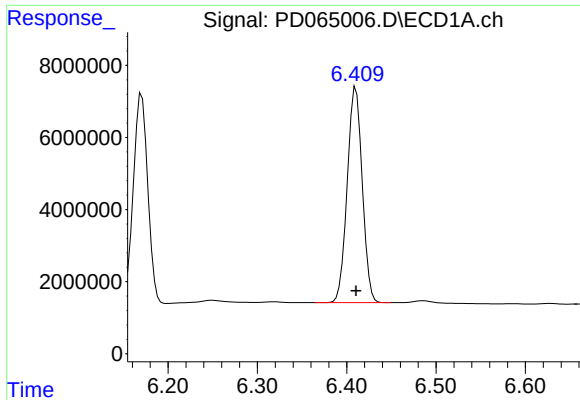

#17 4,4'-DDT


R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 69873311
Conc: 78.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

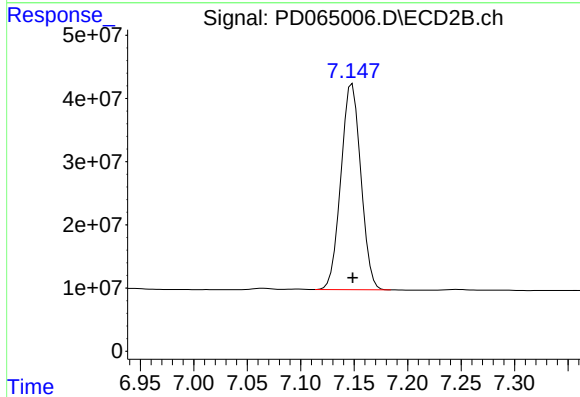


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 423022428
Conc: 77.32 ng/ml

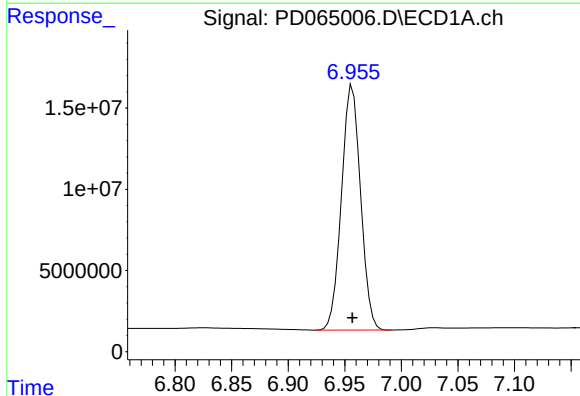


#20 Methoxychlor

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 177229808
Conc: 385.50 ng/ml

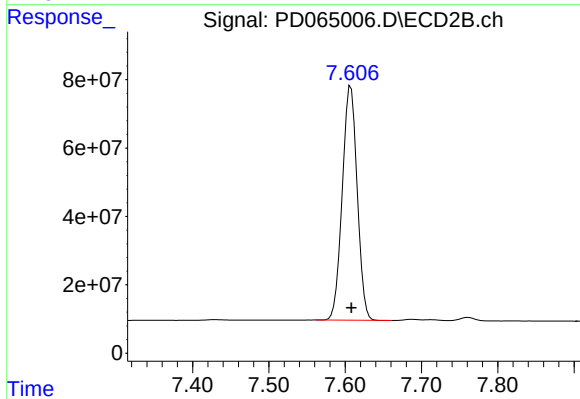

#20 Methoxychlor


R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 932537960
Conc: 371.75 ng/ml

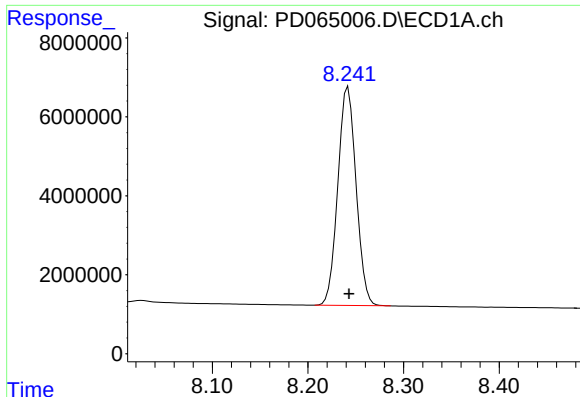

#27 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: 0.000 min
Response: 73532235
Conc: 73.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

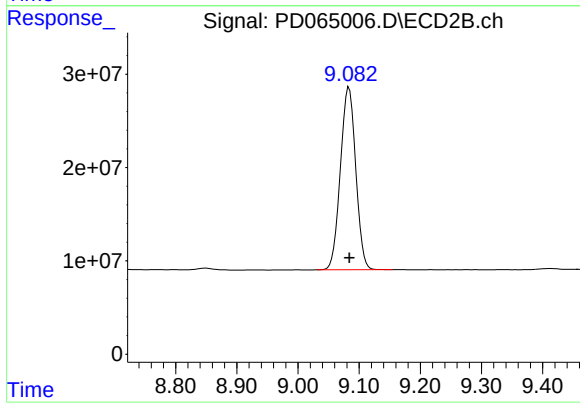

#27 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 341296965
Conc: 73.13 ng/ml