

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 18:03
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:08:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 01:07:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	37549865	297.9E6	38.366	37.938
27)	SA Decachlor...	8.242	9.085	76550376	353.2E6	74.637	73.809
Target Compounds							
5)	MB Aldrin	4.766	5.504	46063465	351.4E6	38.955	38.726
6)	B beta-BHC	4.467	4.870	23372950	186.8E6	36.749	36.702
7)	B delta-BHC	4.672	5.088	49597156	388.2E6	39.789	39.334
8)	B Heptachlo...	5.208	5.894	43328228	309.1E6	38.385	39.191
10)	B trans-Chl...	5.433	6.127	43752564	304.8E6	38.466	39.226
11)	B cis-Chlor...	5.492	6.199	42739382	292.5E6	38.253	38.993
12)	B 4,4'-DDE	5.655	6.357	81883106	558.9E6	79.928	79.322
15)	B Endosulfa...	6.320	6.941	72634371	441.5E6	78.225	77.666
18)	B Endrin al...	6.488	7.066	62344796	377.5E6	76.934	76.560
19)	B Endosulfa...	6.700	7.288	74515459	431.4E6	76.825	77.299
21)	B Endrin ke...	7.194	7.761	88494892	480.4E6	77.879	76.011

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 18:03
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:08:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 01:07:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

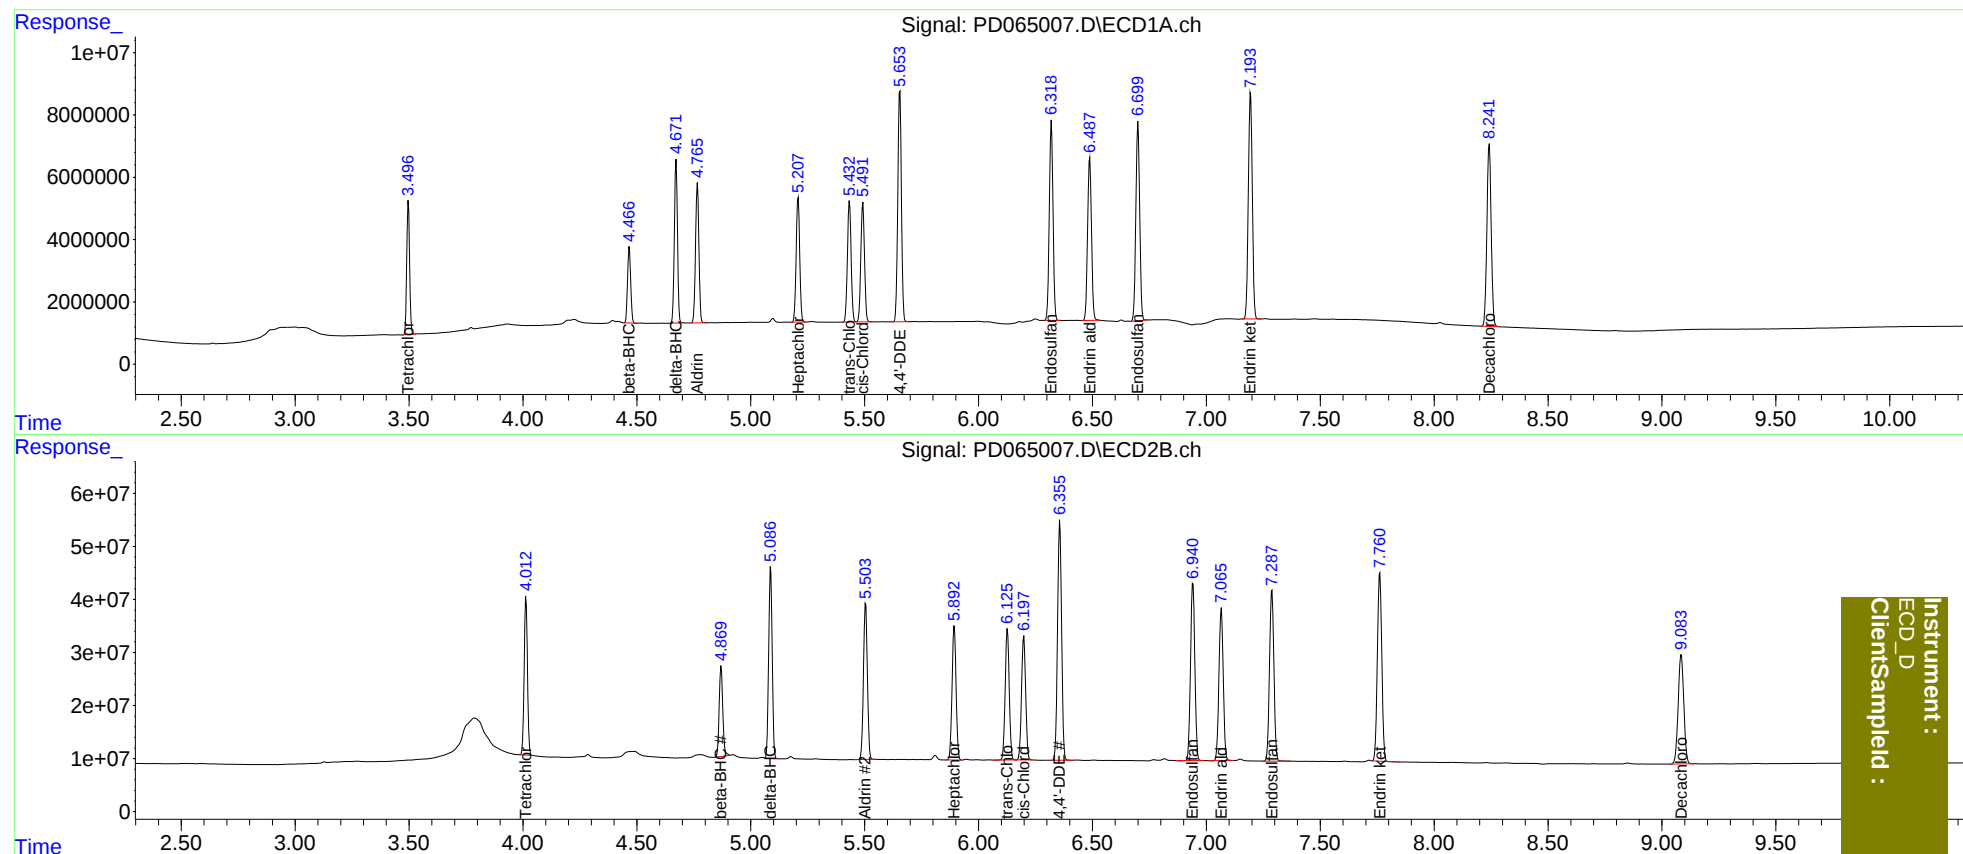


Instrument :
ECD_D
ClientSampled :

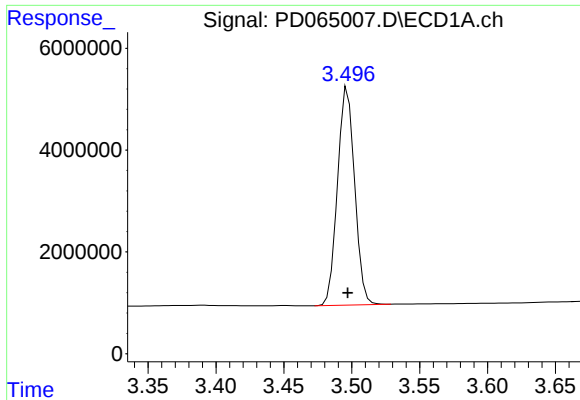

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 37549865
Conc: 38.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

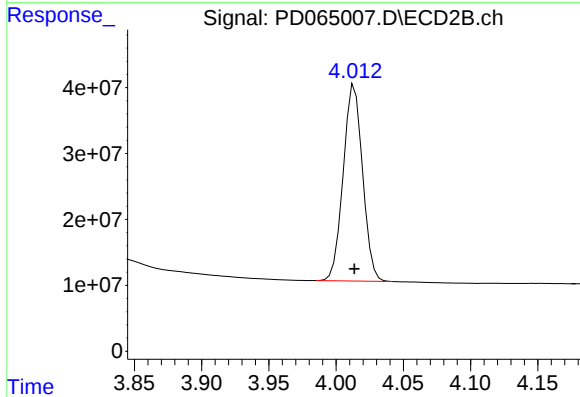


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 297927837
Conc: 37.94 ng/ml

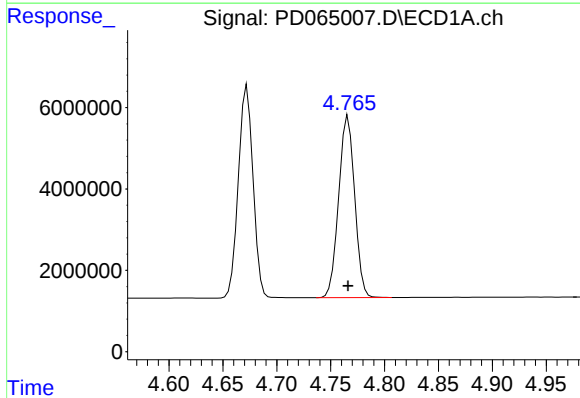


#5 Aldrin

R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 46063465
Conc: 38.95 ng/ml

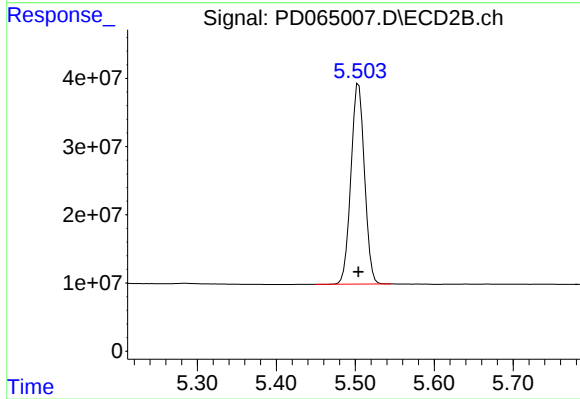

#5 Aldrin


R.T.: 5.504 min
Delta R.T.: 0.000 min
Response: 351381246
Conc: 38.73 ng/ml

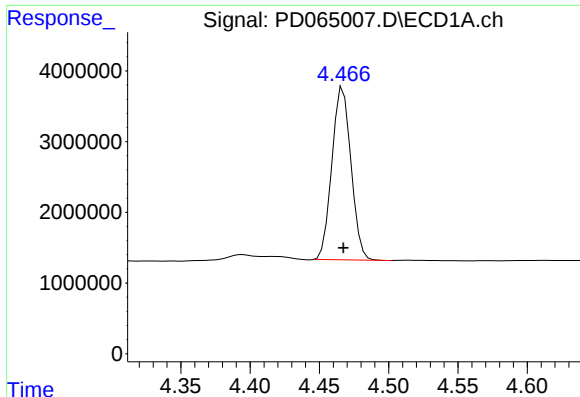

#6 beta-BHC


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 23372950
Conc: 36.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

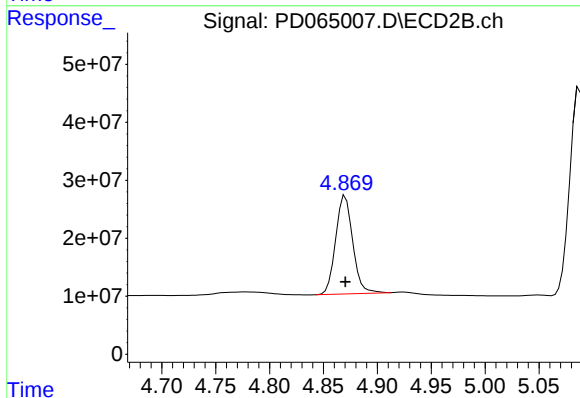


#6 beta-BHC

R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 186775730
Conc: 36.70 ng/ml

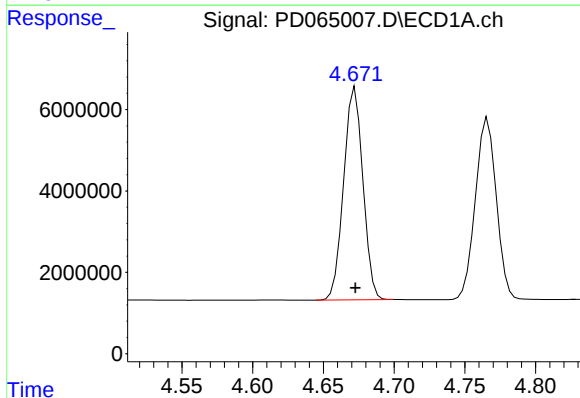


#7 delta-BHC

R.T.: 4.672 min
Delta R.T.: 0.000 min
Response: 49597156
Conc: 39.79 ng/ml

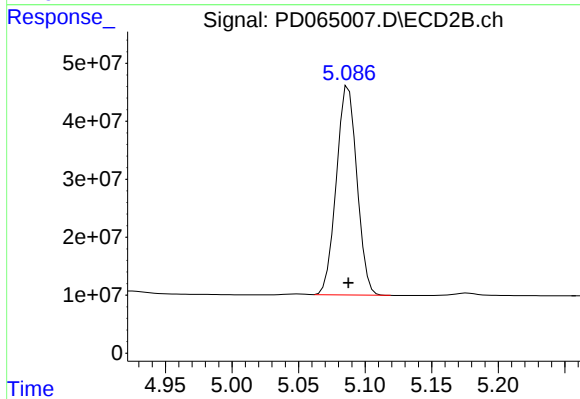

#7 delta-BHC


R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 388172835
Conc: 39.33 ng/ml

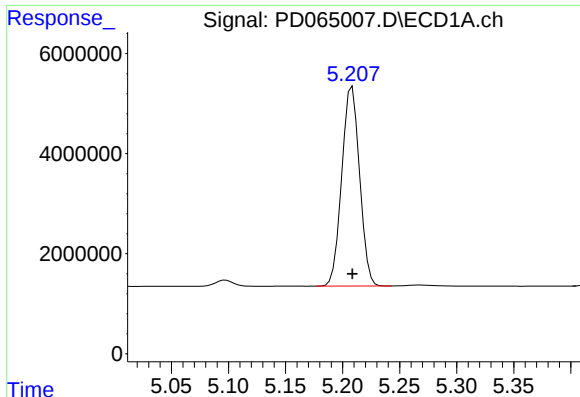

#8 Heptachlor epoxide


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 43328228
Conc: 38.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

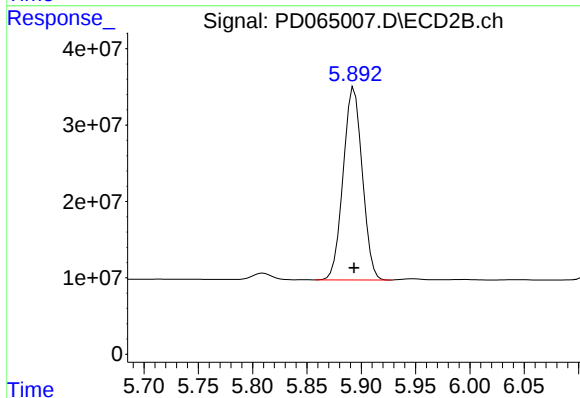


#8 Heptachlor epoxide

R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 309060873
Conc: 39.19 ng/ml

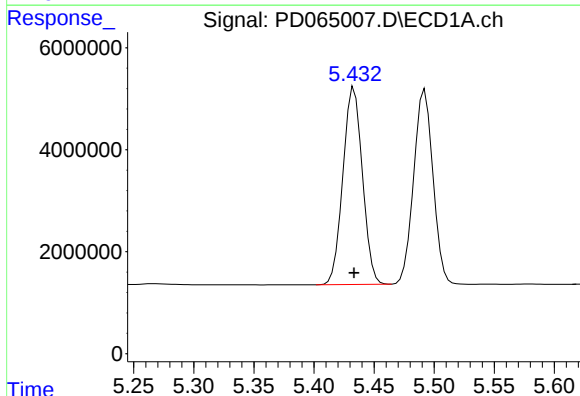


#10 trans-Chlordane

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 43752564
Conc: 38.47 ng/ml

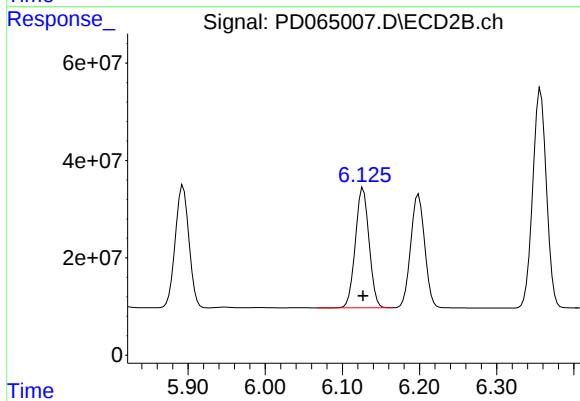

#10 trans-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 304790264
Conc: 39.23 ng/ml

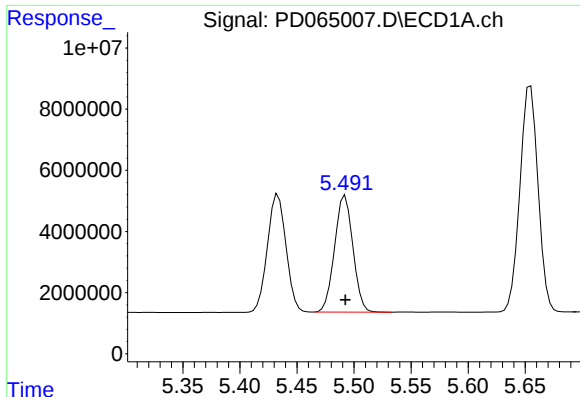

#11 cis-Chlordane


R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 42739382
Conc: 38.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

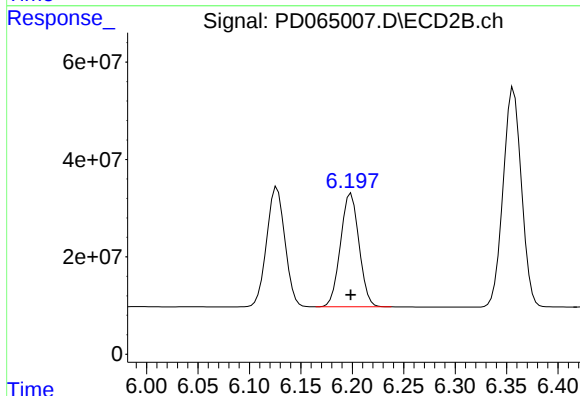


#11 cis-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 292549348
Conc: 38.99 ng/ml

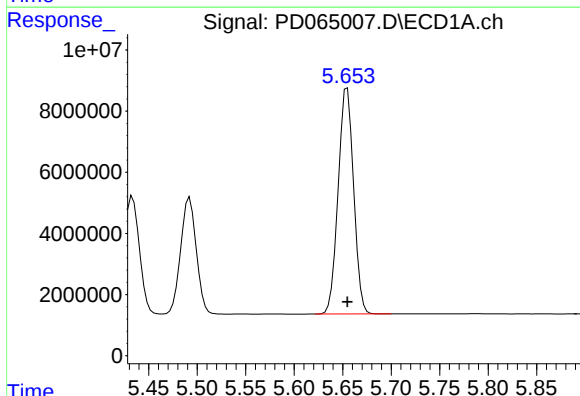


#12 4,4'-DDE

R.T.: 5.655 min
Delta R.T.: 0.000 min
Response: 81883106
Conc: 79.93 ng/ml

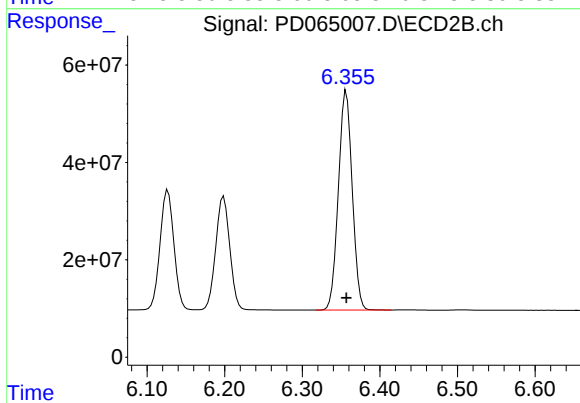

#12 4,4'-DDE


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 558915369
Conc: 79.32 ng/ml

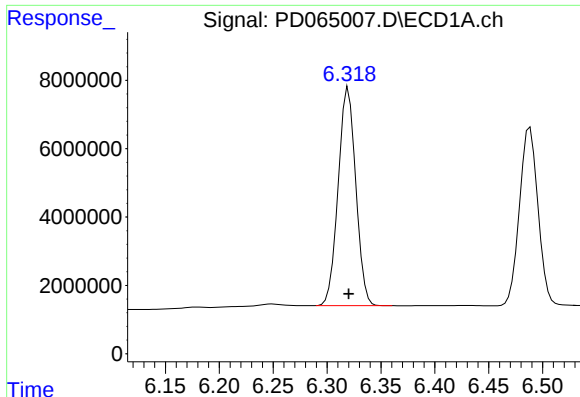

#15 Endosulfan II


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 72634371
Conc: 78.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

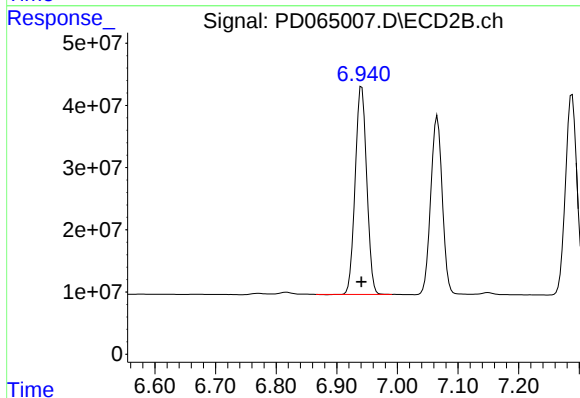


#15 Endosulfan II

R.T.: 6.941 min
Delta R.T.: 0.000 min
Response: 441494486
Conc: 77.67 ng/ml

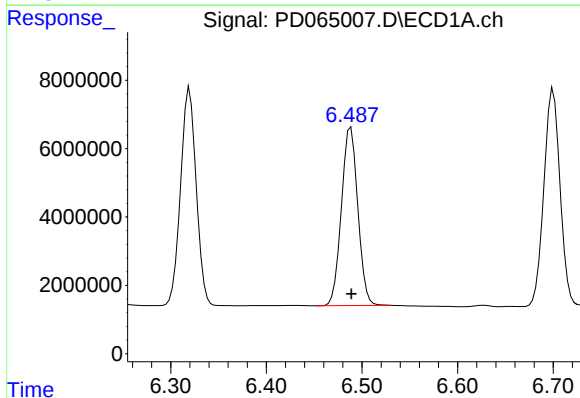


#18 Endrin aldehyde

R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 62344796
Conc: 76.93 ng/ml

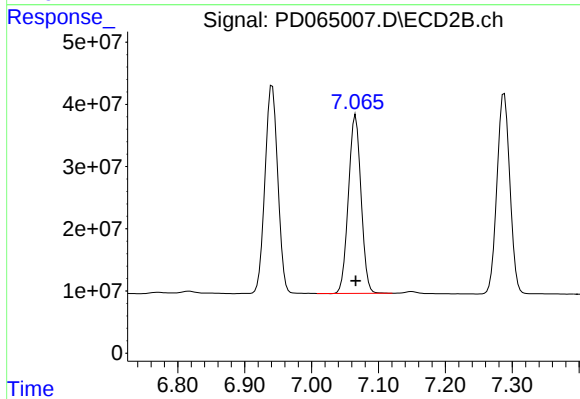

#18 Endrin aldehyde


R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 377500000
Conc: 76.56 ng/ml

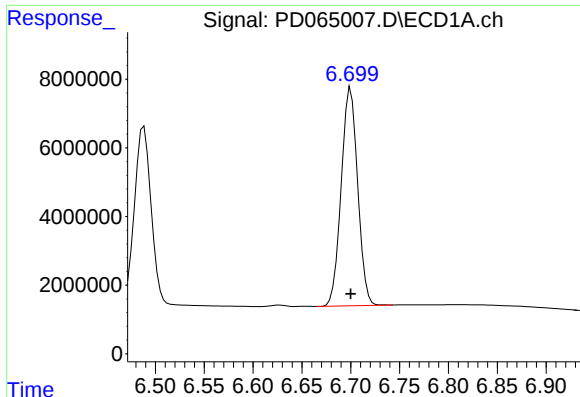

#19 Endosulfan Sulfate


R.T.: 6.700 min
Delta R.T.: 0.000 min
Response: 74515459
Conc: 76.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

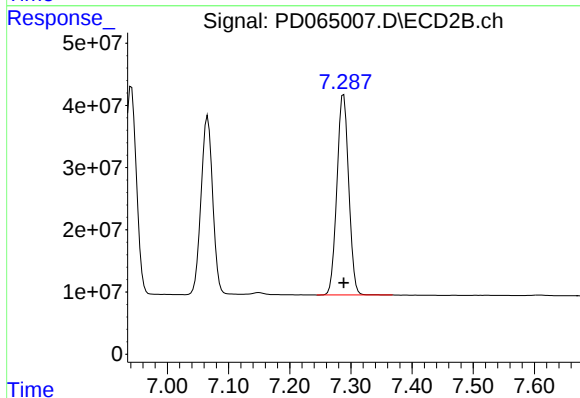


#19 Endosulfan Sulfate

R.T.: 7.288 min
Delta R.T.: 0.000 min
Response: 431404335
Conc: 77.30 ng/ml

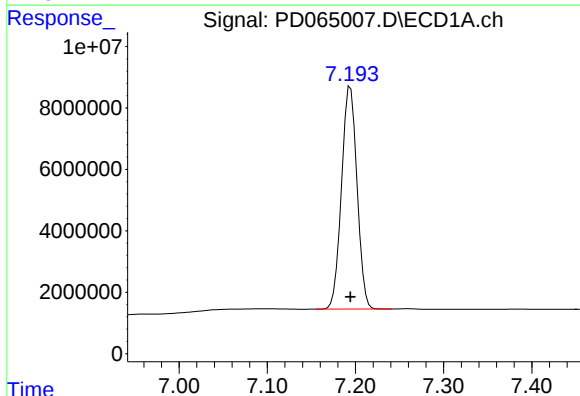


#21 Endrin ketone

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 88494892
Conc: 77.88 ng/ml

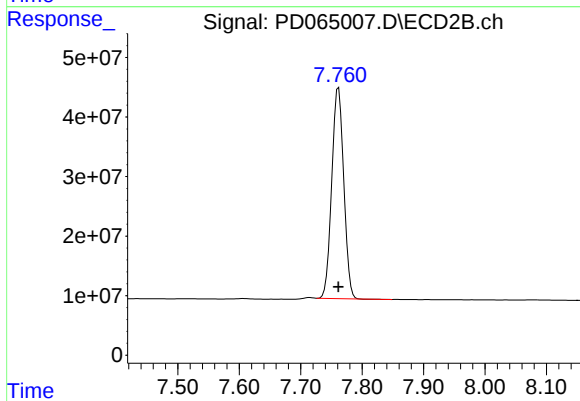

#21 Endrin ketone


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 480408782
Conc: 76.01 ng/ml

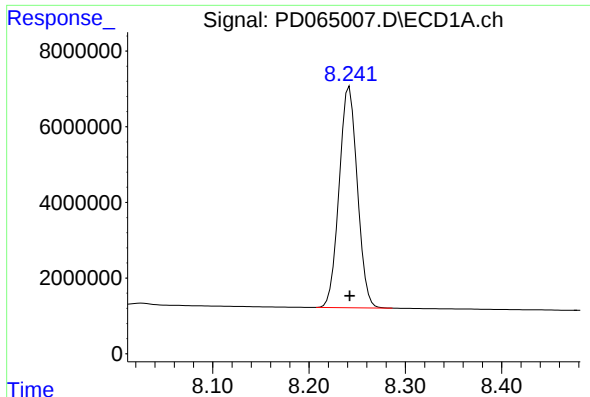

#27 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: 0.000 min
Response: 76550376
Conc: 74.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

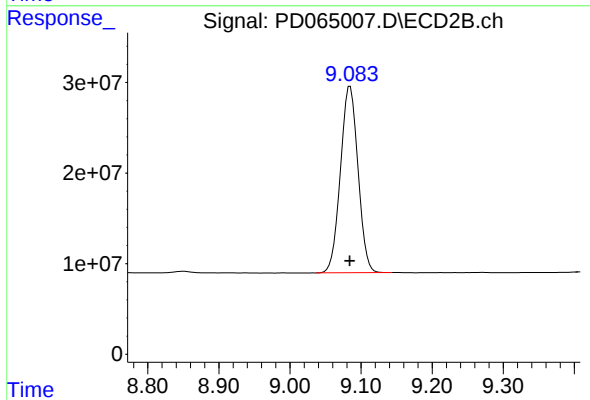

#27 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 353194448
Conc: 73.81 ng/ml