

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD065008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 18:17
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 02:04:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:03:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	69717948	543.0E6	72.278	70.231
27)	SA Decachlor...	8.242	9.084	137.1E6	628.3E6	137.466	134.623
Target Compounds							
2)	A alpha-BHC	3.937	4.408	102.5E6	811.9E6	78.123	75.221
3)	MA gamma-BHC...	4.220	4.695	95842967	737.7E6	74.375	73.203
4)	MA Heptachlor	4.518	5.199	87674084	668.1E6	73.733	72.183
9)	A Endosulfan I	5.547	6.251	72649330	489.8E6	71.197	72.017
13)	MA Dieldrin	5.790	6.509	163.3E6	1034.6E6	153.224	147.541
14)	MA Endrin	6.048	6.728	142.4E6	819.2E6	154.112	147.000
16)	A 4,4'-DDD	6.170	6.851	132.3E6	805.4E6	156.466	148.693
17)	MA 4,4'-DDT	6.410	7.148	141.8E6	815.9E6	159.674	149.129
20)	A Methoxychlor	6.957	7.607	348.8E6	1723.6E6	758.724	687.097


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD065008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 18:17
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:04:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:03:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

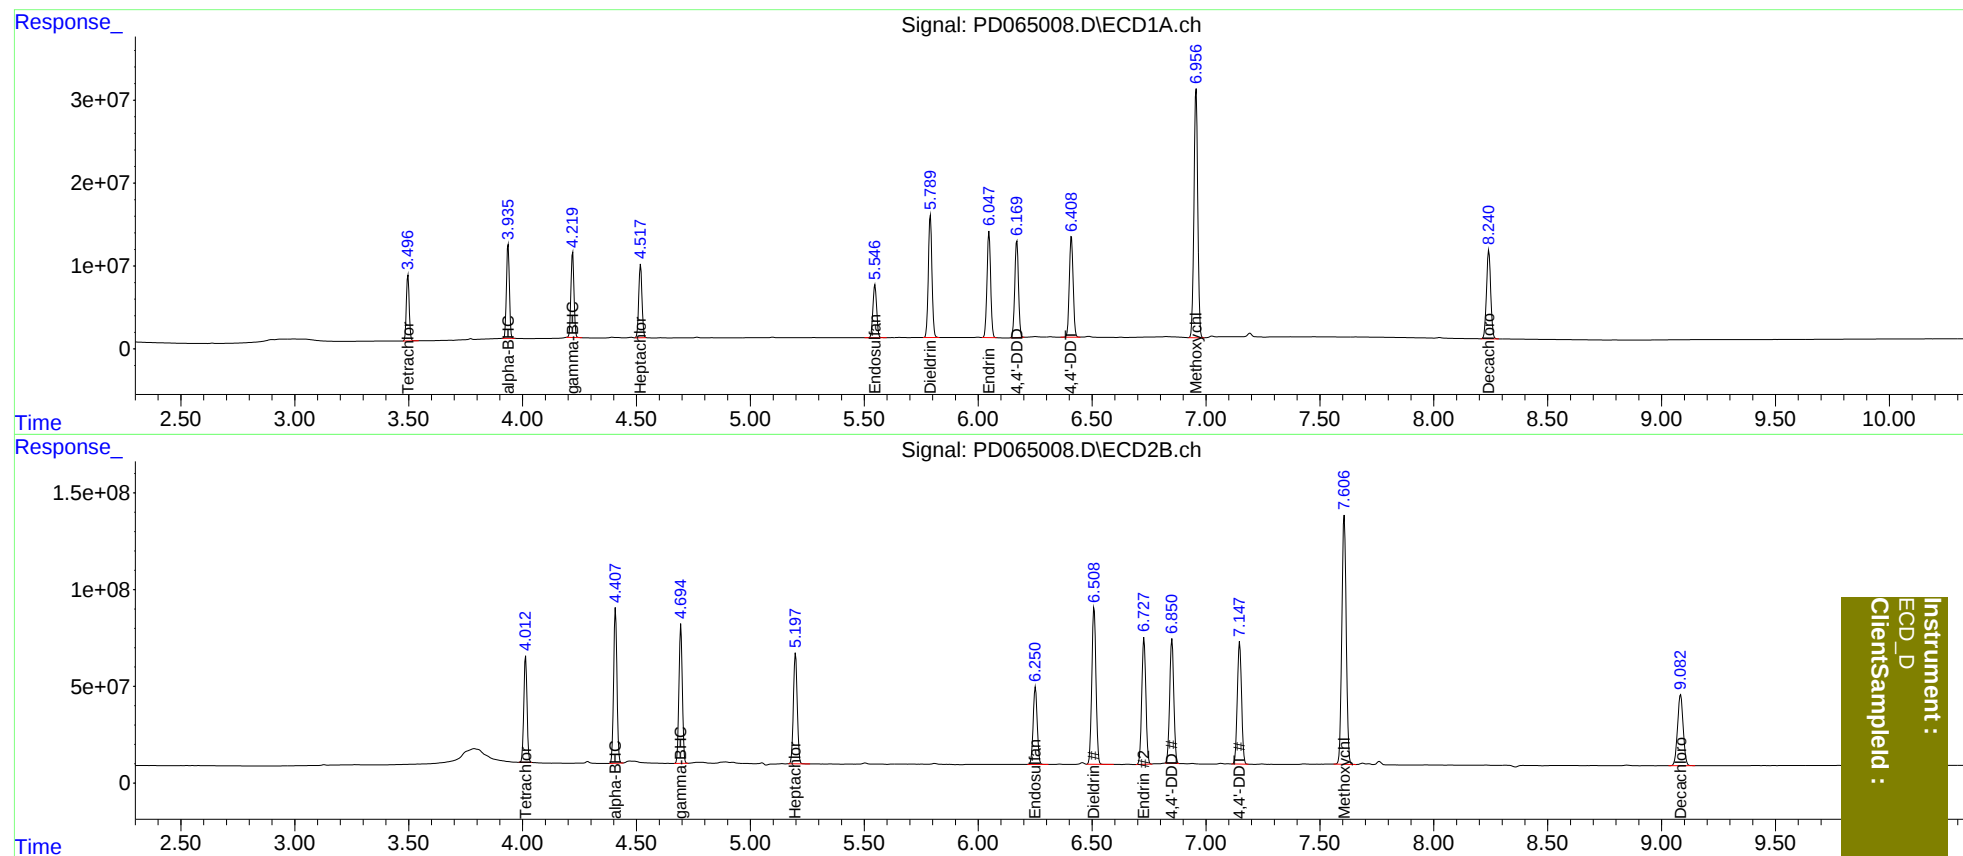


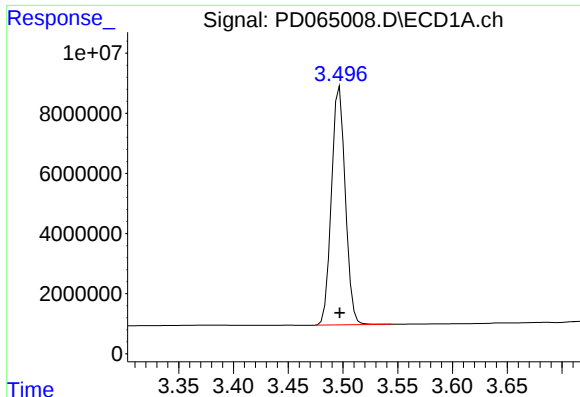

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 69717948
Conc: 72.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

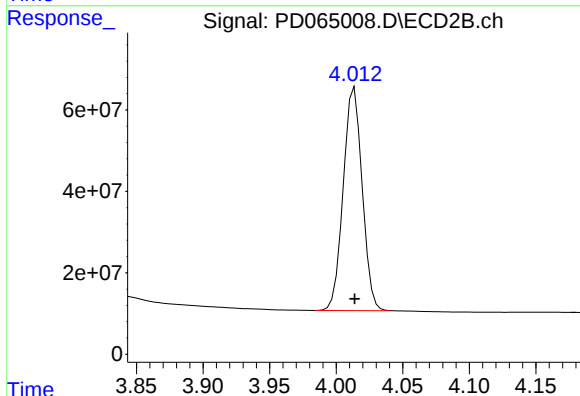


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 542995740
Conc: 70.23 ng/ml

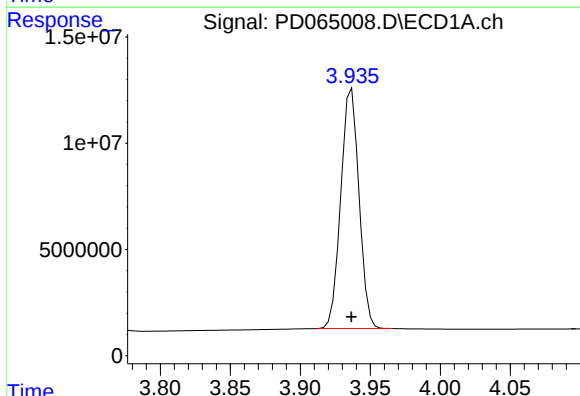


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 102519112
Conc: 78.12 ng/ml

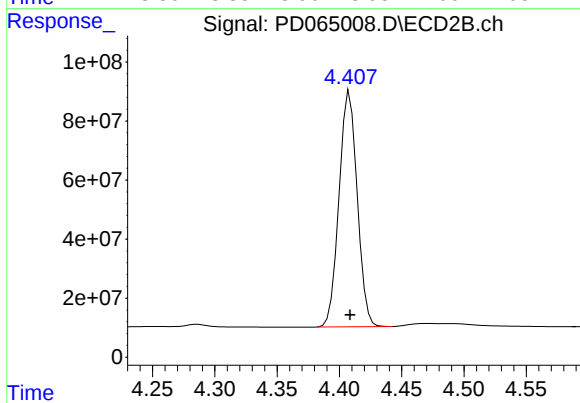

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 811887036
Conc: 75.22 ng/ml

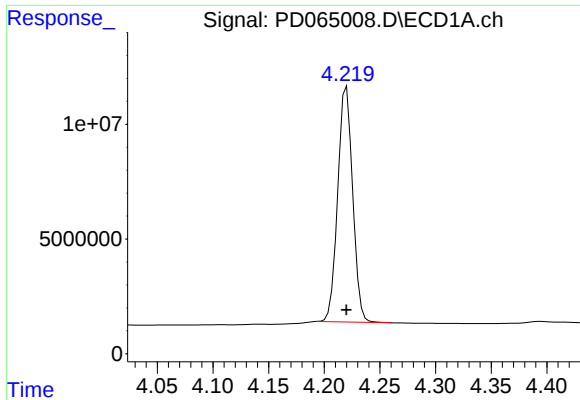

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 95842967
Conc: 74.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

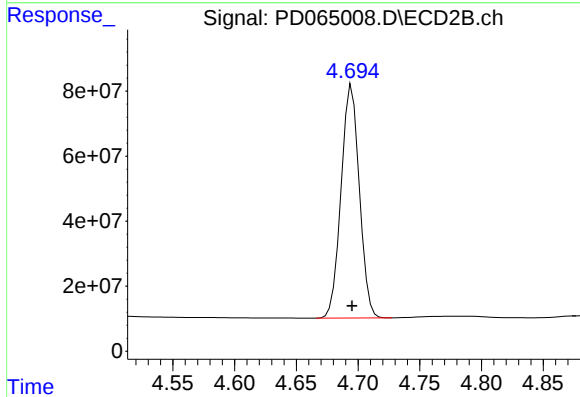


#3 gamma-BHC (Lindane)

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 737670754
Conc: 73.20 ng/ml

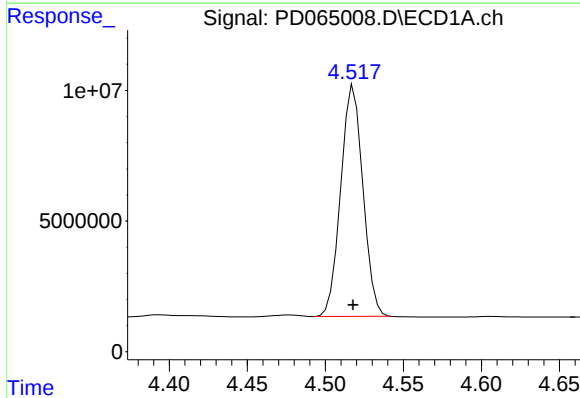


#4 Heptachlor

R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 87674084
Conc: 73.73 ng/ml

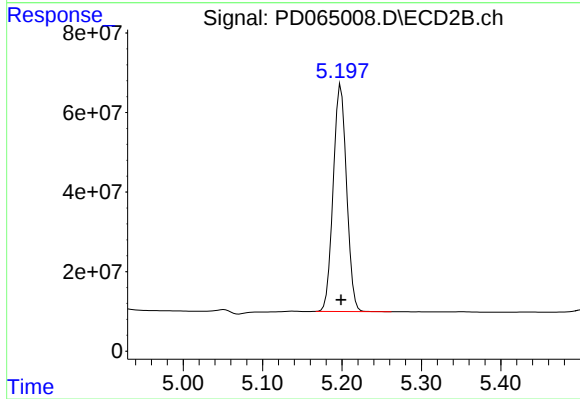

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 668063801
Conc: 72.18 ng/ml

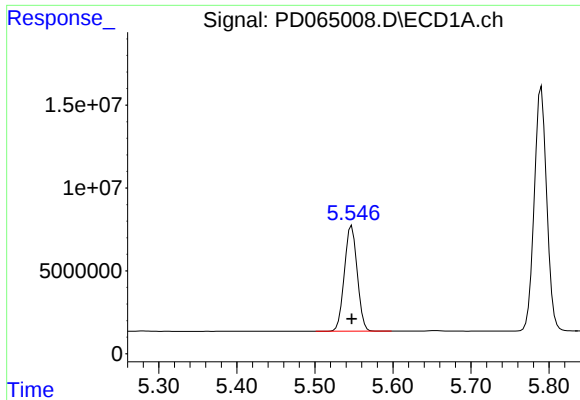

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 72649330
Conc: 71.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

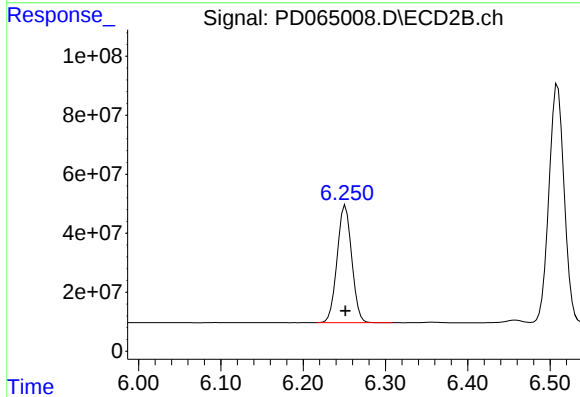


#9 Endosulfan I

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 489786531
Conc: 72.02 ng/ml

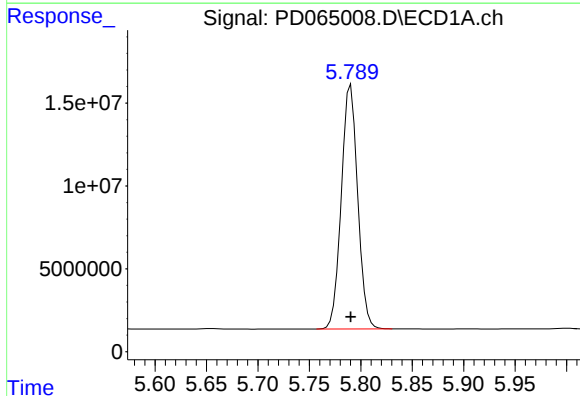


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 163278263
Conc: 153.22 ng/ml

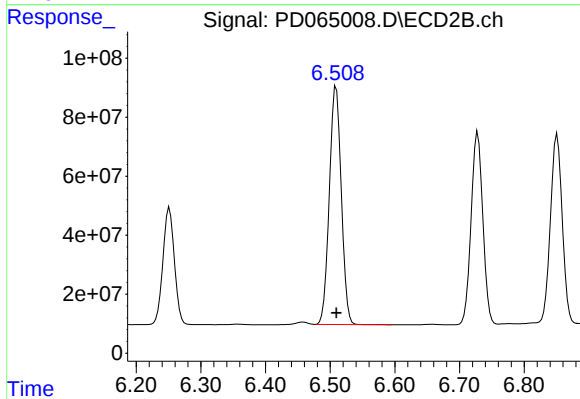

#13 Dieldrin


R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 1034576477
Conc: 147.54 ng/ml

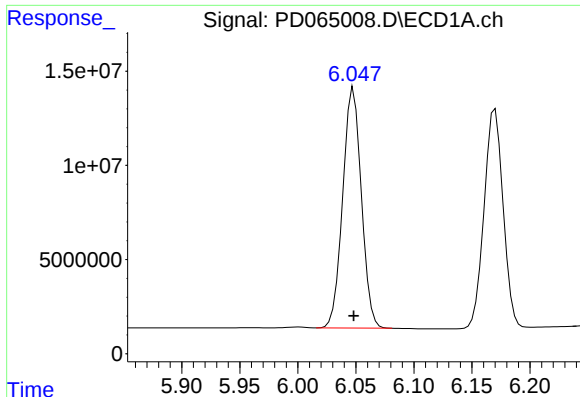

#14 Endrin


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 142381467
Conc: 154.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

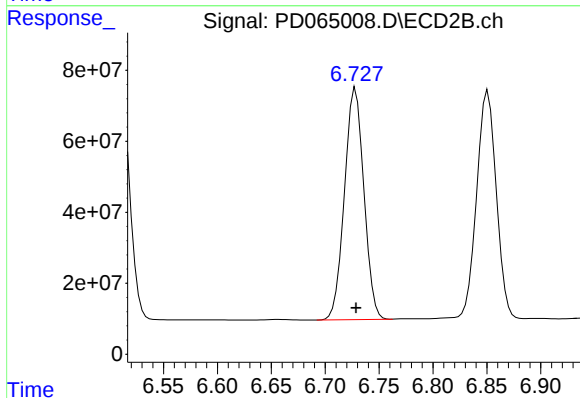


#14 Endrin

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 819240130
Conc: 147.00 ng/ml

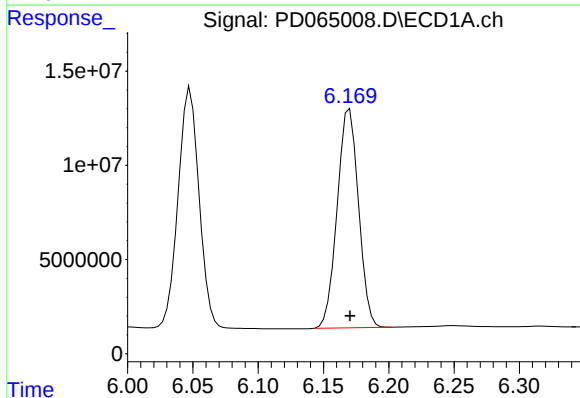


#16 4,4'-DDD

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 132285695
Conc: 156.47 ng/ml

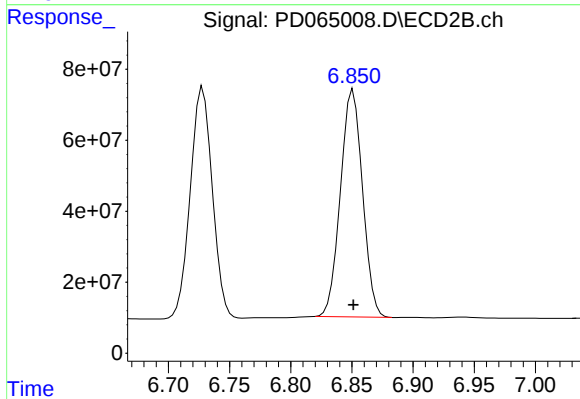

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 805418383
Conc: 148.69 ng/ml

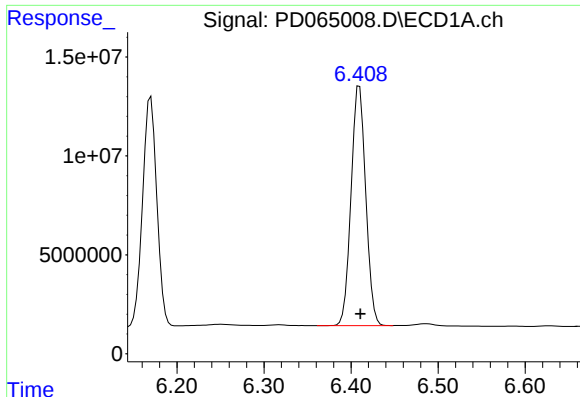

#17 4,4'-DDT


R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 141793464
Conc: 159.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

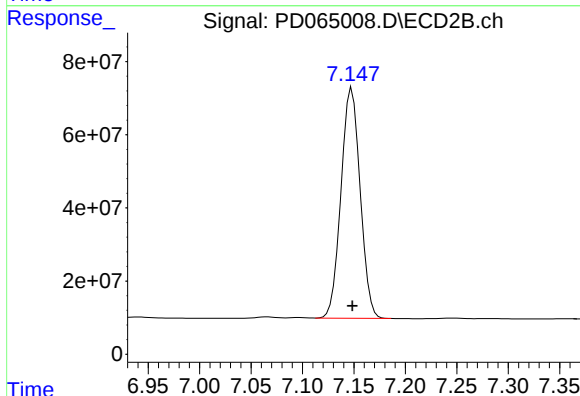


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 815874760
Conc: 149.13 ng/ml

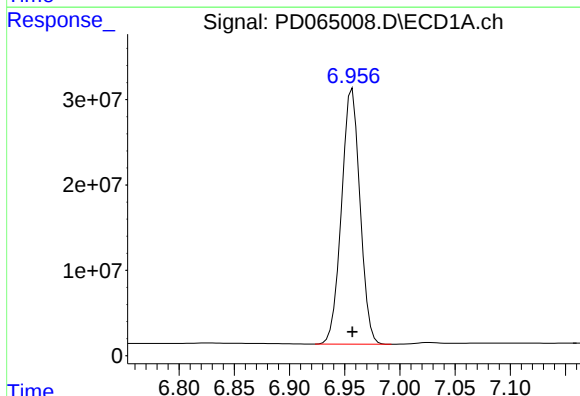


#20 Methoxychlor

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 348812126
Conc: 758.72 ng/ml

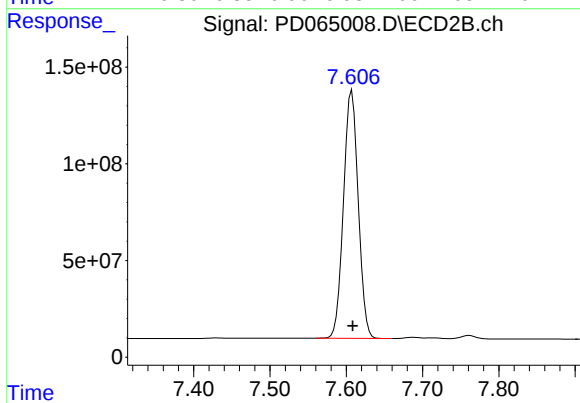

#20 Methoxychlor


R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 1723593026
Conc: 687.10 ng/ml

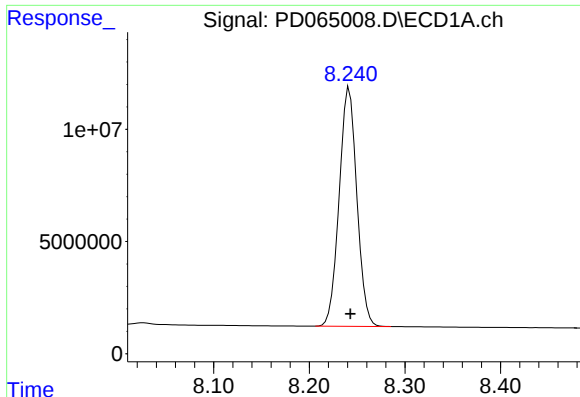

#27 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: -0.001 min
Response: 137099620
Conc: 137.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

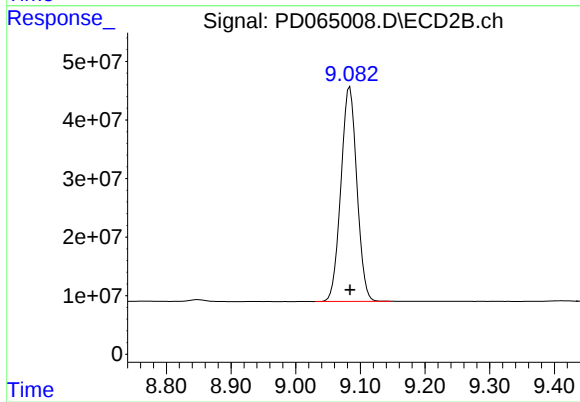

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 628322534
Conc: 134.62 ng/ml