

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
 Data File : PD064993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 14:50
 Operator : AR\AJ
 Sample : RESC10
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:03:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:57:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	19649800	157.4E6	20.506	20.529
27)	SA Decachlor...	8.243	9.084	37858719	186.4E6	38.297	40.906
Target Compounds							
2)	A alpha-BHC	3.937	4.409	13239705	112.3E6	10.123	10.523
3)	MA gamma-BHC...	4.220	4.695	13369259	106.1E6	10.206	10.598
4)	MA Heptachlor	4.519	5.199	12101241	97670648	10.227	10.608
5)	MB Aldrin	4.767	5.504	11934032	96108172	10.267	10.672
6)	B beta-BHC	4.468	4.871	6806941	58486627	10.940	11.120
7)	B delta-BHC	4.673	5.087	12320666	102.4E6	10.003	10.456
8)	B Heptachlo...	5.209	5.893	11336104	83965255	10.206	10.712
9)	A Endosulfan I	5.547	6.251	9976561	69117543	9.931	10.228
10)	B trans-Chl...	5.434	6.127	11341428	81518444	10.114	10.581
11)	B cis-Chlor...	5.493	6.199	11014724	77334488	10.016	10.448
12)	B 4,4'-DDE	5.655	6.357	19612332	146.1E6	19.404	20.977
13)	MA Dieldrin	5.790	6.510	20481589	144.4E6	19.335	20.760
14)	MA Endrin	6.049	6.729	18039997	114.6E6	19.517	20.983
15)	B Endosulfa...	6.320	6.942	18441990	118.2E6	20.054	21.166
16)	A 4,4'-DDD	6.171	6.851	16163131	108.2E6	19.259	20.441
17)	MA 4,4'-DDT	6.411	7.149	16904804	110.1E6	19.151	20.591
18)	B Endrin al...	6.489	7.066	16515230	103.4E6	20.539	21.400
19)	B Endosulfa...	6.700	7.288	19418163	115.2E6	20.236	21.058
20)	A Methoxychlor	6.957	7.608	44380040	259.9E6	97.364	105.722
21)	B Endrin ke...	7.195	7.762	22835574	133.2E6	20.367	21.584

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD064993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 14:50
Operator : AR\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:03:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:57:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

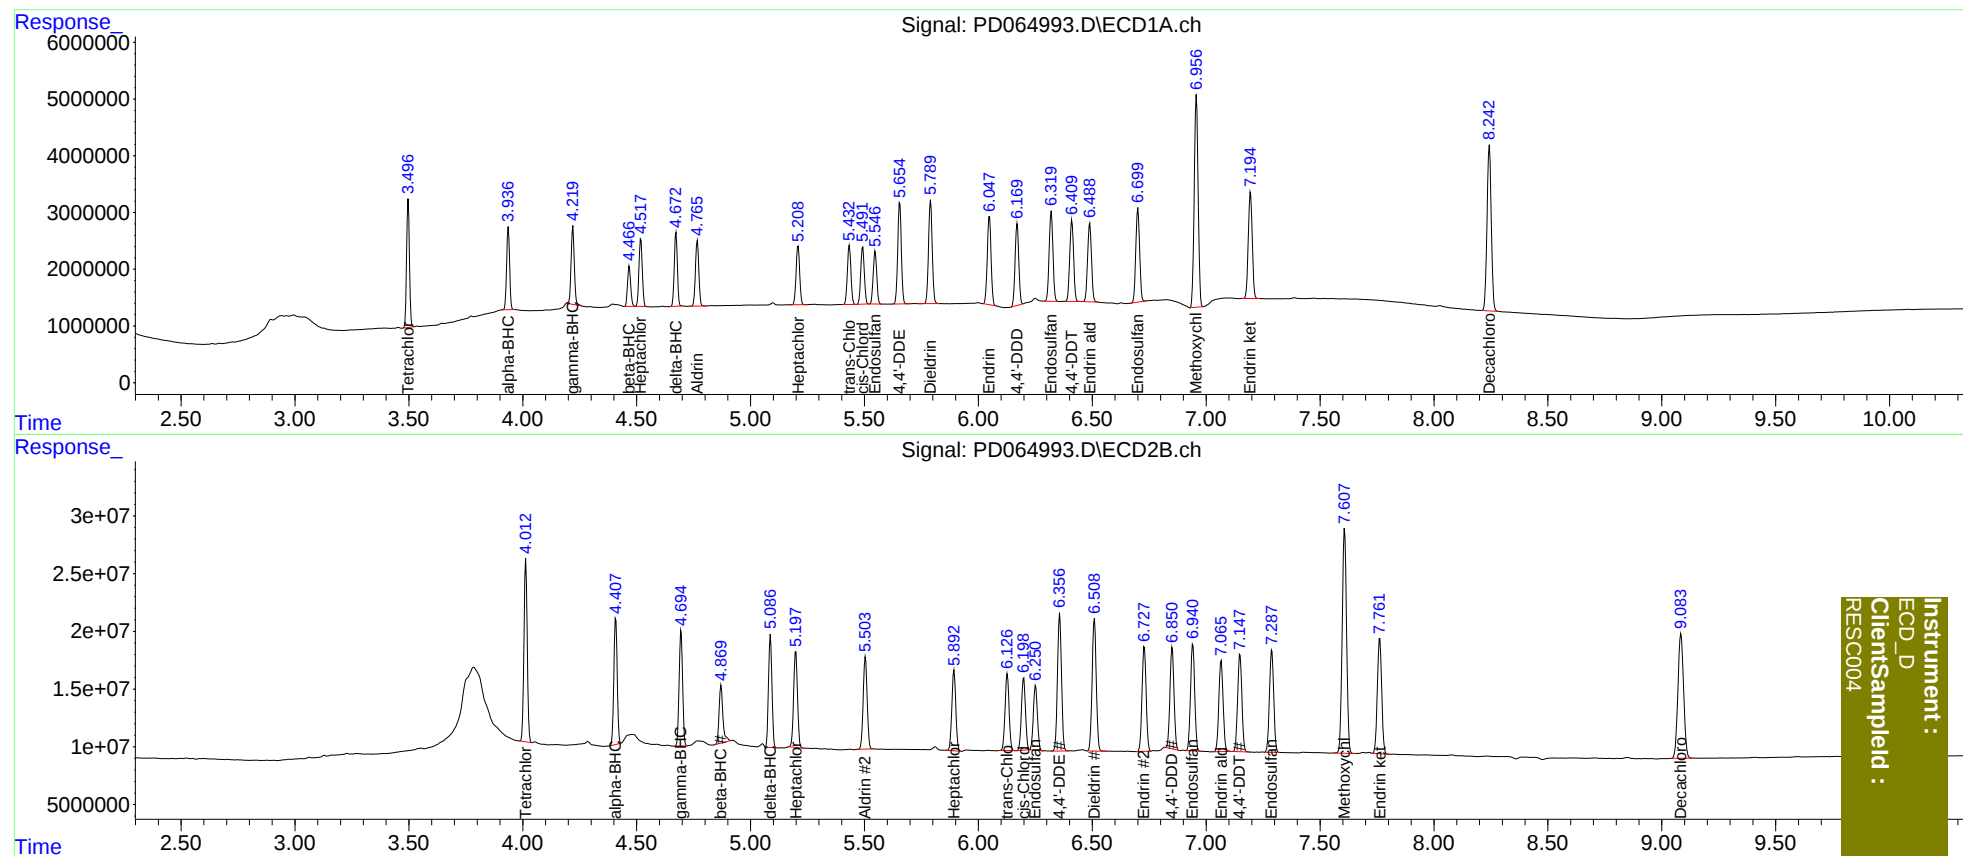

Instrument :
ECD_D
ClientSampled :
RESC004

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081721\
Data File : PD064993.D
Acq On : 17 Aug 2021 14:50
Operator : AR\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Title : GC Extractables
Last Update : Wed Aug 18 02:57:59 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.497	3.937	100.00%
3.937	4.220	100.00%
4.220	4.468	100.00%
4.468	4.519	100.00%
4.519	4.673	100.00%
4.673	4.767	100.00%
4.767	5.209	100.00%
5.209	5.434	100.00%
5.434	5.493	100.00%
5.493	5.547	100.00%
5.547	5.655	100.00%
5.655	5.790	100.00%
5.790	6.049	100.00%
6.049	6.171	100.00%
6.171	6.320	100.00%
6.320	6.411	100.00%
6.411	6.489	100.00%
6.489	6.700	100.00%
6.700	6.957	100.00%
6.957	7.195	100.00%
7.195	8.243	100.00%

Signal #2

4.014	4.409	100.00%
4.409	4.695	100.00%
4.695	4.871	100.00%
4.871	5.087	100.00%
5.087	5.199	100.00%
5.199	5.504	100.00%
5.504	5.893	100.00%
5.893	6.127	100.00%
6.127	6.199	100.00%
6.199	6.251	99.12%
6.251	6.357	100.00%
6.357	6.510	100.00%
6.510	6.729	100.00%
6.729	6.851	100.00%
6.851	6.942	100.00%
6.942	7.066	100.00%
7.066	7.149	100.00%
7.149	7.288	100.00%
7.288	7.608	100.00%
7.608	7.762	100.00%
7.762	9.084	100.00%

