

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081722\
 Data File : PD071619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2022 13:28
 Operator : AR\AJ
 Sample : INDA303
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3139

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 00:22:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 10 22:43:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.806	3.563	47374139	527.2E6	16.730	17.018
27)	SA Decachlor...	8.000	9.090	91306102	333.9E6	35.811	35.232
Target Compounds							
2)	A alpha-BHC	3.316	4.030	69315458	705.5E6	16.471	17.435
3)	MA gamma-BHC...	3.650	4.365	65634332	589.4E6	16.852	17.726
4)	MA Heptachlor	3.996	4.943	70188765	449.0E6	17.432	18.412
9)	A Endosulfan I	5.160	6.105	56363282	282.2E6	16.862	18.374
13)	MA Dieldrin	5.428	6.382	134.8E6	584.6E6	35.819	36.853
14)	MA Endrin	5.705	6.614	115.3E6	437.9E6	35.830	34.005
16)	A 4,4'-DDD	5.853	6.746	101.8E6	447.7E6	38.944	38.746
17)	MA 4,4'-DDT	6.107	7.058	103.9E6	431.7E6	37.325	37.391
20)	A Methoxychlor	6.686	7.534	273.1E6	979.3E6	197.387	196.525

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081722\
Data File : PD071619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2022 13:28
Operator : AR\AJ
Sample : INDA303
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 00:22:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 22:43:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

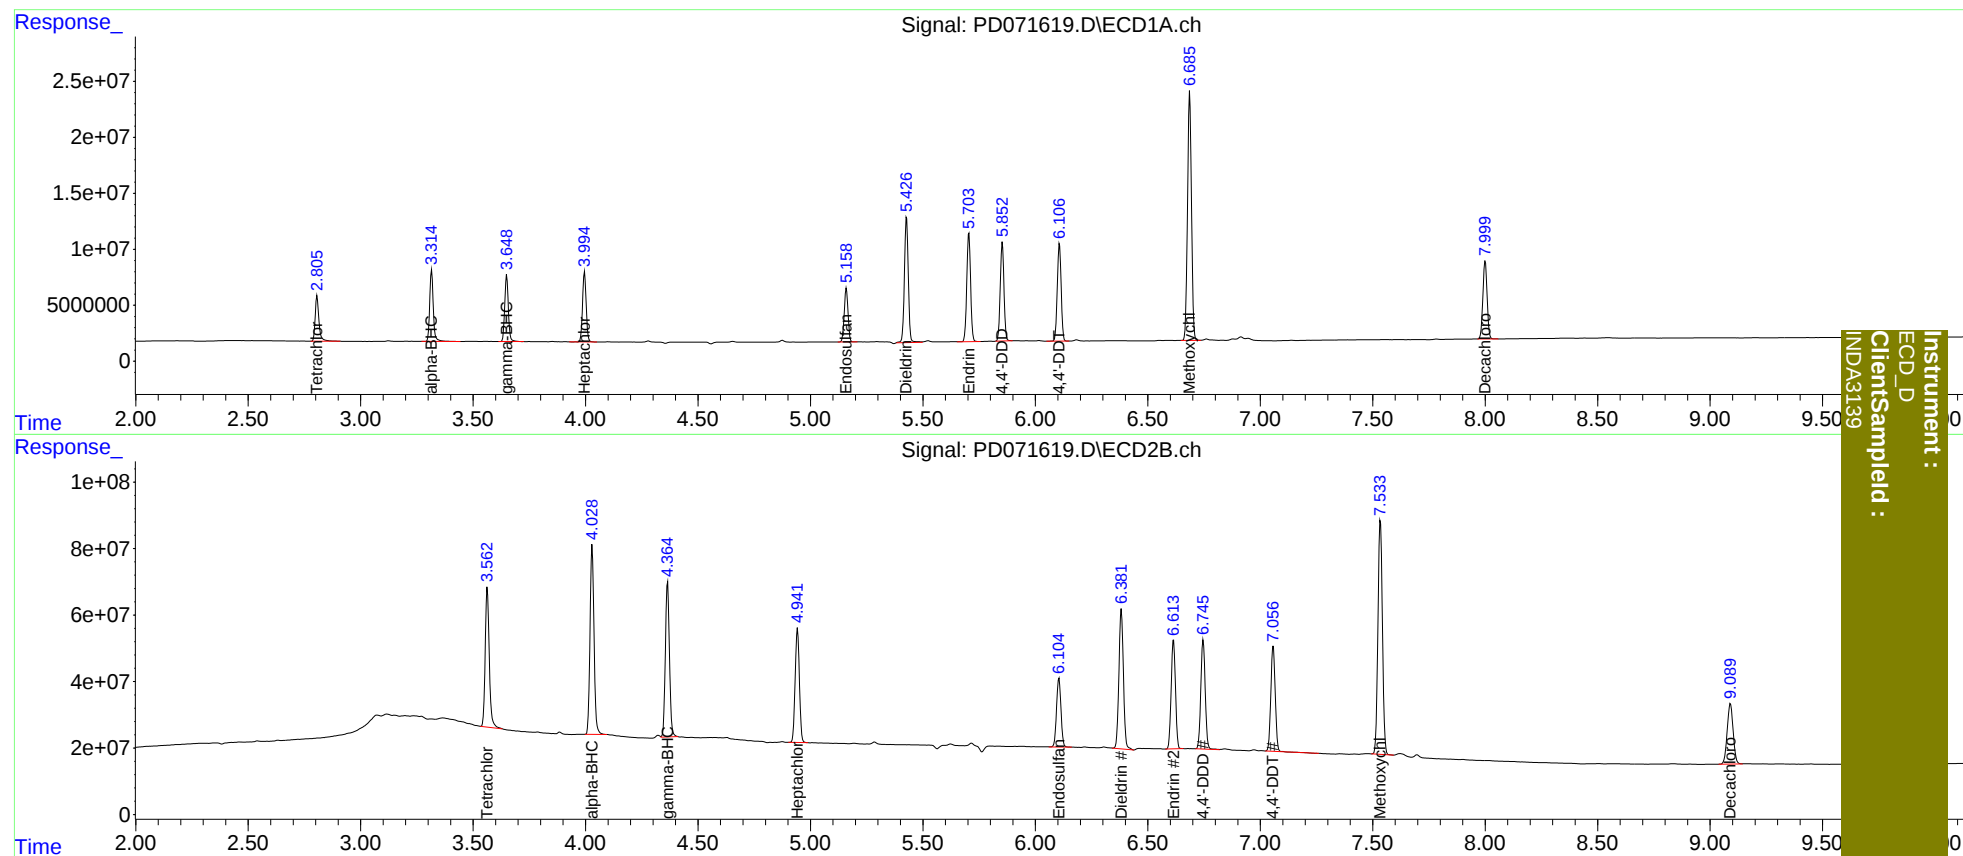

Instrument :
ECD_D
Client Sampled :
INDA3139