

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081723\
 Data File : PD077213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 08:30
 Operator : AR\AJ
 Sample : PIBLK232
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:14:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.761	46510058	25826054	21.185	20.731
27)	SA Decachlor...	9.087	7.903	123.0E6	62771688	48.355	50.357
Target Compounds							
4)	MA Heptachlor	0.000	3.896f	0	243774	N.D.	0.141
5)	MB Aldrin	0.000	4.219	0	1177003	N.D.	0.680
6)	B beta-BHC	0.000	3.896	0	243774	N.D.	0.299
7)	B delta-BHC	4.771	0.000	5718807	0	1.725	N.D. #
8)	B Heptachlo...	5.690	4.739	3478943	371819	1.090	0.227 #
10)	B trans-Chl...	5.986	0.000	2193044	0	0.710	N.D. #
11)	B cis-Chlor...	5.986f	0.000	2193044	0	0.685	N.D. #
13)	MA Dieldrin	0.000	5.397f	0	65853	N.D.	<MDL
14)	MA Endrin	0.000	5.643	0	265861	N.D.	0.192
15)	B Endosulfa...	6.812	5.879f	1998466	184558	0.707	0.138 #
18)	B Endrin al...	0.000	6.116	0	433664	N.D.	0.399
23)	Toxaphene-2	0.000	5.643	0	265861	N.D.	30.390


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081723\
Data File : PD077213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 08:30
Operator : AR\AJ
Sample : PIBLK232
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:14:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

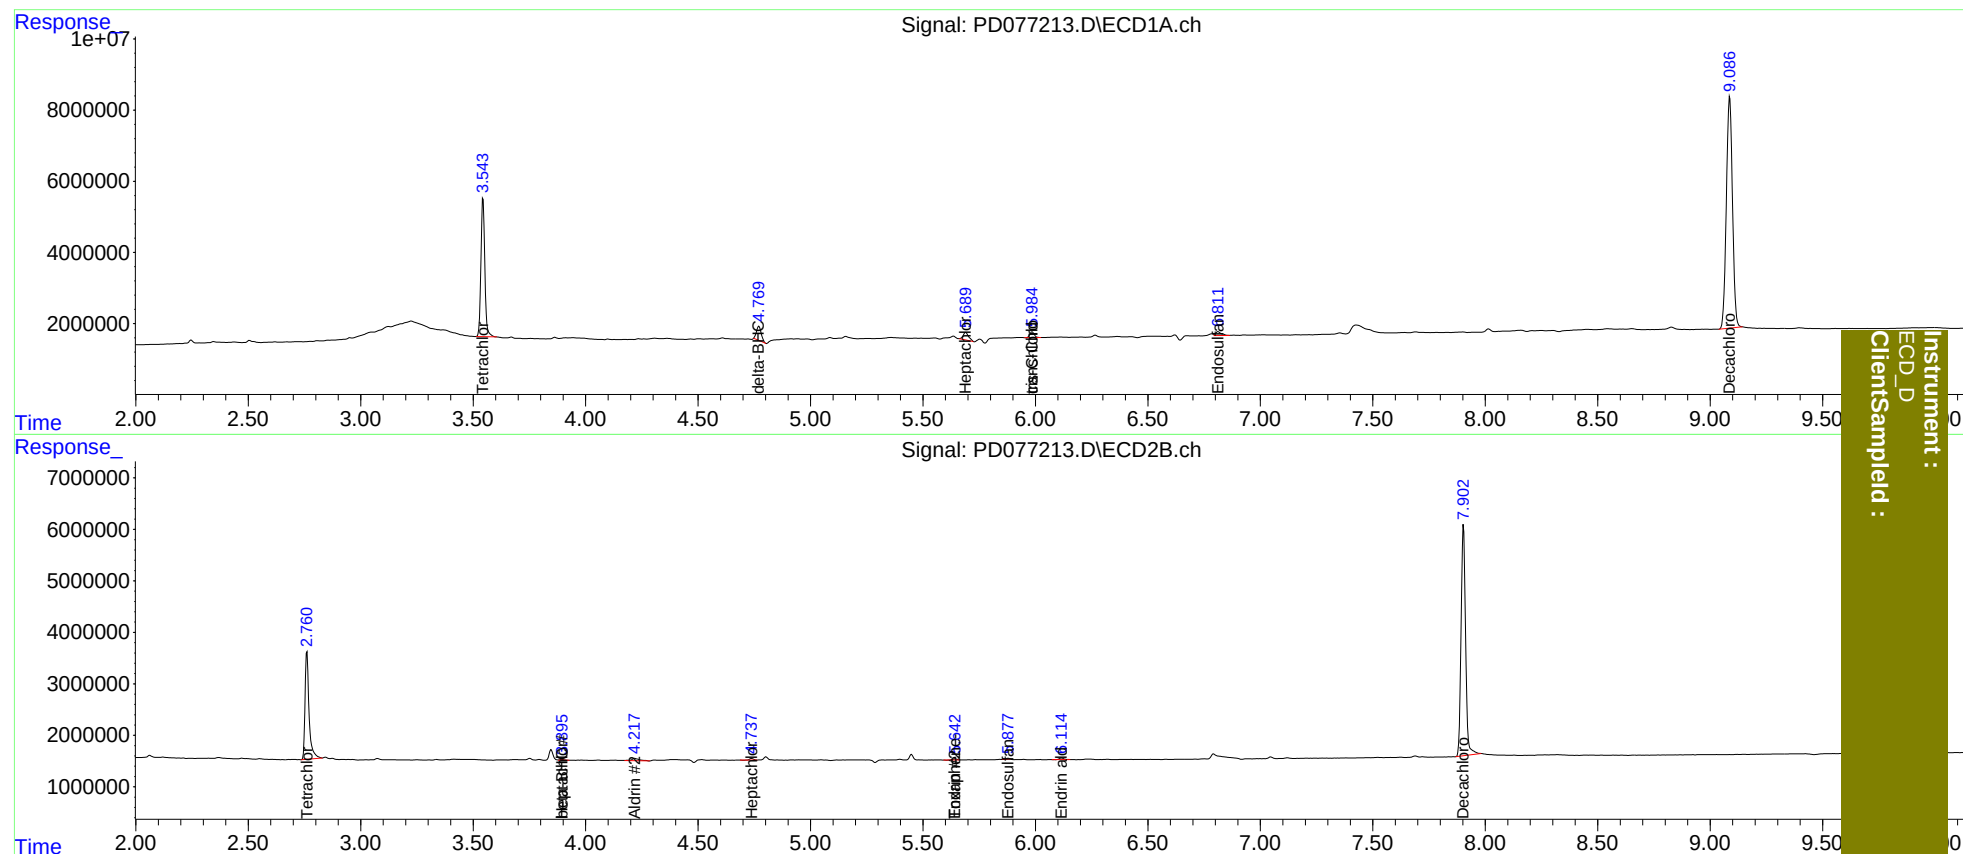


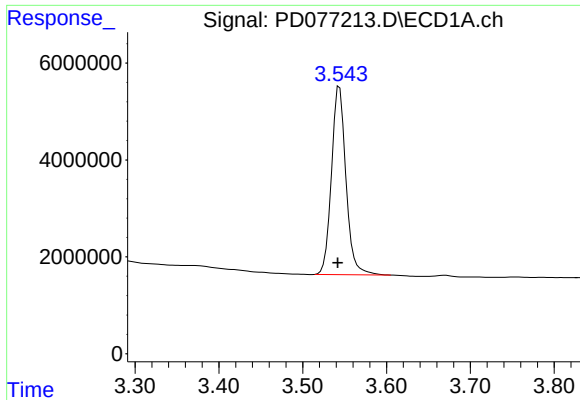

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.002 min
Response: 46510058
Conc: 21.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

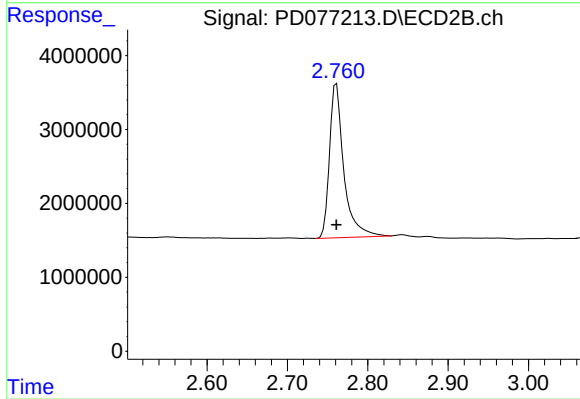


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 25826054
Conc: 20.73 ng/ml

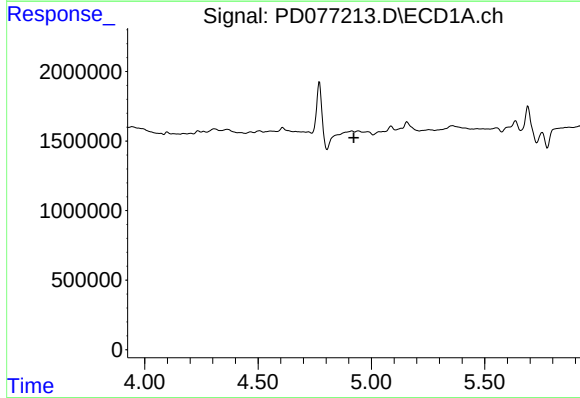


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.923 min
Response: 0
Conc: N.D.

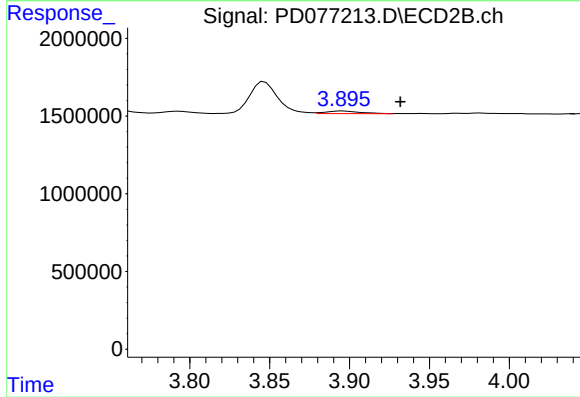

#4 Heptachlor


R.T.: 3.896 min
Delta R.T.: -0.036 min
Response: 243774
Conc: 0.14 ng/ml

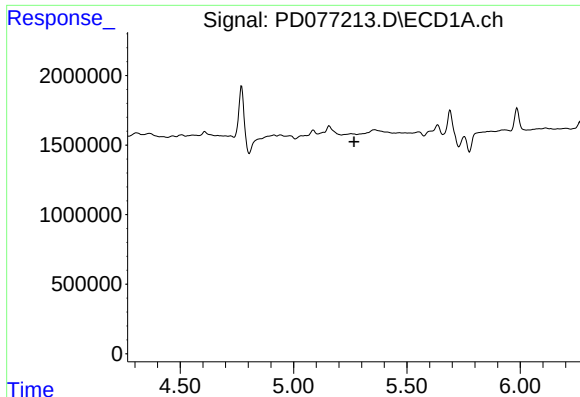

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

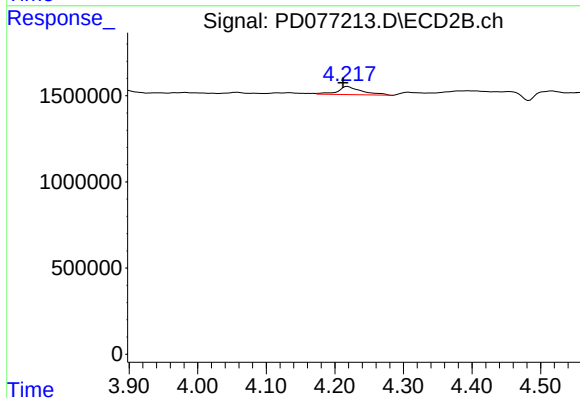


#5 Aldrin

R.T.: 4.219 min
Delta R.T.: 0.007 min
Response: 1177003
Conc: 0.68 ng/ml

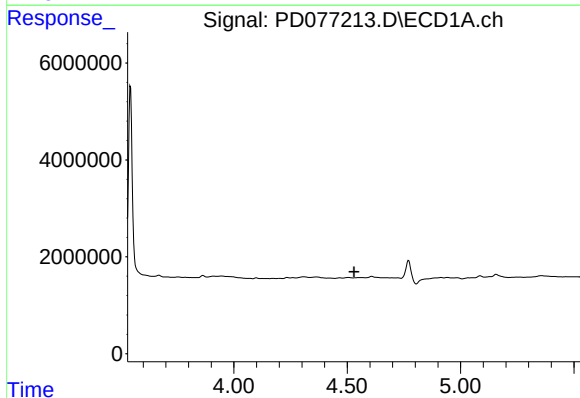


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.530 min
Response: 0
Conc: N.D.

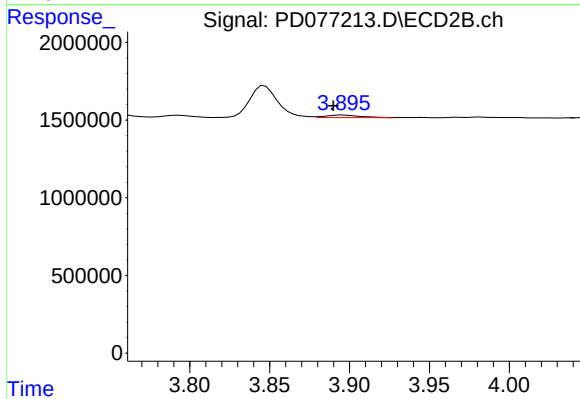

#6 beta-BHC


R.T.: 3.896 min
Delta R.T.: 0.006 min
Response: 243774
Conc: 0.30 ng/ml

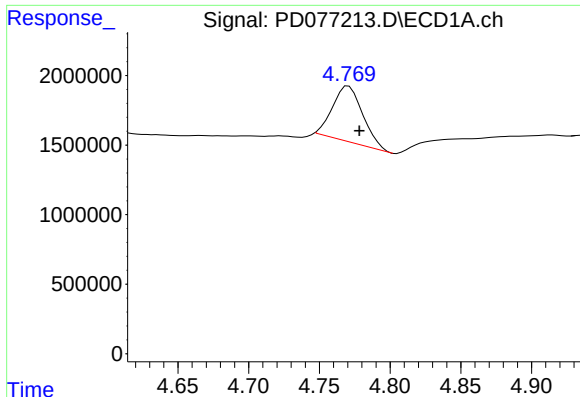

#7 delta-BHC


R.T.: 4.771 min
Delta R.T.: -0.008 min
Response: 5718807
Conc: 1.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

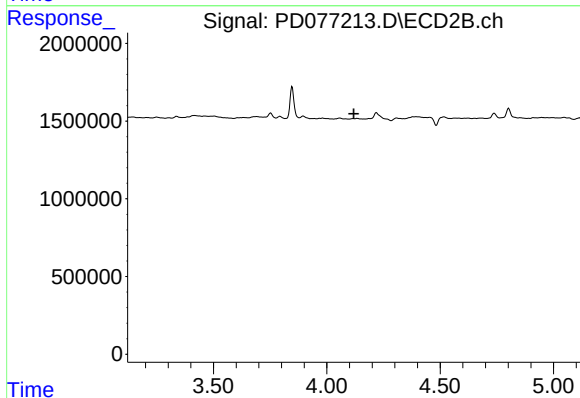


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.119 min
Response: 0
Conc: N.D.

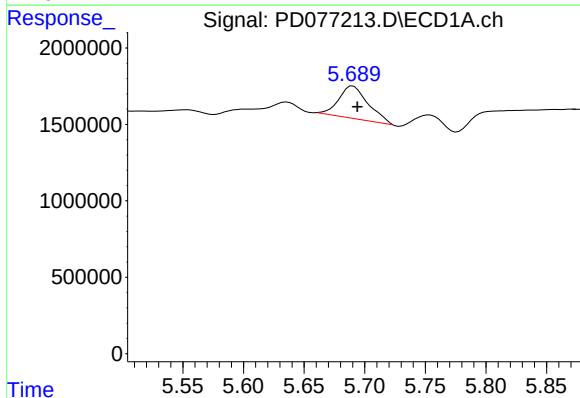


#8 Heptachlor epoxide

R.T.: 5.690 min
Delta R.T.: -0.004 min
Response: 3478943
Conc: 1.09 ng/ml

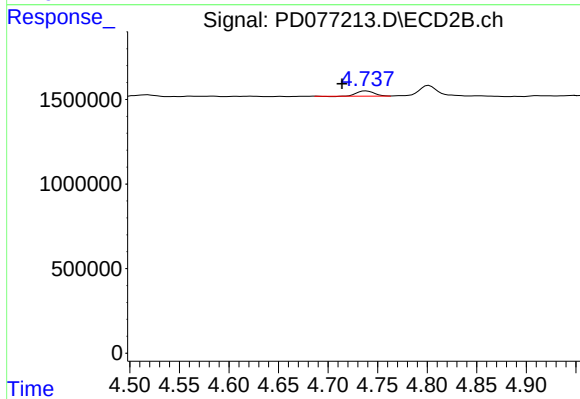

#8 Heptachlor epoxide


R.T.: 4.739 min
Delta R.T.: 0.024 min
Response: 371819
Conc: 0.23 ng/ml

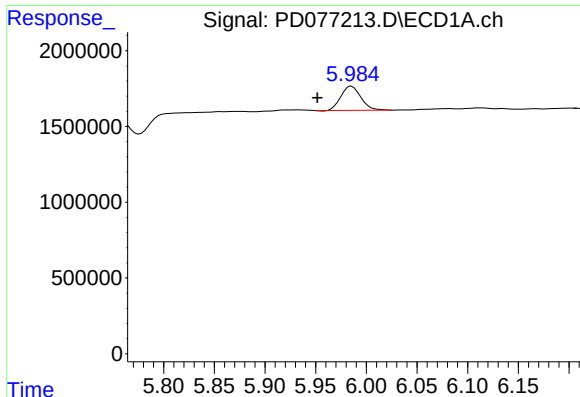

#10 trans-Chlordane


R.T.: 5.986 min
Delta R.T.: 0.034 min
Response: 2193044
Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

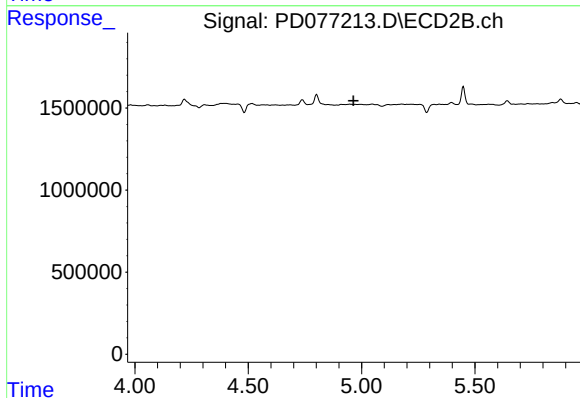


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

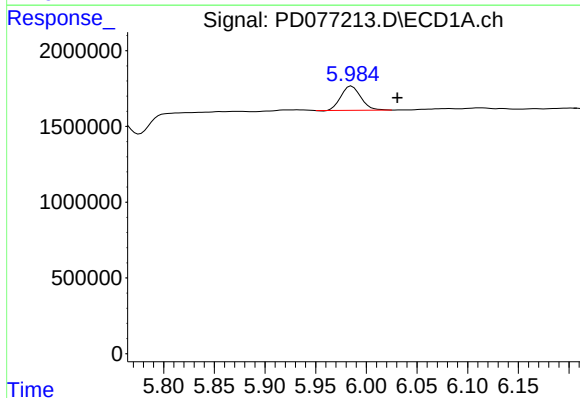


#11 cis-Chlordane

R.T.: 5.986 min
Delta R.T.: -0.045 min
Response: 2193044
Conc: 0.68 ng/ml

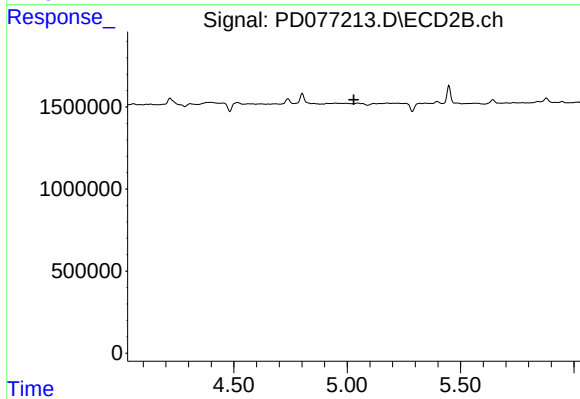

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.029 min
Response: 0
Conc: N.D.

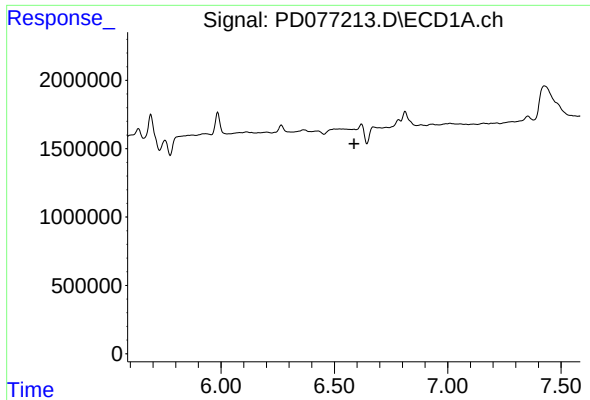

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

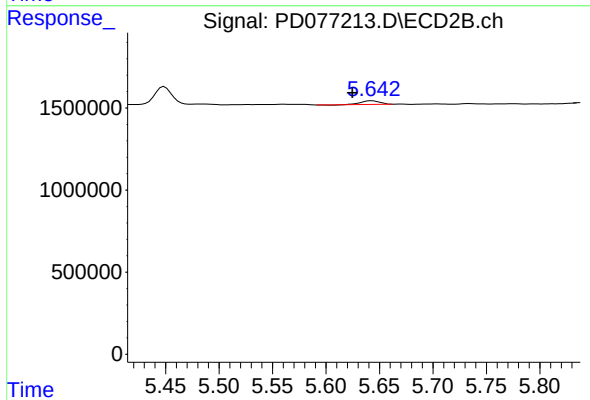


#14 Endrin

R.T.: 5.643 min
Delta R.T.: 0.018 min
Response: 265861
Conc: 0.19 ng/ml

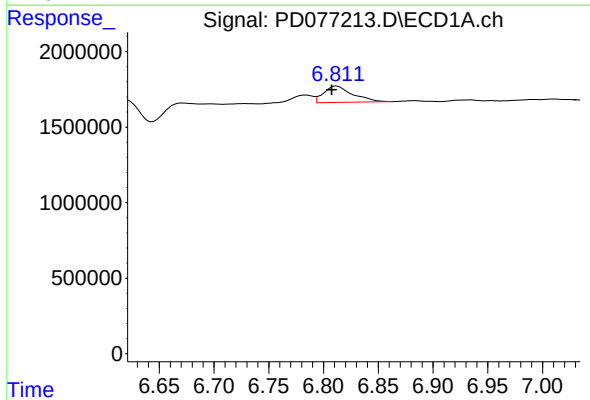


#15 Endosulfan II

R.T.: 6.812 min
Delta R.T.: 0.005 min
Response: 1998466
Conc: 0.71 ng/ml

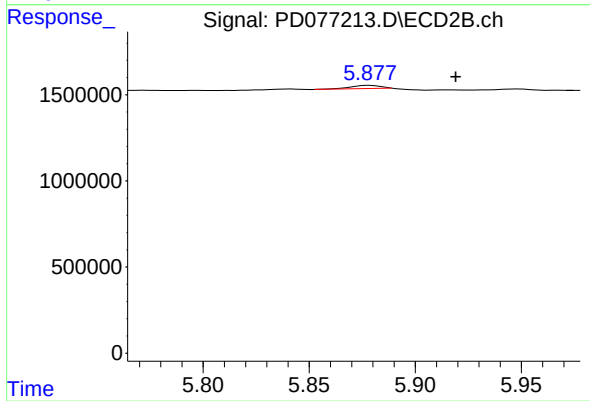

#15 Endosulfan II


R.T.: 5.879 min
Delta R.T.: -0.040 min
Response: 184558
Conc: 0.14 ng/ml

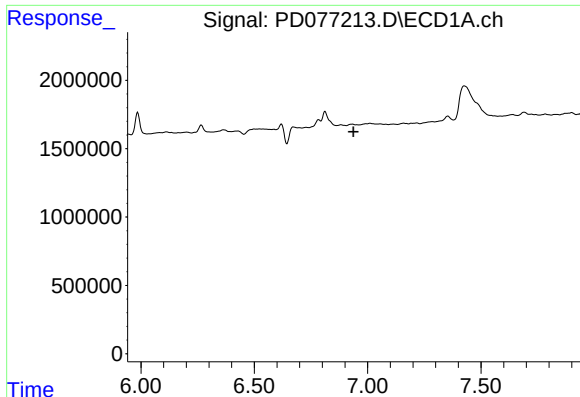

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.938 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

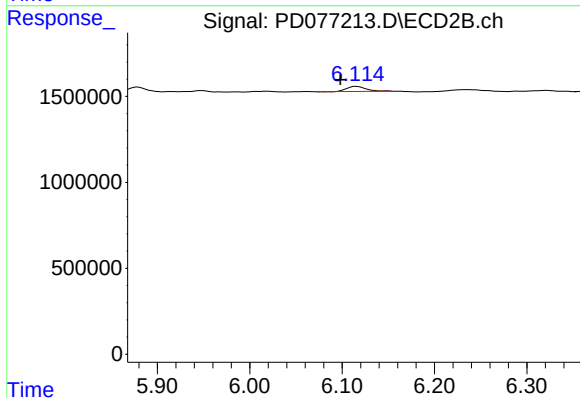


#18 Endrin aldehyde

R.T.: 6.116 min
Delta R.T.: 0.017 min
Response: 433664
Conc: 0.40 ng/ml

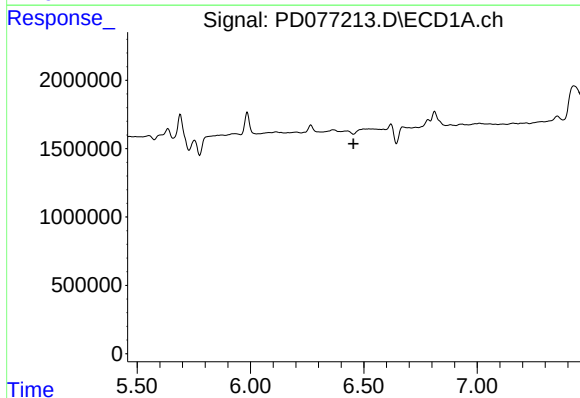


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

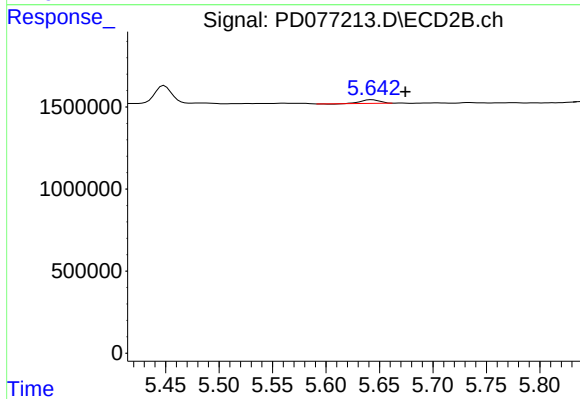

#23 Toxaphene-2


R.T.: 5.643 min
Delta R.T.: -0.031 min
Response: 265861
Conc: 30.39 ng/ml

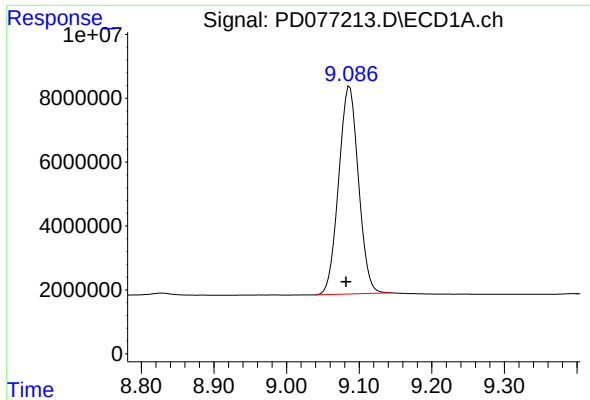

#27 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.005 min
Response: 123045458
Conc: 48.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

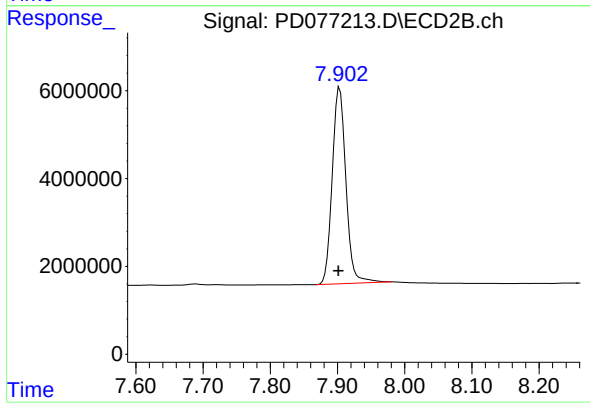

#27 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.002 min
Response: 62771688
Conc: 50.36 ng/ml