

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081723\
 Data File : PD077216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 09:45
 Operator : AR\AJ
 Sample : PB154795BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:15:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.761	42534127	23466583	19.374	18.837
2)	SA Decachlor...	9.095	7.906	96669163	47197162	37.990	37.863
Target Compounds							
3)	MA gamma-BHC...	0.000	3.607	0	263693	N.D.	0.153
6)	B beta-BHC	0.000	3.850f	0	4019289	N.D.	4.923
7)	B delta-BHC	4.780	0.000	5511583	0	1.663	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081723\
Data File : PD077216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 09:45
Operator : AR\AJ
Sample : PB154795BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:15:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

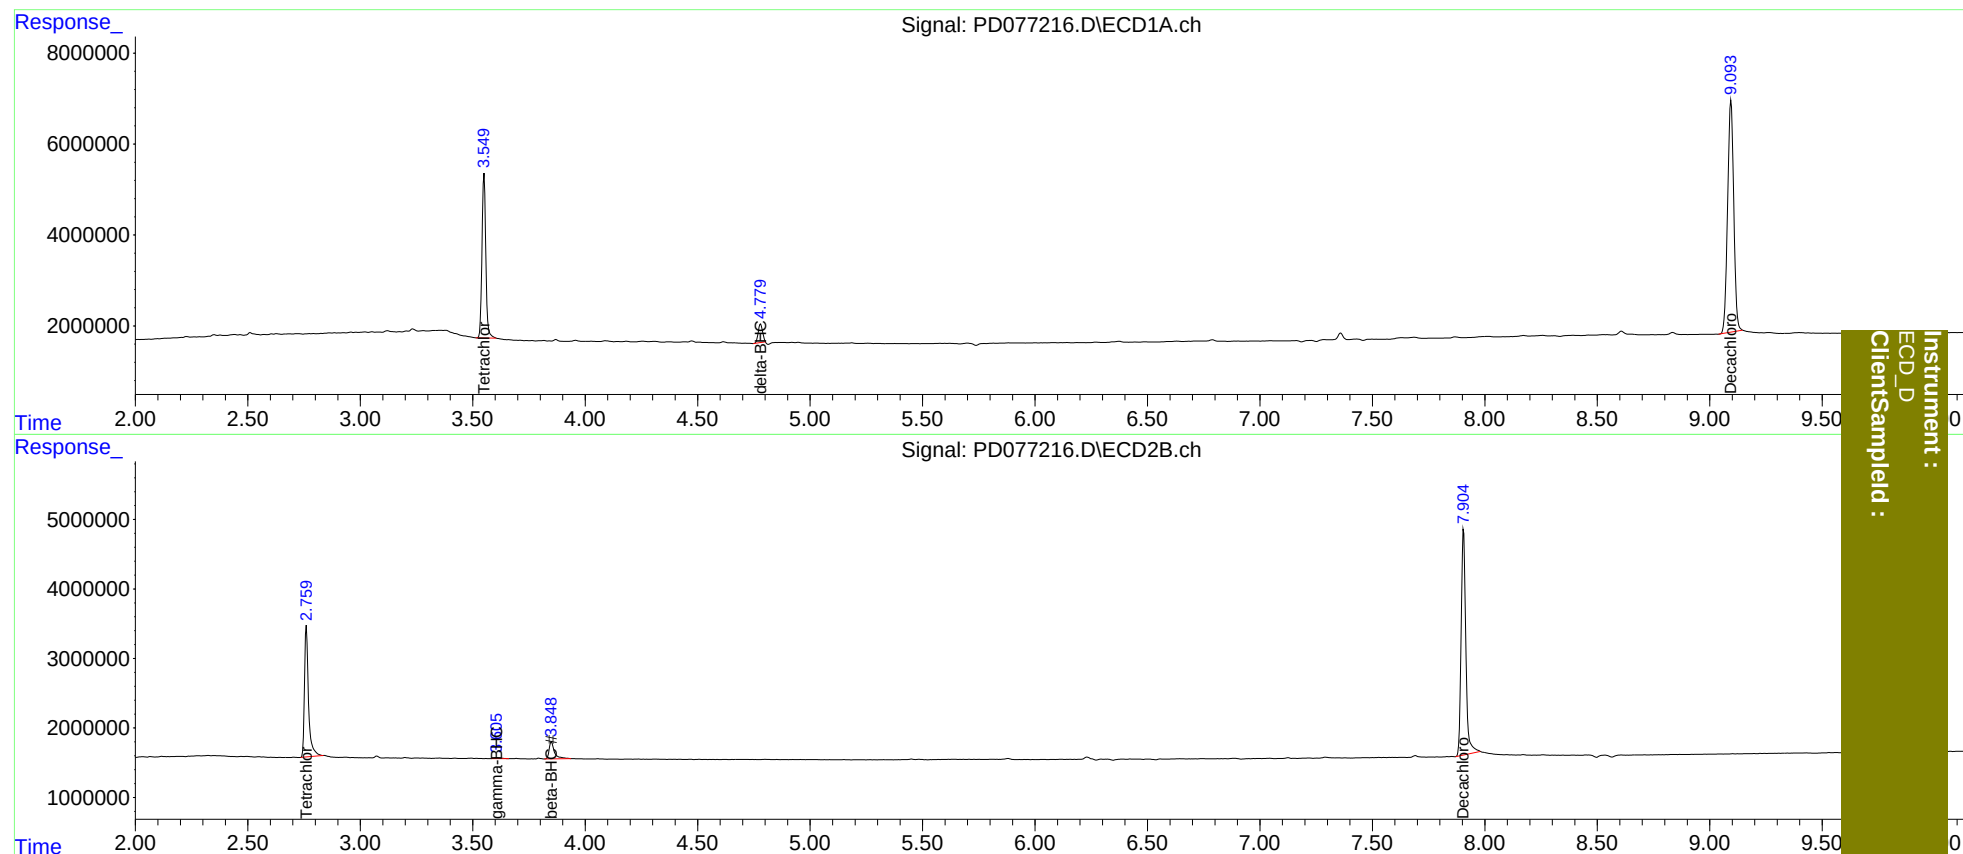


Instrument :
ECD_D
ClientSampled :
0

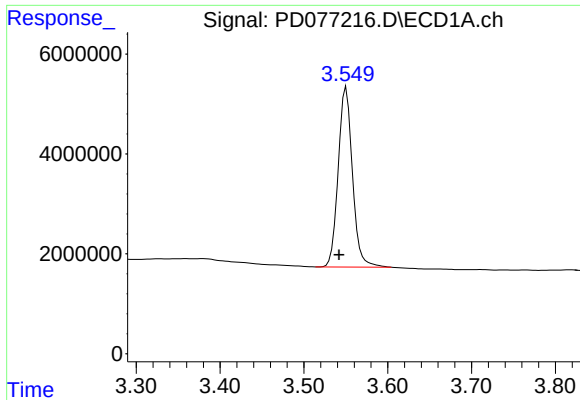

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.008 min
Response: 42534127
Conc: 19.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

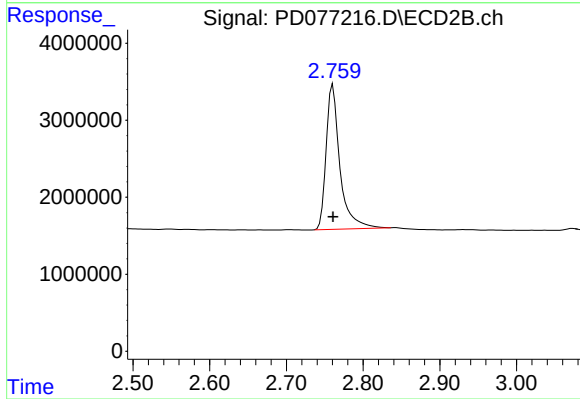


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 23466583
Conc: 18.84 ng/ml

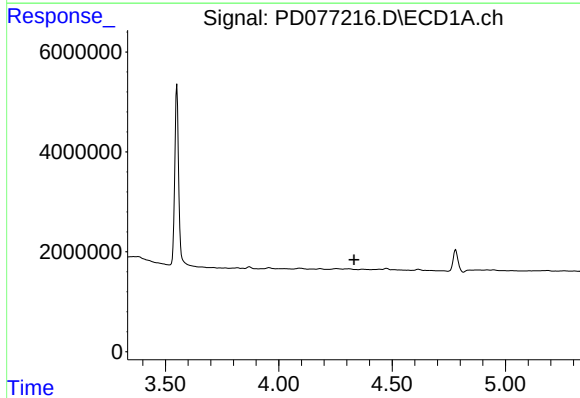


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.332 min
Response: 0
Conc: N.D.

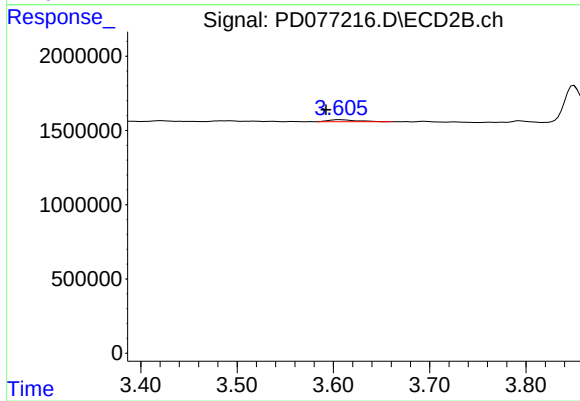

#3 gamma-BHC (Lindane)


R.T.: 3.607 min
Delta R.T.: 0.014 min
Response: 263693
Conc: 0.15 ng/ml

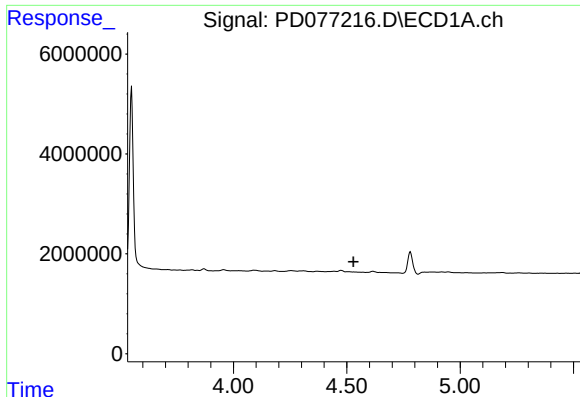

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

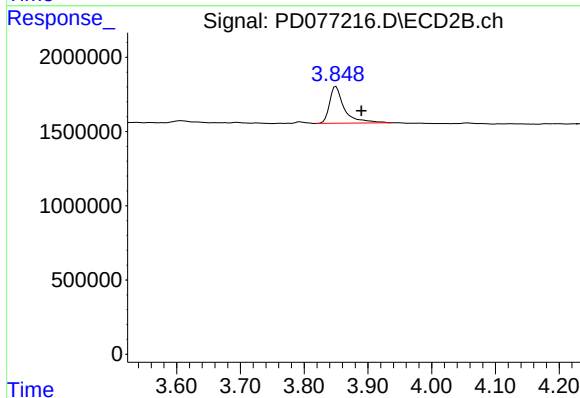


#6 beta-BHC

R.T.: 3.850 min
Delta R.T.: -0.040 min
Response: 4019289
Conc: 4.92 ng/ml

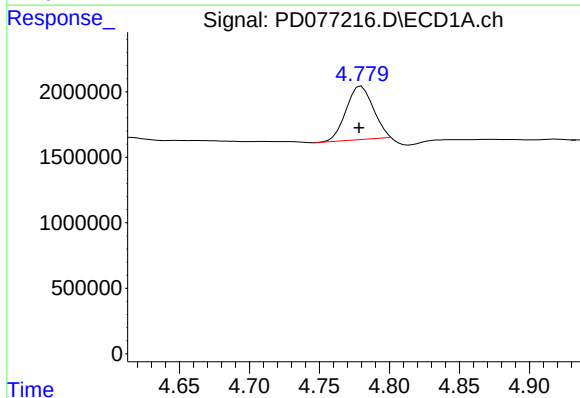


#7 delta-BHC

R.T.: 4.780 min
Delta R.T.: 0.002 min
Response: 5511583
Conc: 1.66 ng/ml

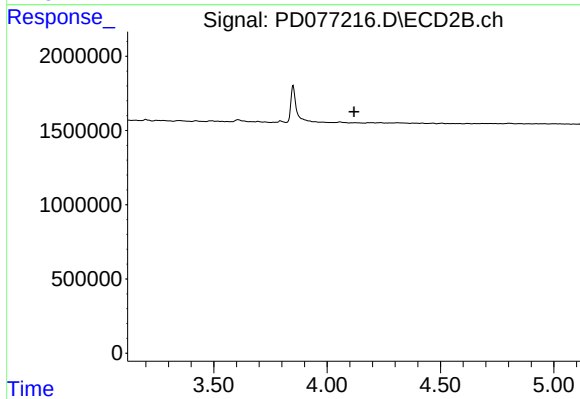

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.119 min
Response: 0
Conc: N.D.

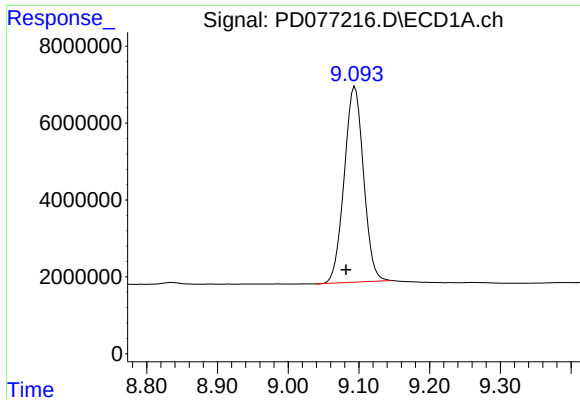

#27 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.013 min
Response: 96669163
Conc: 37.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

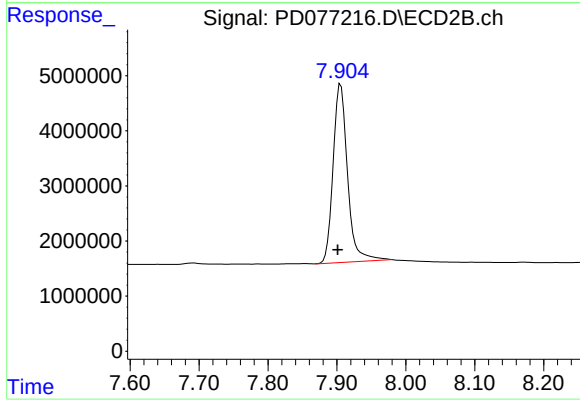

#27 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.004 min
Response: 47197162
Conc: 37.86 ng/ml