

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
 Data File : PD059006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 09:57
 Operator : DD\AJ
 Sample : L3611-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFL0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:42:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	11205516	17074420	11.587	11.790
27)	SA Decachlor...	7.842	8.861	16317849	20657793	15.492	15.063
Target Compounds							
6)	B beta-BHC	4.102f	0.000	1072899	0	1.822	N.D. #
8)	B Heptachlo...	0.000	5.777f	0	9764194	N.D.	5.864
9)	A Endosulfan I	0.000	6.085	0	408528	N.D.	0.263
10)	B trans-Chl...	0.000	5.933	0	997498	N.D.	0.599
11)	B cis-Chlor...	0.000	6.004	0	2017964	N.D.	1.199
15)	B Endosulfa...	0.000	6.771	0	173123	N.D.	0.123
16)	A 4,4'-DDD	0.000	6.625f	0	863108	N.D.	0.658
19)	B Endosulfa...	6.344	0.000	2337764	0	2.284	N.D. #
23)	Toxaphene-2	5.503	0.000	52284253	0	7225.997	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
Data File : PD059006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 09:57
Operator : DD\AJ
Sample : L3611-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFL0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:42:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

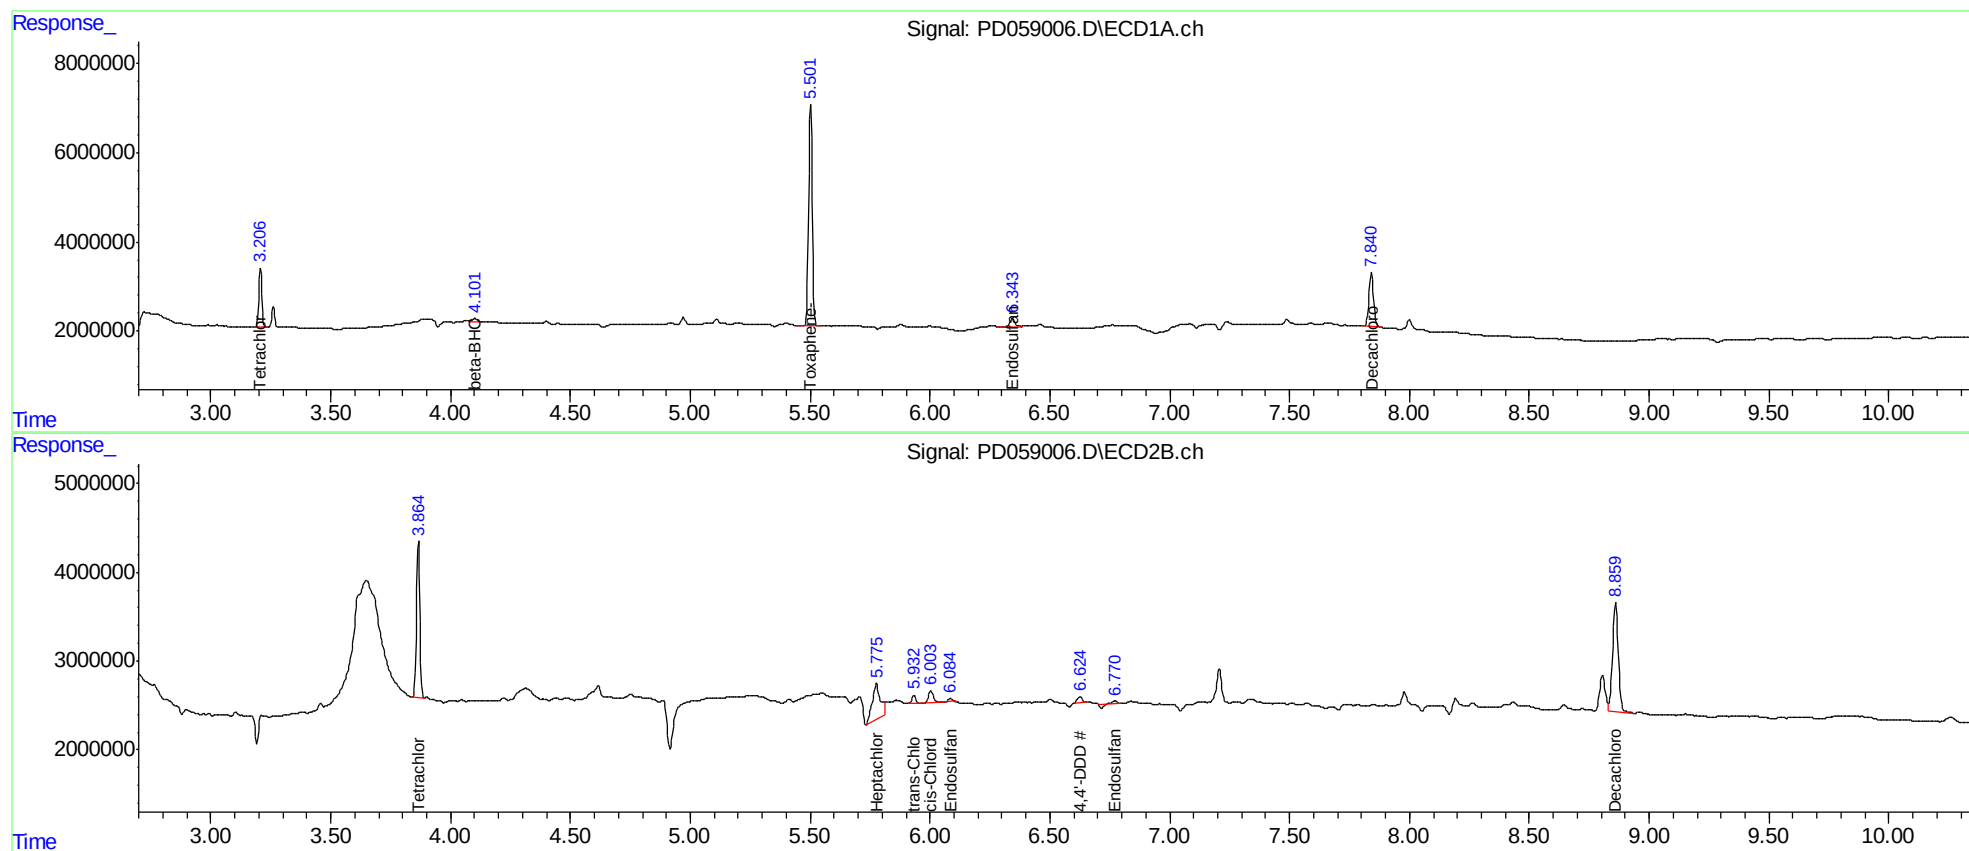


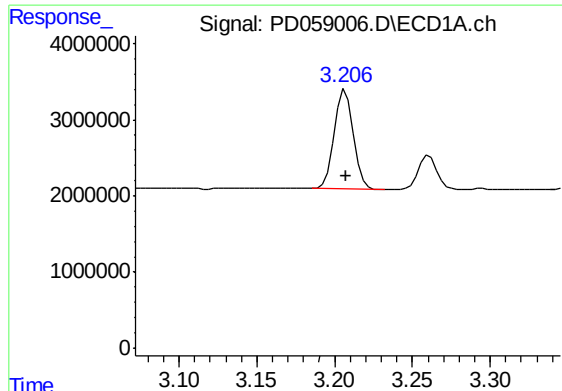

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 11205516
Conc: 11.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

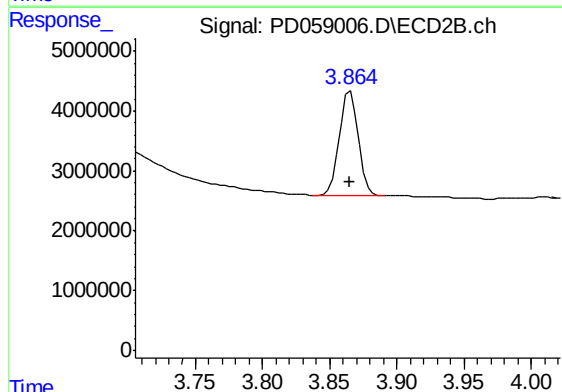


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 17074420
Conc: 11.79 ng/ml

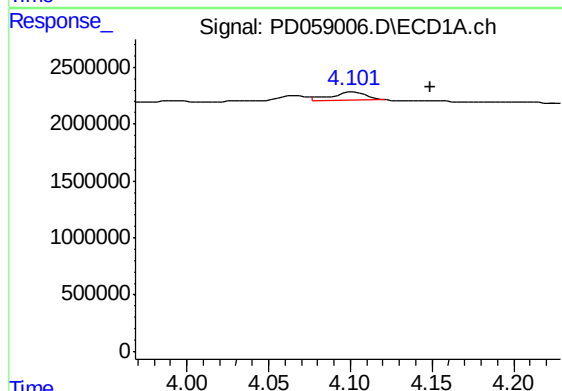


#6 beta-BHC

R.T.: 4.102 min
Delta R.T.: -0.047 min
Response: 1072899
Conc: 1.82 ng/ml

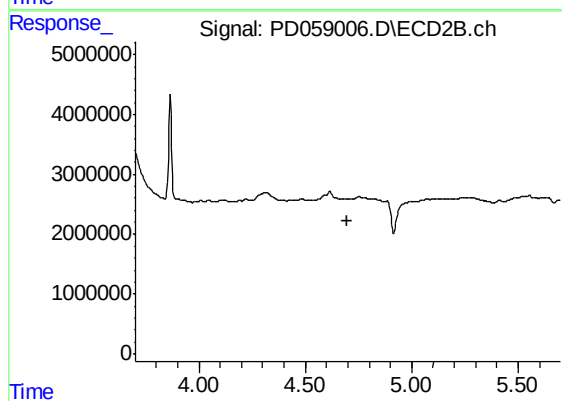

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

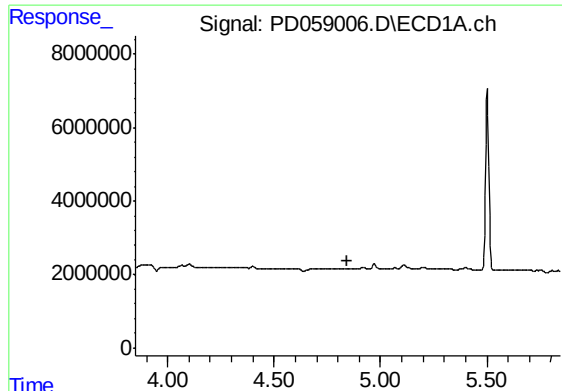

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL0

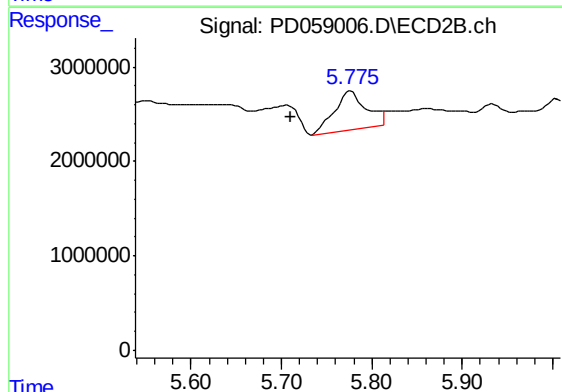


#8 Heptachlor epoxide

R.T.: 5.777 min
Delta R.T.: 0.066 min
Response: 9764194
Conc: 5.86 ng/ml

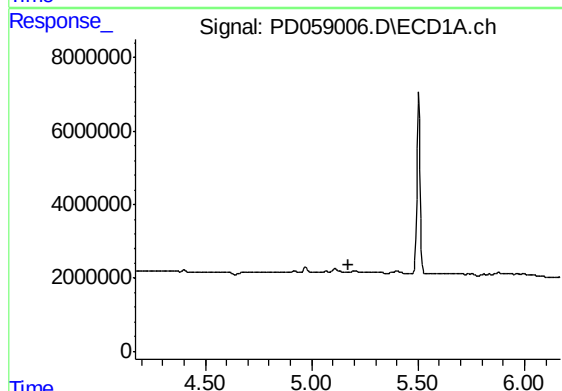


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

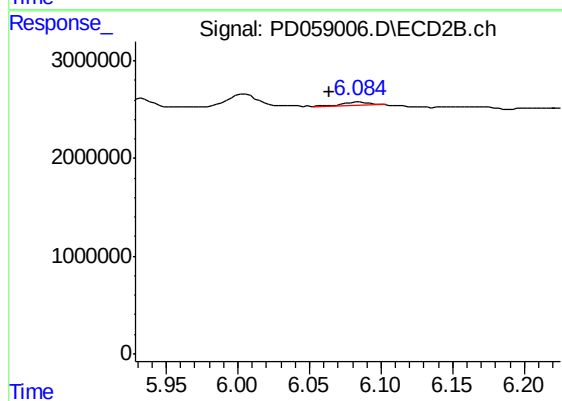

#9 Endosulfan I


R.T.: 6.085 min
Delta R.T.: 0.021 min
Response: 408528
Conc: 0.26 ng/ml

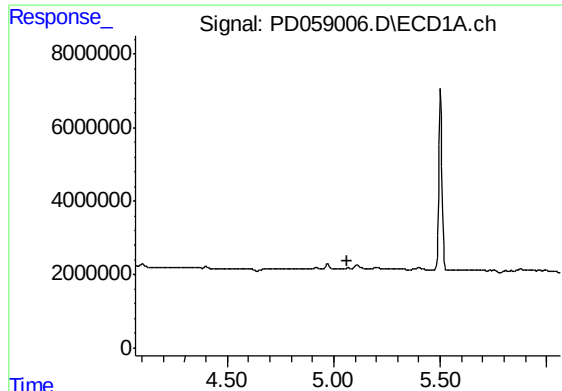

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL0

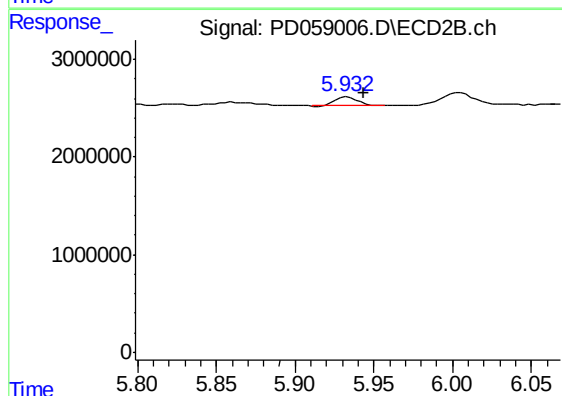


#10 trans-Chlordane

R.T.: 5.933 min
Delta R.T.: -0.011 min
Response: 997498
Conc: 0.60 ng/ml

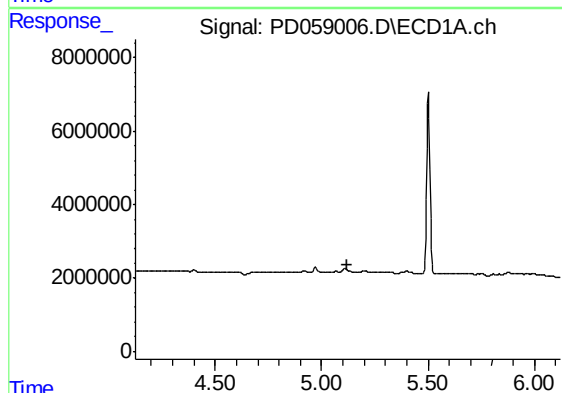


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

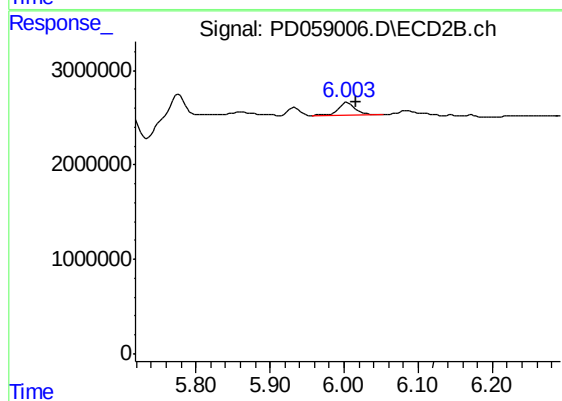

#11 cis-Chlordane


R.T.: 6.004 min
Delta R.T.: -0.012 min
Response: 2017964
Conc: 1.20 ng/ml

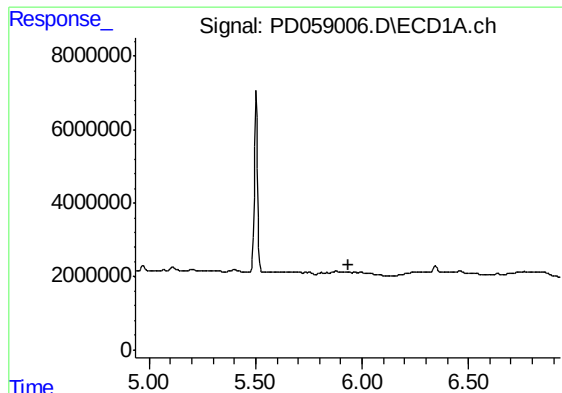

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL0

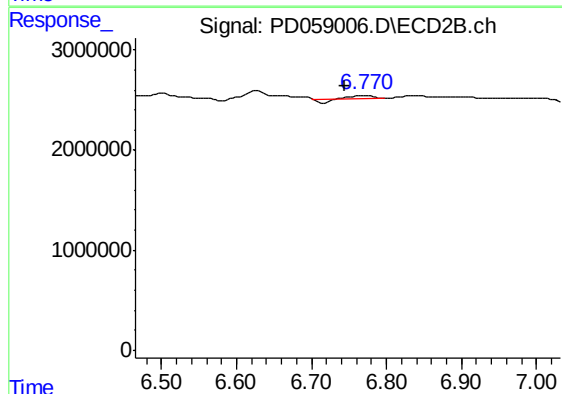


#15 Endosulfan II

R.T.: 6.771 min
Delta R.T.: 0.027 min
Response: 173123
Conc: 0.12 ng/ml

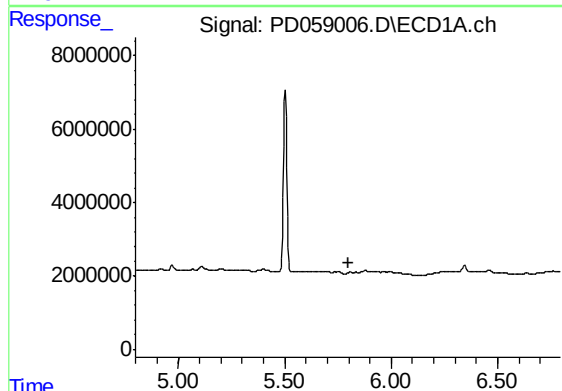


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.798 min
Response: 0
Conc: N.D.

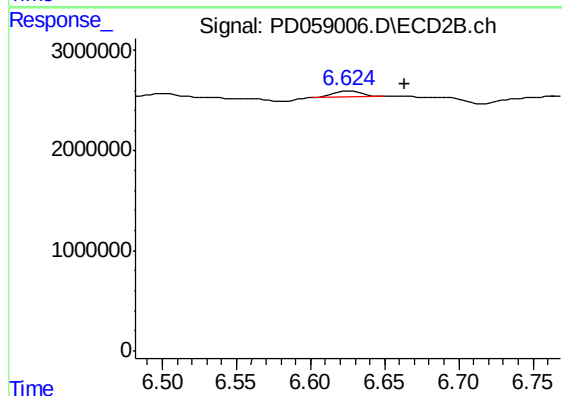

#16 4,4'-DDD


R.T.: 6.625 min
Delta R.T.: -0.038 min
Response: 863108
Conc: 0.66 ng/ml

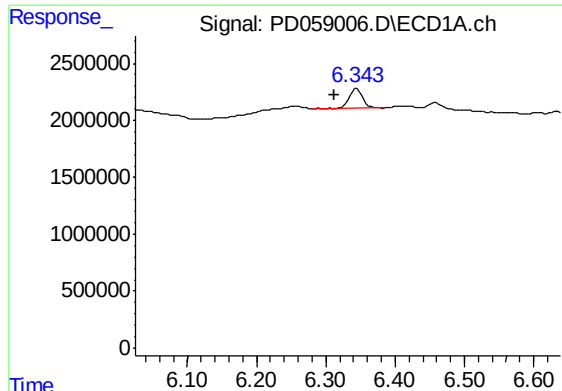

#19 Endosulfan Sulfate


R.T.: 6.344 min
Delta R.T.: 0.032 min
Response: 2337764
Conc: 2.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

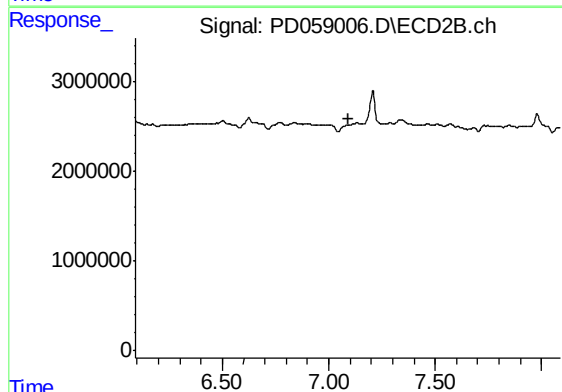


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

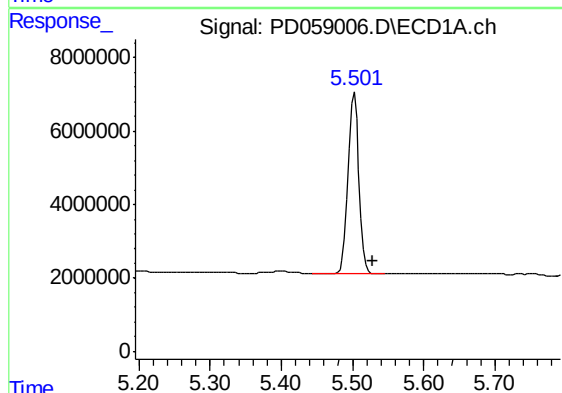


#23 Toxaphene-2

R.T.: 5.503 min
Delta R.T.: -0.026 min
Response: 52284253
Conc: 7226.00 ng/ml

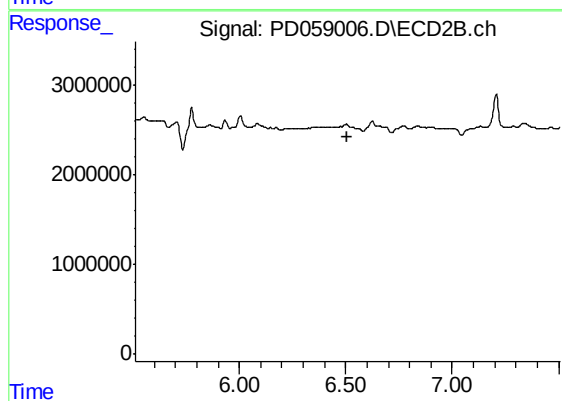

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

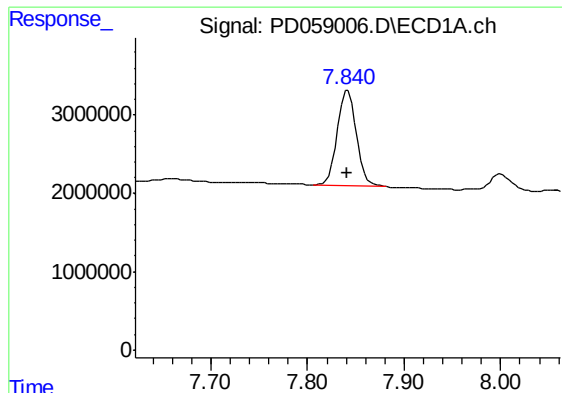

#27 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.001 min
Response: 16317849
Conc: 15.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL0

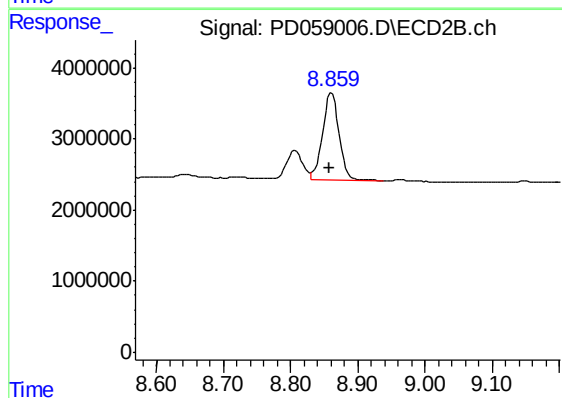

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.002 min
Response: 20657793
Conc: 15.06 ng/ml