

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
 Data File : PD059007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 10:11
 Operator : DD\AJ
 Sample : L3611-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFL1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:42:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	18974687	29046563	19.620	20.056
27)	SA Decachlor...	7.842	8.861	28302146	35139888	26.870	25.623
Target Compounds							
6)	B beta-BHC	4.103f	0.000	1786571	0	3.034	N.D. #
9)	A Endosulfan I	0.000	6.087	0	436289	N.D.	0.281
15)	B Endosulfa...	0.000	6.770	0	201756	N.D.	0.143
16)	A 4,4'-DDD	0.000	6.624f	0	1295210	N.D.	0.988
19)	B Endosulfa...	0.000	7.138f	0	823637	N.D.	0.573
20)	A Methoxychlor	0.000	7.424	0	854420	N.D.	1.237
23)	Toxaphene-2	5.502	0.000	27819408	0	3844.809	N.D. #
26)	Toxaphene-5	0.000	7.424	0	854420	N.D.	47.930


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
Data File : PD059007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 10:11
Operator : DD\AJ
Sample : L3611-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFL1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:42:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

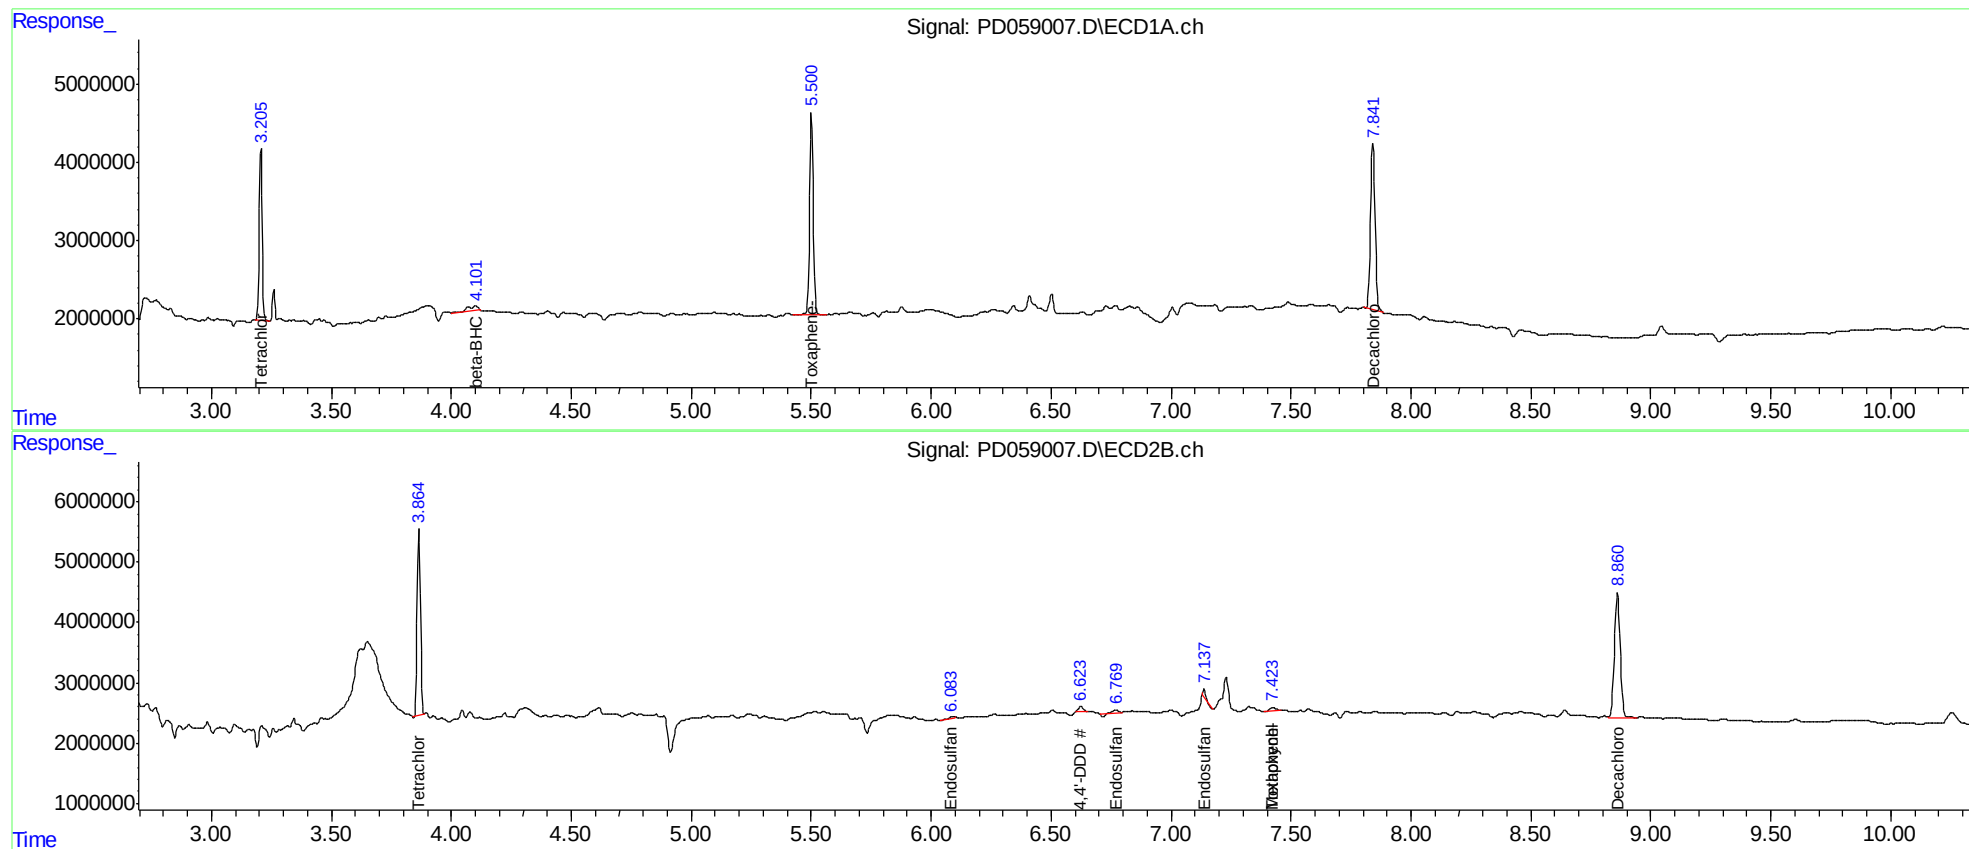


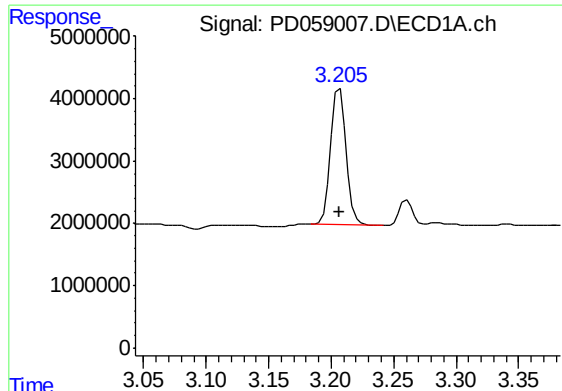

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 18974687
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFL1

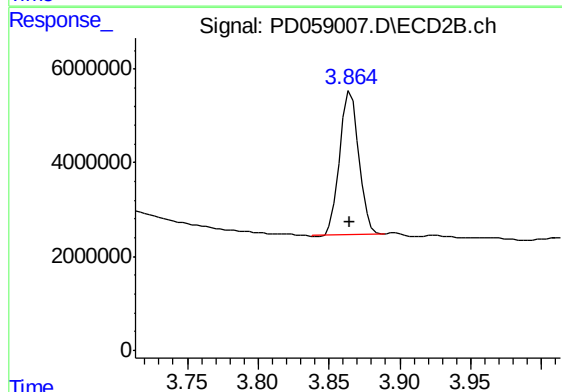


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 29046563
Conc: 20.06 ng/ml

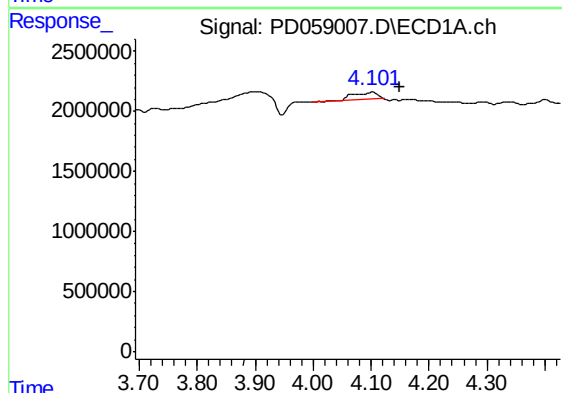


#6 beta-BHC

R.T.: 4.103 min
Delta R.T.: -0.046 min
Response: 1786571
Conc: 3.03 ng/ml

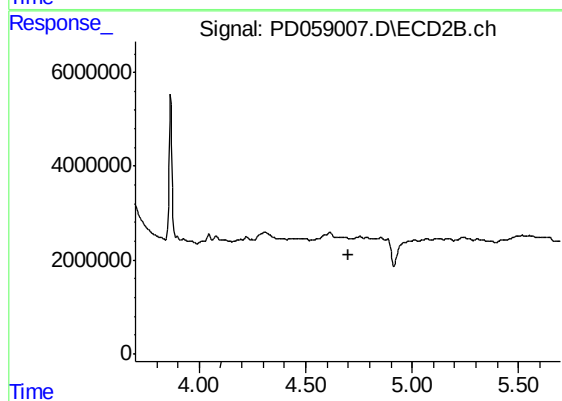

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

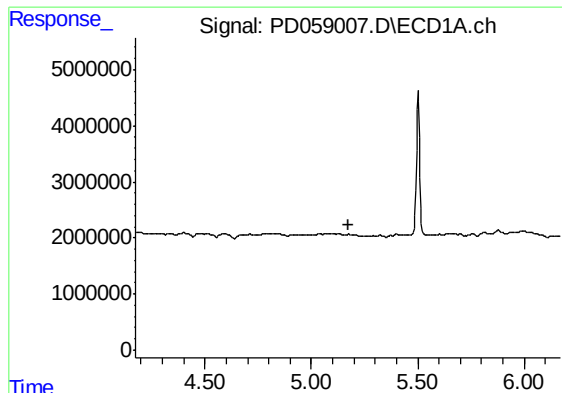

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL1

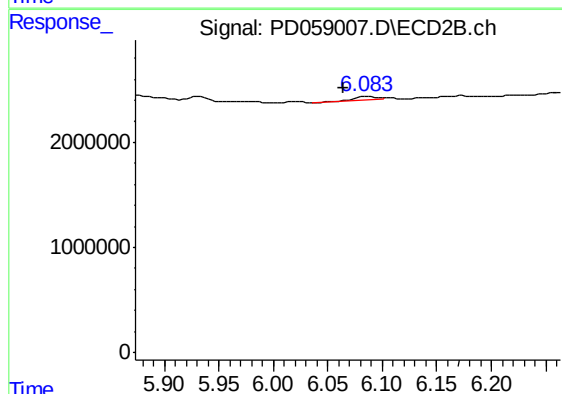


#9 Endosulfan I

R.T.: 6.087 min
Delta R.T.: 0.023 min
Response: 436289
Conc: 0.28 ng/ml

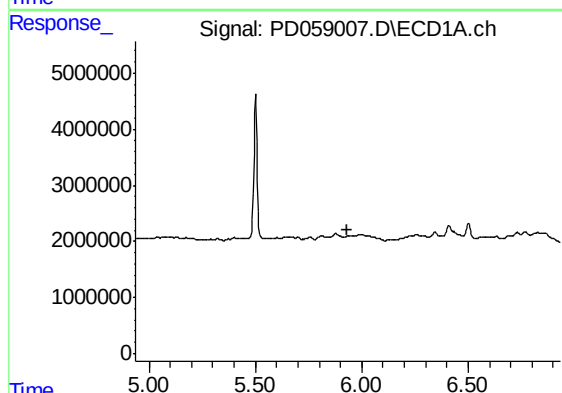


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.934 min
Response: 0
Conc: N.D.

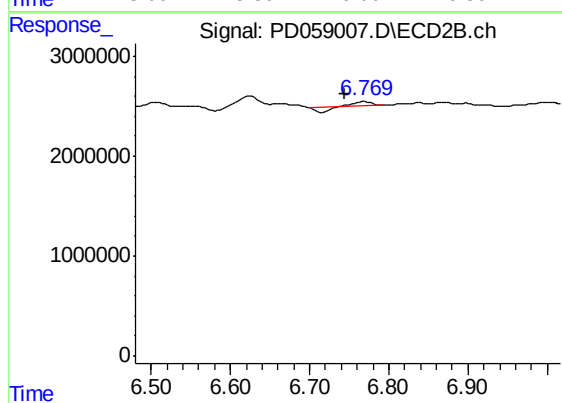

#15 Endosulfan II


R.T.: 6.770 min
Delta R.T.: 0.026 min
Response: 201756
Conc: 0.14 ng/ml

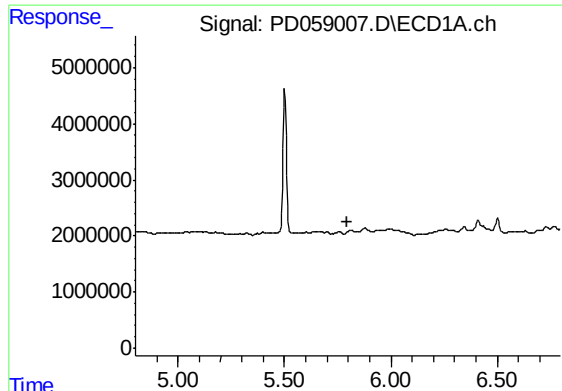

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL1

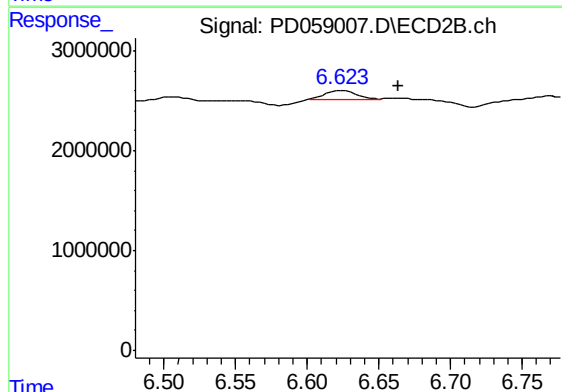


#16 4,4'-DDD

R.T.: 6.624 min
Delta R.T.: -0.039 min
Response: 1295210
Conc: 0.99 ng/ml

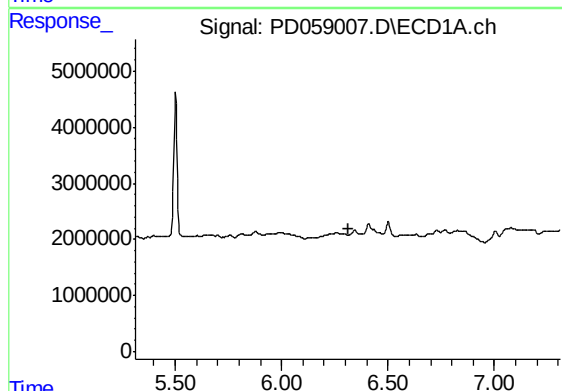


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.312 min
Response: 0
Conc: N.D.

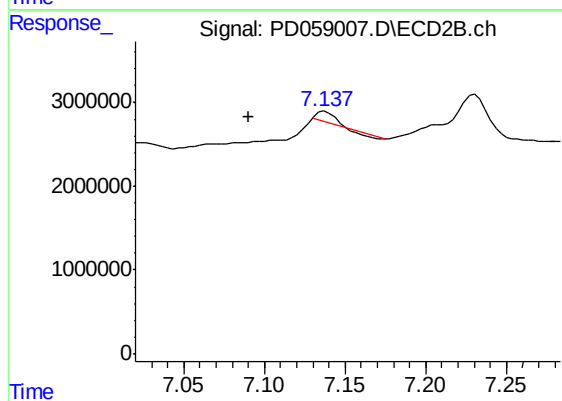

#19 Endosulfan Sulfate


R.T.: 7.138 min
Delta R.T.: 0.048 min
Response: 823637
Conc: 0.57 ng/ml

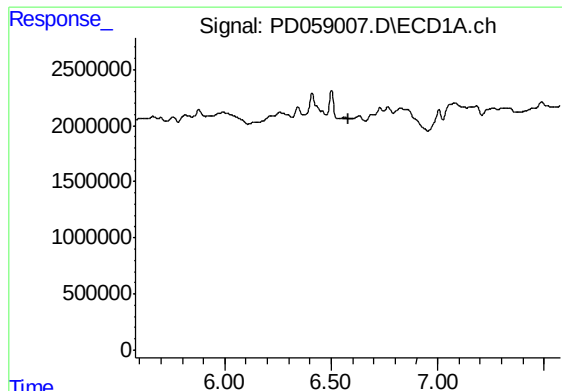

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.580 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL1

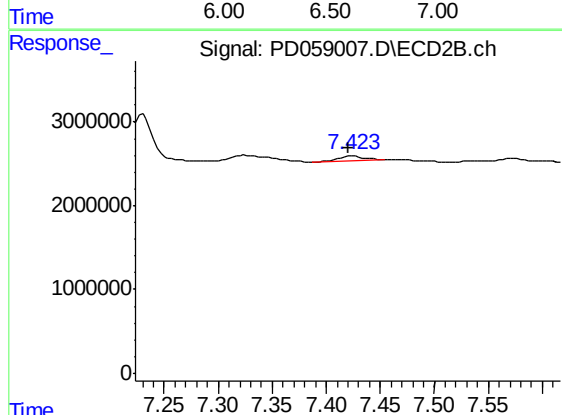


#20 Methoxychlor

R.T.: 7.424 min
Delta R.T.: 0.004 min
Response: 854420
Conc: 1.24 ng/ml

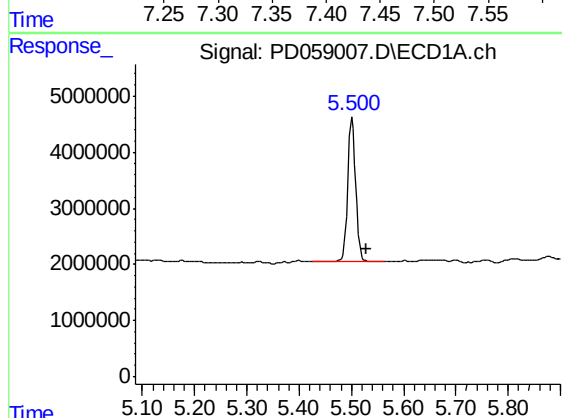


#23 Toxaphene-2

R.T.: 5.502 min
Delta R.T.: -0.027 min
Response: 27819408
Conc: 3844.81 ng/ml

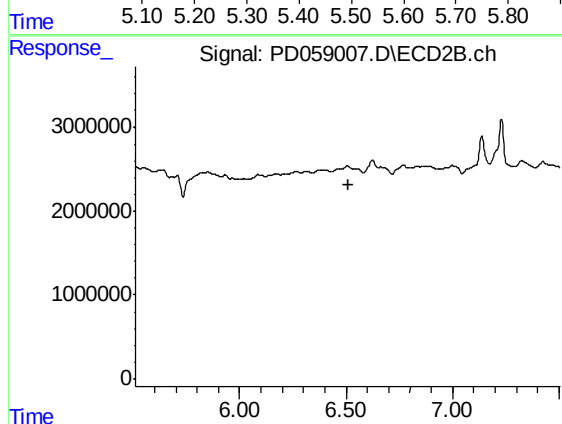

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

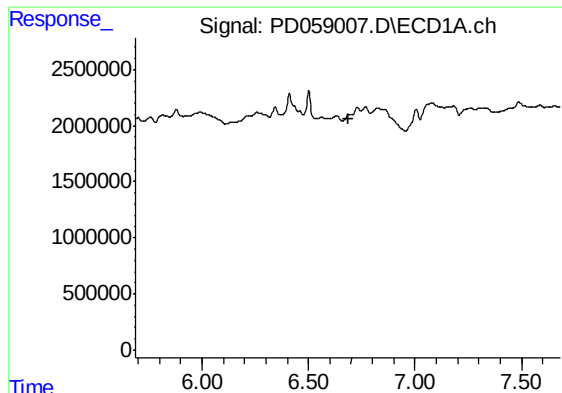

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 6.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFL1

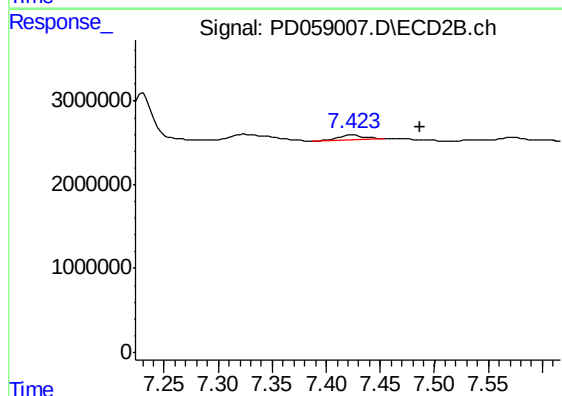


#26 Toxaphene-5

R.T.: 7.424 min
Delta R.T.: -0.062 min
Response: 854420
Conc: 47.93 ng/ml

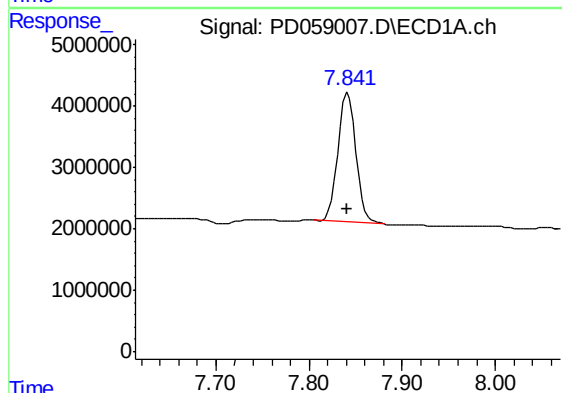

#27 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.001 min
Response: 28302146
Conc: 26.87 ng/ml

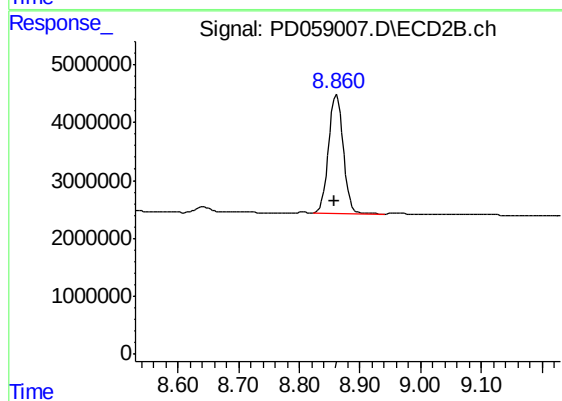

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.003 min
Response: 35139888
Conc: 25.62 ng/ml