

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
 Data File : PD059012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 11:22
 Operator : DD\AJ
 Sample : L3611-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:43:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.207	3.866	12817922	18754951	13.254	12.950
27) SA	Decachlor...	7.842	8.861	18866522	21574291	17.912	15.731
Target Compounds							
8) B	Heptachlo...	0.000	5.762f	0	1769197	N.D.	1.063
9) A	Endosulfan I	0.000	6.019f	0	776100	N.D.	0.501
10) B	trans-Chl...	0.000	5.933	0	1597034	N.D.	0.959
11) B	cis-Chlor...	0.000	6.019	0	776100	N.D.	0.461
16) A	4,4'-DDD	0.000	6.627f	0	3455861	N.D.	2.636


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
Data File : PD059012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 11:22
Operator : DD\AJ
Sample : L3611-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFM1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:43:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

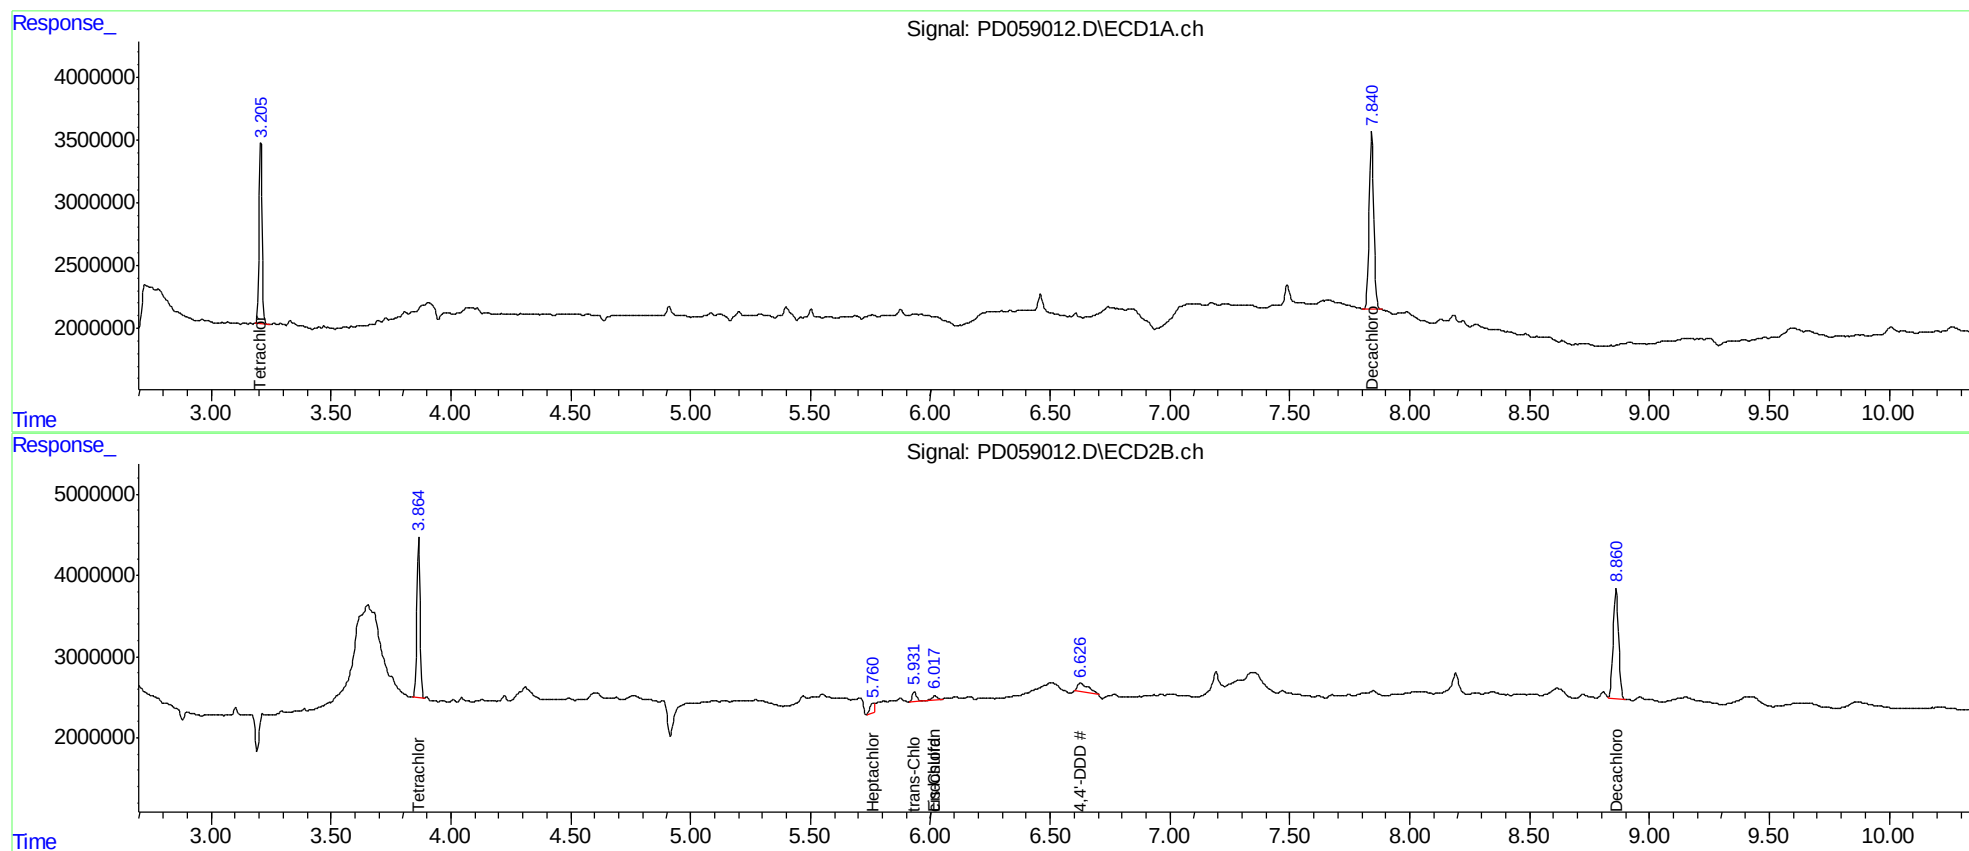


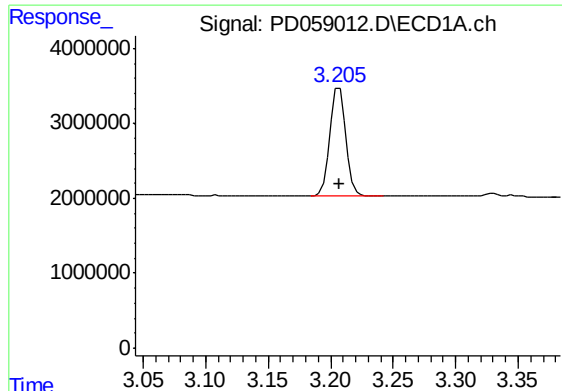

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 12817922
Conc: 13.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFM1

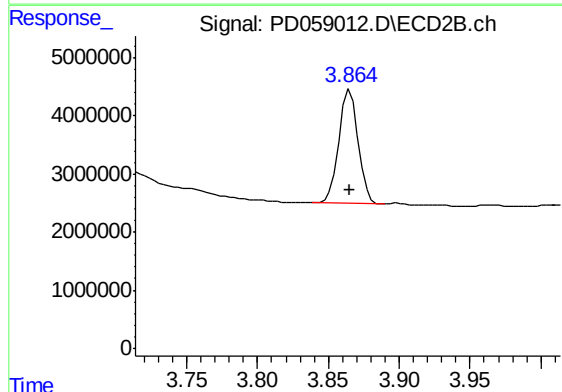


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 18754951
Conc: 12.95 ng/ml

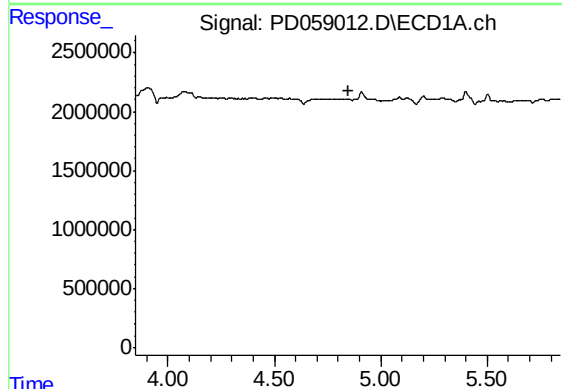


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

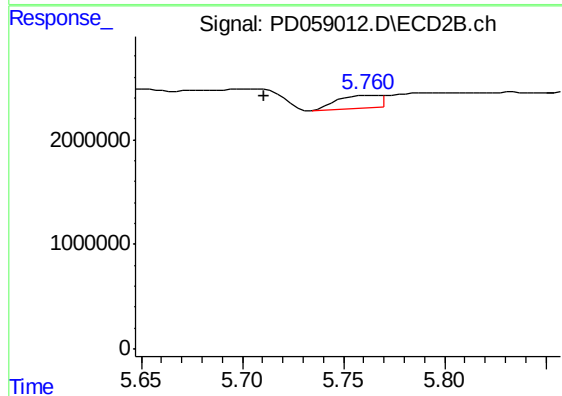

#8 Heptachlor epoxide


R.T.: 5.762 min
Delta R.T.: 0.052 min
Response: 1769197
Conc: 1.06 ng/ml

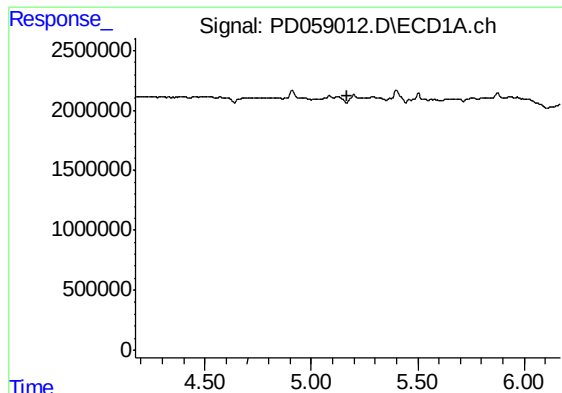

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFM1

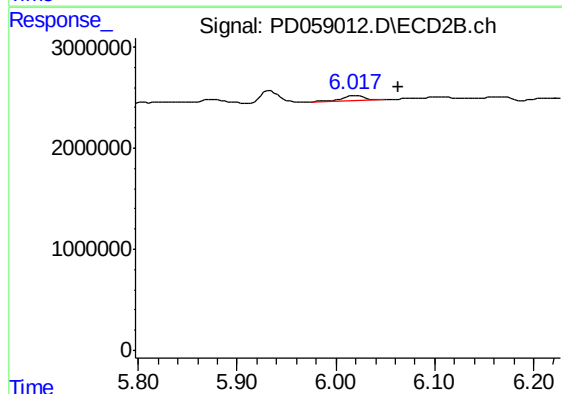


#9 Endosulfan I

R.T.: 6.019 min
Delta R.T.: -0.045 min
Response: 776100
Conc: 0.50 ng/ml

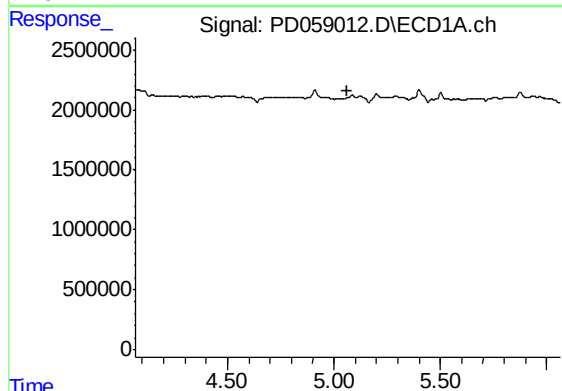


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

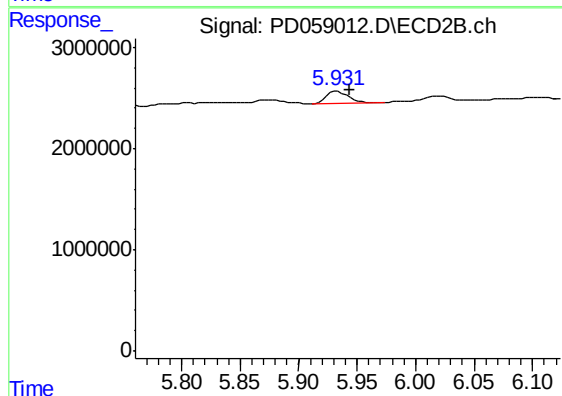

#10 trans-Chlordane


R.T.: 5.933 min
Delta R.T.: -0.011 min
Response: 1597034
Conc: 0.96 ng/ml

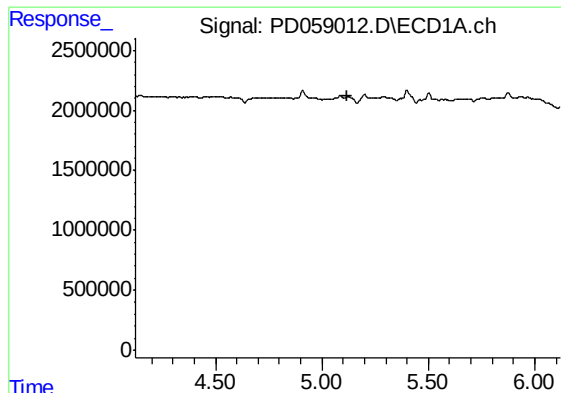

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFM1

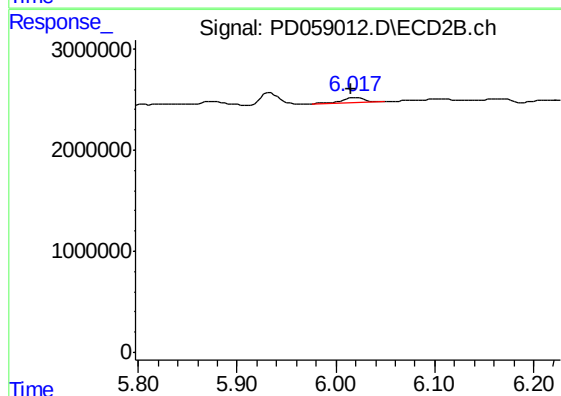


#11 cis-Chlordane

R.T.: 6.019 min
Delta R.T.: 0.004 min
Response: 776100
Conc: 0.46 ng/ml

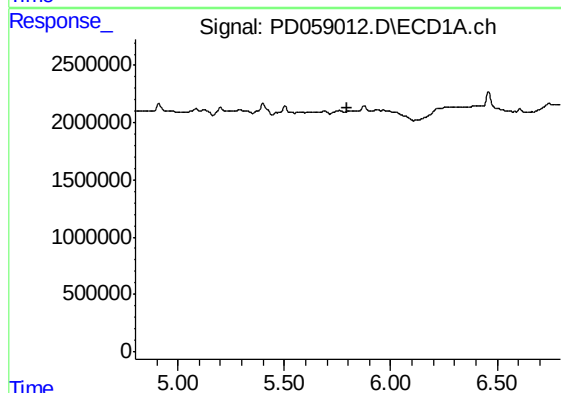


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

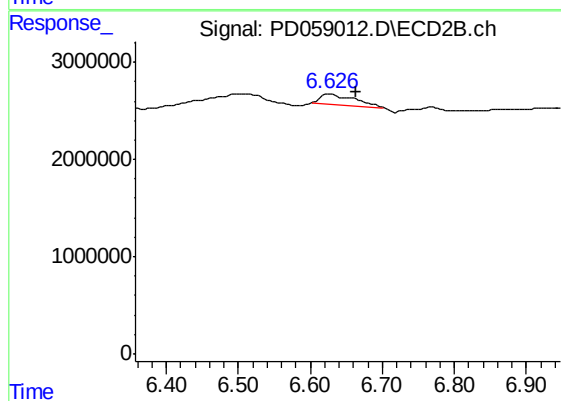

#16 4,4'-DDD


R.T.: 6.627 min
Delta R.T.: -0.036 min
Response: 3455861
Conc: 2.64 ng/ml

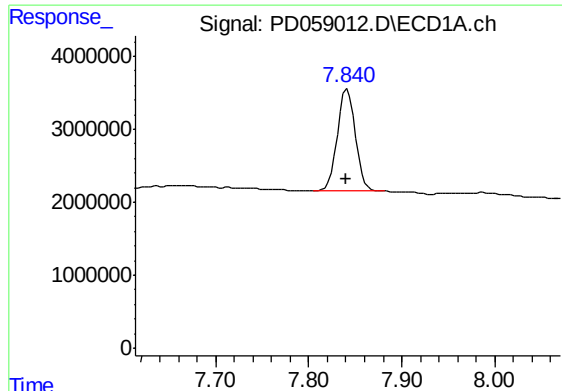

#27 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.000 min
Response: 18866522
Conc: 17.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFM1

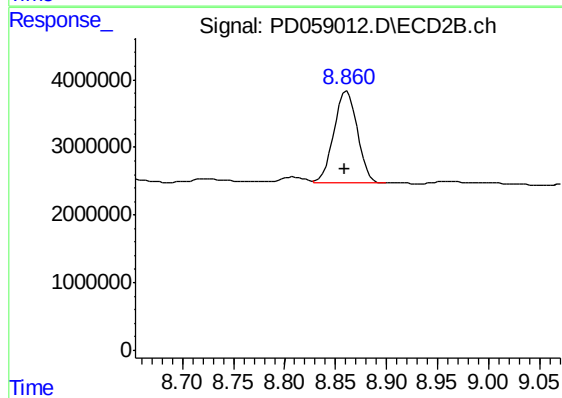

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.003 min
Response: 21574291
Conc: 15.73 ng/ml