

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
 Data File : PD059023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 13:57
 Operator : DD\AJ
 Sample : L3611-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFM3

Manual Integrations
 APPROVED

Ankita
 8/20/2020 2:06:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 08:36:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	13221423	18437095	13.671	12.731
27)	SA Decachlor...	7.841	8.860	23881336	24997411	22.673	18.228
Target Compounds							
8)	B Heptachlo...	4.845	5.708	869375	3550635	0.770m	2.132 #
10)	B trans-Chl...	5.067	5.931	1309749	76943821	1.133m	46.190 #
11)	B cis-Chlor...	5.112	6.019	4026402	11820075	3.460	7.021 #
12)	B 4,4'-DDE	5.291	6.167	2747018	2627085	2.387m	1.658 #
14)	MA Endrin	5.663	6.533	1188845	1070778	1.197m	0.789m#
16)	A 4,4'-DDD	5.802	6.658	2880222	18522152	3.054m	14.130 #
17)	MA 4,4'-DDT	6.029	6.964	4299786	2406289	4.781m	1.823 #
19)	B Endosulfa...	6.304	7.098	4586667	4615901	4.482	3.212 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081820\
Data File : PD059023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 13:57
Operator : DD\AJ
Sample : L3611-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 08:36:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

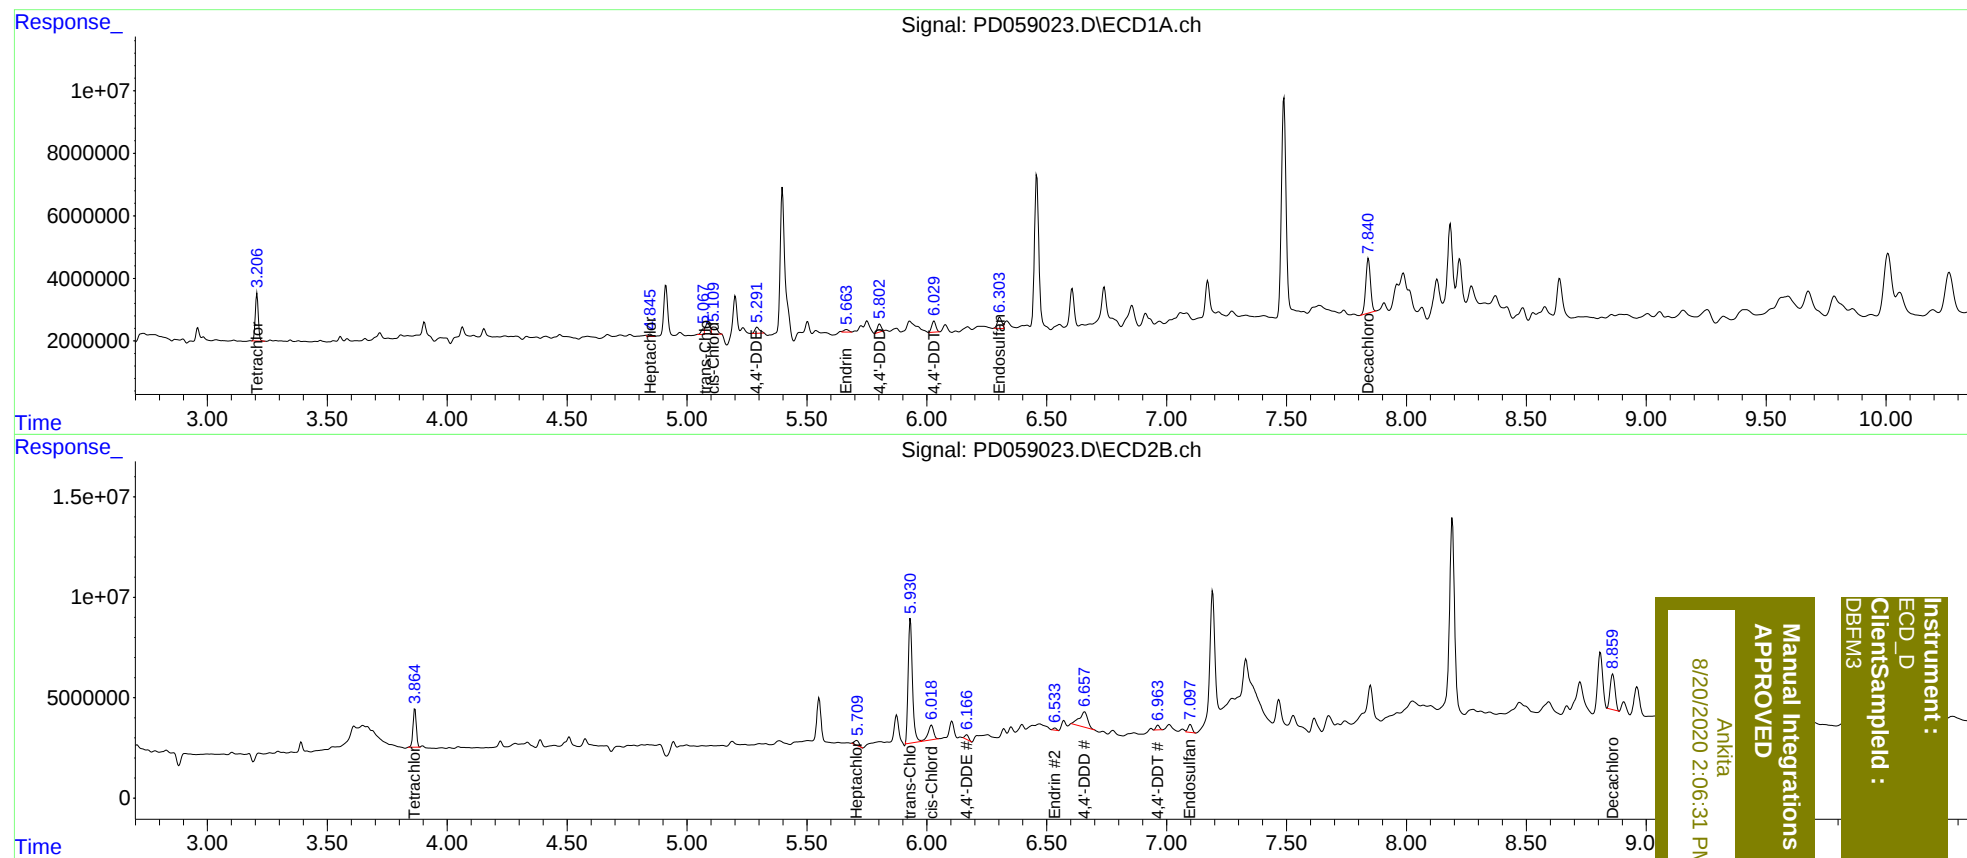

8/20/2020 2:06:31 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
DBFM3