

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081821\
 Data File : PD065038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 00:39
 Operator : AR\AJ
 Sample : M3287-12MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGB11MSD

Manual Integrations
 APPROVED

mohammad
 8/19/2021 6:06:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 08:51:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:57:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.012	8193123	64303111	8.550	8.387
2)	SA Decachlor...	8.247	9.104	11836822	95677858	11.974	21.001 #
Target Compounds							
2)	A alpha-BHC	3.939	4.408	74085883	522.9E6	56.644	49.000
3)	MA gamma-BHC...	4.223	4.695	71831412	459.6E6	54.837	45.907
4)	MA Heptachlor	4.522	5.198	62781002	388.9E6	53.056	42.239
5)	MB Aldrin	4.770	5.504	60538672	346.8E6	52.080	38.516 #
6)	B beta-BHC	4.471	4.870	29445049	184.0E6	47.325	34.991 #
7)	B delta-BHC	4.676	5.087	66891869	412.0E6	54.308	42.044
8)	B Heptachlo...	5.213	5.894	52729764	274.7E6	47.473	35.052 #
9)	A Endosulfan I	5.552	6.251	42001337	269.1E6	41.811	39.813
10)	B trans-Chl...	5.438	6.125	52108593	334.8E6	46.468	43.454m
11)	B cis-Chlor...	5.497	6.199	48816609	277.9E6	44.390	37.544
12)	B 4,4'-DDE	5.660	6.357	116.5E6	529.3E6	115.224	75.996 #
13)	MA Dieldrin	5.794	6.510	112.3E6	483.4E6	106.014m	69.512 #
14)	MA Endrin	6.053	6.729	95605496	439.2E6	103.436	80.406
15)	B Endosulfa...	6.325	6.942	88395840	397.9E6	96.122	71.230 #
16)	A 4,4'-DDD	6.175	6.851	82360279	407.1E6	98.135	76.911
17)	MA 4,4'-DDT	6.415	7.149	95534008	447.4E6	108.228	83.654
18)	B Endrin al...	6.494	7.067	68593274	315.8E6	85.306	65.359
19)	B Endosulfa...	6.706	7.289	94548240	400.0E6	98.529	73.132 #
20)	A Methoxychlor	6.962	7.609	216.0E6	856.1E6	473.808	348.236 #
21)	B Endrin ke...	7.199	7.761	93483946	386.8E6	83.380	62.690m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081821\
Data File : PD065038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 00:39
Operator : AR\AJ
Sample : M3287-12MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 08:51:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:57:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

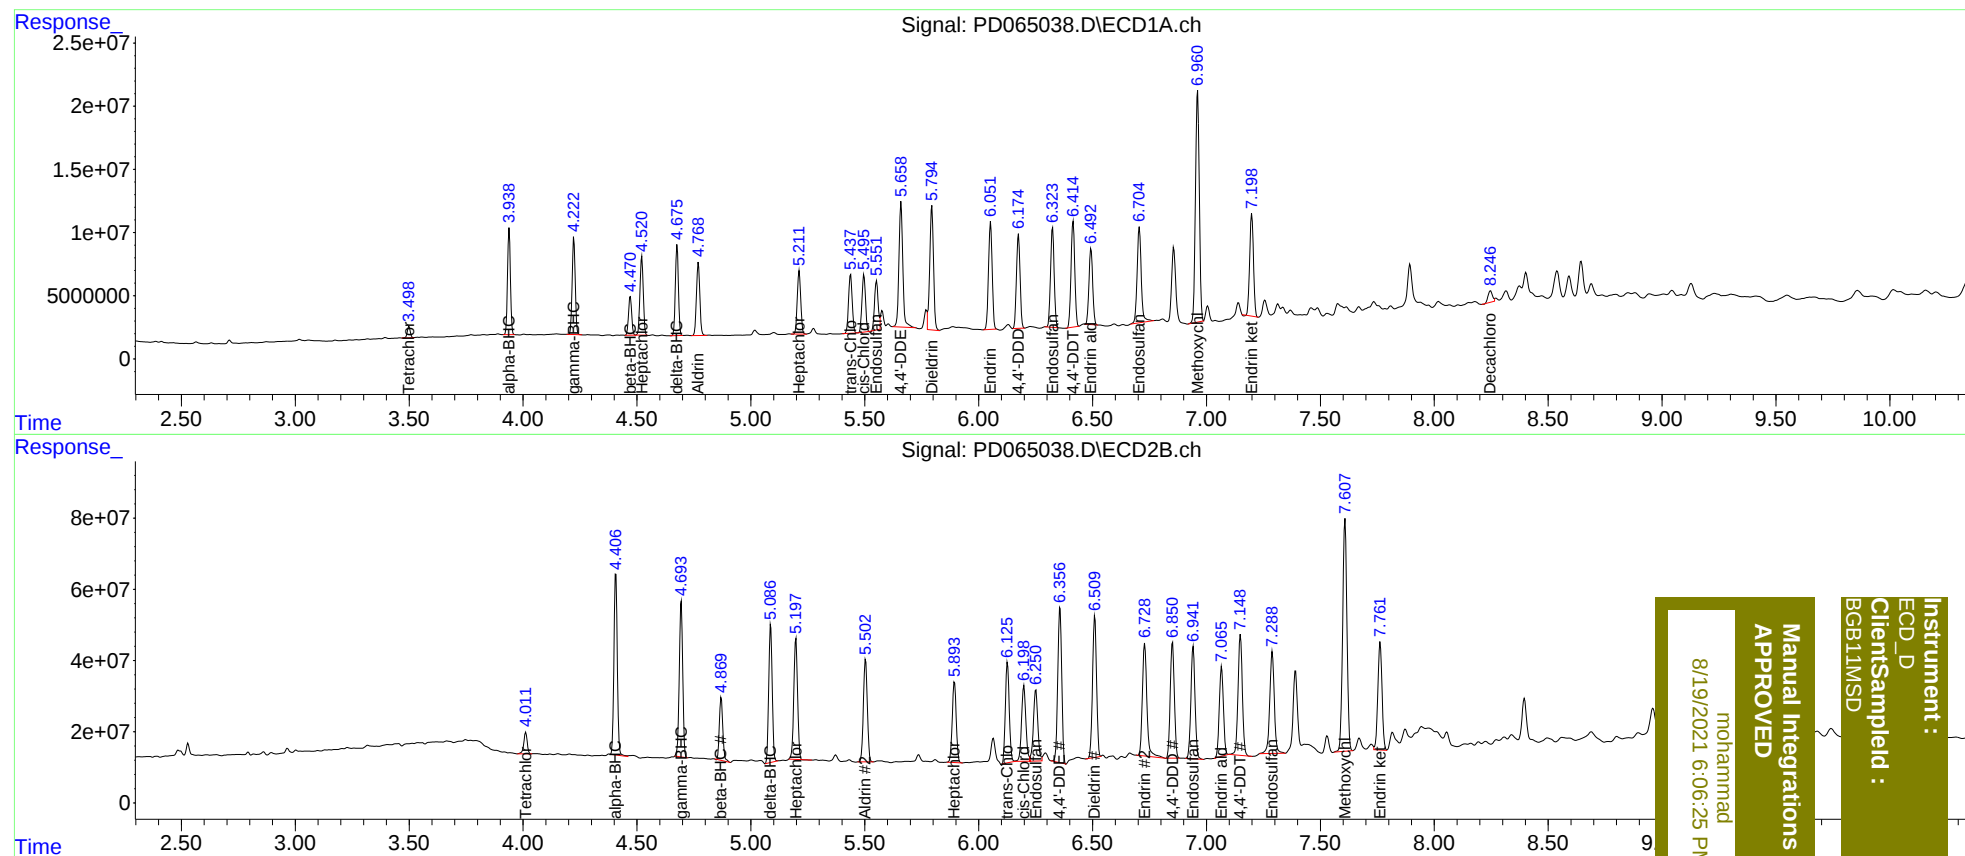

Manual Integrations
APPROVED

8/19/2021 6:06:25 PM
mohammad

Instrument :
ECD_D
Client Sampled :
BGB11MSD