

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081821\
 Data File : PD065030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 18:06
 Operator : AR\AJ
 Sample : M3287-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGB04

Manual Integrations
 APPROVED

mohammad
 8/19/2021 6:06:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 08:26:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 18 02:57:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	14382203	118.3E6	15.009	15.427
27)	SA Decachlor...	8.240	9.097	31882654	212.0E6	32.252	46.543 #
Target Compounds							
3)	MA gamma-BHC...	4.227	4.677	20296083	99219674	15.494	9.912m#
15)	B Endosulfa...	6.321	6.931	4642012	8329891	5.048	1.491 #
16)	A 4,4'-DDD	6.175	6.850	4976085	59088444	5.929	11.162 #
17)	MA 4,4'-DDT	6.409	7.149	4335348	40358960	4.911	7.546m#
18)	B Endrin al...	6.504	7.059	4413613	14673974	5.489m	3.037m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081821\
Data File : PD065030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 18:06
Operator : AR\AJ
Sample : M3287-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 08:26:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 18 02:57:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

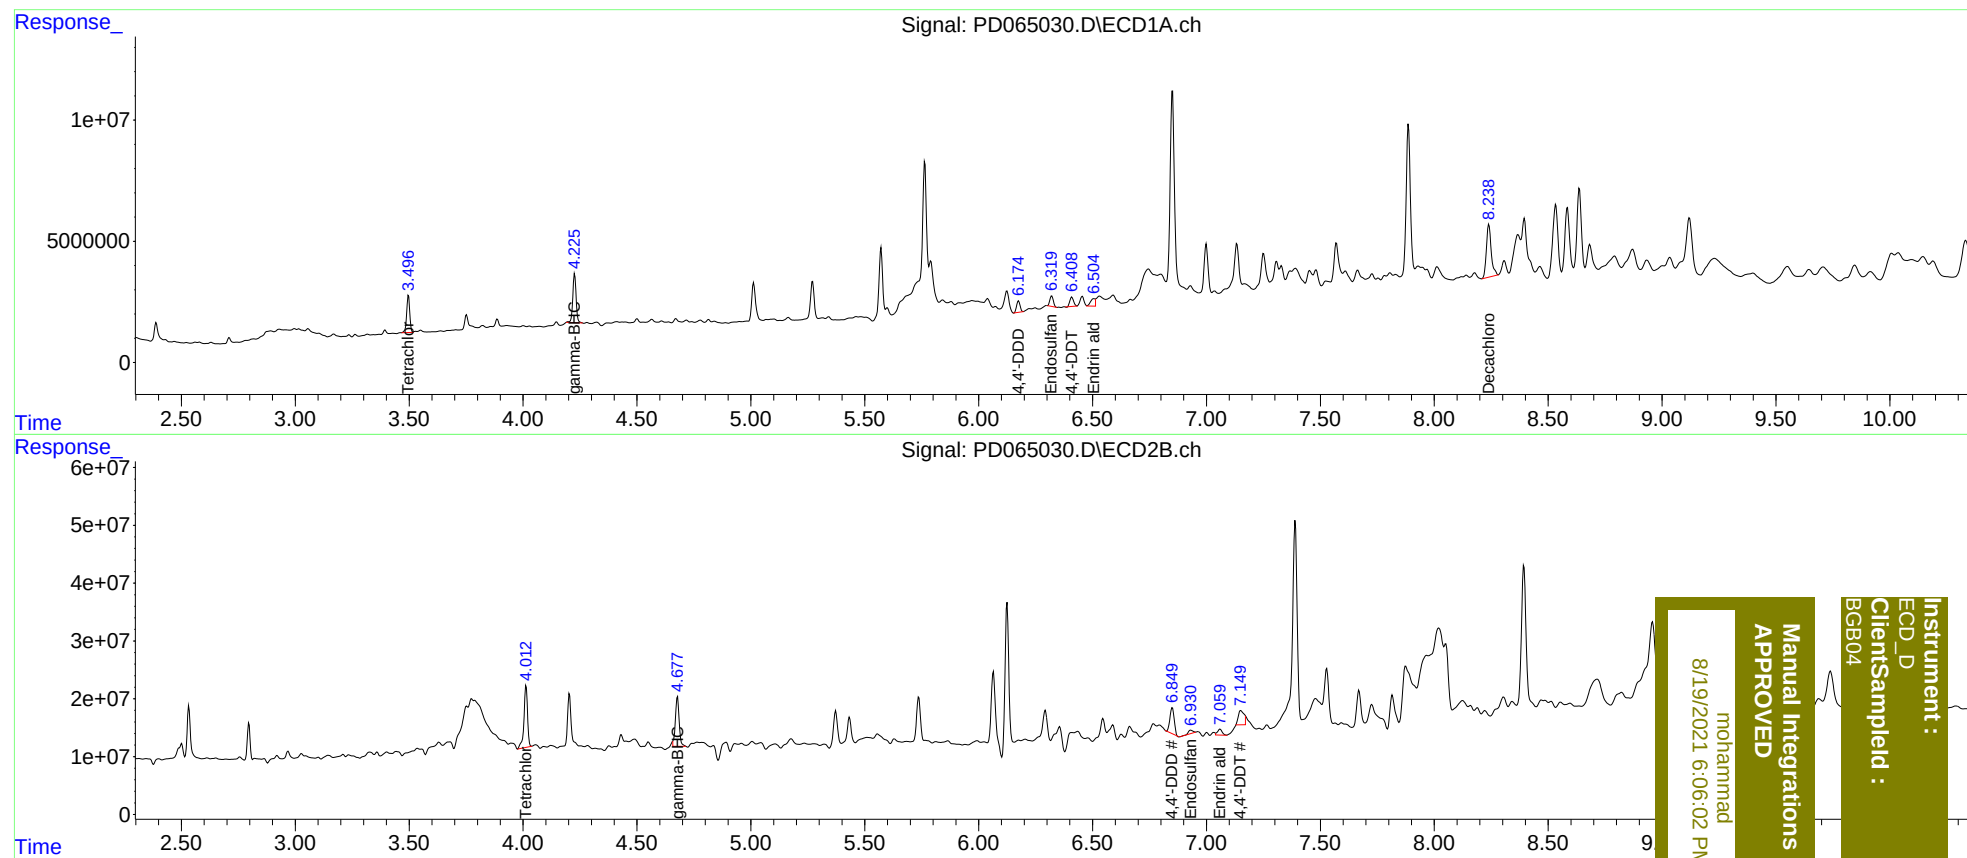

8/19/2021 6:06:02 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
Client Sample :
BGB04