

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 10:31
 Operator : AR\AJ
 Sample : PB147082BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS082

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:58:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	52243035	596.3E6	18.314	18.192
27)	SA Decachlor...	8.000	9.089	103.6E6	376.5E6	36.892	39.272
Target Compounds							
2)	A alpha-BHC	3.314	4.029	18219788	220.3E6	4.429	5.216
3)	MA gamma-BHC...	3.648	4.364	18364241	192.8E6	4.666	5.487
4)	MA Heptachlor	3.993	4.941	18980509	142.6E6	4.667m	5.544
5)	MB Aldrin	4.279	5.284	19288101	125.9E6	4.654	5.625
6)	B beta-BHC	3.945	4.571	8702086	77589309	4.917m	5.371
7)	B delta-BHC	4.181	4.818	15657251	128.3E6	3.944	4.575
8)	B Heptachlo...	4.785	5.716	18443890	104.9E6	4.838	5.269
9)	A Endosulfan I	5.157	6.104	17346930	90986698	5.096m	5.643
10)	B trans-Chl...	5.038	5.971	18732309	98838645	4.708	5.407
11)	B cis-Chlor...	5.101	6.048	18296462	97194466	4.699m	5.441
12)	B 4,4'-DDE	5.294	6.221	33136284	175.2E6	9.323	11.128
13)	MA Dieldrin	5.426	6.381	36488101	189.3E6	9.621	11.426
14)	MA Endrin	5.703	6.613	31484910	146.5E6	9.602	11.543
15)	B Endosulfa...	5.998	6.839	31732493	149.8E6	10.173	11.461
16)	A 4,4'-DDD	5.852	6.745	28484069	141.0E6	10.470	11.579
17)	MA 4,4'-DDT	6.106	7.057	28547319	141.2E6	10.104	11.932
18)	B Endrin al...	6.179	6.970	24709603	113.8E6	9.213	10.355
19)	B Endosulfa...	6.404	7.203	29753265	128.3E6	9.670	10.467
20)	A Methoxychlor	6.685	7.532	84121477	329.9E6	58.265	62.720
21)	B Endrin ke...	6.914	7.695	35633521	152.5E6	10.427	11.620

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 10:31
Operator : AR\AJ
Sample : PB147082BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:58:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

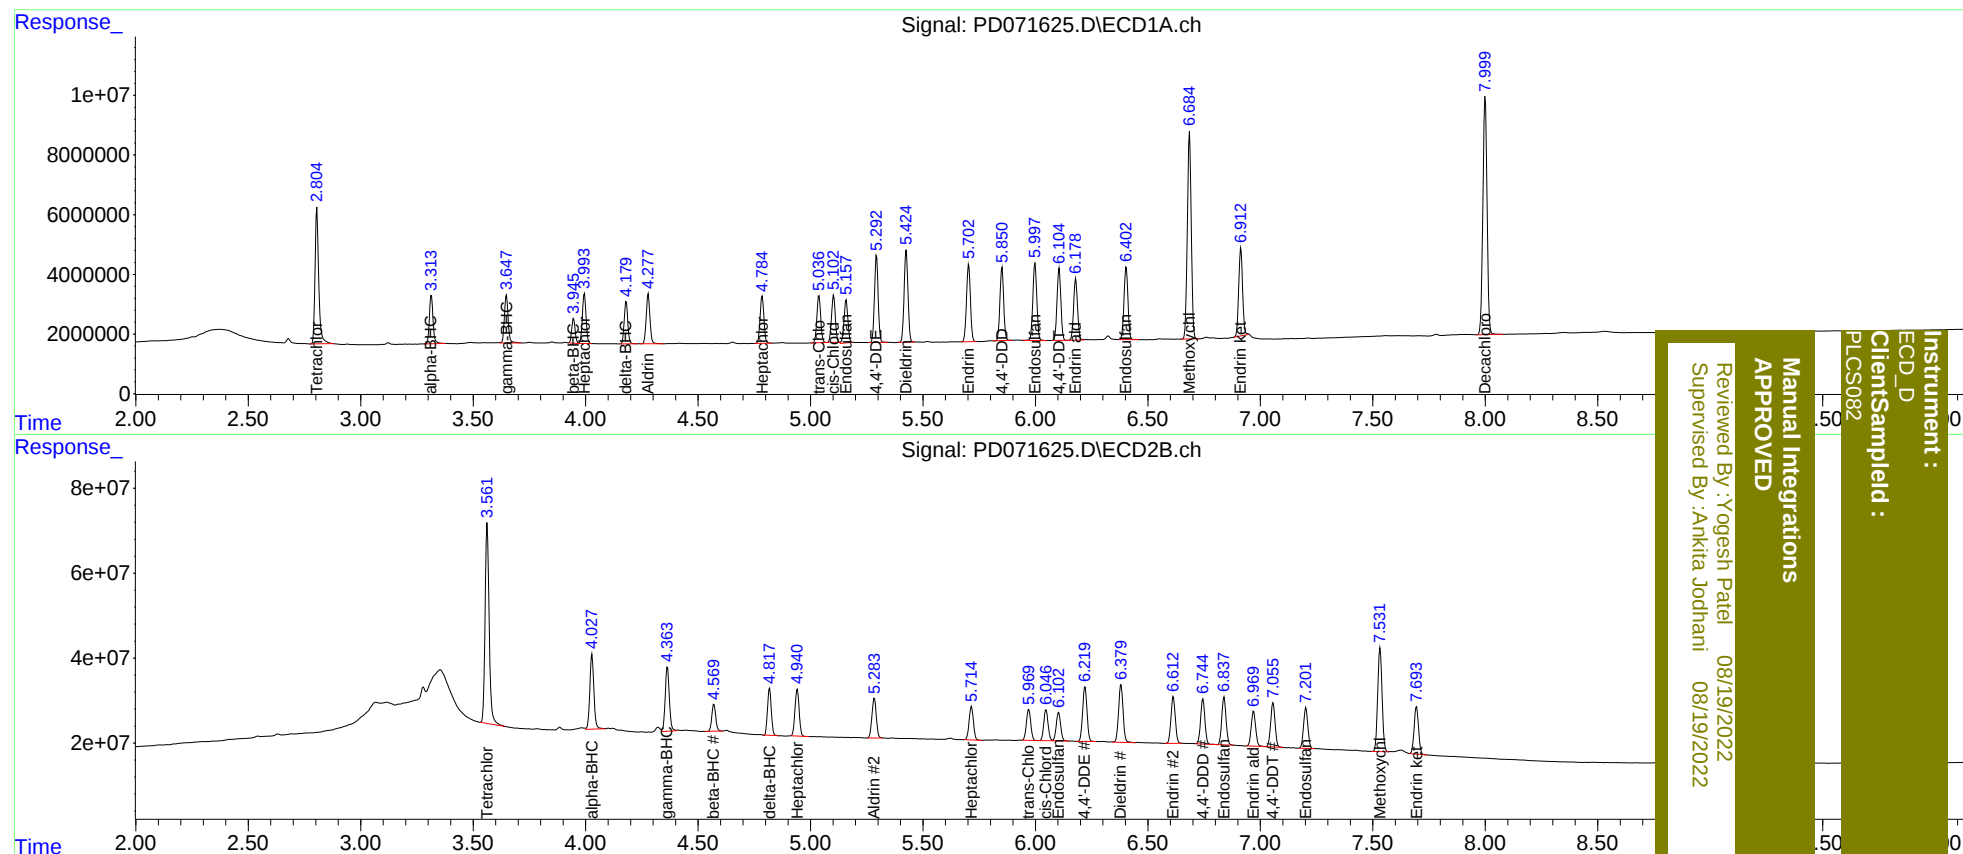

Instrument :
ECD_D
ClientSampled :
PLCS082

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022