

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 11:01
 Operator : AR\AJ
 Sample : N4210-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC46MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:58:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.806	3.563	42892122	491.7E6	15.036	15.000
27)	SA Decachlor...	8.000	9.089	79497236	296.4E6	28.315	30.916
Target Compounds							
2)	A alpha-BHC	3.315	4.029	203.7E6	1907.9E6	49.518	45.174
3)	MA gamma-BHC...	3.648	4.365	195.3E6	1547.0E6	49.634	44.014
4)	MA Heptachlor	3.994	4.942	200.5E6	1100.2E6	49.296m	42.782
5)	MB Aldrin	4.279	5.285	199.9E6	966.0E6	48.229	43.170
6)	B beta-BHC	3.946	4.570	79646910	590.6E6	45.001m	40.890m
7)	B delta-BHC	4.181	4.819	192.6E6	1095.6E6	48.513	39.070
8)	B Heptachlo...	4.786	5.717	179.1E6	772.7E6	46.977	38.818
9)	A Endosulfan I	5.159	6.104	151.7E6	711.6E6	44.557m	44.138
10)	B trans-Chl...	5.039	5.971	182.0E6	792.5E6	45.736	43.355
11)	B cis-Chlor...	5.104	6.049	163.3E6	767.9E6	41.927	42.987
12)	B 4,4'-DDE	5.295	6.221	348.8E6	1379.6E6	98.132	87.652
13)	MA Dieldrin	5.427	6.382	371.8E6	1498.0E6	98.034	90.419
14)	MA Endrin	5.705	6.614	331.7E6	1240.7E6	101.165	97.763
15)	B Endosulfa...	6.000	6.840	299.5E6	1203.6E6	96.024	92.056
16)	A 4,4'-DDD	5.853	6.746	282.1E6	1159.2E6	103.692	95.202
17)	MA 4,4'-DDT	6.107	7.057	306.8E6	1203.0E6	108.586	101.688
18)	B Endrin al...	6.180	6.971	233.0E6	943.0E6	86.883	85.768
19)	B Endosulfa...	6.405	7.204	278.8E6	1071.9E6	90.603	87.443
20)	A Methoxychlor	6.687	7.533	767.2E6	2524.7E6	531.382	479.971
21)	B Endrin ke...	6.915	7.696	322.6E6	1209.3E6	94.409	92.148

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 11:01
Operator : AR\AJ
Sample : N4210-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:58:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

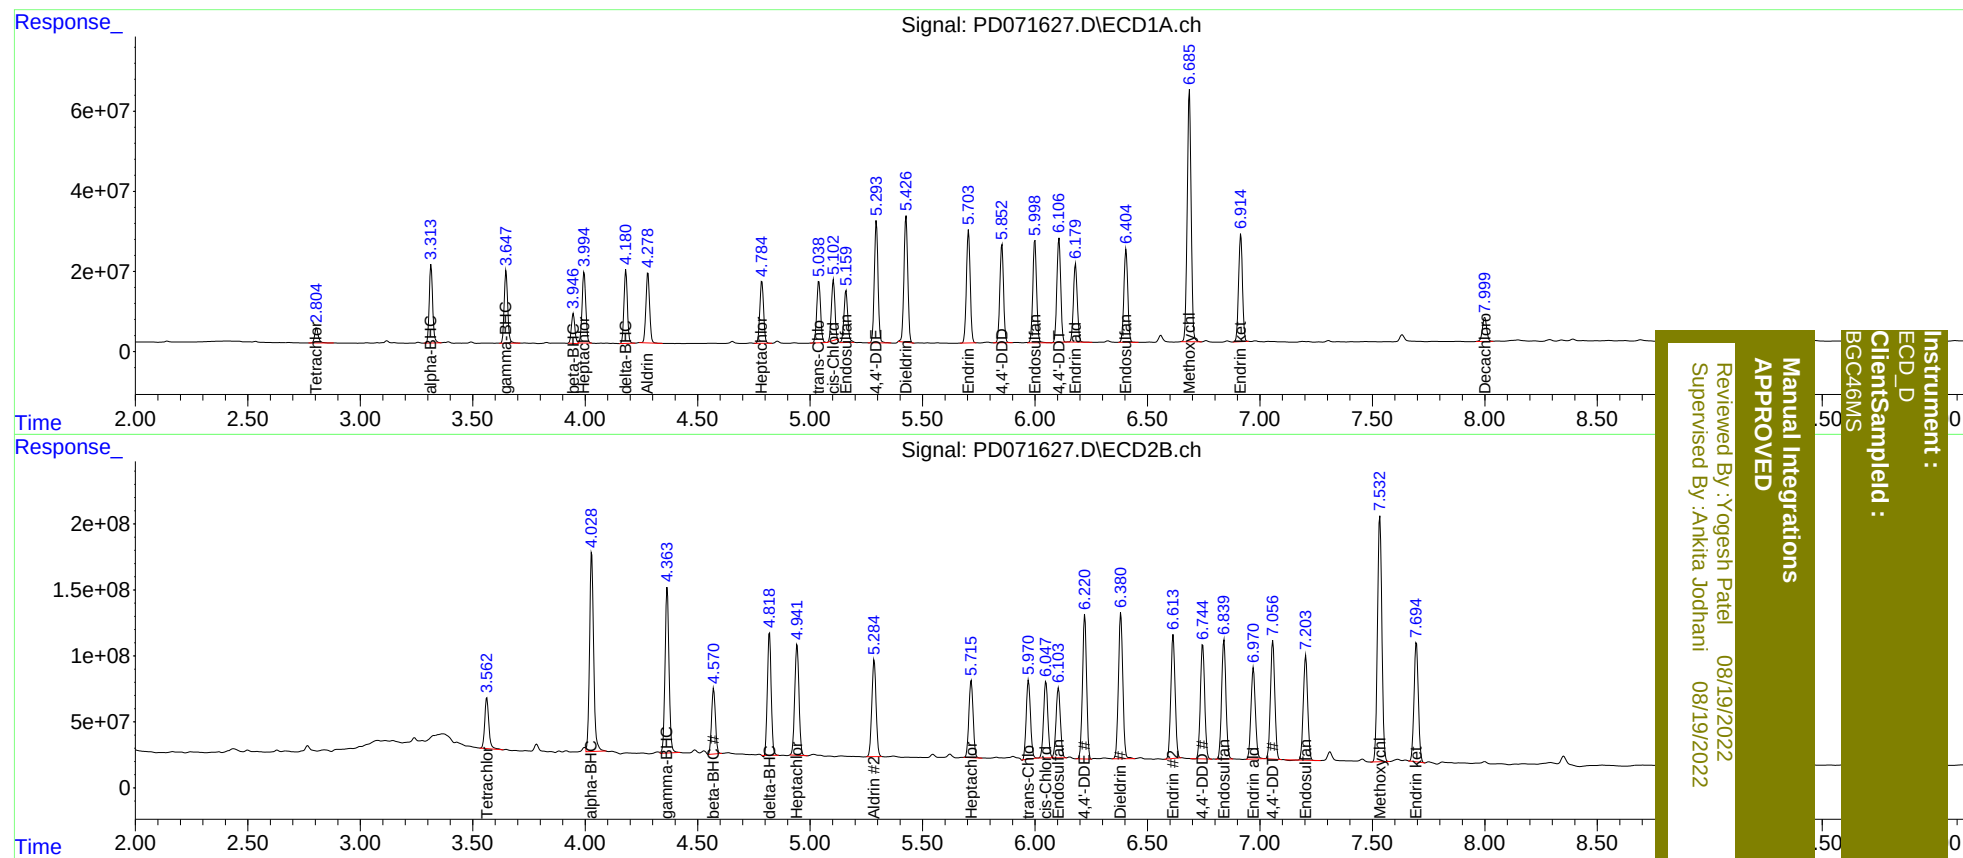

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGC46MS