

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 11:14
 Operator : AR\AJ
 Sample : N4210-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC46MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:58:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	41873506	481.0E6	14.679	14.675
27)	SA Decachlor...	7.999	9.089	77611184	292.8E6	27.643	30.545
Target Compounds							
2)	A alpha-BHC	3.315	4.029	200.0E6	1873.6E6	48.605	44.362
3)	MA gamma-BHC...	3.648	4.365	192.6E6	1519.8E6	48.931	43.242
4)	MA Heptachlor	3.994	4.942	197.3E6	1078.5E6	48.505m	41.938
5)	MB Aldrin	4.279	5.285	196.2E6	947.2E6	47.347	42.331
6)	B beta-BHC	3.945	4.570	76946140	576.9E6	43.475m	39.942m
7)	B delta-BHC	4.181	4.819	189.6E6	1081.7E6	47.759	38.573
8)	B Heptachlo...	4.786	5.716	176.9E6	757.5E6	46.394	38.051
9)	A Endosulfan I	5.158	6.104	147.7E6	697.4E6	43.376m	43.255
10)	B trans-Chl...	5.038	5.971	179.2E6	787.8E6	45.040	43.098
11)	B cis-Chlor...	5.102	6.048	174.8E6	756.3E6	44.882m	42.338
12)	B 4,4'-DDE	5.294	6.221	344.5E6	1356.3E6	96.923	86.171
13)	MA Dieldrin	5.426	6.381	365.9E6	1477.2E6	96.479	89.164
14)	MA Endrin	5.703	6.614	328.5E6	1221.2E6	100.171	96.229
15)	B Endosulfa...	5.999	6.840	295.9E6	1184.4E6	94.868	90.590
16)	A 4,4'-DDD	5.852	6.746	278.4E6	1142.0E6	102.324	93.792
17)	MA 4,4'-DDT	6.106	7.056	304.5E6	1178.7E6	107.778	99.641
18)	B Endrin al...	6.179	6.971	229.3E6	921.3E6	85.486	83.797
19)	B Endosulfa...	6.404	7.204	274.0E6	1062.6E6	89.048	86.683
20)	A Methoxychlor	6.685	7.533	762.9E6	2500.9E6	528.411	475.431
21)	B Endrin ke...	6.914	7.695	319.6E6	1193.2E6	93.526	90.916

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 11:14
Operator : AR\AJ
Sample : N4210-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:58:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

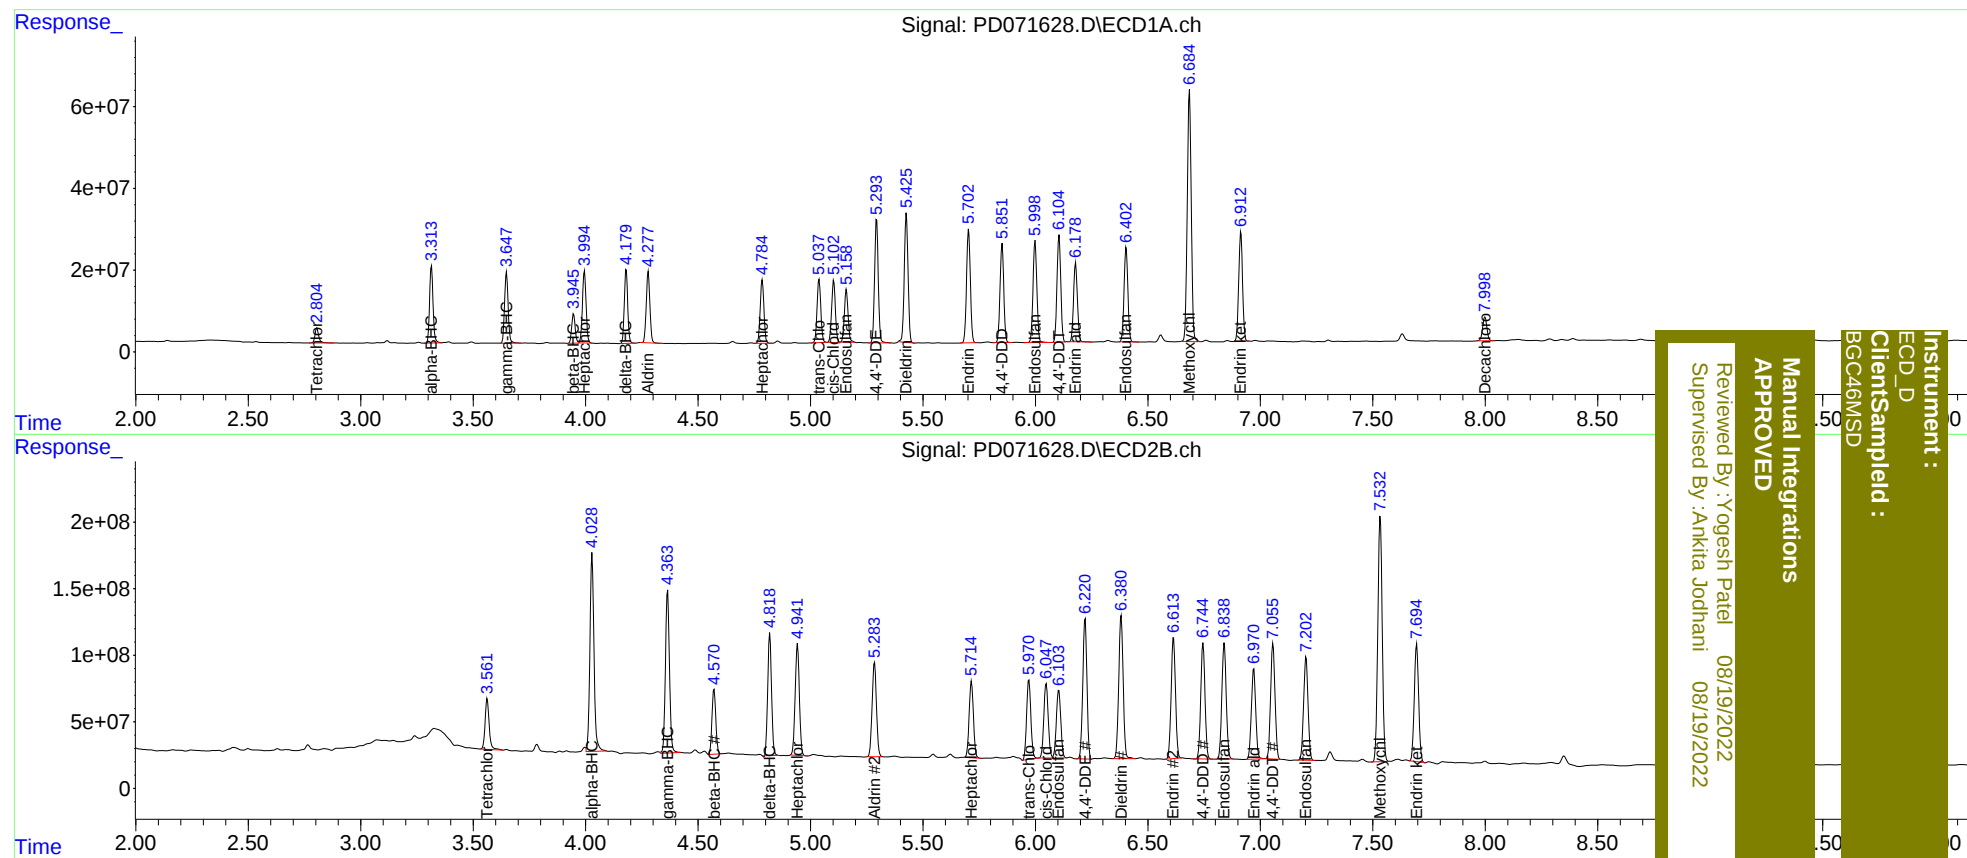

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGC46MSD