

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 11:28
 Operator : AR\AJ
 Sample : N4210-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC47

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:59:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.804	3.561	44527543	525.9E6	15.610m	16.043m
27) SA Decachlor...	8.000	9.091	81416128	303.6E6	28.998	31.669
Target Compounds						
16) A 4,4'-DDD	5.847	6.746	1768092	25806223	0.650m	2.119m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 11:28
Operator : AR\AJ
Sample : N4210-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:59:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

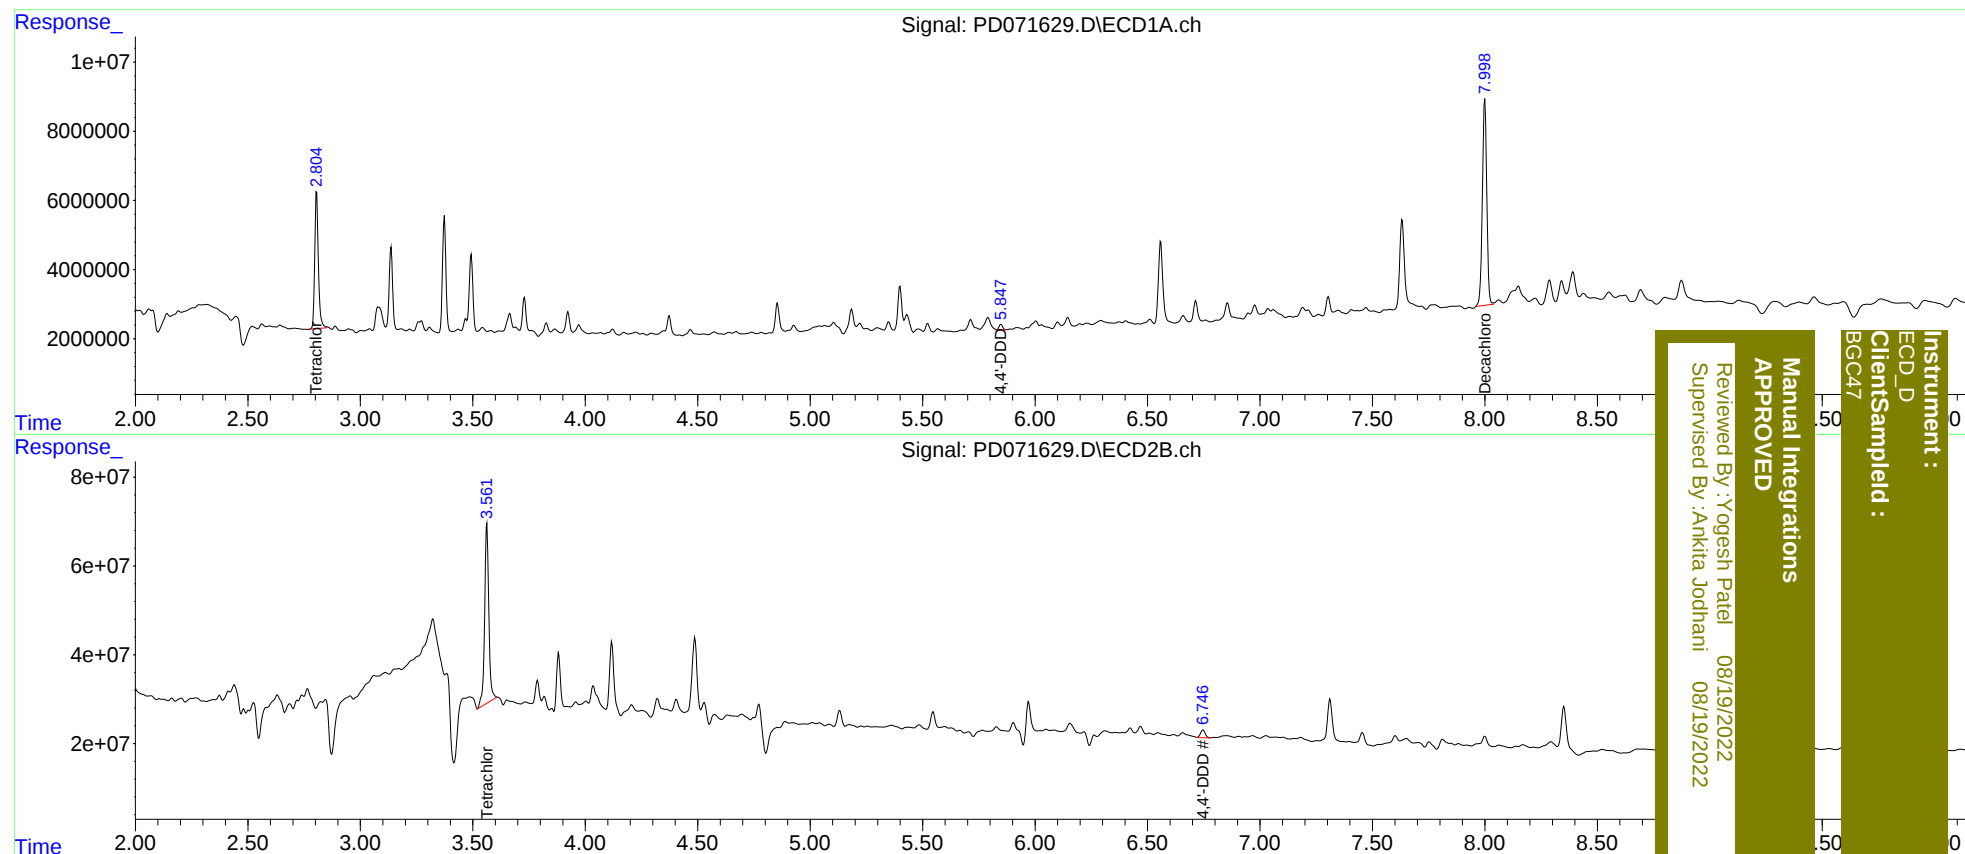

Instrument :
ECD_D
ClientSampled :
BGC47

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022

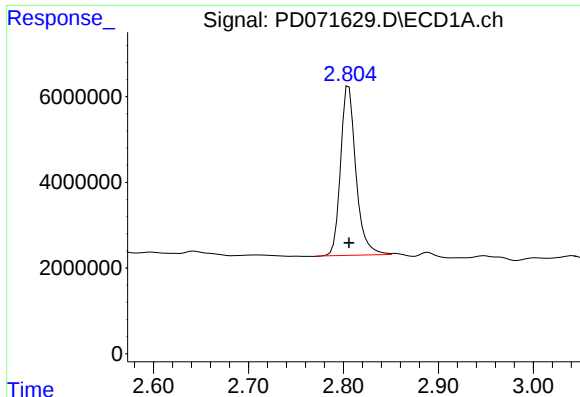


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: -0.002 min
Response: 44527543
Conc: 15.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC47


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

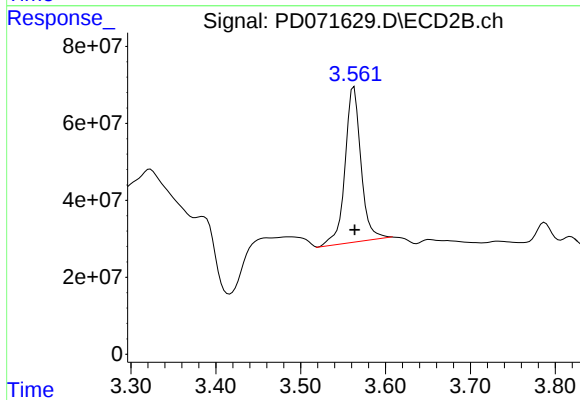


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.002 min
Response: 525877995
Conc: 16.04 ng/ml m

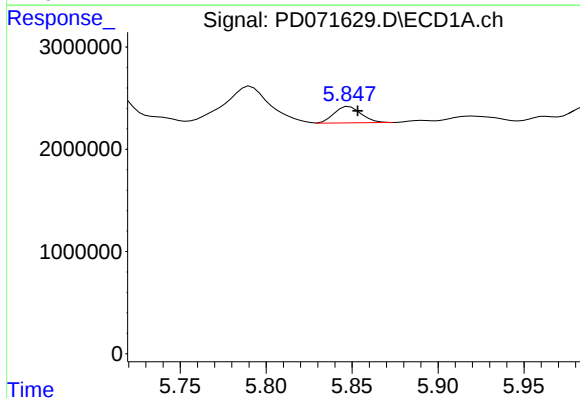


#16 4,4'-DDD

R.T.: 5.847 min
Delta R.T.: -0.006 min
Response: 1768092
Conc: 0.65 ng/ml m

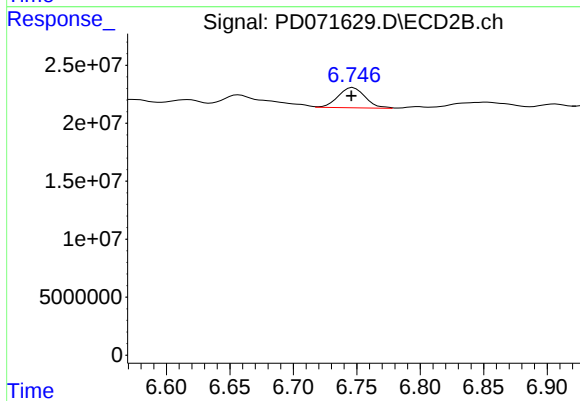

#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 25806223
Conc: 2.12 ng/ml m

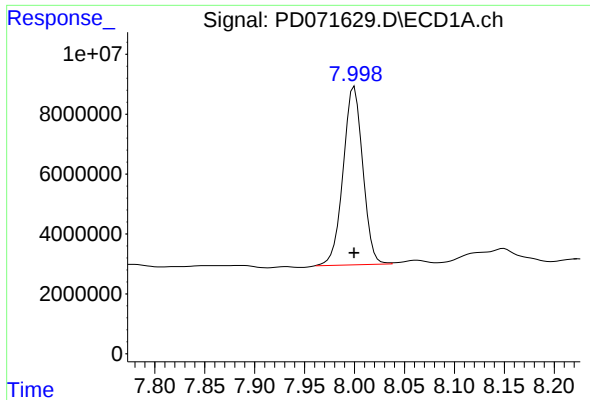


#27 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: 0.000 min
Response: 81416128
Conc: 29.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC47

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

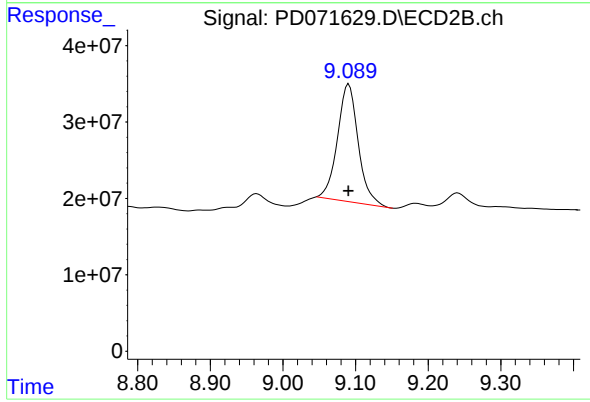

#27 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 303595697
Conc: 31.67 ng/ml