

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 12:08
 Operator : AR\AJ
 Sample : N4210-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC50

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:59:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.806	3.564	35938589	447.3E6	12.599	13.646
2)	SA Decachlor...	7.999	9.071	62938145	441.3E6	22.417	46.031m#
Target Compounds							
3)	MA gamma-BHC...	3.655	4.346	26237613	131.8E6	6.667	3.750m#
16)	A 4,4'-DDD	5.847	6.746	7587718	85808262	2.789m	7.047m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 12:08
Operator : AR\AJ
Sample : N4210-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:59:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

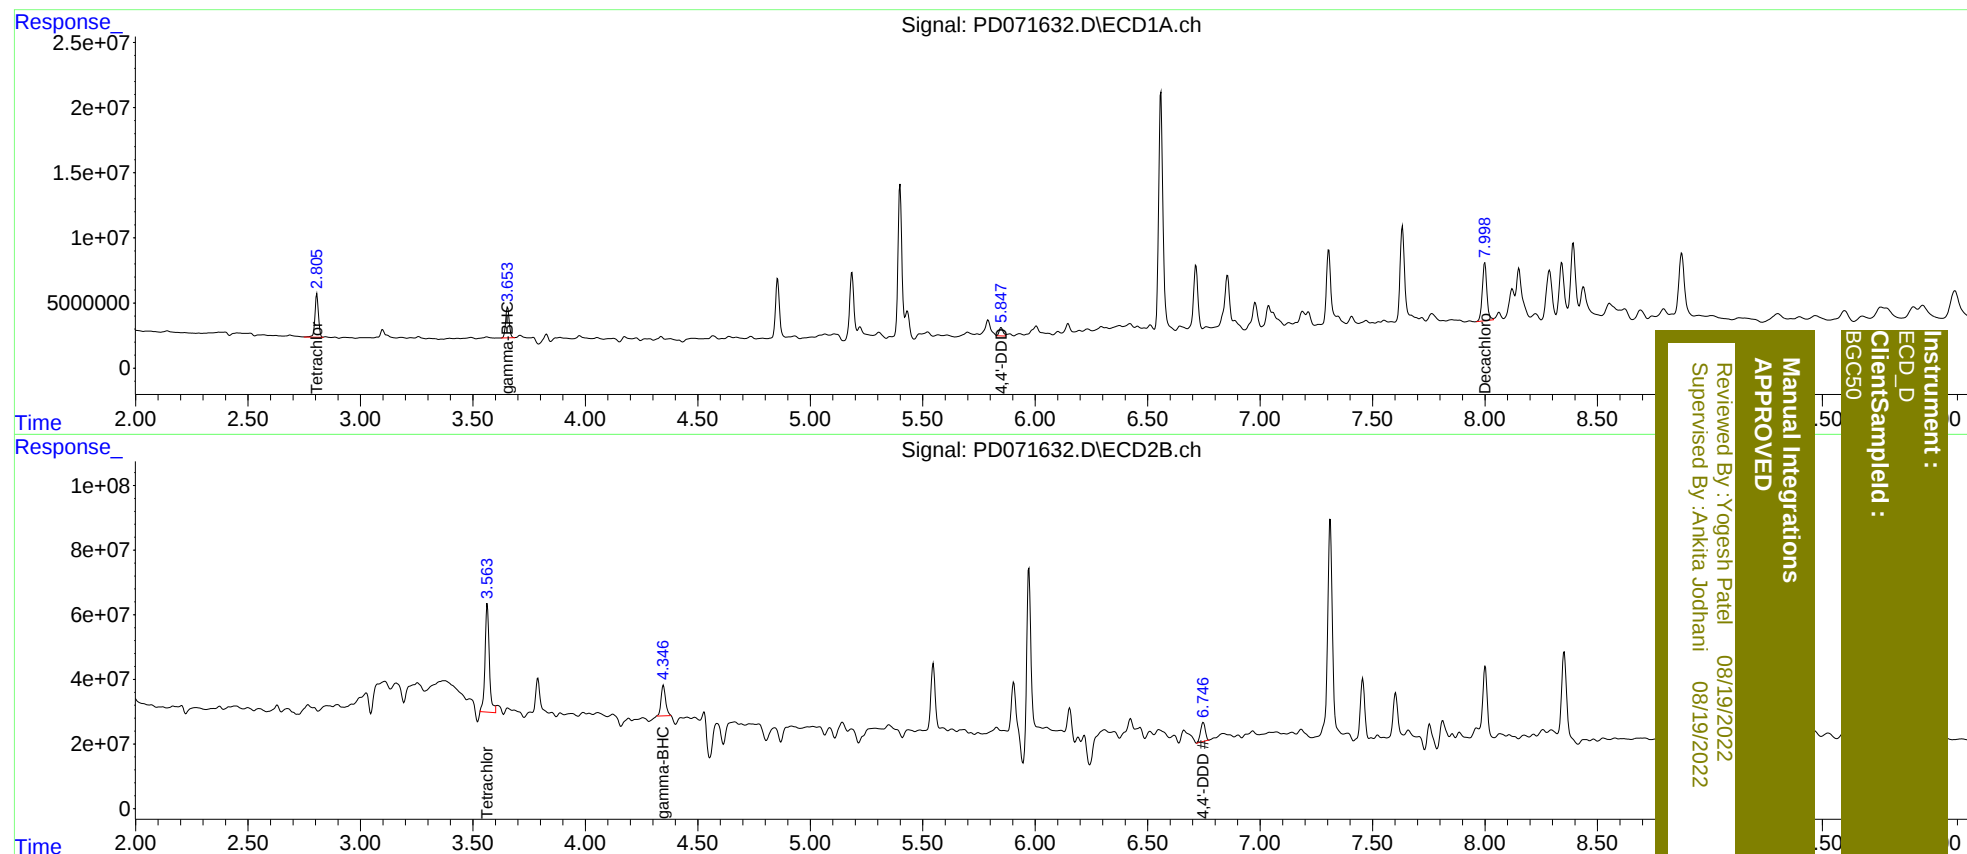

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGC50

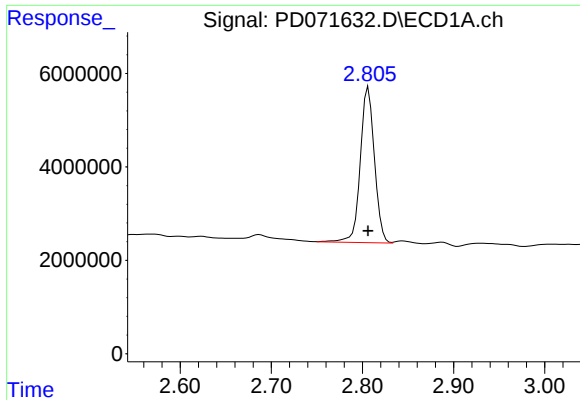


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 35938589
Conc: 12.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC50


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

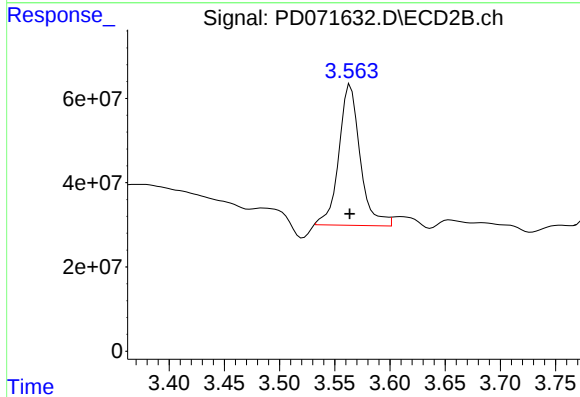


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 447304724
Conc: 13.65 ng/ml

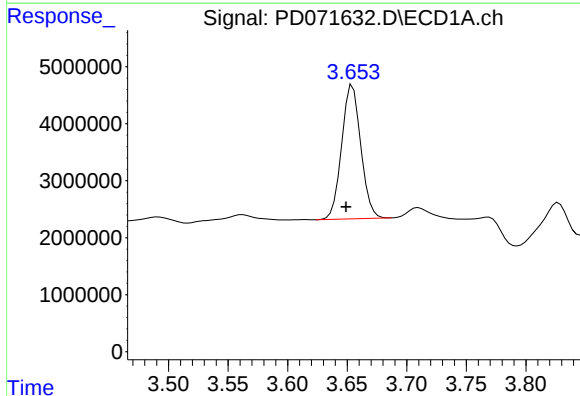


#3 gamma-BHC (Lindane)

R.T.: 3.655 min
Delta R.T.: 0.006 min
Response: 26237613
Conc: 6.67 ng/ml

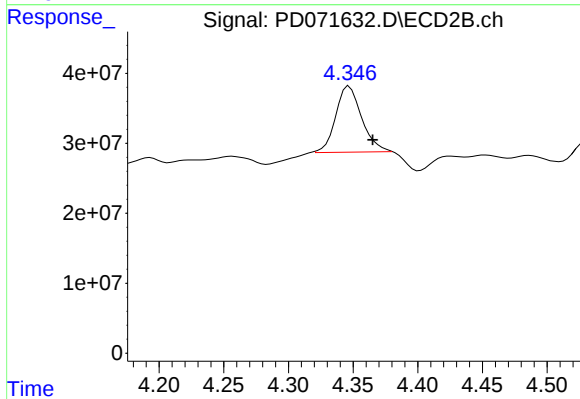

#3 gamma-BHC (Lindane)

R.T.: 4.346 min
Delta R.T.: -0.019 min
Response: 131801358
Conc: 3.75 ng/ml m

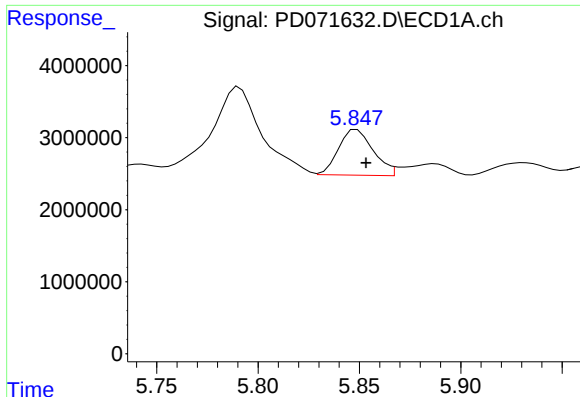


#16 4,4'-DDD

R.T.: 5.847 min
Delta R.T.: -0.006 min
Response: 7587718
Conc: 2.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC50


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

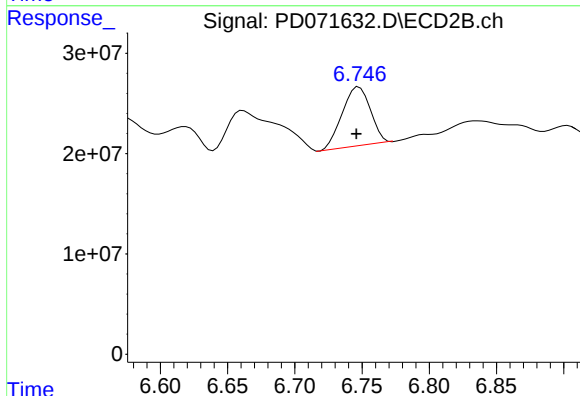


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 85808262
Conc: 7.05 ng/ml m

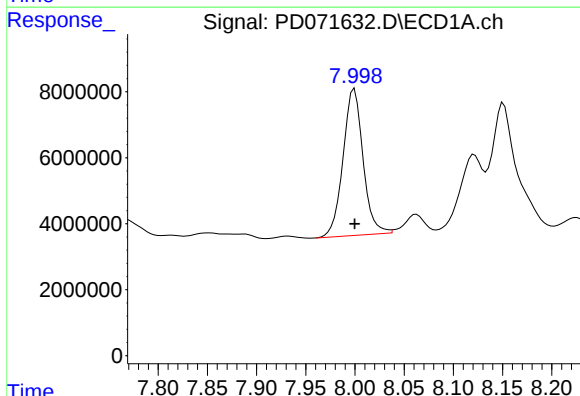

#27 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 62938145
Conc: 22.42 ng/ml

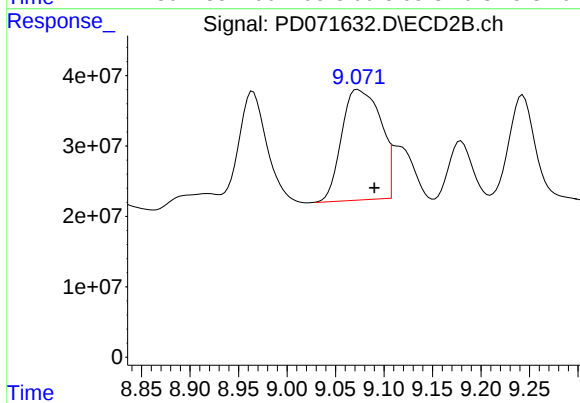

#27 Decachlorobiphenyl

R.T.: 9.071 min
Delta R.T.: -0.019 min
Response: 441276644
Conc: 46.03 ng/ml m