

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 12:21
 Operator : AR\AJ
 Sample : N4210-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC51

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:00:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.807	3.565	35585636	380.3E6	12.475	11.602
27) SA Decachlor...	8.000	9.088	52039002	163.9E6	18.535	17.098m
Target Compounds						
16) A 4,4'-DDD	5.849	6.746	1039493	19534429	0.382m	1.604m#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 12:21
Operator : AR\AJ
Sample : N4210-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:00:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

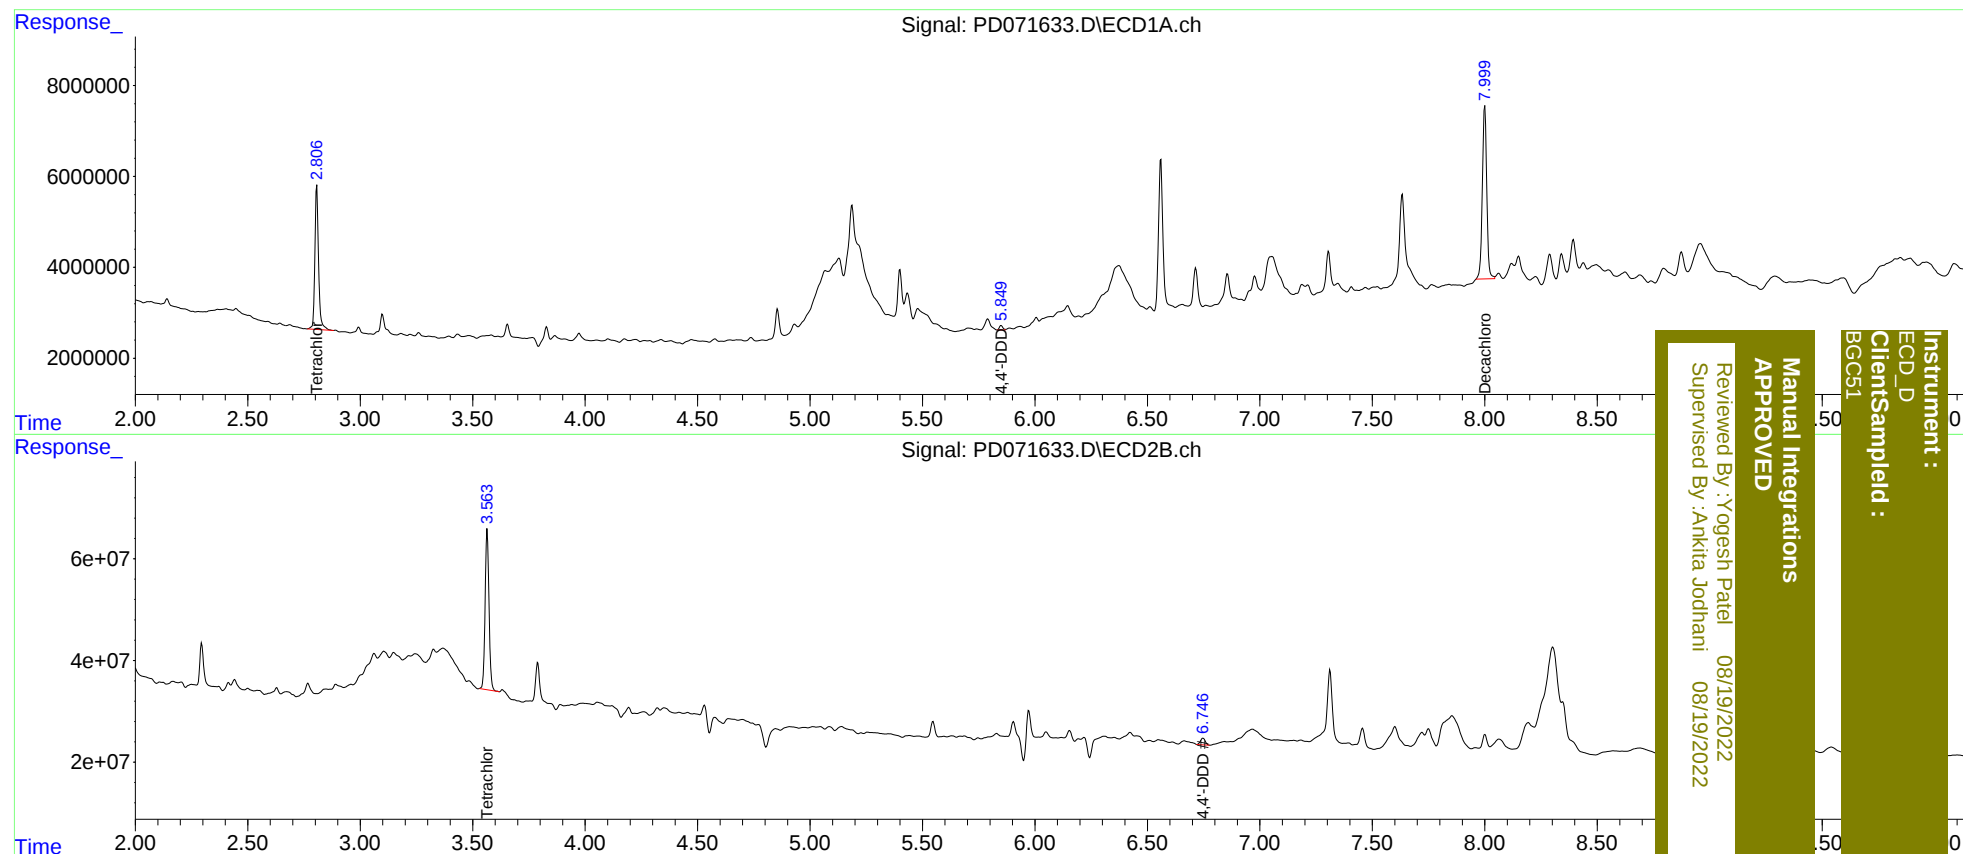

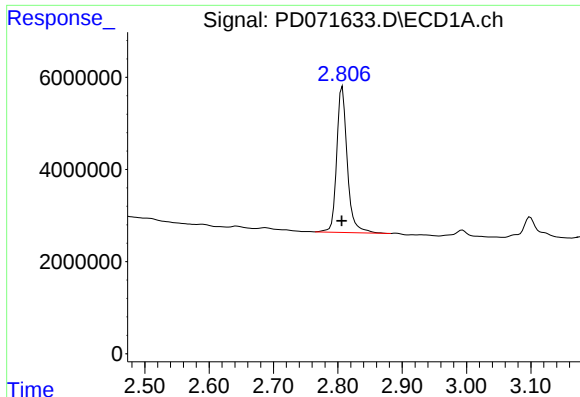


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 35585636
Conc: 12.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC51


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

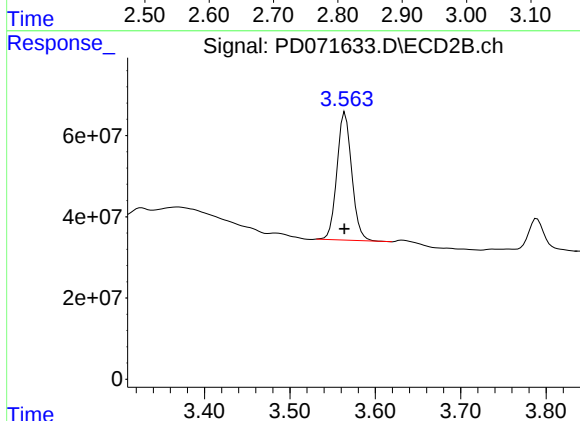


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.001 min
Response: 380293848
Conc: 11.60 ng/ml

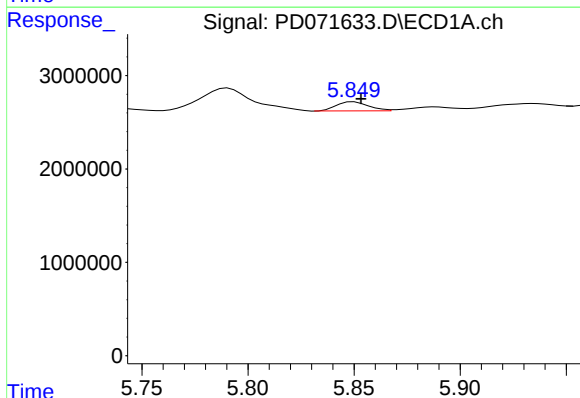


#16 4,4'-DDD

R.T.: 5.849 min
Delta R.T.: -0.005 min
Response: 1039493
Conc: 0.38 ng/ml m

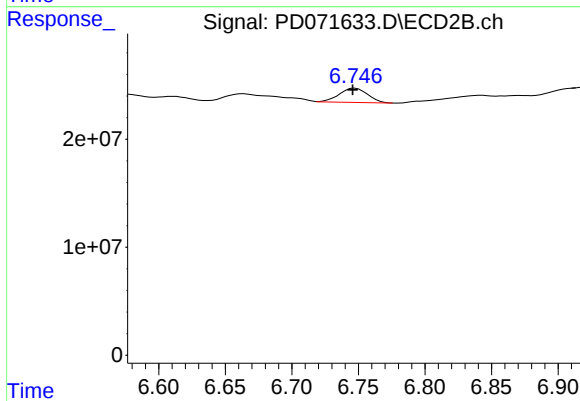

#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 19534429
Conc: 1.60 ng/ml m

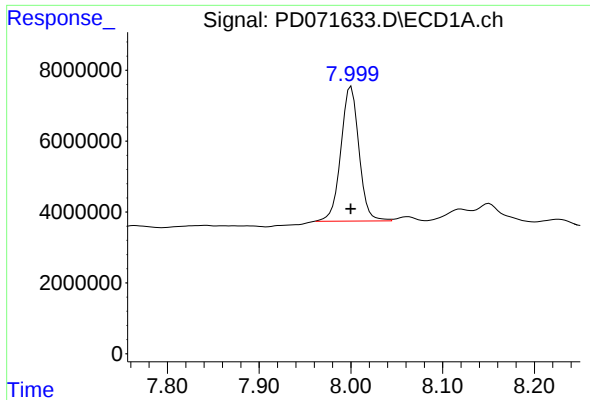


#27 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: 0.000 min
Response: 52039002
Conc: 18.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC51

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

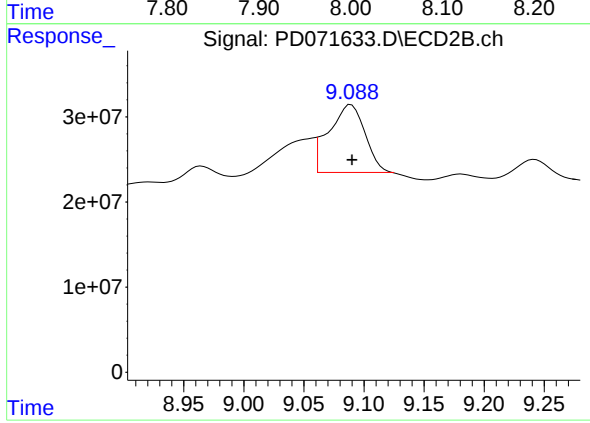

#27 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.002 min
Response: 163912399
Conc: 17.10 ng/ml m