

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 13:14
 Operator : AR\AJ
 Sample : INDA307
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3141

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:01:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.806	3.564	47853856	544.9E6	16.776	16.622
27)	SA Decachlor...	8.000	9.091	85298616	317.7E6	30.381	33.141
Target Compounds							
2)	A alpha-BHC	3.315	4.030	70335516	731.4E6	17.097	17.319
3)	MA gamma-BHC...	3.649	4.366	67477434	602.8E6	17.145	17.149
4)	MA Heptachlor	3.995	4.943	71124580	451.3E6	17.487	17.547
9)	A Endosulfan I	5.159	6.105	54225026	275.8E6	15.929	17.103
13)	MA Dieldrin	5.427	6.382	129.2E6	598.4E6	34.064	36.121
14)	MA Endrin	5.704	6.614	113.0E6	422.4E6	34.455	33.283
16)	A 4,4'-DDD	5.853	6.747	100.4E6	452.0E6	36.895	37.119
17)	MA 4,4'-DDT	6.106	7.058	96550928	400.2E6	34.174	33.828
20)	A Methoxychlor	6.686	7.535	264.2E6	964.8E6	182.968	183.423


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 13:14
Operator : AR\AJ
Sample : INDA307
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:01:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

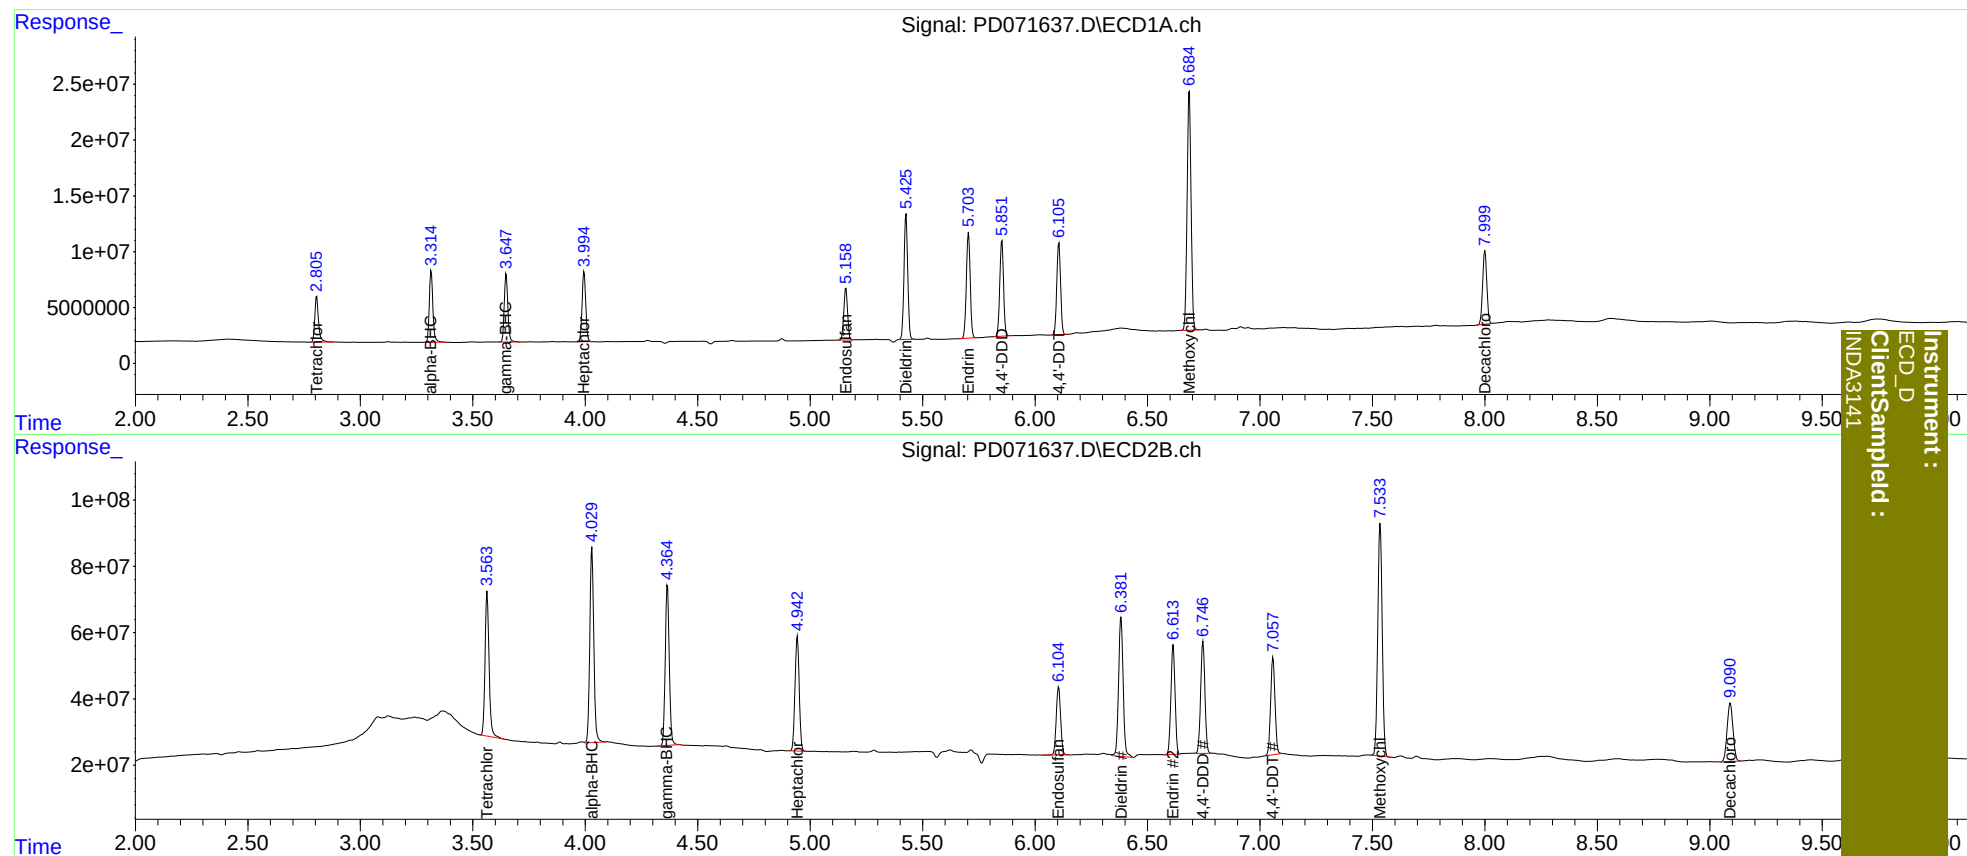


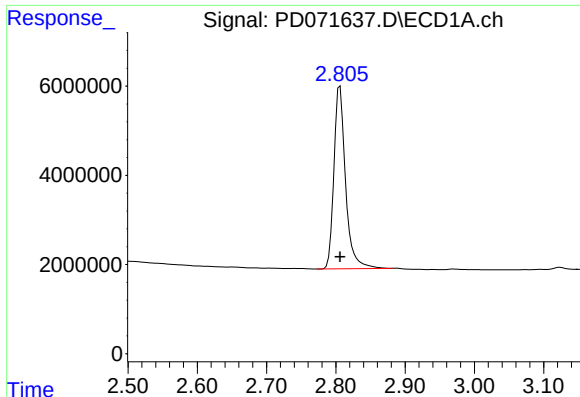

#1 Tetrachloro-m-xylene


R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 47853856
Conc: 16.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

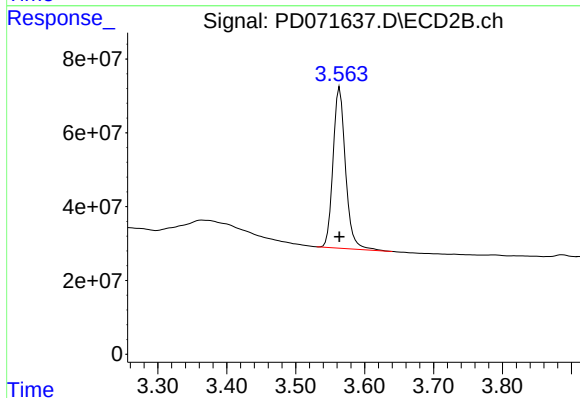


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 544852124
Conc: 16.62 ng/ml

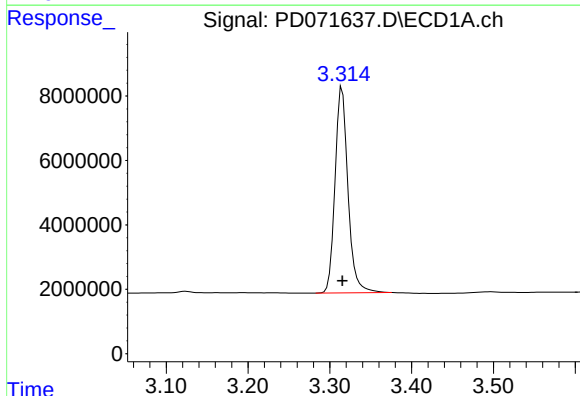


#2 alpha-BHC

R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 70335516
Conc: 17.10 ng/ml

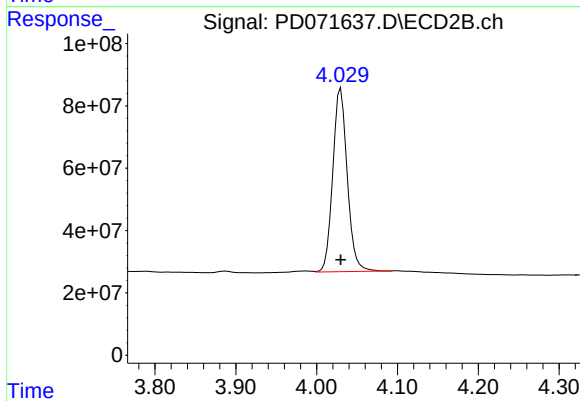

#2 alpha-BHC


R.T.: 4.030 min
Delta R.T.: 0.000 min
Response: 731449478
Conc: 17.32 ng/ml

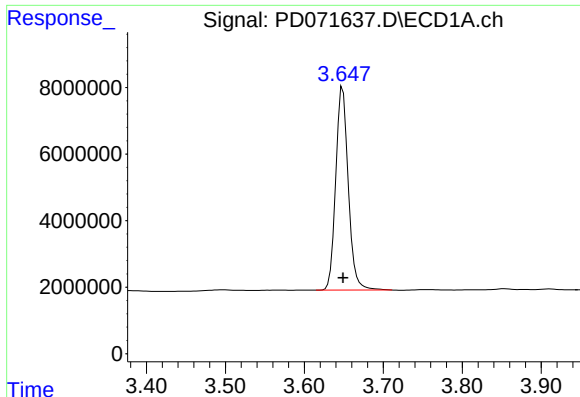

#3 gamma-BHC (Lindane)


R.T.: 3.649 min
Delta R.T.: 0.000 min
Response: 67477434
Conc: 17.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

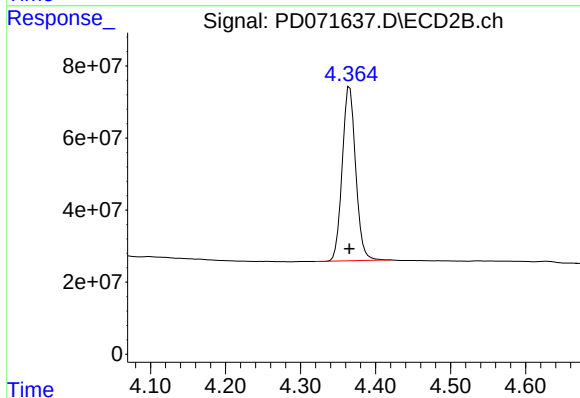


#3 gamma-BHC (Lindane)

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 602753682
Conc: 17.15 ng/ml

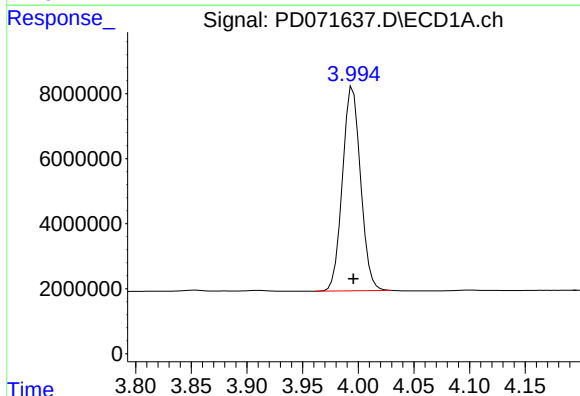


#4 Heptachlor

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 71124580
Conc: 17.49 ng/ml

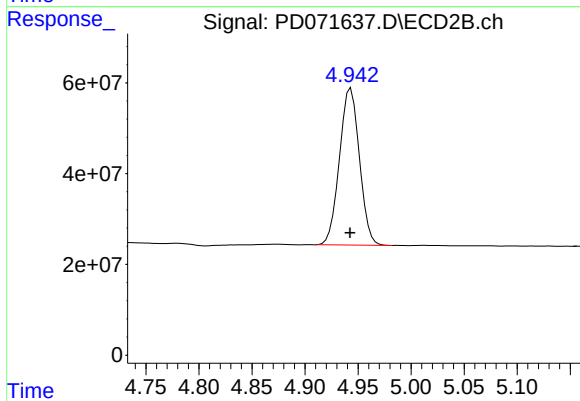

#4 Heptachlor


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 451272922
Conc: 17.55 ng/ml

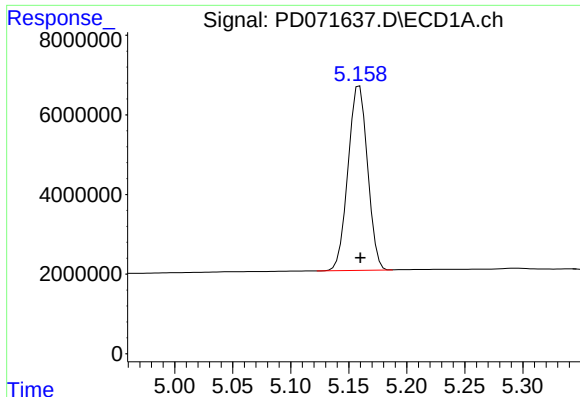

#9 Endosulfan I


R.T.: 5.159 min
Delta R.T.: 0.000 min
Response: 54225026
Conc: 15.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

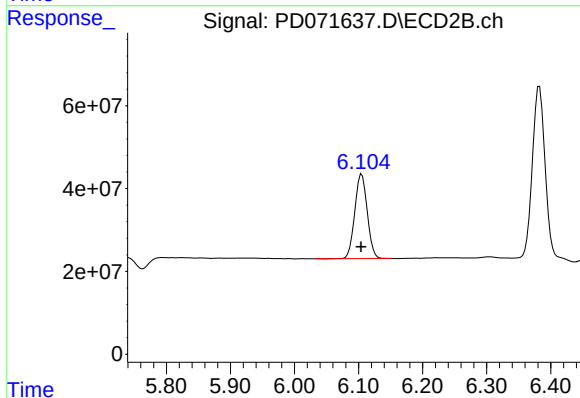


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 275760545
Conc: 17.10 ng/ml

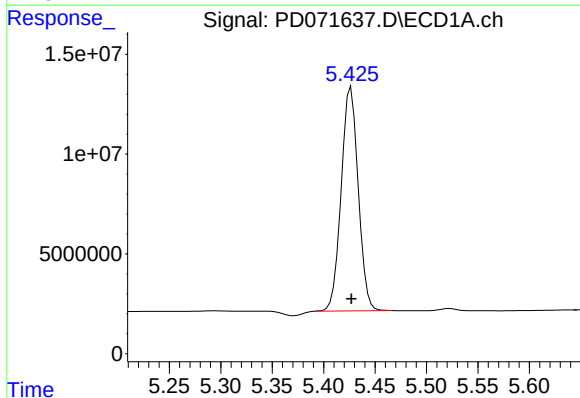


#13 Dieldrin

R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 129186287
Conc: 34.06 ng/ml

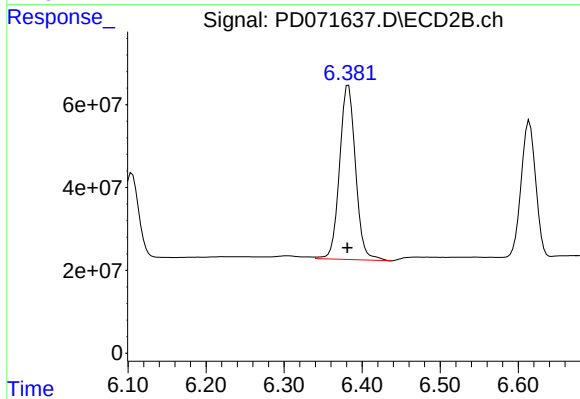

#13 Dieldrin


R.T.: 6.382 min
Delta R.T.: 0.001 min
Response: 598420069
Conc: 36.12 ng/ml

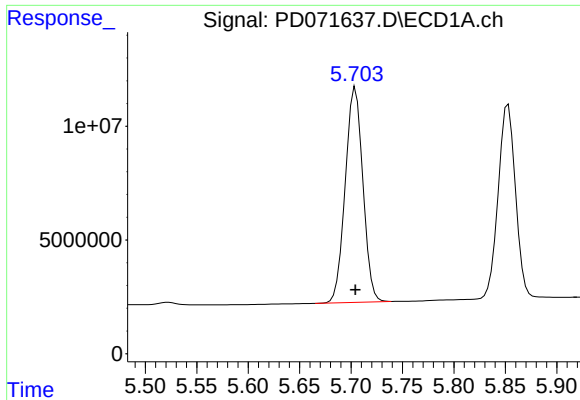

#14 Endrin


R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 112977980
Conc: 34.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

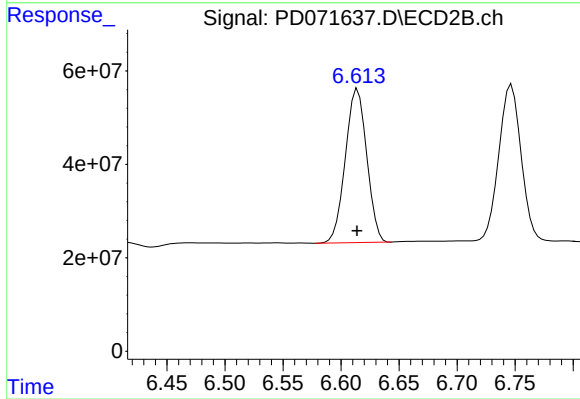


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 422389595
Conc: 33.28 ng/ml

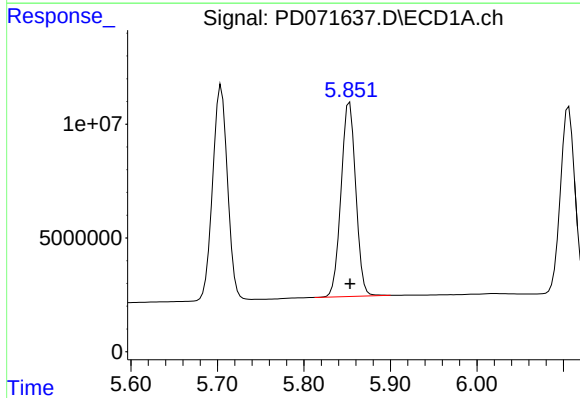


#16 4,4'-DDD

R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 100372817
Conc: 36.89 ng/ml

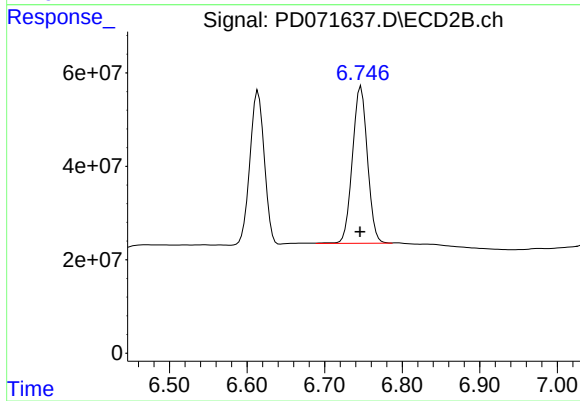

#16 4,4'-DDD


R.T.: 6.747 min
Delta R.T.: 0.001 min
Response: 451952183
Conc: 37.12 ng/ml

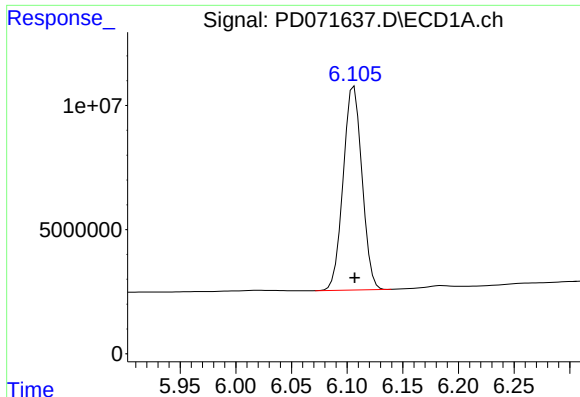

#17 4,4'-DDT


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 96550928
Conc: 34.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

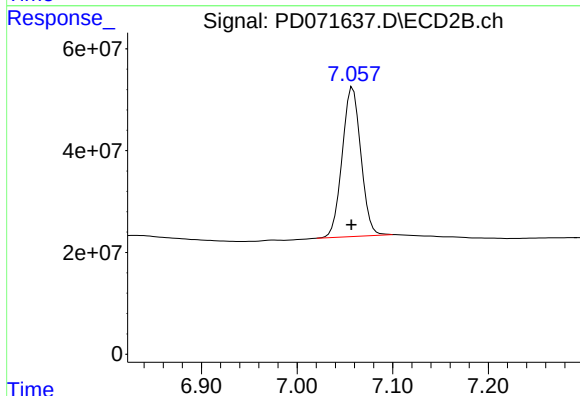


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.001 min
Response: 400178022
Conc: 33.83 ng/ml

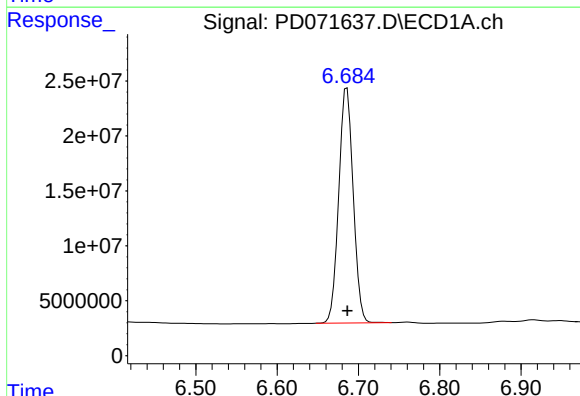


#20 Methoxychlor

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 264162385
Conc: 182.97 ng/ml

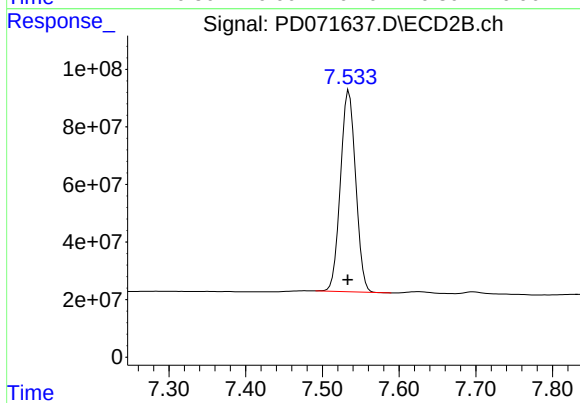

#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.001 min
Response: 964838553
Conc: 183.42 ng/ml

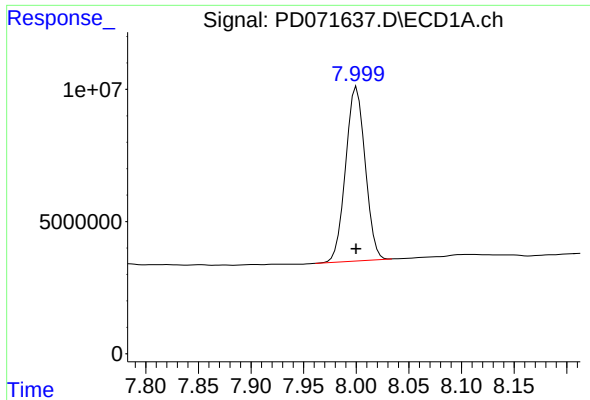

#27 Decachlorobiphenyl


R.T.: 8.000 min

Delta R.T.: 0.000 min

Response: 85298616

Conc: 30.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3141

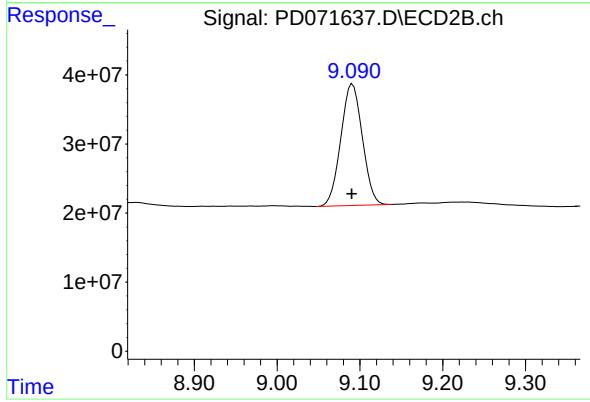

#27 Decachlorobiphenyl

R.T.: 9.091 min

Delta R.T.: 0.001 min

Response: 317710977

Conc: 33.14 ng/ml