

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
 Data File : PD071639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 13:47
 Operator : AR\AJ
 Sample : N4210-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC51

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:01:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.810	3.563	35928376	398.5E6	12.595	12.157
27) SA Decachlor...	8.002	9.090	53538678	231.2E6	19.069	24.114 #
Target Compounds						
16) A 4,4'-DDD	5.851	6.747	897458	19203352	0.330m	1.577 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081822\
Data File : PD071639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 13:47
Operator : AR\AJ
Sample : N4210-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:01:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

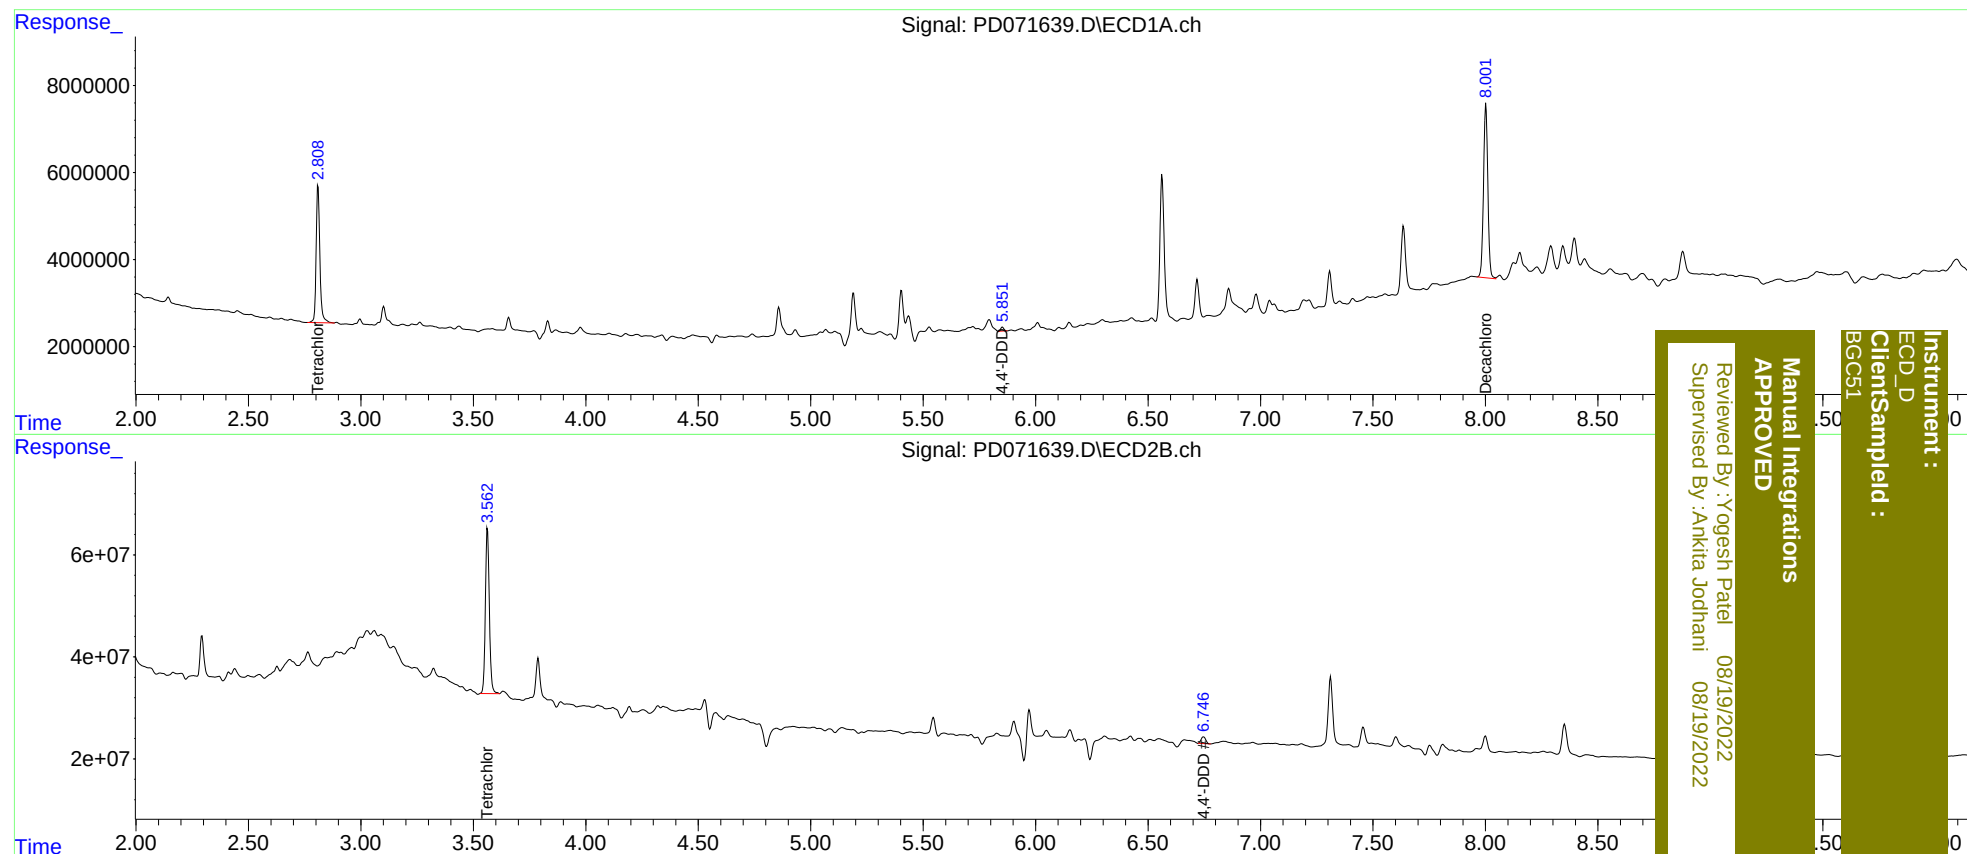

Instrument :
ECD_D
ClientSampled :
BGC51

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/19/2022
Supervised By : Ankita Jodhani 08/19/2022

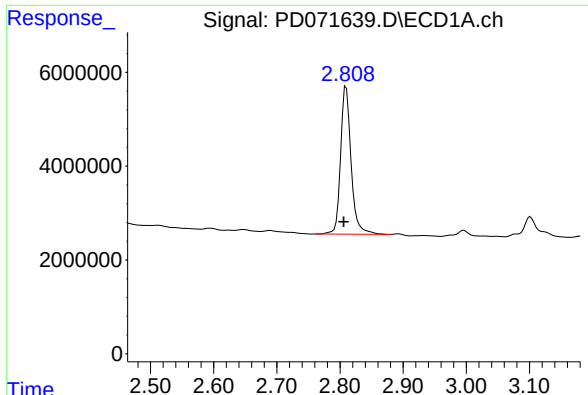

#1 Tetrachloro-m-xylene

R.T.: 2.810 min
Delta R.T.: 0.004 min
Response: 35928376
Conc: 12.60 ng/ml

Instrument :


ECD_D

ClientSampleId :

BGC51


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

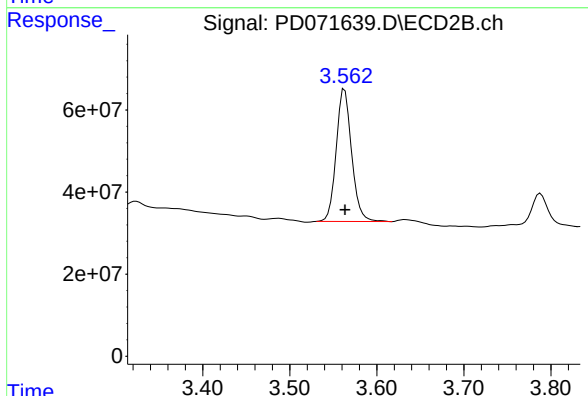


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 398471323
Conc: 12.16 ng/ml

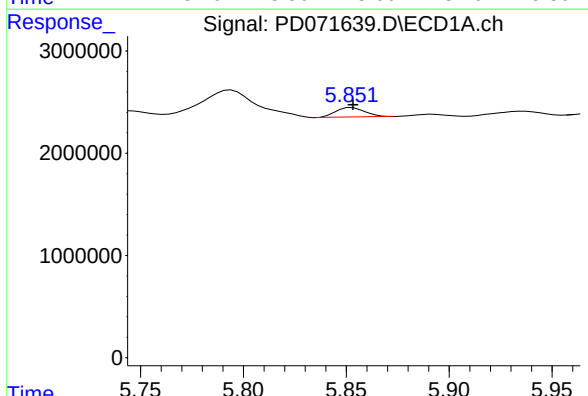


#16 4,4'-DDD

R.T.: 5.851 min
Delta R.T.: -0.002 min
Response: 897458
Conc: 0.33 ng/ml m

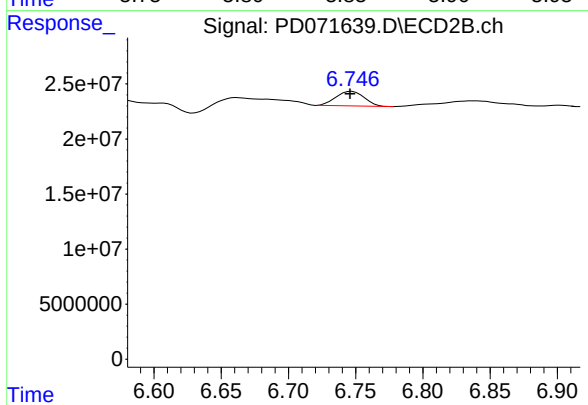

#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.001 min
Response: 19203352
Conc: 1.58 ng/ml

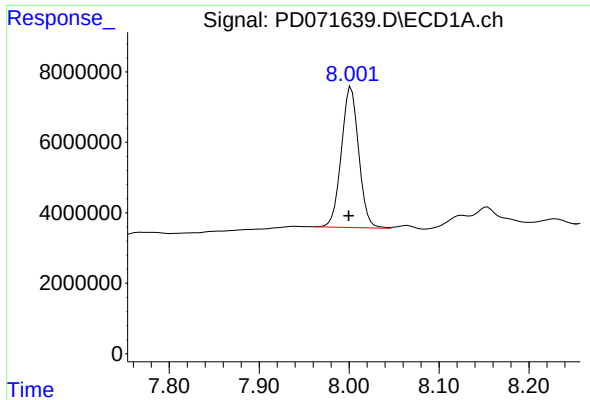


#27 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.003 min
Response: 53538678
Conc: 19.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
BGC51

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

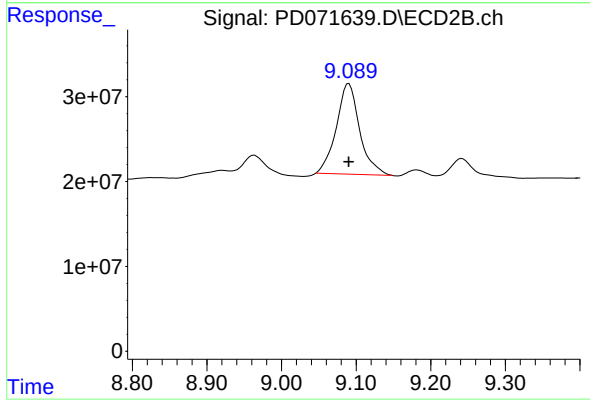

#27 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 231169068
Conc: 24.11 ng/ml