

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081823\
 Data File : PD077226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 12:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 17:58:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds							
28) SA Decachlor...	9.078	0.000	236187	0	0.086	N.D.	#
Target Compounds							
7) B delta-BHC	4.778	0.000	1207533	0	0.346	N.D.	#
8) B Heptachlo...	5.697	0.000	4912632	0	1.484	N.D.	#
13) MA Dieldrin	6.375f	0.000	334441	0	0.102	N.D.	#
14) MA Endrin	0.000	5.644f	0	430809	N.D.	0.294	#
15) B Endosulfa...	6.788f	0.000	641509	0	0.202	N.D.	#
21) B Endrin ke...	7.669	0.000	2094496	0	0.695	N.D.	#
24) Chlordane-2	0.000	4.331	0	1802930	N.D.	32.060	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081823\
Data File : PD077226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 12:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 17:58:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

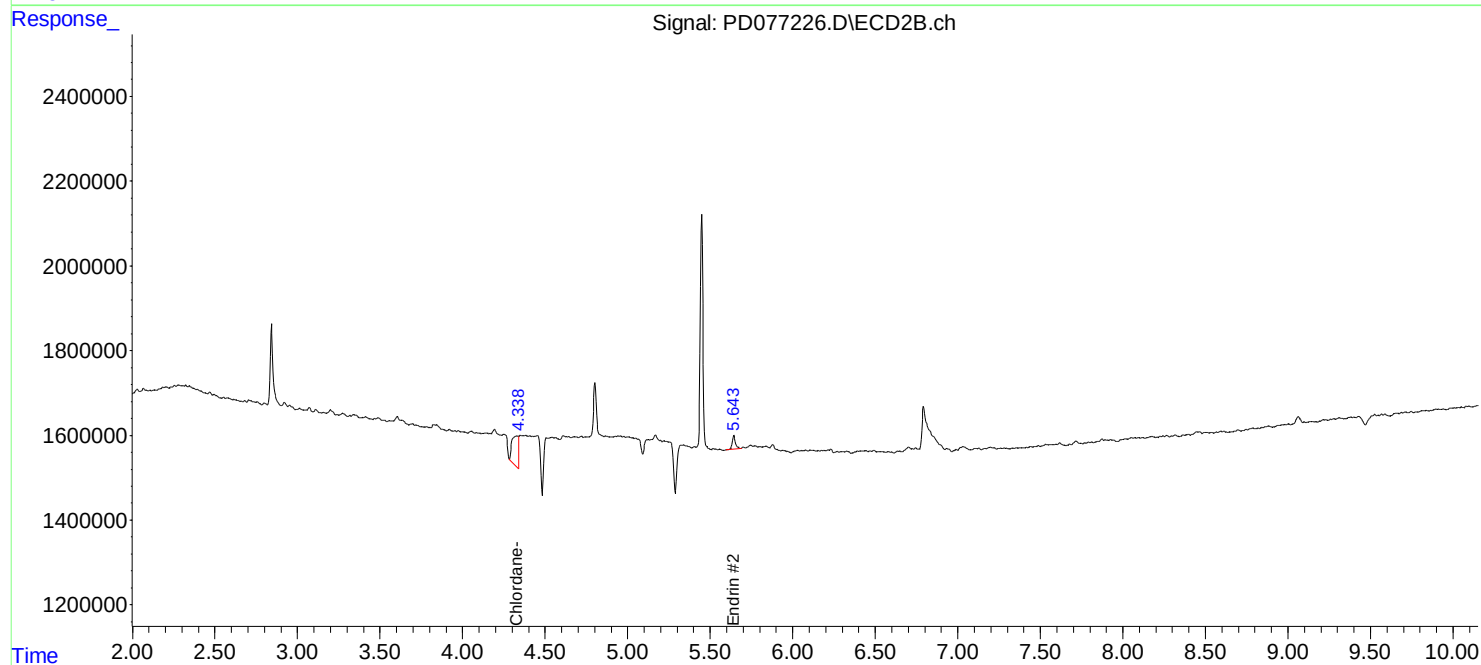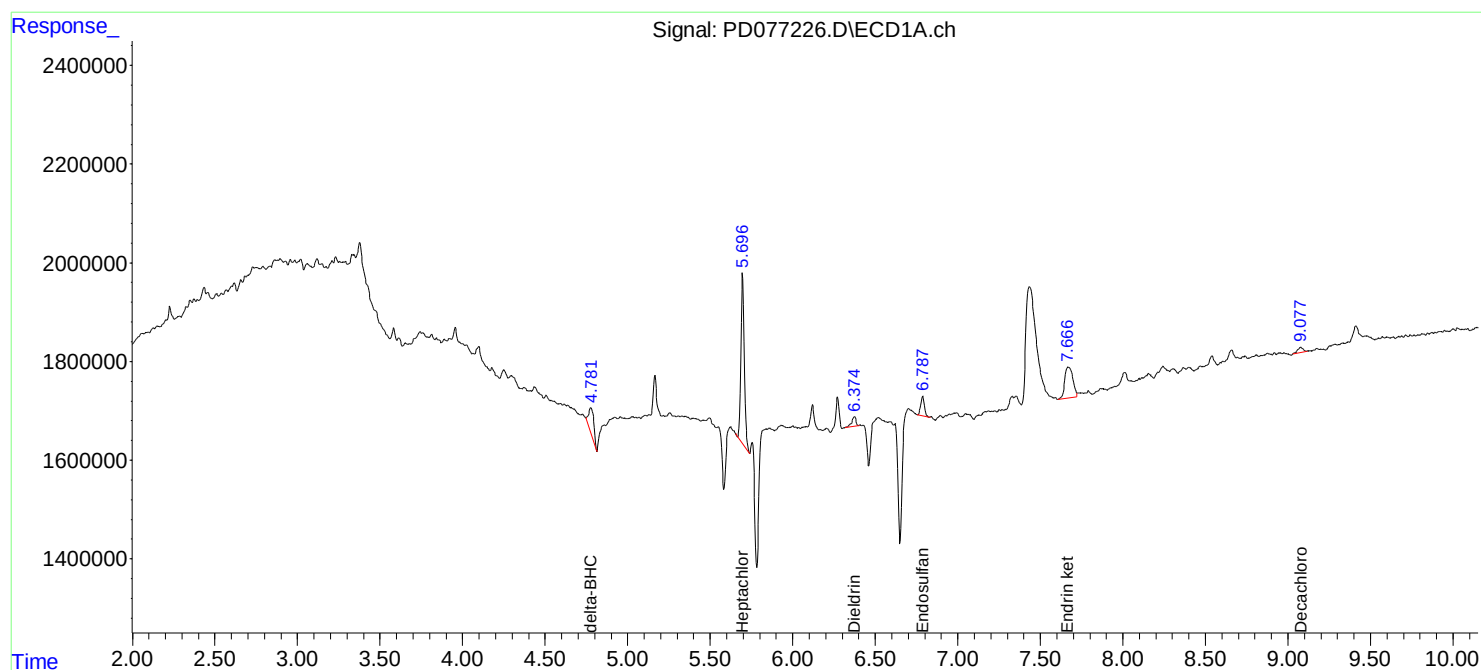


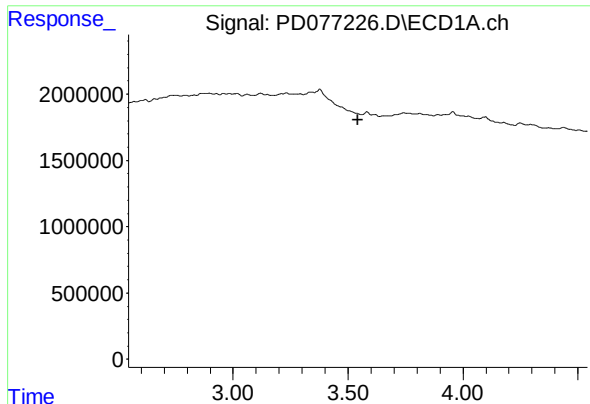

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

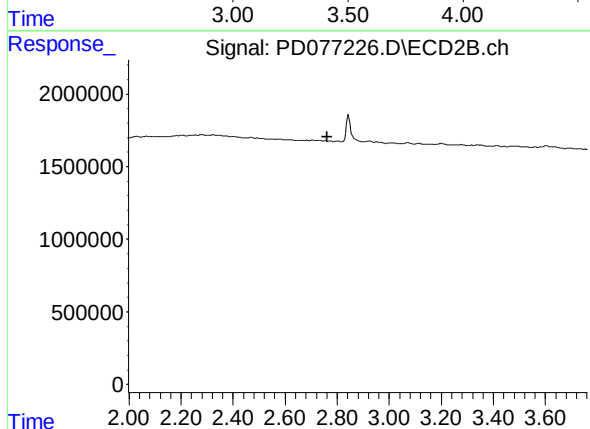


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.762 min
Response: 0
Conc: N.D.

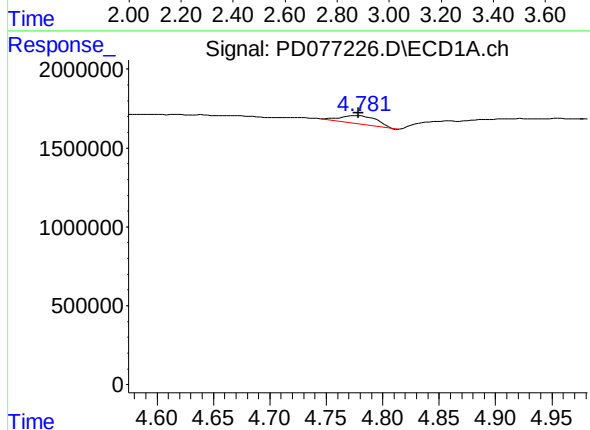


#7 delta-BHC

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 1207533
Conc: 0.35 ng/ml

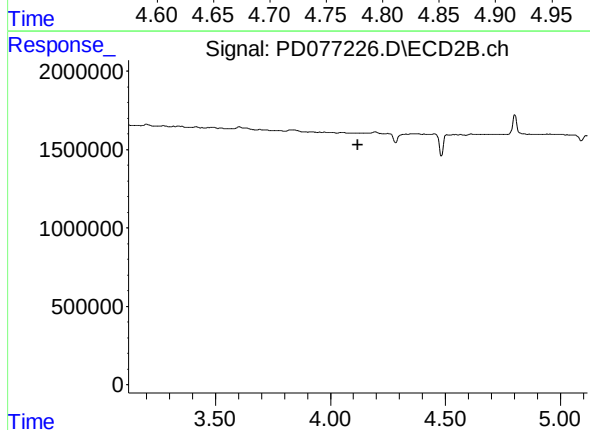

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.120 min
Response: 0
Conc: N.D.

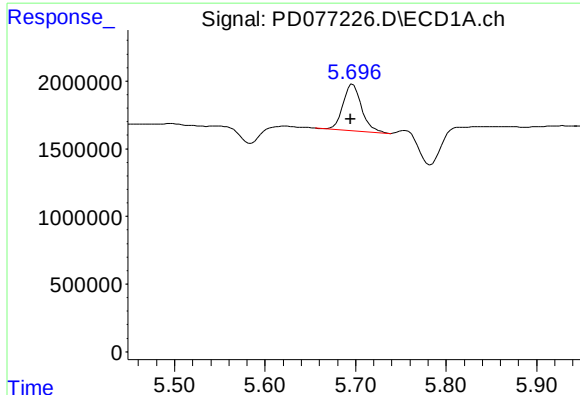

#8 Heptachlor epoxide


R.T.: 5.697 min
Delta R.T.: 0.002 min
Response: 4912632
Conc: 1.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

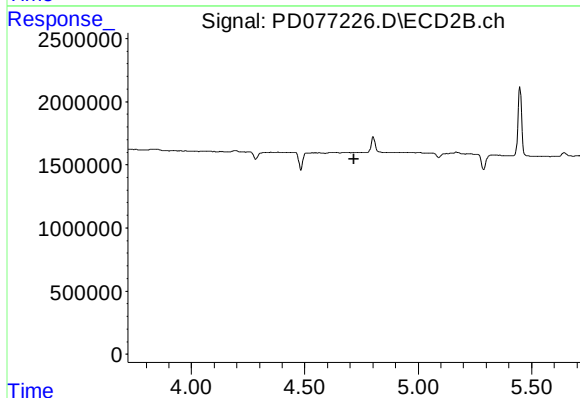


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

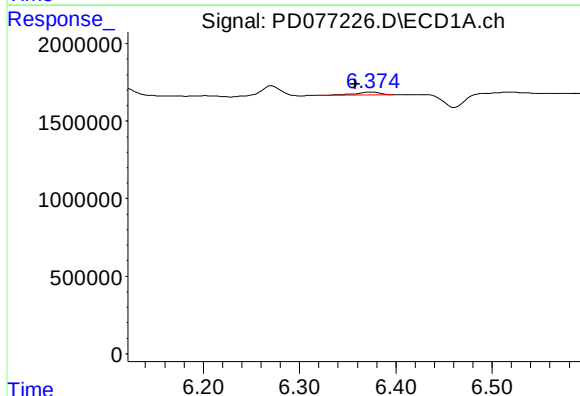


#13 Dieldrin

R.T.: 6.375 min
Delta R.T.: 0.017 min
Response: 334441
Conc: 0.10 ng/ml

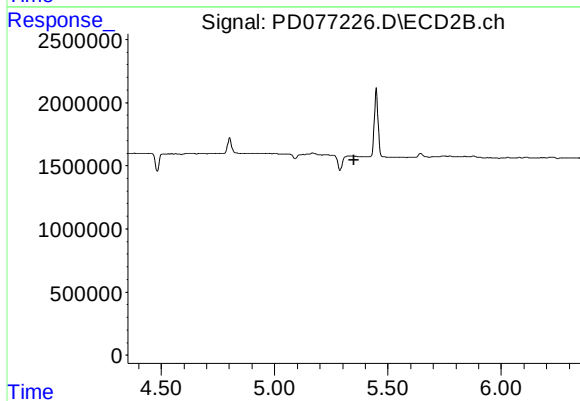

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

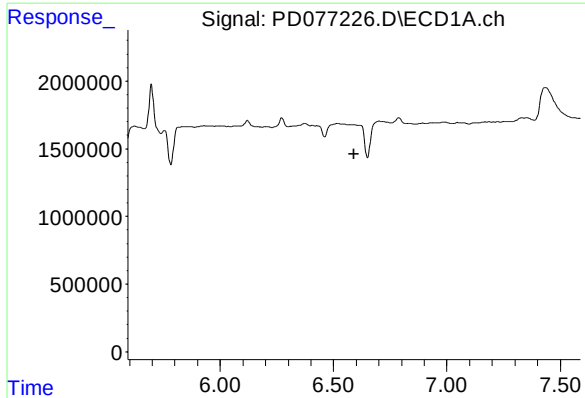

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

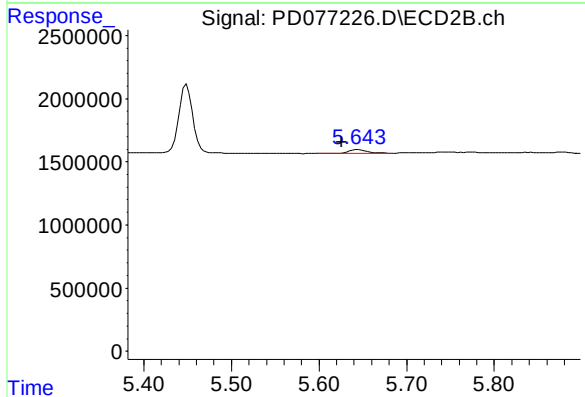


#14 Endrin

R.T.: 5.644 min
Delta R.T.: 0.018 min
Response: 430809
Conc: 0.29 ng/ml

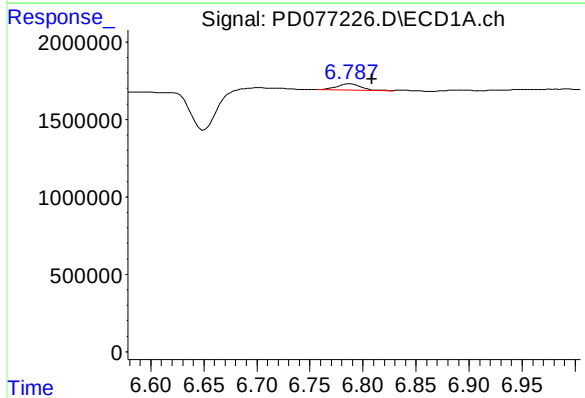


#15 Endosulfan II

R.T.: 6.788 min
Delta R.T.: -0.021 min
Response: 641509
Conc: 0.20 ng/ml

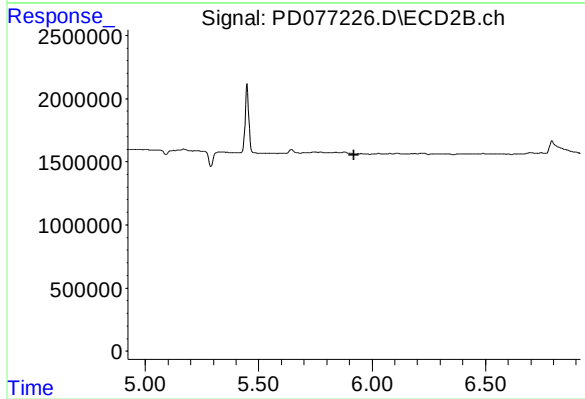

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

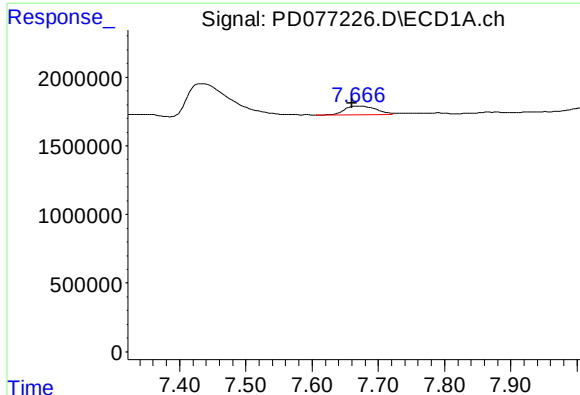

#21 Endrin ketone


R.T.: 7.669 min
Delta R.T.: 0.008 min
Response: 2094496
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

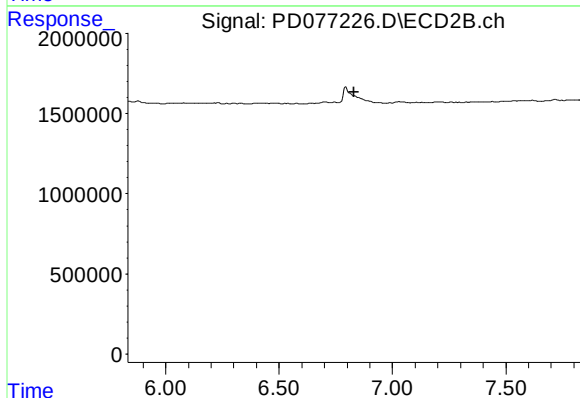


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

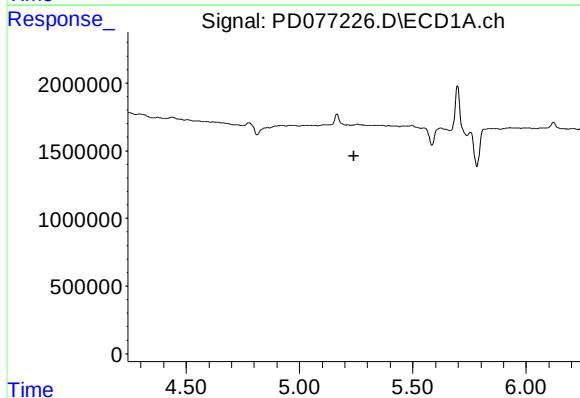


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

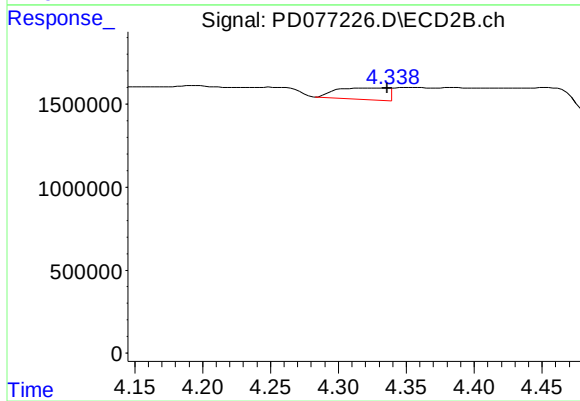

#24 Chlordane-2


R.T.: 4.331 min
Delta R.T.: -0.005 min
Response: 1802930
Conc: 32.06 ng/ml

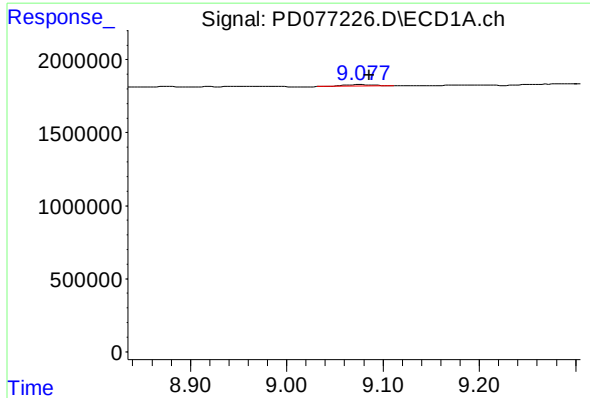

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: -0.008 min
Response: 236187
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

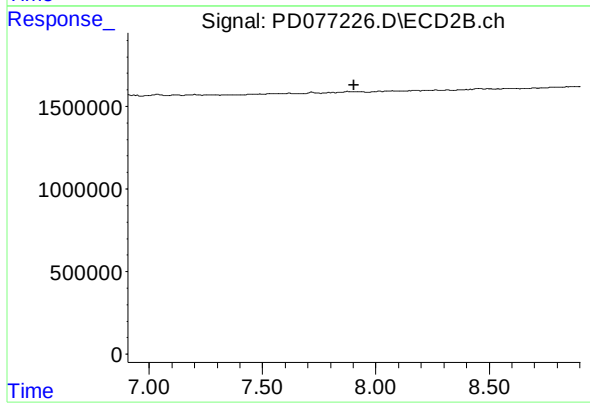

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.