

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081823\
 Data File : PD077227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 12:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 17:58:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.761	51279137	29522835	21.669	21.674
28)	SA Decachlor...	9.086	7.903	65517351	31247459	23.910	21.835
Target Compounds							
4)	MA Heptachlor	4.912	0.000	289514	0	0.080	N.D. #
7)	B delta-BHC	4.769	0.000	1890377	0	0.542	N.D. #
8)	B Heptachlo...	5.690	0.000	3060928	0	0.924	N.D. #
9)	A Endosulfan I	6.111f	5.114f	297969	155622	0.098	0.100
13)	MA Dieldrin	6.367	0.000	333530	0	0.102	N.D. #
14)	MA Endrin	0.000	5.644f	0	317685	N.D.	0.217 #
15)	B Endosulfa...	6.784f	0.000	1102992	0	0.347	N.D. #
21)	B Endrin ke...	7.691f	0.000	556259	0	0.185	N.D. #
24)	Chlordane-2	0.000	4.333	0	410796	N.D.	7.305 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081823\
Data File : PD077227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 12:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 17:58:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

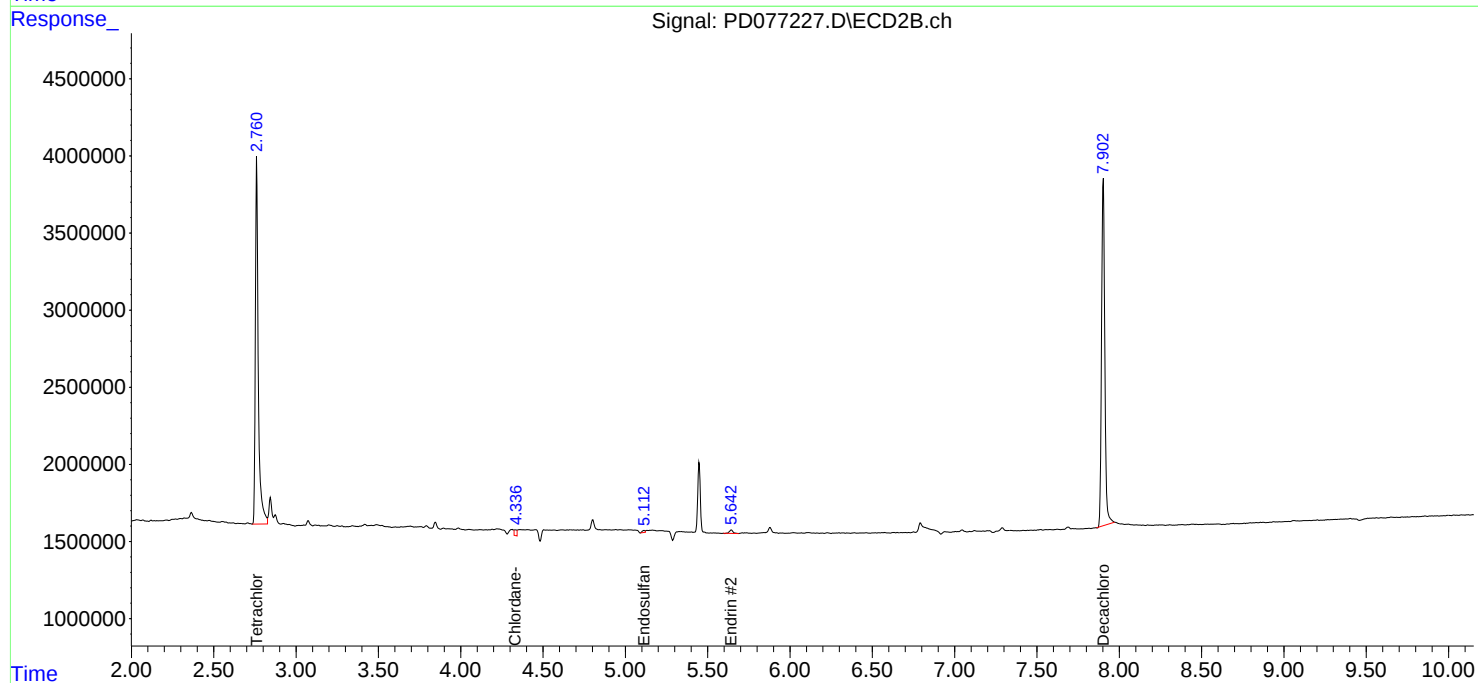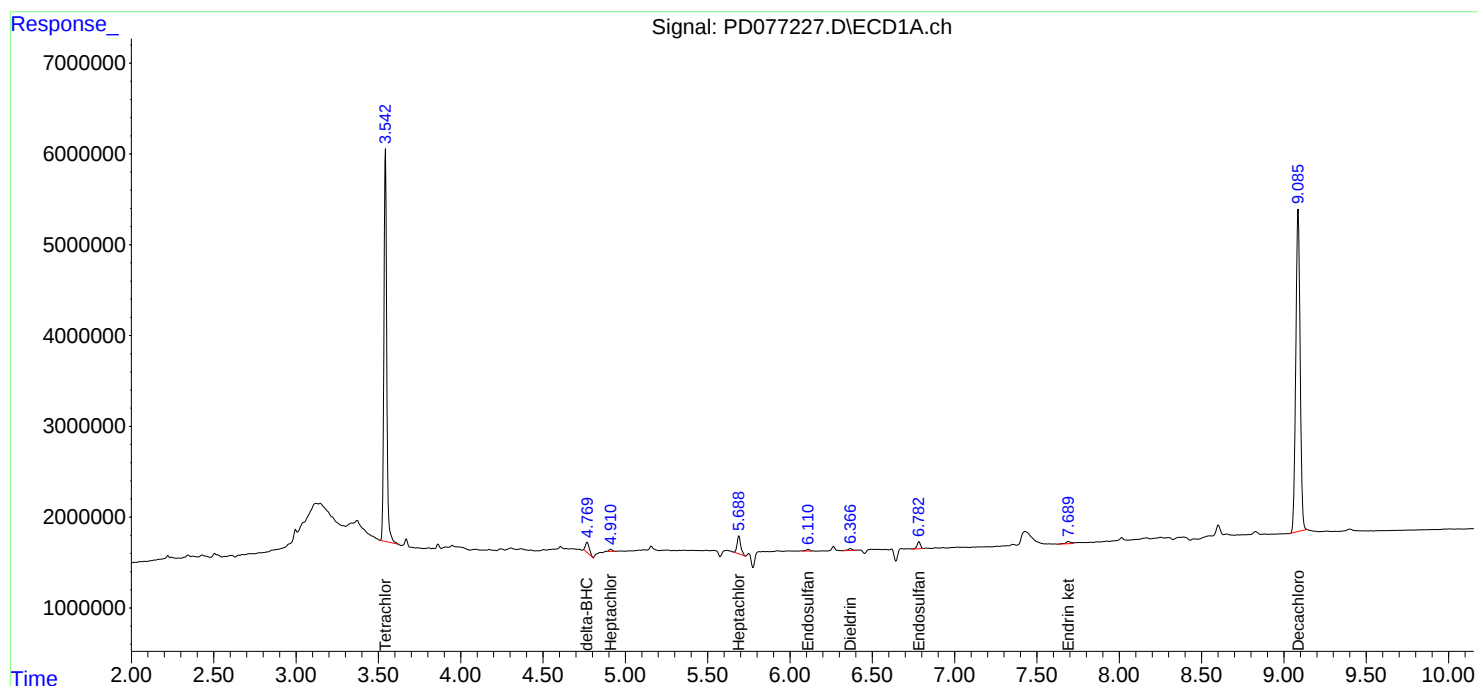


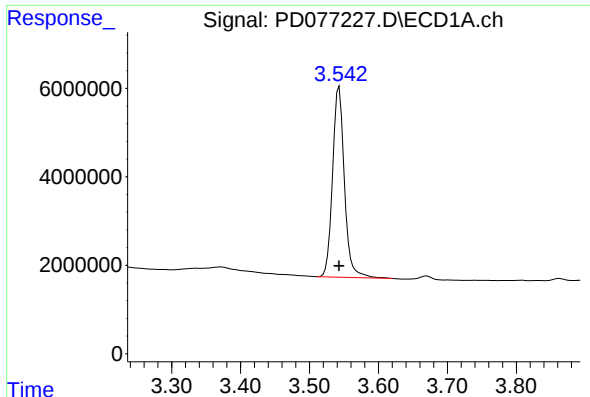

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 51279137
Conc: 21.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

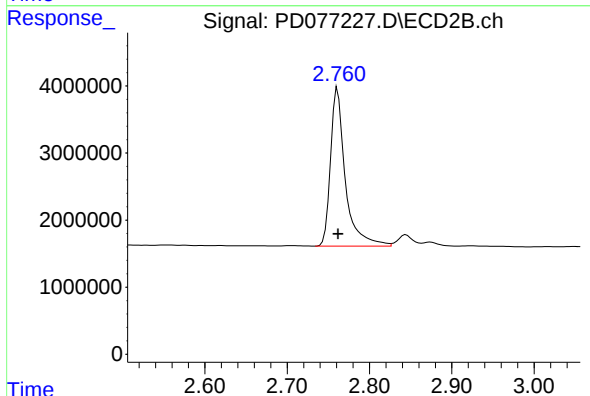


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 29522835
Conc: 21.67 ng/ml

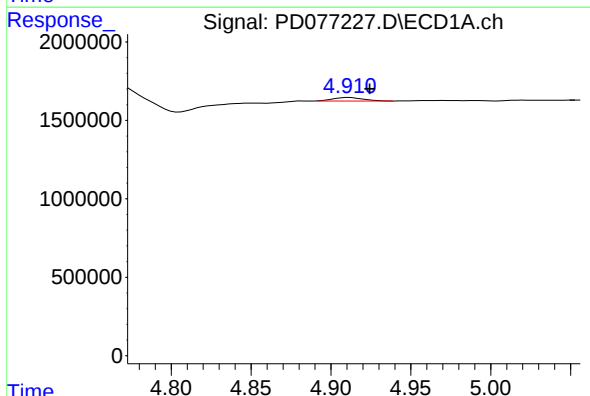


#4 Heptachlor

R.T.: 4.912 min
Delta R.T.: -0.013 min
Response: 289514
Conc: 0.08 ng/ml

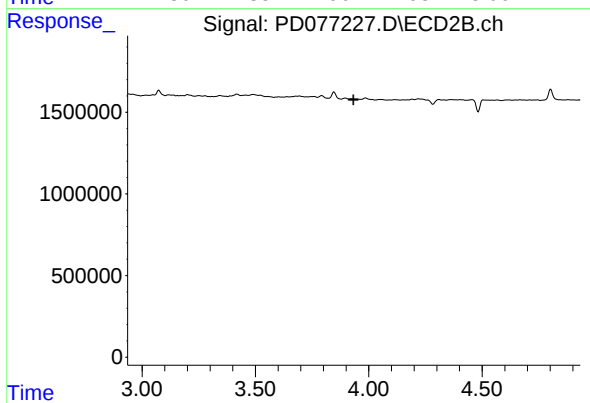

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

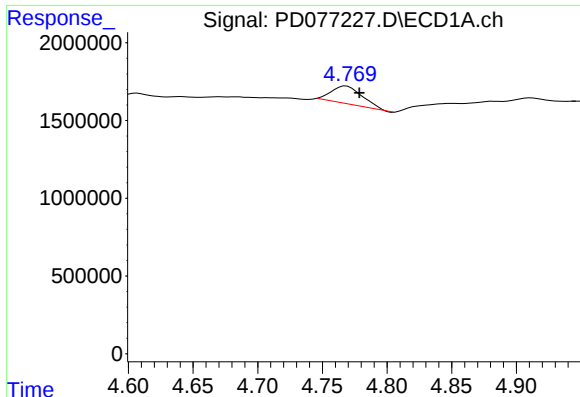

#7 delta-BHC


R.T.: 4.769 min
Delta R.T.: -0.010 min
Response: 1890377
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

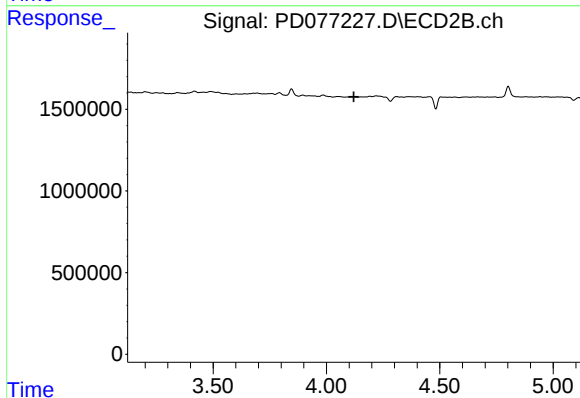


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

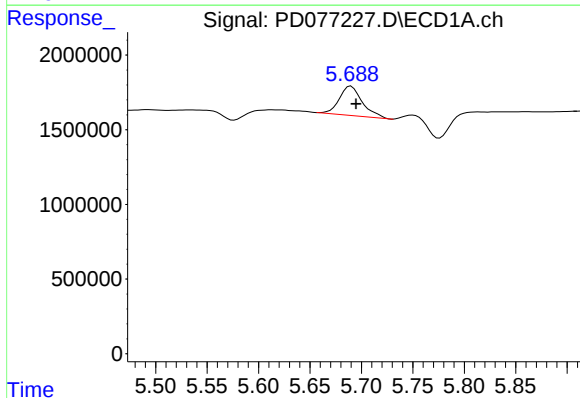


#8 Heptachlor epoxide

R.T.: 5.690 min
Delta R.T.: -0.005 min
Response: 3060928
Conc: 0.92 ng/ml

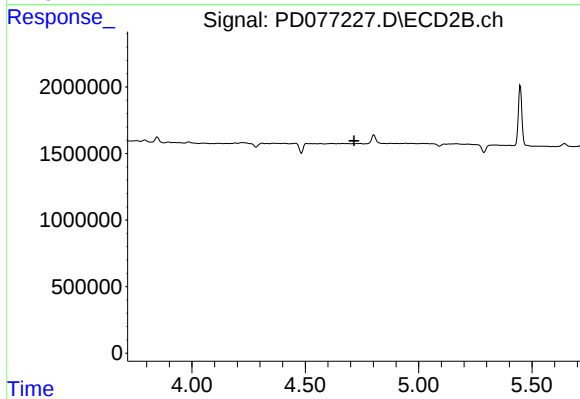

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

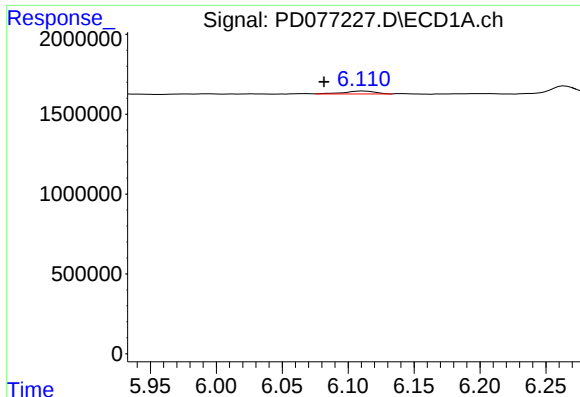

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.029 min
Response: 297969
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

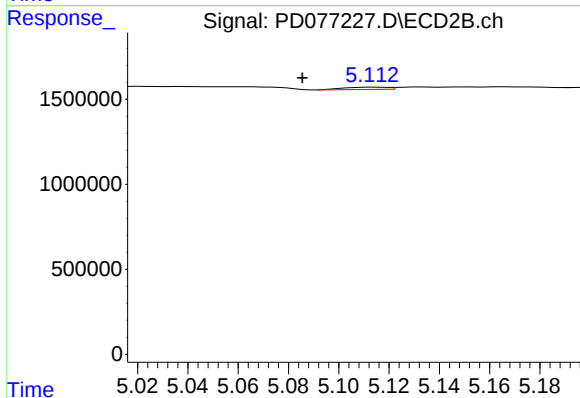


#9 Endosulfan I

R.T.: 5.114 min
Delta R.T.: 0.028 min
Response: 155622
Conc: 0.10 ng/ml

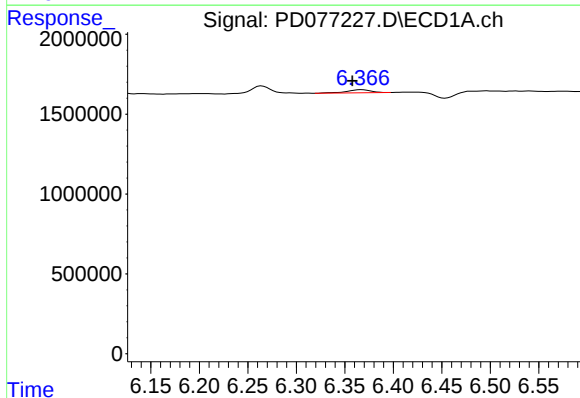


#13 Dieldrin

R.T.: 6.367 min
Delta R.T.: 0.010 min
Response: 333530
Conc: 0.10 ng/ml

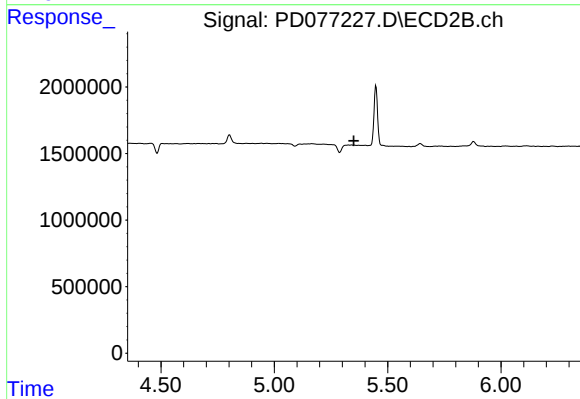

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

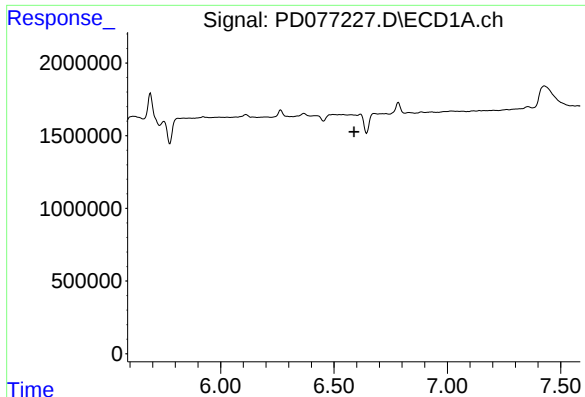

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

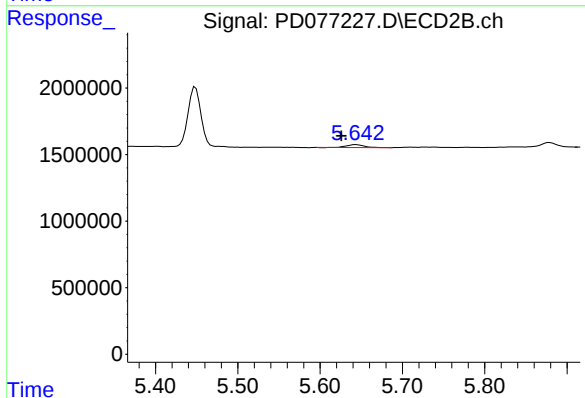


#14 Endrin

R.T.: 5.644 min
Delta R.T.: 0.018 min
Response: 317685
Conc: 0.22 ng/ml

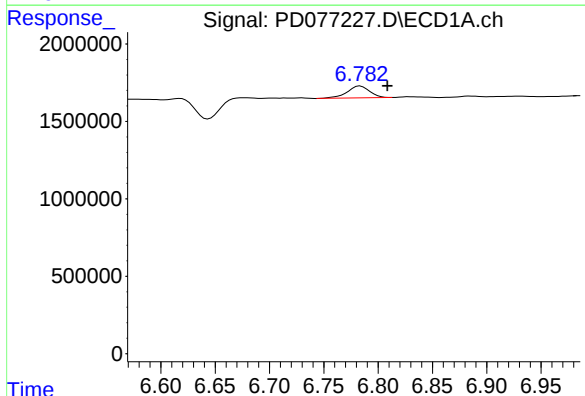


#15 Endosulfan II

R.T.: 6.784 min
Delta R.T.: -0.025 min
Response: 1102992
Conc: 0.35 ng/ml

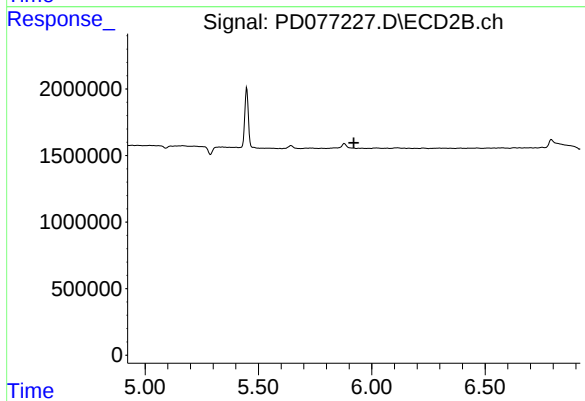

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

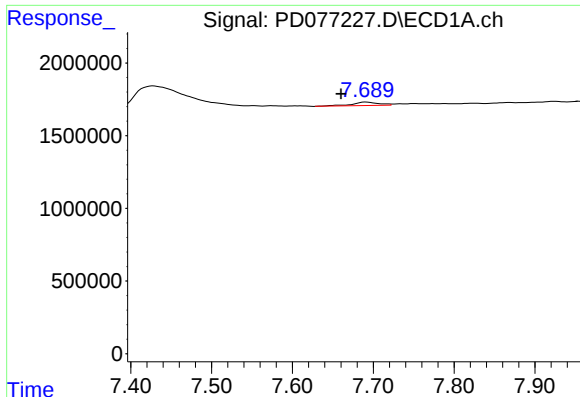

#21 Endrin ketone


R.T.: 7.691 min
Delta R.T.: 0.031 min
Response: 556259
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

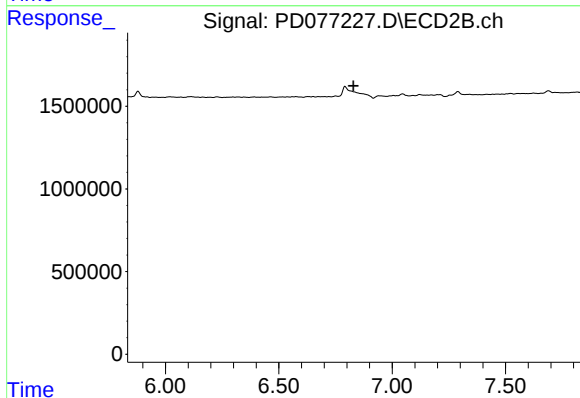


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

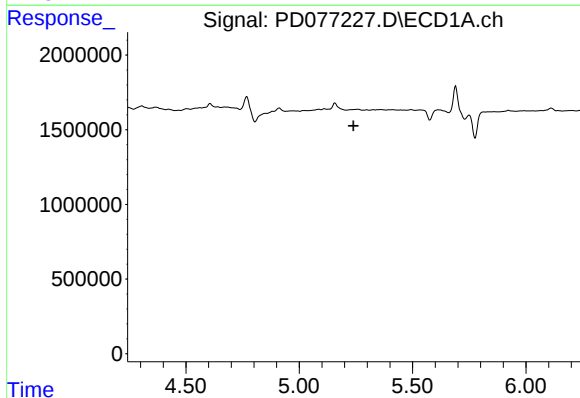


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

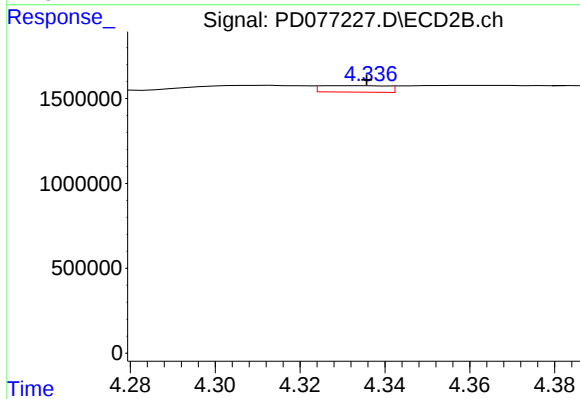

#24 Chlordane-2


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 410796
Conc: 7.30 ng/ml

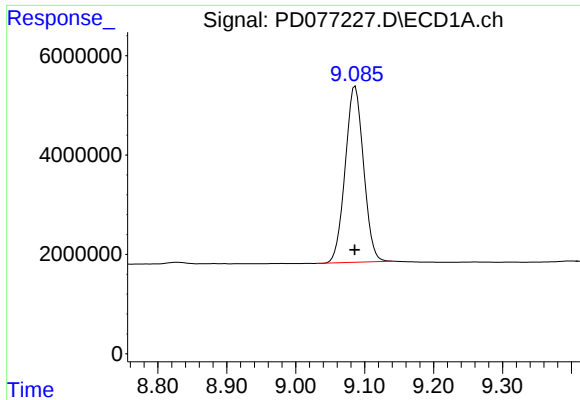

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 65517351
Conc: 23.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

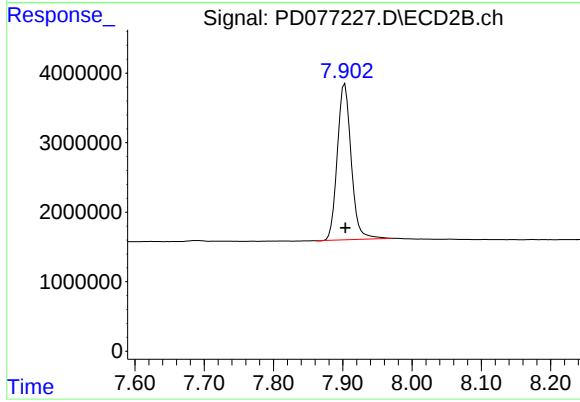

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 31247459
Conc: 21.83 ng/ml