

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081920\
 Data File : PD059040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2020 10:33
 Operator : DD\AJ
 Sample : L3613-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFP9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:56:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	13624020	21490315	14.088	14.839
27)	SA Decachlor...	7.841	8.862	24175597	28769874	22.952	20.978
Target Compounds							
6)	B beta-BHC	4.101f	0.000	1022313	0	1.736	N.D. #
9)	A Endosulfan I	0.000	6.086	0	680957	N.D.	0.439
10)	B trans-Chl...	0.000	5.932	0	706071	N.D.	0.424
16)	A 4,4'-DDD	0.000	6.627f	0	773788	N.D.	0.590
19)	B Endosulfa...	6.344	0.000	10610176	0	10.368	N.D. #
20)	A Methoxychlor	0.000	7.362f	0	13991945	N.D.	20.252
21)	B Endrin ke...	0.000	7.572	0	1887163	N.D.	1.298
23)	Toxaphene-2	5.502	0.000	95410889	0	13186.357	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081920\
Data File : PD059040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2020 10:33
Operator : DD\AJ
Sample : L3613-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DBFP9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:56:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

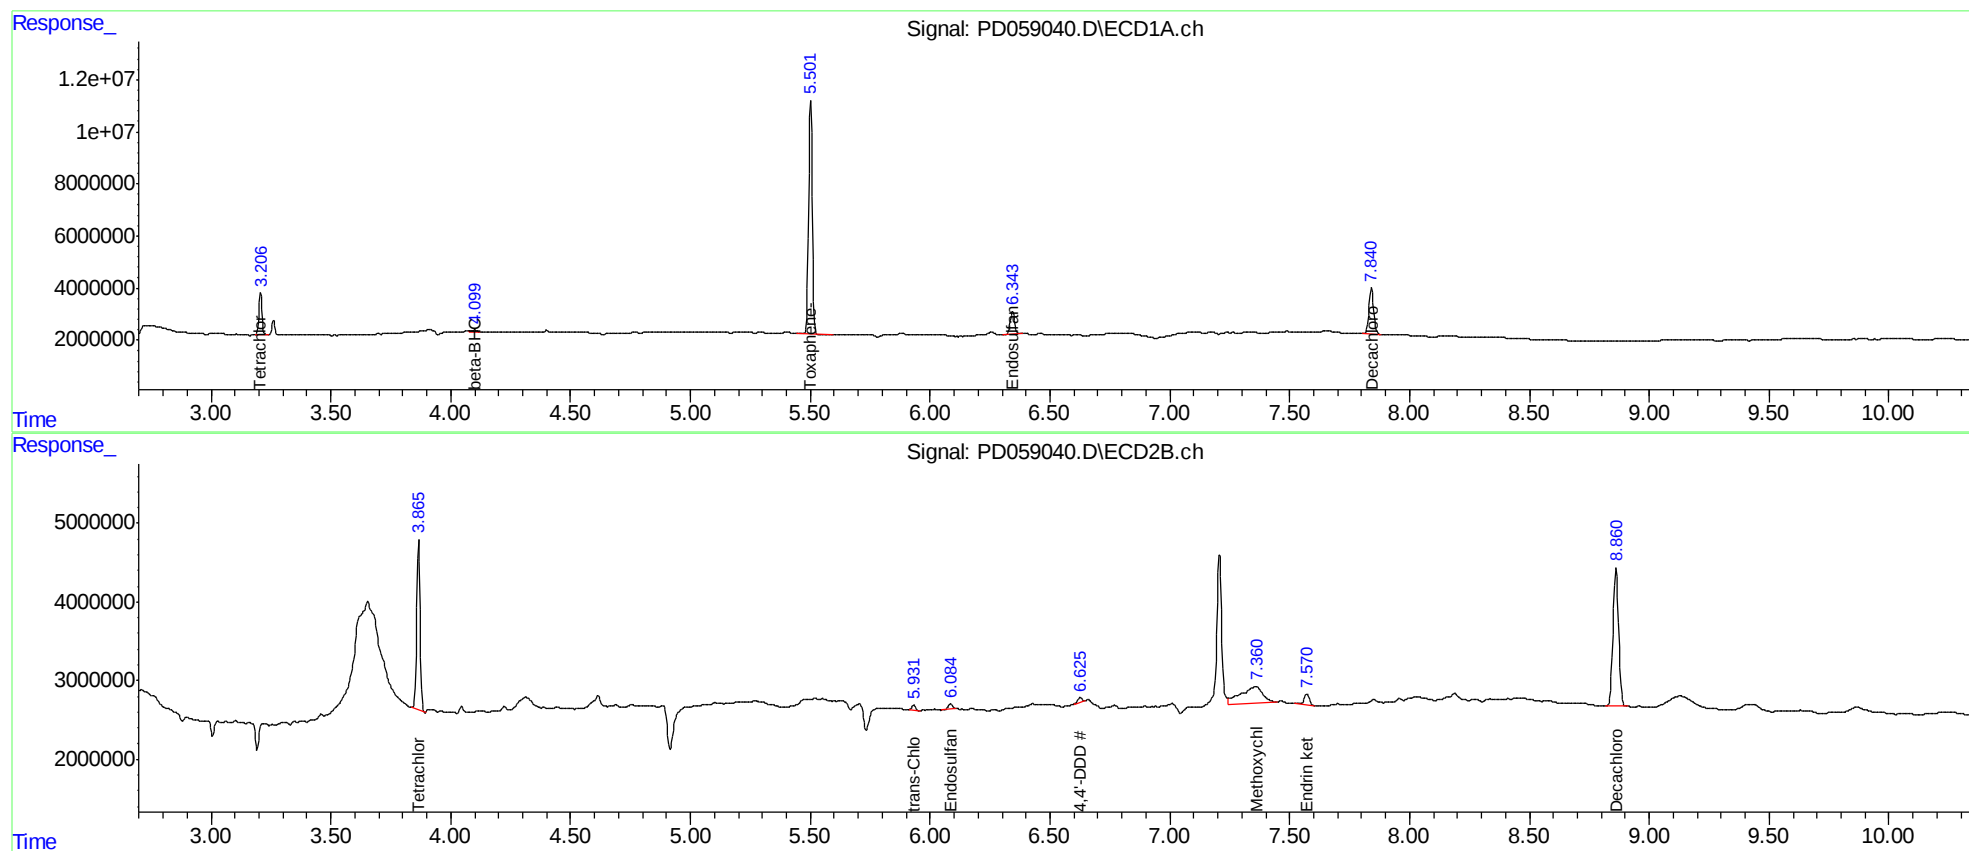


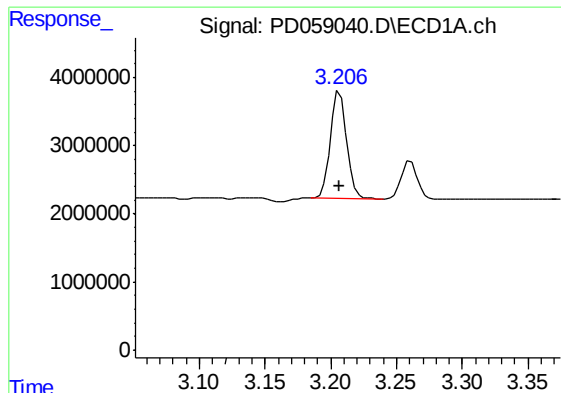

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 13624020
Conc: 14.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFP9

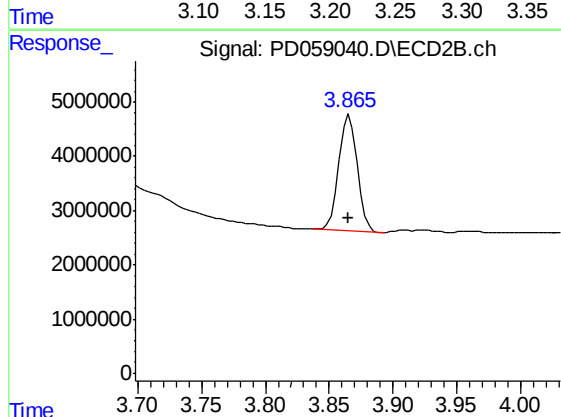


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.001 min
Response: 21490315
Conc: 14.84 ng/ml

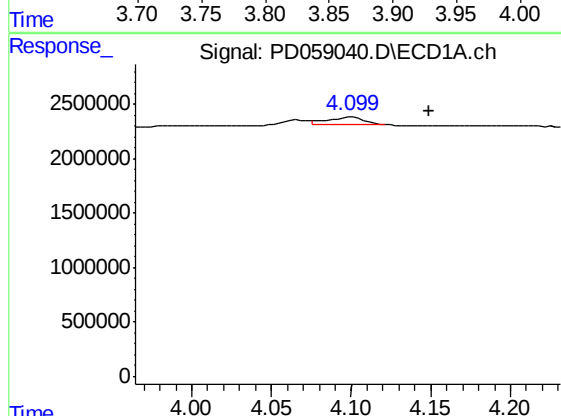


#6 beta-BHC

R.T.: 4.101 min
Delta R.T.: -0.048 min
Response: 1022313
Conc: 1.74 ng/ml

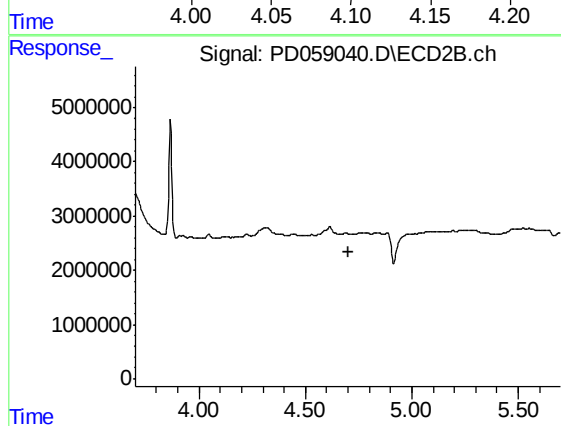

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

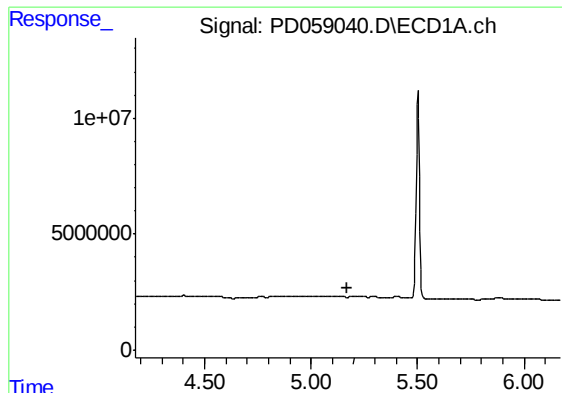

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFP9

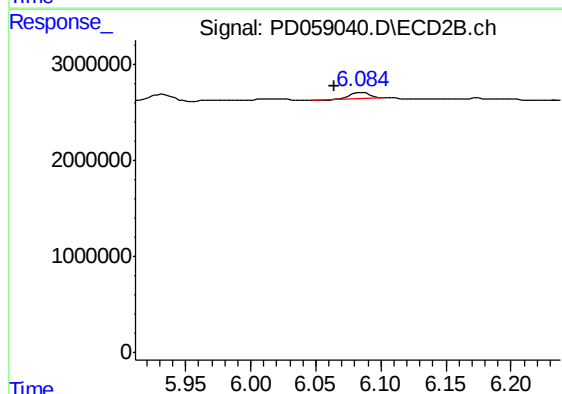


#9 Endosulfan I

R.T.: 6.086 min
Delta R.T.: 0.022 min
Response: 680957
Conc: 0.44 ng/ml

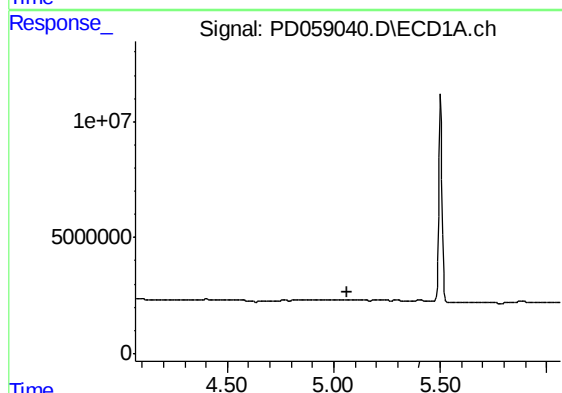


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.065 min
Response: 0
Conc: N.D.

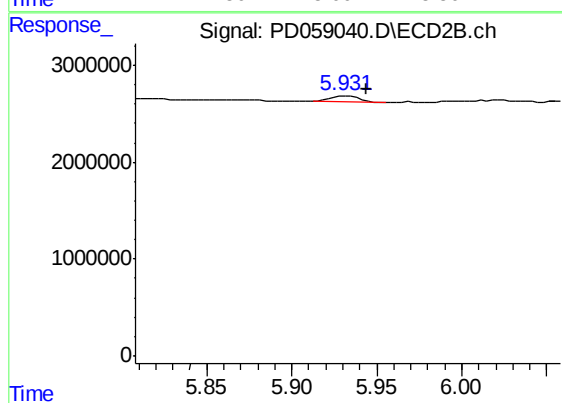

#10 trans-Chlordane


R.T.: 5.932 min
Delta R.T.: -0.012 min
Response: 706071
Conc: 0.42 ng/ml

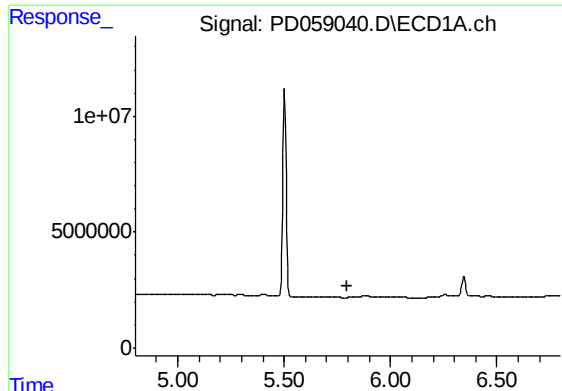

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFP9

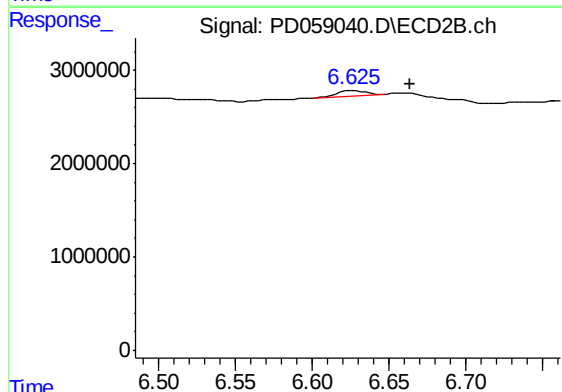


#16 4,4'-DDD

R.T.: 6.627 min
Delta R.T.: -0.036 min
Response: 773788
Conc: 0.59 ng/ml

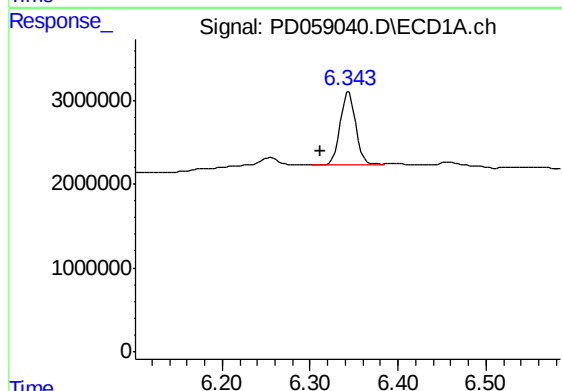


#19 Endosulfan Sulfate

R.T.: 6.344 min
Delta R.T.: 0.032 min
Response: 10610176
Conc: 10.37 ng/ml

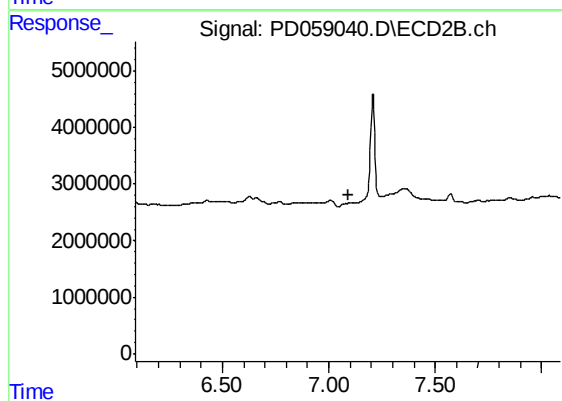

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

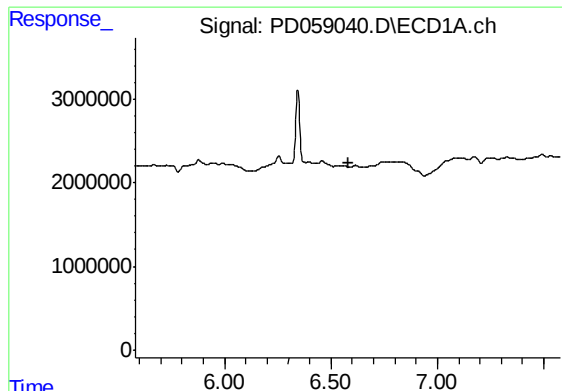

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.580 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DBFP9

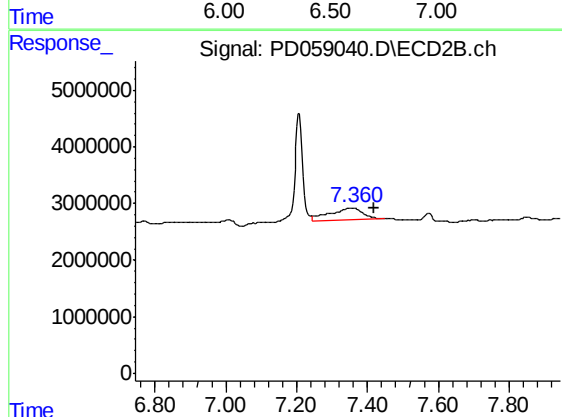


#20 Methoxychlor

R.T.: 7.362 min
Delta R.T.: -0.058 min
Response: 13991945
Conc: 20.25 ng/ml

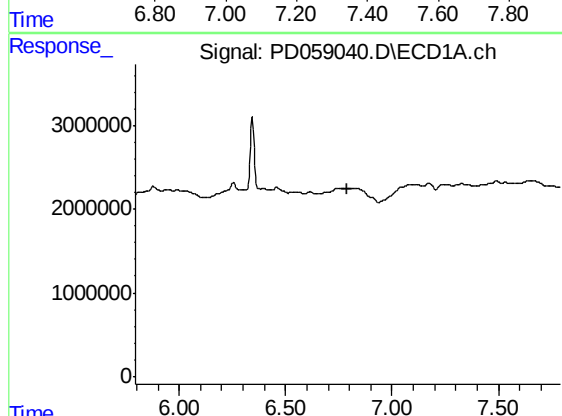


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.792 min
Response: 0
Conc: N.D.

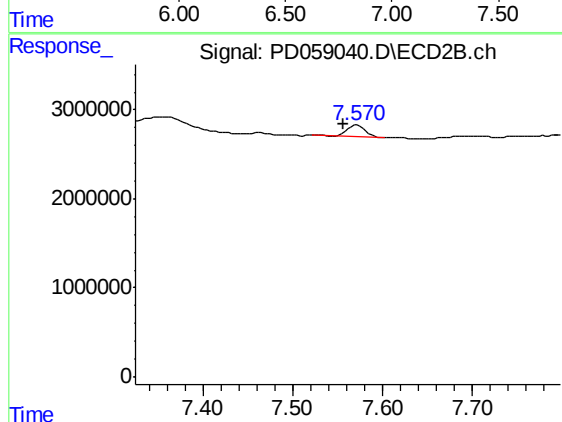

#21 Endrin ketone


R.T.: 7.572 min
Delta R.T.: 0.016 min
Response: 1887163
Conc: 1.30 ng/ml

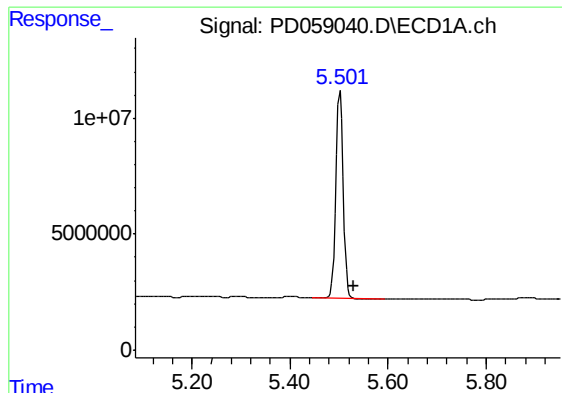

#23 Toxaphene-2


R.T.: 5.502 min
Delta R.T.: -0.027 min
Response: 95410889
Conc: 13186.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
DBFP9

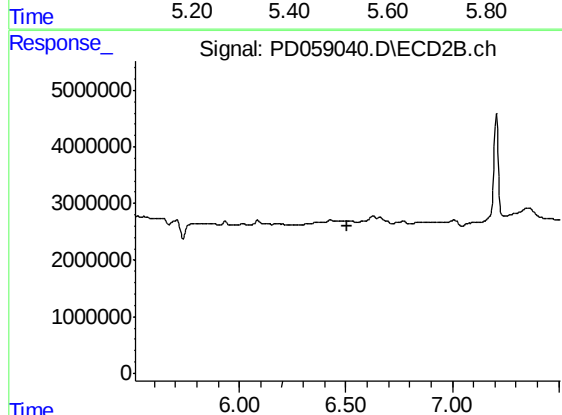


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

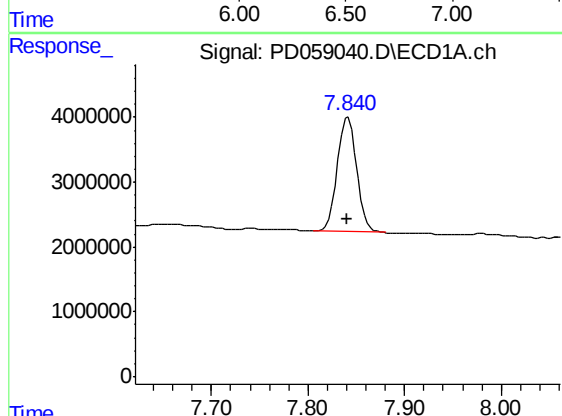

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 24175597
Conc: 22.95 ng/ml

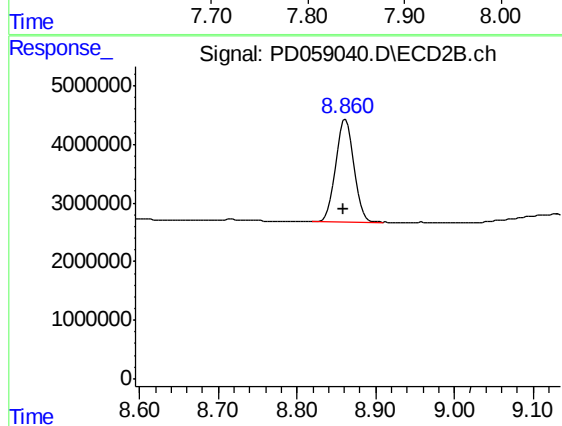

#27 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.003 min
Response: 28769874
Conc: 20.98 ng/ml