

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081920\
 Data File : PD059049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2020 12:41
 Operator : DD\AJ
 Sample : L3613-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFR1

Manual Integrations
 APPROVED

Ankita
 8/20/2020 2:27:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 07:19:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	16386153	24495501	16.944	16.914
27)	SA Decachlor...	7.840	8.861	24264649	28448486	23.037	20.744
Target Compounds							
10)	B trans-Chl...	5.064	5.938	1215423	4708625	1.051m	2.827 #
11)	B cis-Chlor...	5.117	6.017	1287396	1896224	1.106m	1.126m
12)	B 4,4'-DDE	5.289	6.171	970765	1562545	0.844m	0.986
13)	MA Dieldrin	5.406	6.320	4639456	1483928	3.819	0.887 #
16)	A 4,4'-DDD	5.798	6.659	802027	5388730	0.851m	4.111 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081920\
Data File : PD059049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2020 12:41
Operator : DD\AJ
Sample : L3613-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 07:19:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

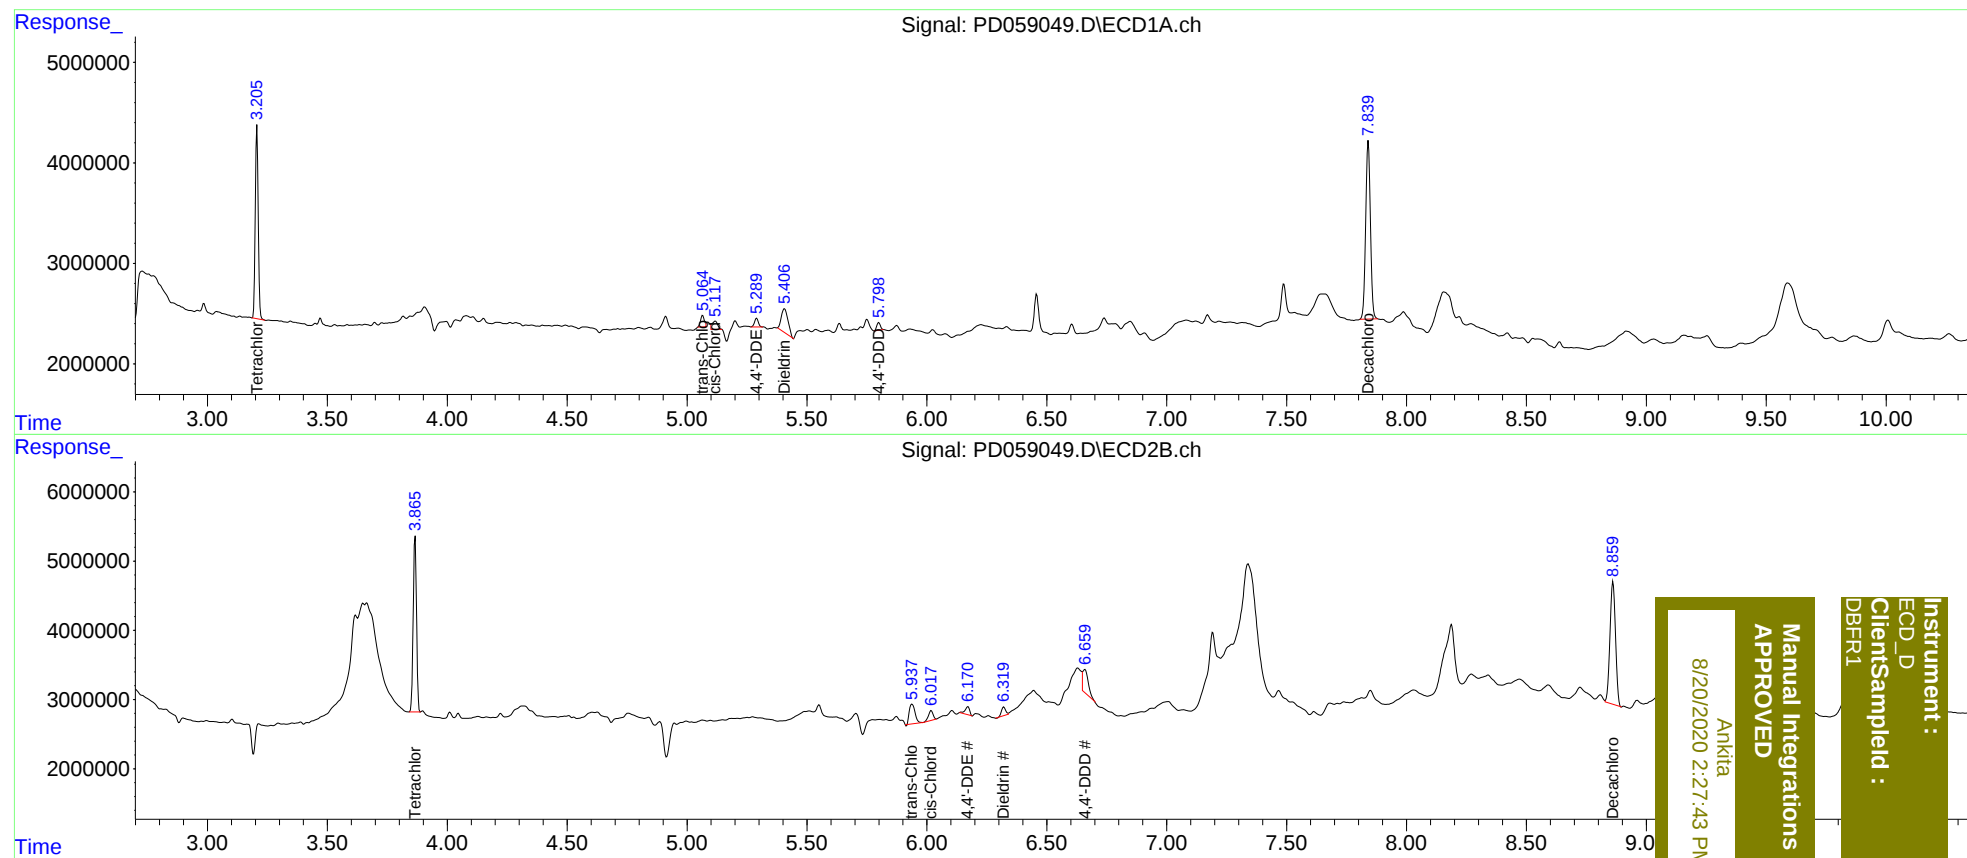

8/20/2020 2:27:43 PM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBFR1