

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081923\
 Data File : PD077234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 08:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 21:35:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	4.027f	0.000	10271	0	0.003	N.D. #
5) MB	Aldrin	5.272	4.194f	47915	546972	0.013	0.295 #
7) B	delta-BHC	4.782	0.000	1045171	0	0.300	N.D. #
8) B	Heptachlo...	5.699	0.000	6518574	0	1.969	N.D. #
13) MA	Dieldrin	6.378f	0.000	240056	0	0.073	N.D. #
14) MA	Endrin	0.000	5.646f	0	448998	N.D.	0.307 #
15) B	Endosulfa...	6.792f	0.000	631067	0	0.198	N.D. #
16) A	4,4'-DDD	6.710	0.000	249307	0	0.106	N.D. #
17) MA	4,4'-DDT	7.058f	0.000	296740	0	0.122	N.D. #
22)	Mirex	8.161f	0.000	14385	0	0.006	N.D. #
24)	Chlordane-2	5.227	4.357f	88467	6216004	0.729	110.535 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081923\
Data File : PD077234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 08:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 21:35:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

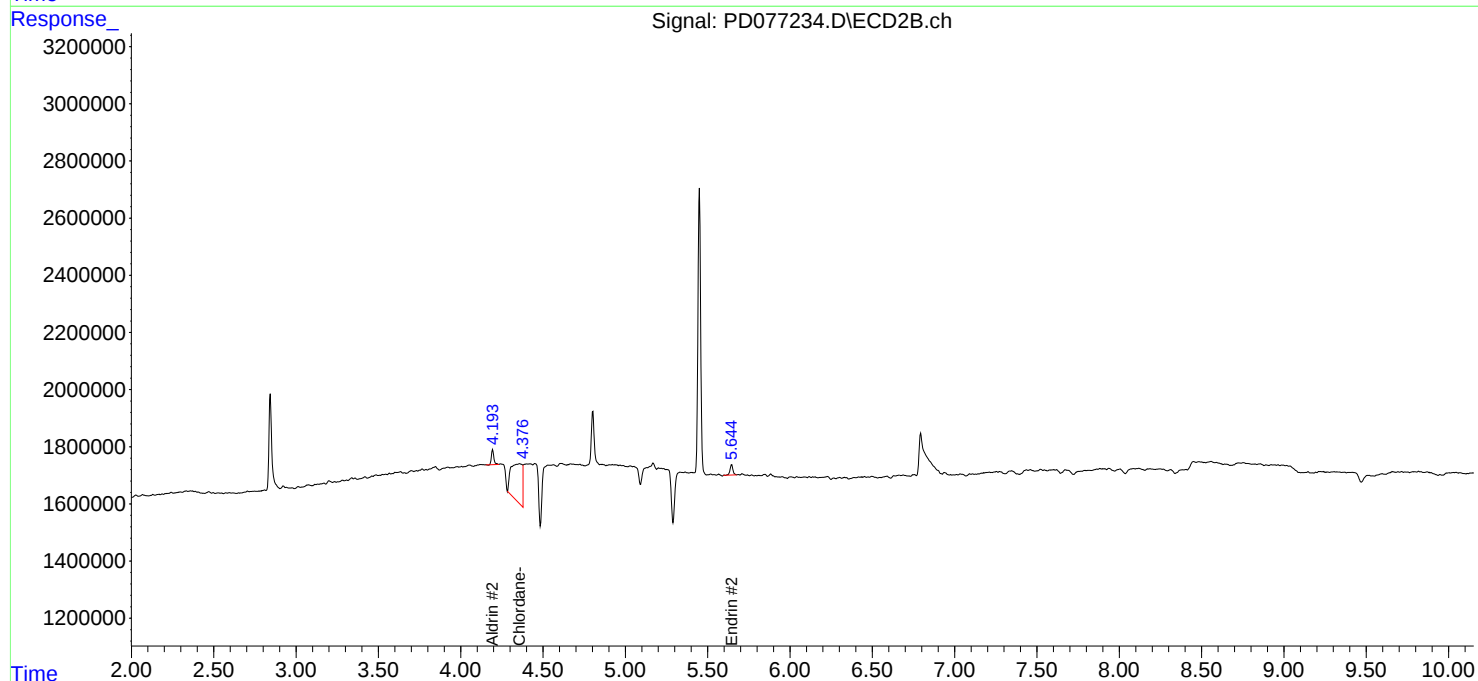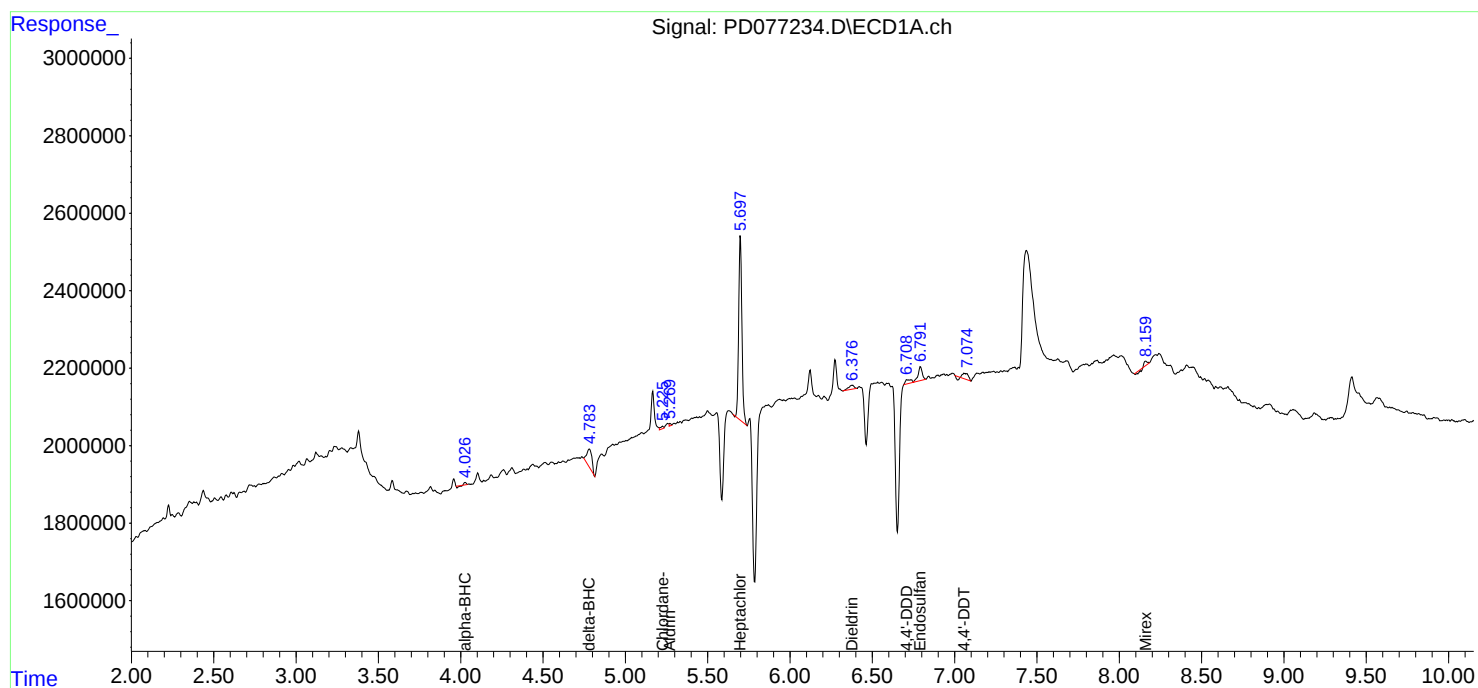


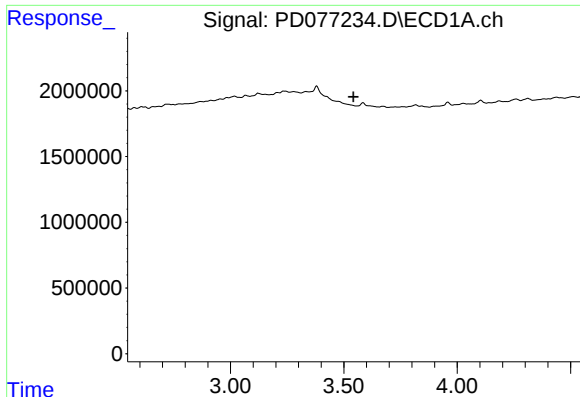

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

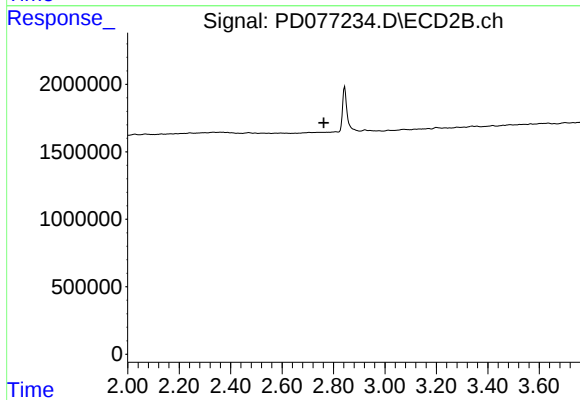


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.762 min
Response: 0
Conc: N.D.

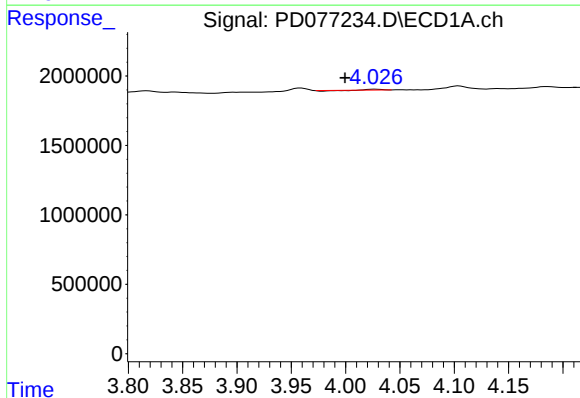


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.027 min
Response: 10271
Conc: 0.00 ng/ml

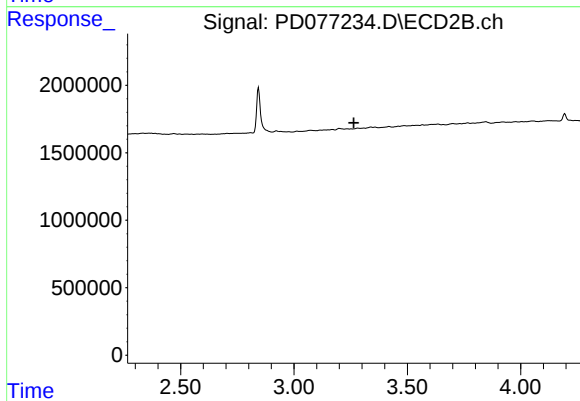

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.264 min
Response: 0
Conc: N.D.

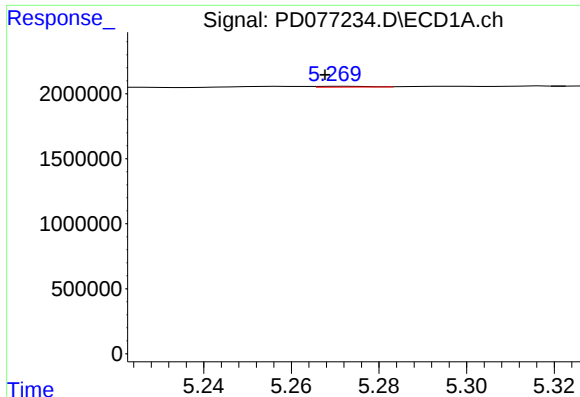

#5 Aldrin


R.T.: 5.272 min
Delta R.T.: 0.004 min
Response: 47915
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

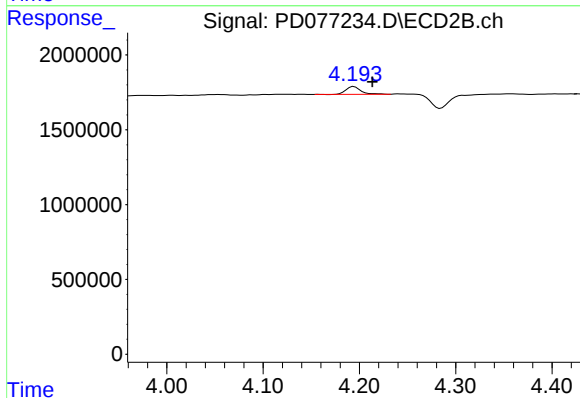


#5 Aldrin

R.T.: 4.194 min
Delta R.T.: -0.019 min
Response: 546972
Conc: 0.30 ng/ml

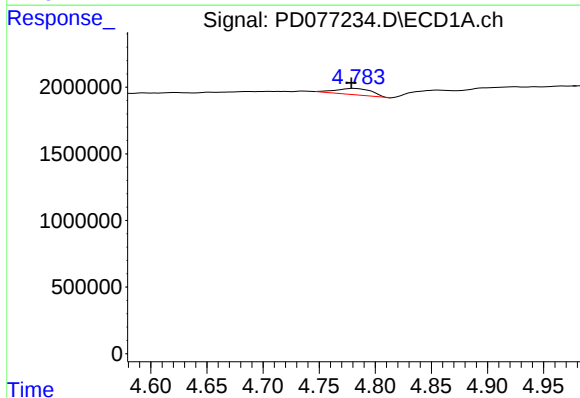


#7 delta-BHC

R.T.: 4.782 min
Delta R.T.: 0.003 min
Response: 1045171
Conc: 0.30 ng/ml

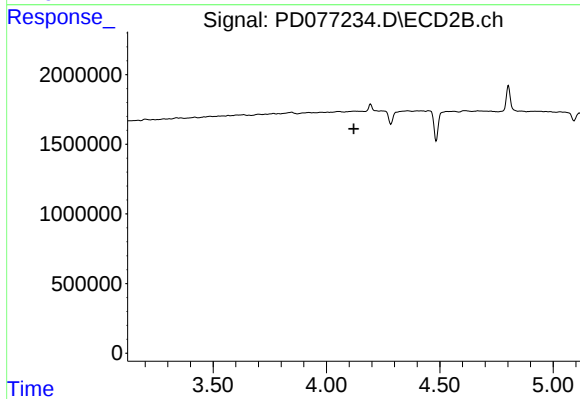

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

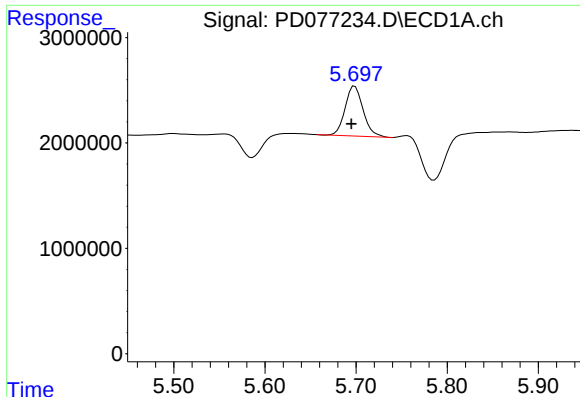

#8 Heptachlor epoxide


R.T.: 5.699 min
Delta R.T.: 0.004 min
Response: 6518574
Conc: 1.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

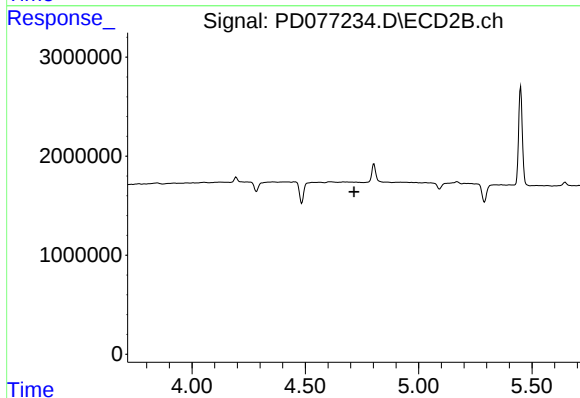


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

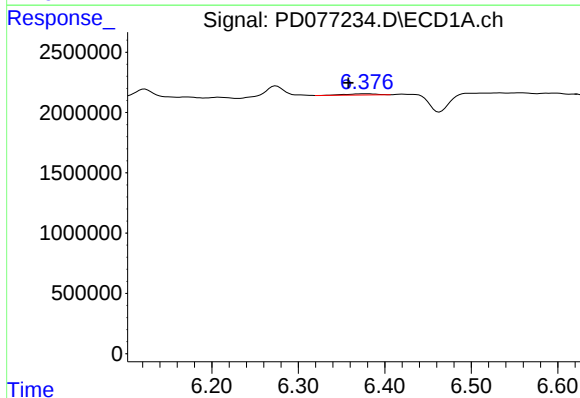


#13 Dieldrin

R.T.: 6.378 min
Delta R.T.: 0.020 min
Response: 240056
Conc: 0.07 ng/ml

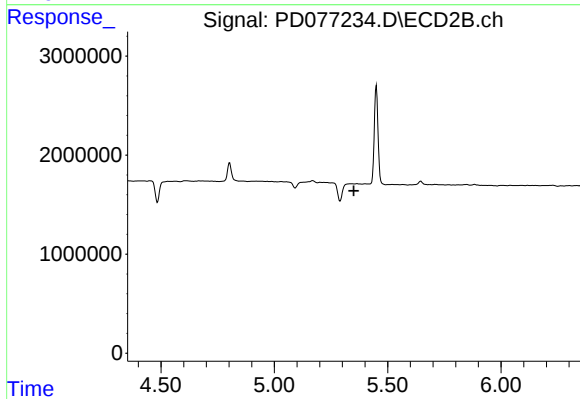

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

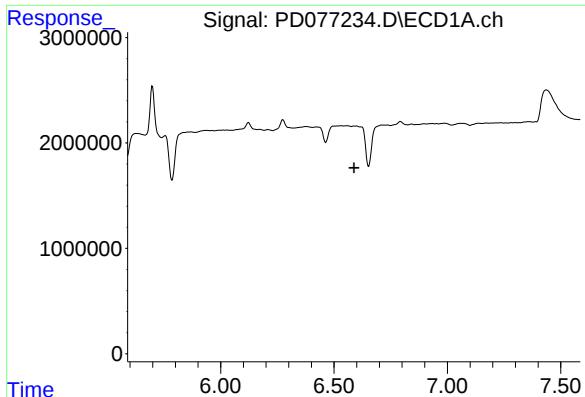

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

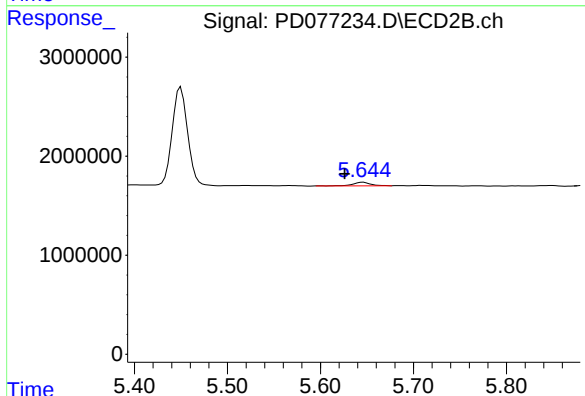


#14 Endrin

R.T.: 5.646 min
Delta R.T.: 0.020 min
Response: 448998
Conc: 0.31 ng/ml

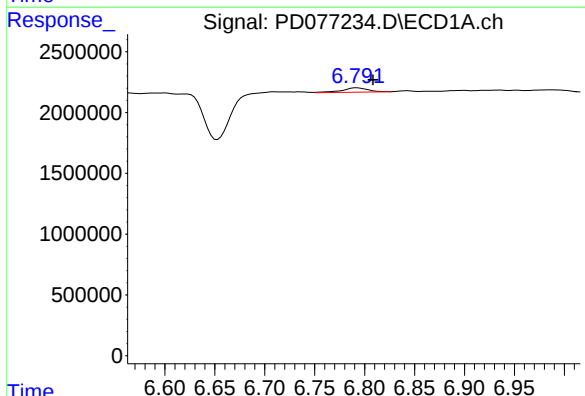


#15 Endosulfan II

R.T.: 6.792 min
Delta R.T.: -0.016 min
Response: 631067
Conc: 0.20 ng/ml

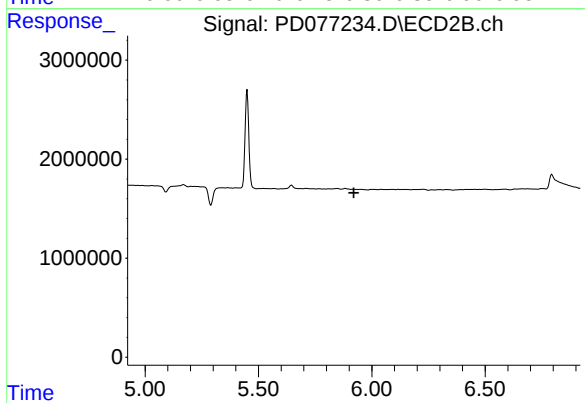

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

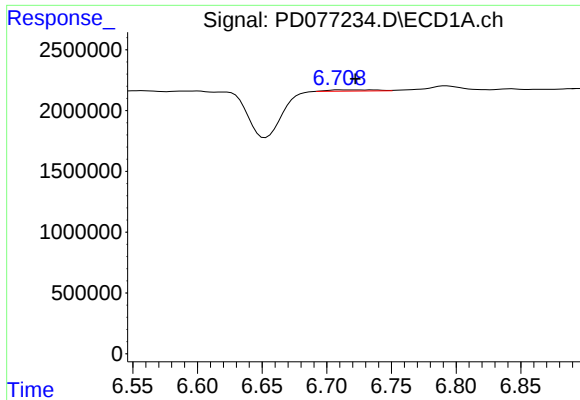

#16 4,4'-DDD


R.T.: 6.710 min
Delta R.T.: -0.013 min
Response: 249307
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

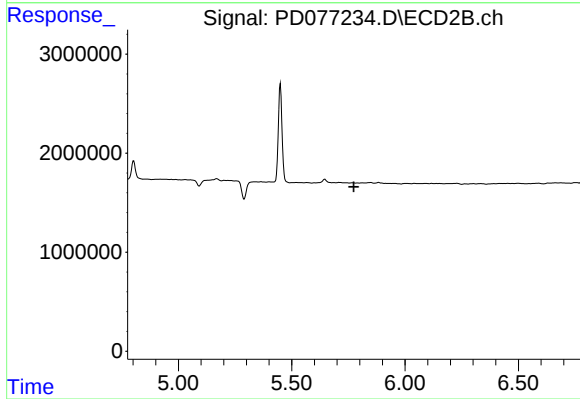


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.773 min
Response: 0
Conc: N.D.

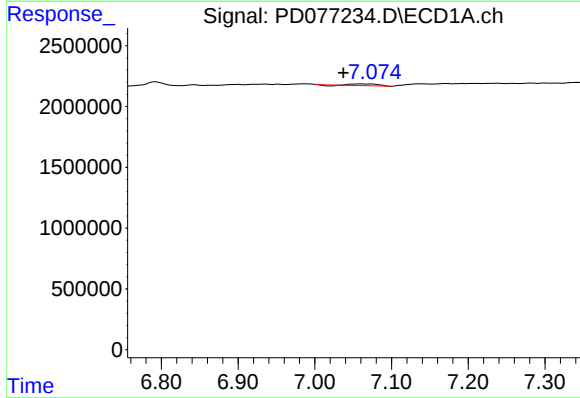


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.021 min
Response: 296740
Conc: 0.12 ng/ml

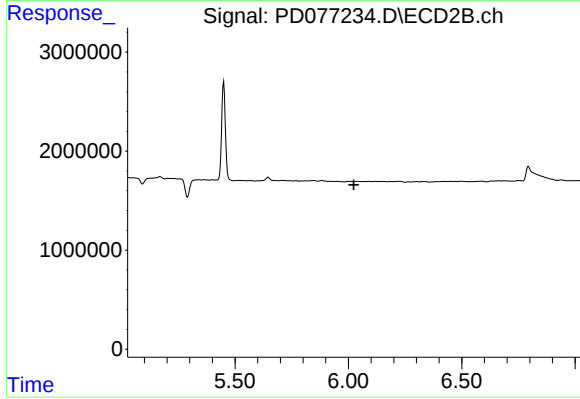

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.025 min
Response: 0
Conc: N.D.

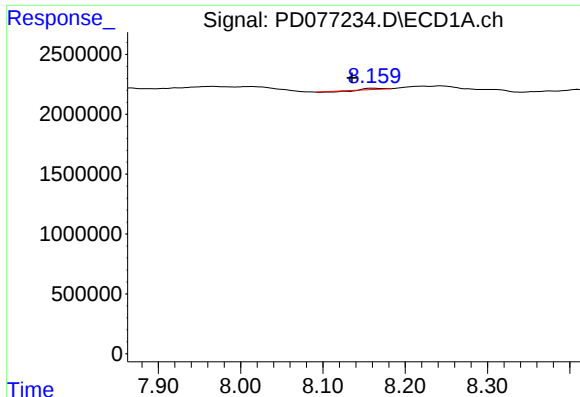

#22 Mirex


R.T.: 8.161 min
Delta R.T.: 0.025 min
Response: 14385
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

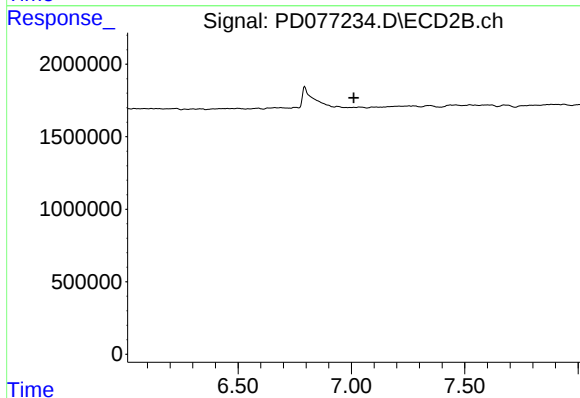


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

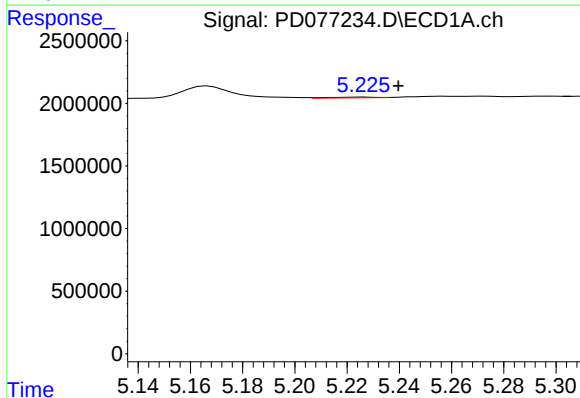


#24 Chlordane-2

R.T.: 5.227 min
Delta R.T.: -0.013 min
Response: 88467
Conc: 0.73 ng/ml

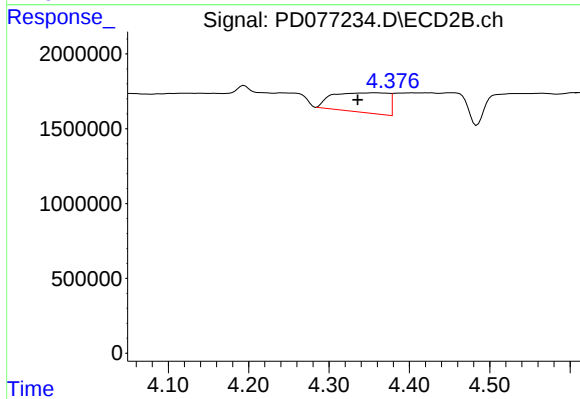

#24 Chlordane-2


R.T.: 4.357 min
Delta R.T.: 0.021 min
Response: 6216004
Conc: 110.53 ng/ml

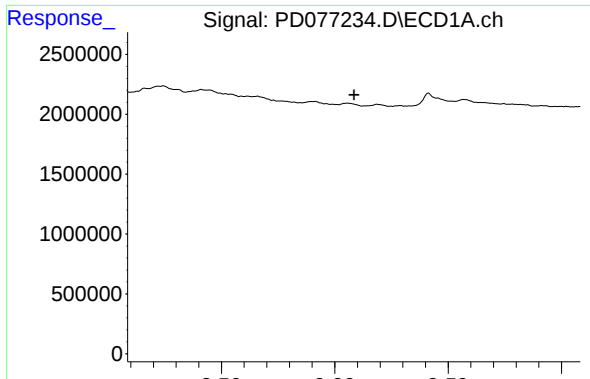

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.086 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

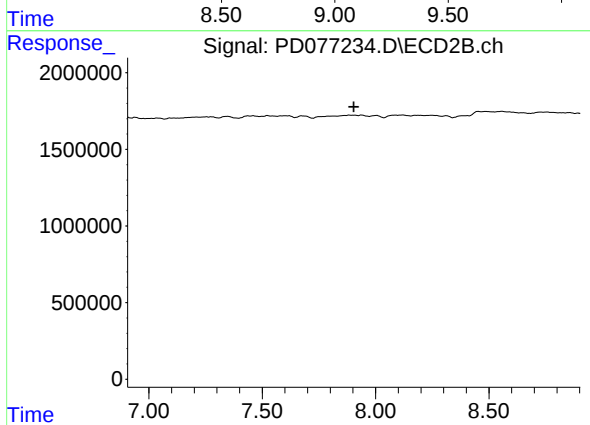

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.