

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081924\
 Data File : PD084520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 14:13
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:06:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081924.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 15:01:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.926	45049326	307.5E6	50.000	50.000
28)	SA Decachlor...	9.115	8.137	74000985	223.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.748	3.954	26272378	113.3E6	500.000	500.000
24)	Chlordane-2	5.274	4.537	29707680	124.7E6	500.000	500.000
25)	Chlordane-3	5.979	5.179	117.6E6	328.5E6	500.000	500.000
26)	Chlordane-4	6.066	5.244	142.7E6	271.0E6	500.000	500.000
27)	Chlordane-5	6.906	6.147	24674745	135.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081924\
Data File : PD084520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 14:13
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:06:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081924.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 15:01:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

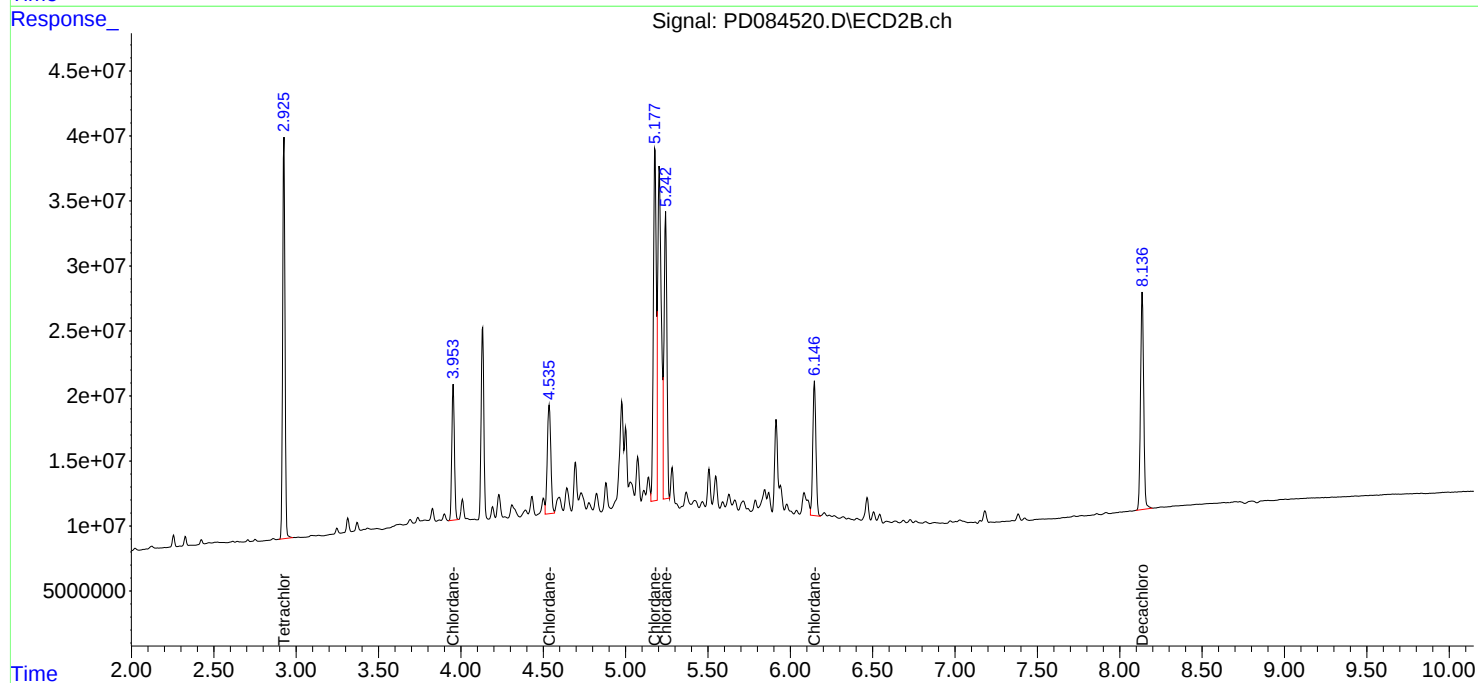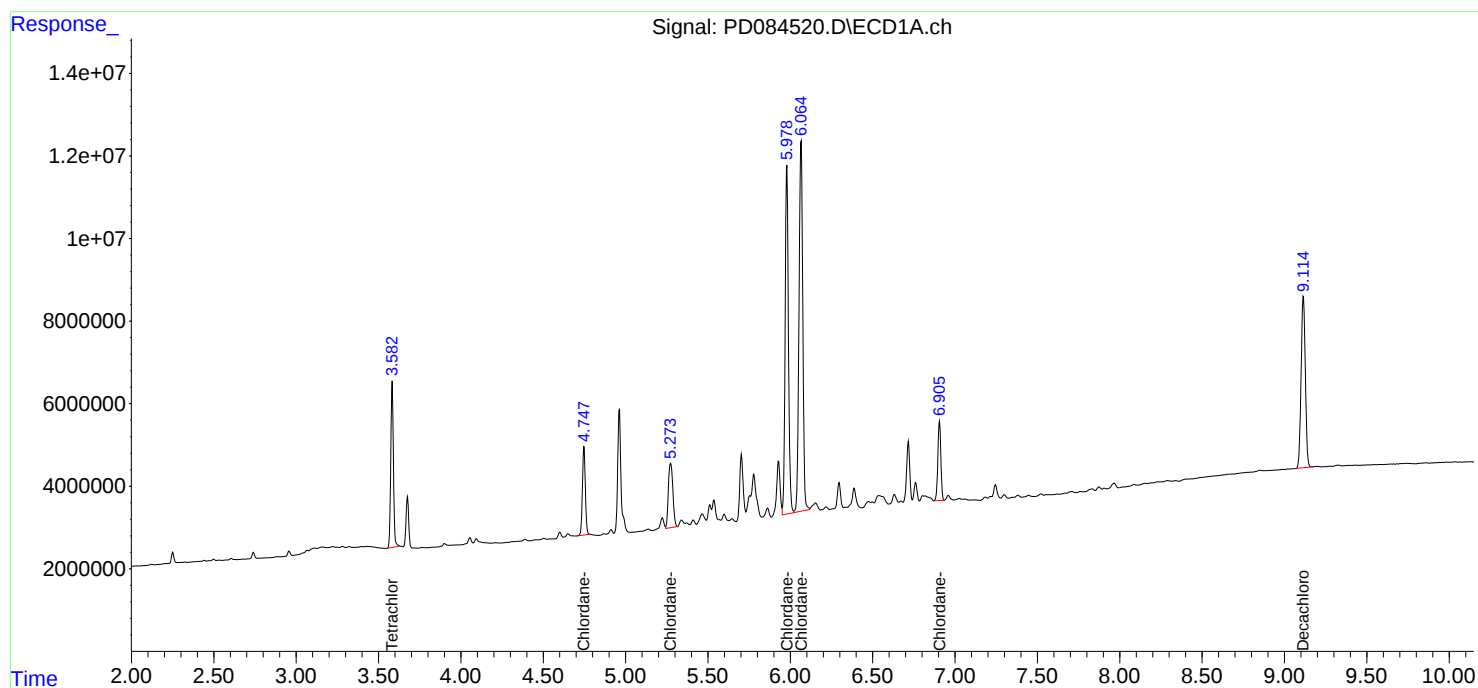


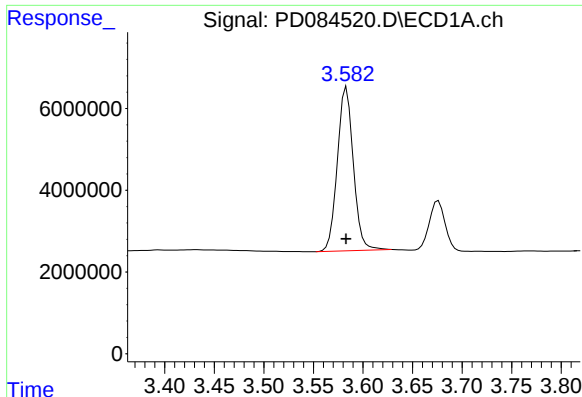

#1 Tetrachloro-m-xylene


R.T.: 3.583 min
Delta R.T.: 0.000 min
Response: 45049326
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

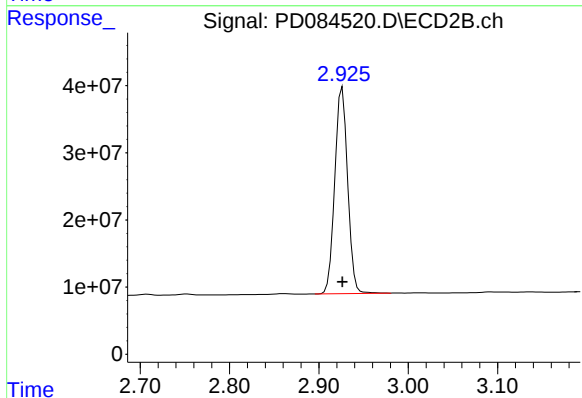


#1 Tetrachloro-m-xylene

R.T.: 2.926 min
Delta R.T.: 0.000 min
Response: 307521145
Conc: 50.00 ng/ml

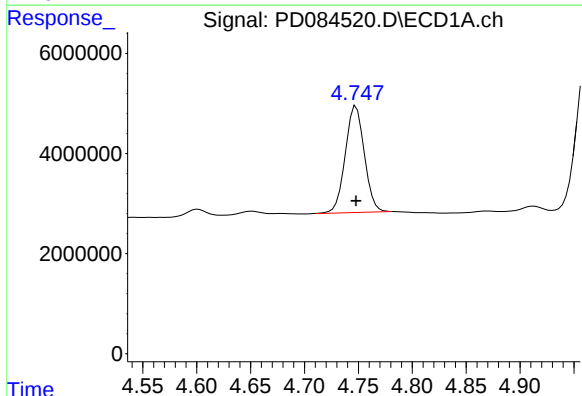


#23 Chlordane-1

R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 26272378
Conc: 500.00 ng/ml

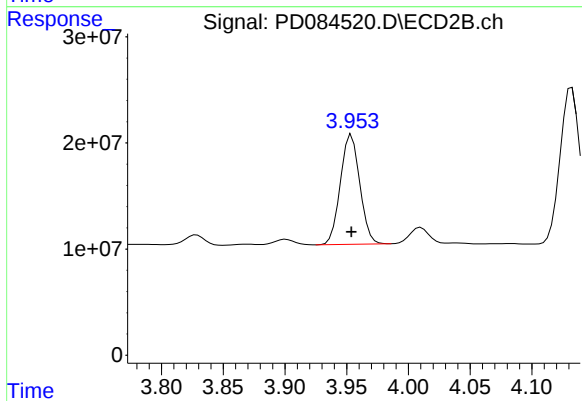

#23 Chlordane-1


R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 113314393
Conc: 500.00 ng/ml

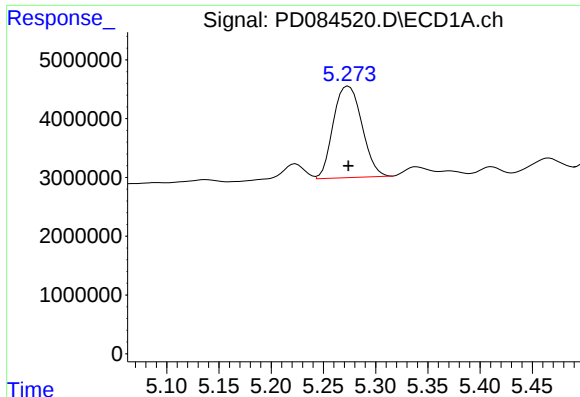

#24 Chlordane-2


R.T.: 5.274 min
Delta R.T.: 0.000 min
Response: 29707680
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

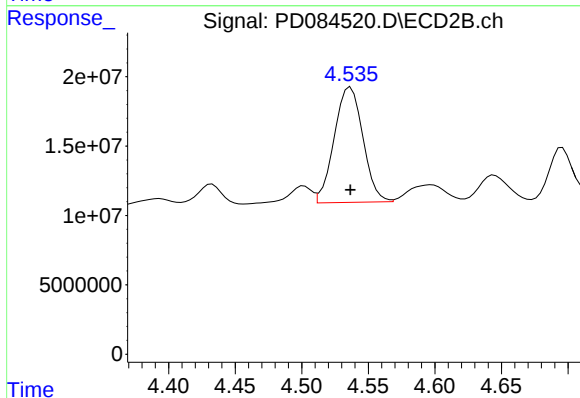


#24 Chlordane-2

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 124684152
Conc: 500.00 ng/ml

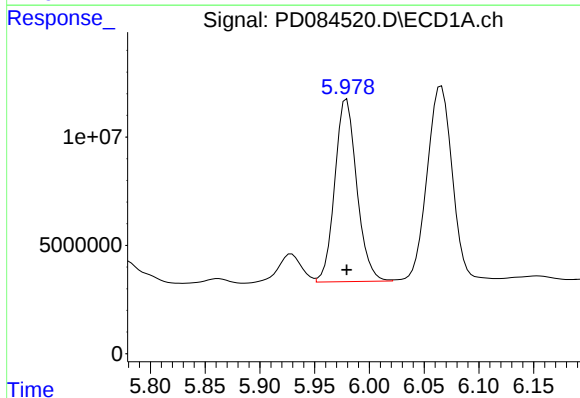


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 117599172
Conc: 500.00 ng/ml

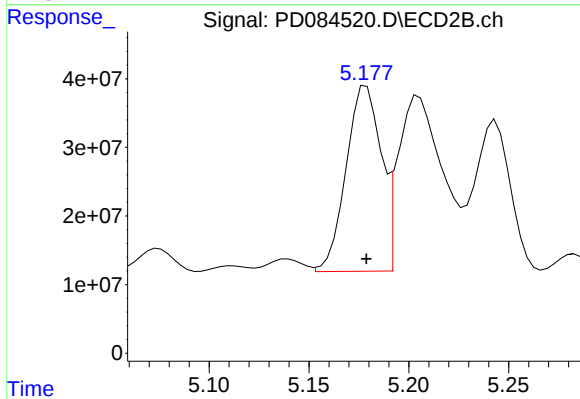

#25 Chlordane-3


R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 328492360
Conc: 500.00 ng/ml

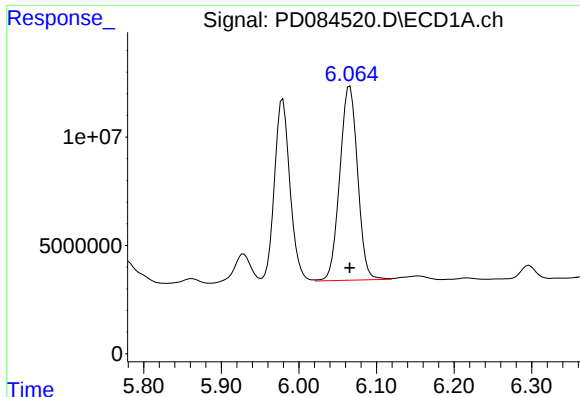

#26 Chlordane-4


R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 142702130
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

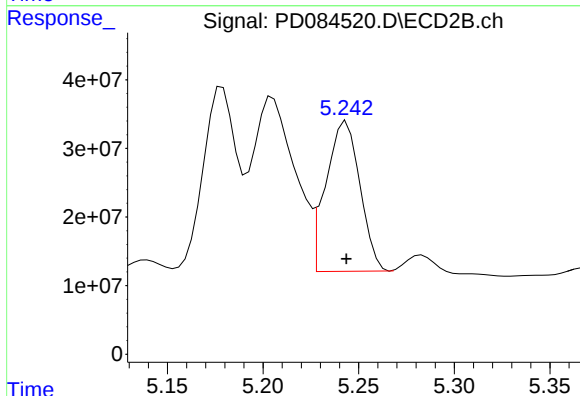


#26 Chlordane-4

R.T.: 5.244 min
Delta R.T.: 0.000 min
Response: 271034141
Conc: 500.00 ng/ml

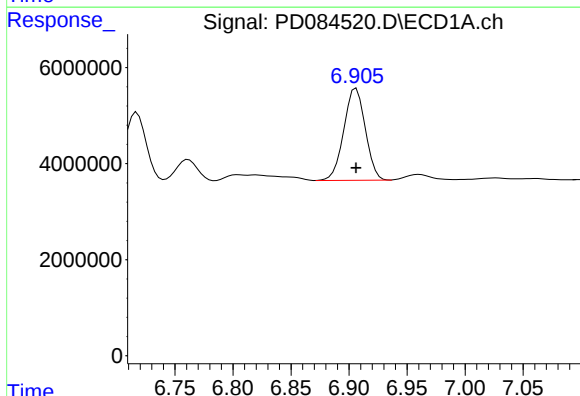


#27 Chlordane-5

R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 24674745
Conc: 500.00 ng/ml

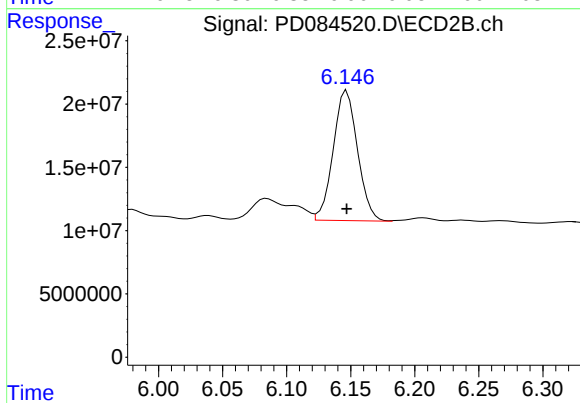

#27 Chlordane-5


R.T.: 6.147 min
Delta R.T.: 0.000 min
Response: 135747473
Conc: 500.00 ng/ml

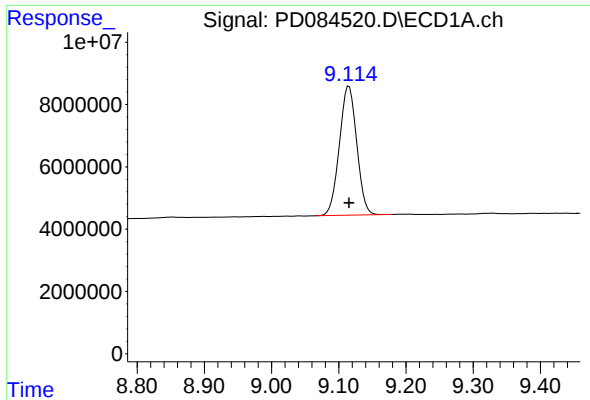

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 74000985
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

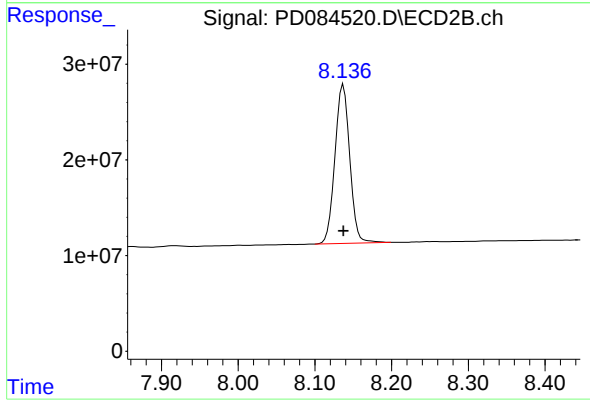

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 223203145
Conc: 50.00 ng/ml