

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081924\
 Data File : PD084519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 14:00
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:09:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081924.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 15:01:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.926	67424178	445.8E6	76.958	74.089
28)	SA Decachlor...	9.114	8.137	109.3E6	319.1E6	74.492	73.998
Target Compounds							
23)	Chlordane-1	4.747	3.954	39713658	164.1E6	763.378	742.928
24)	Chlordane-2	5.274	4.536	43420722	179.1E6	751.346	742.893
25)	Chlordane-3	5.979	5.178	179.7E6	469.4E6	748.446	742.159
26)	Chlordane-4	6.065	5.243	216.0E6	383.8E6	745.442	740.209
27)	Chlordane-5	6.906	6.147	36874441	196.1E6	731.880	742.967



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081924\
Data File : PD084519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 14:00
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:09:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081924.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 15:01:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

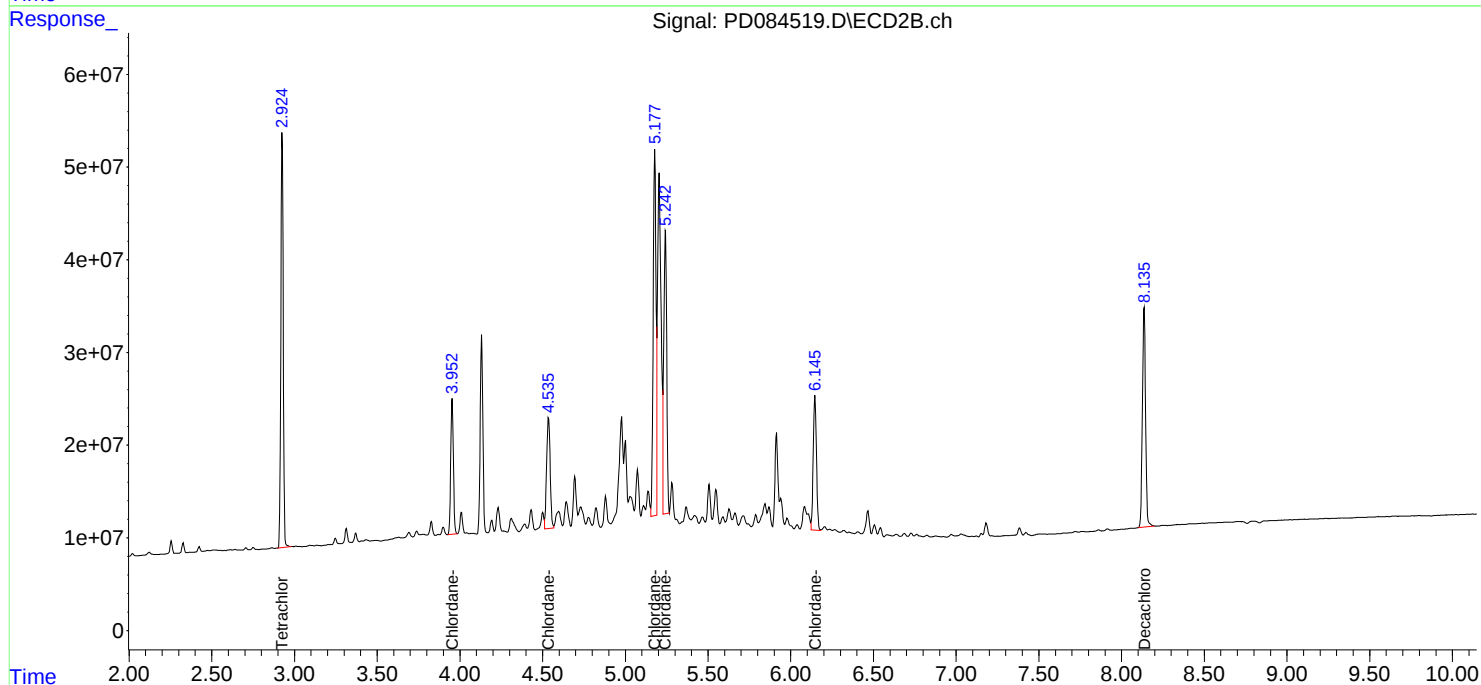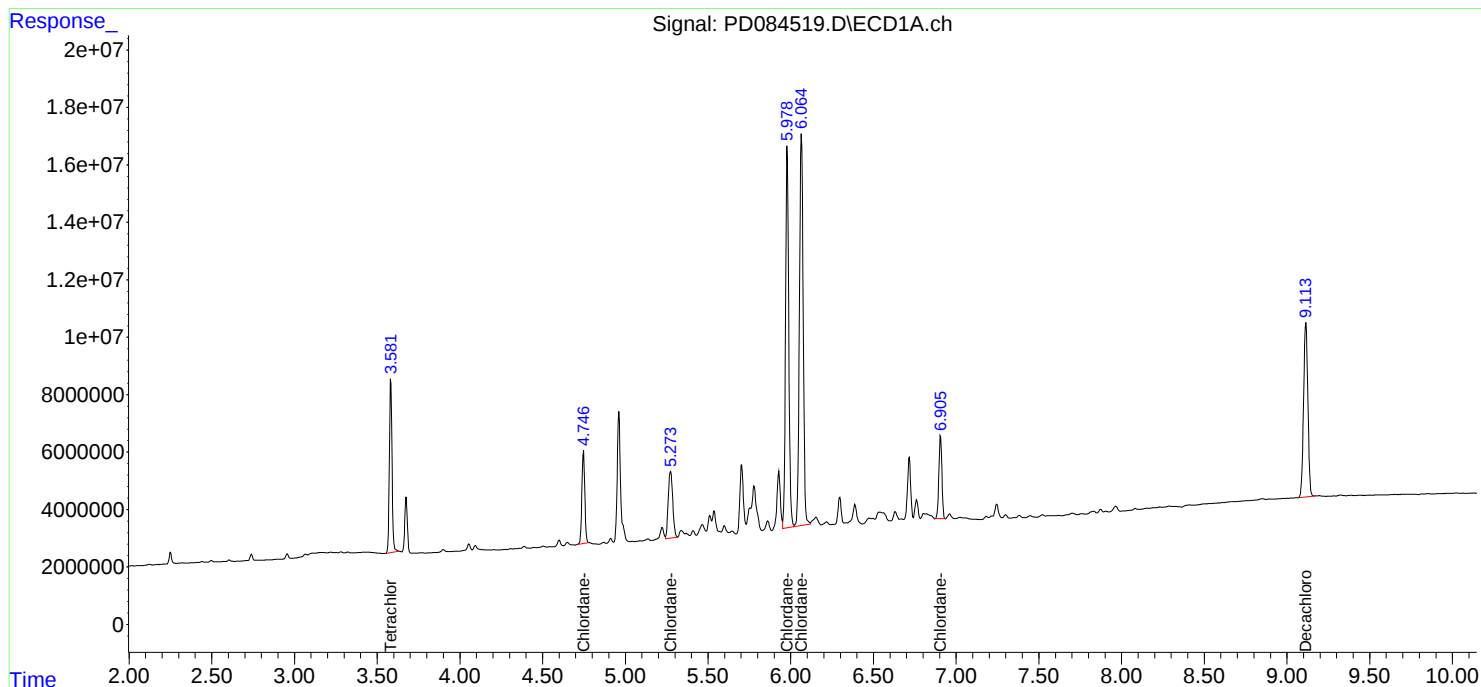


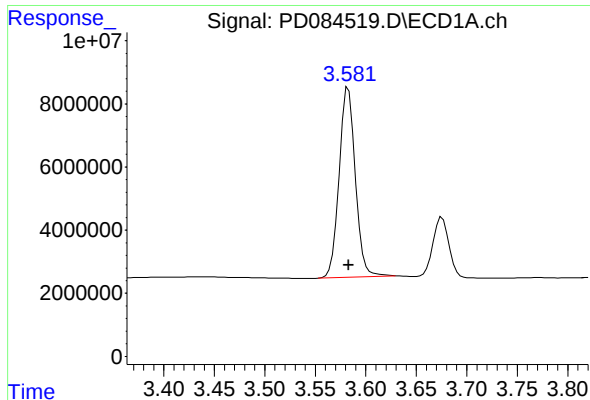

#1 Tetrachloro-m-xylene


R.T.: 3.583 min
Delta R.T.: 0.000 min
Response: 67424178
Conc: 76.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

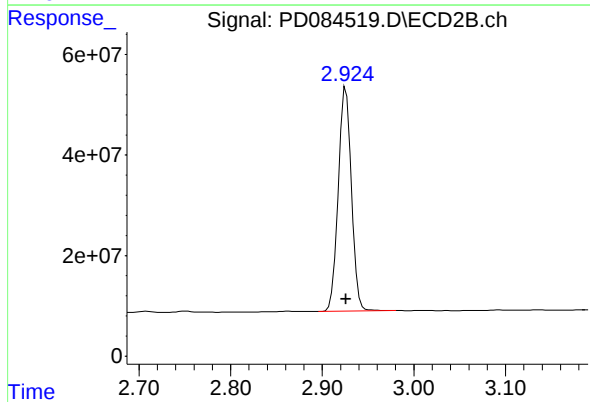


#1 Tetrachloro-m-xylene

R.T.: 2.926 min
Delta R.T.: 0.000 min
Response: 445772663
Conc: 74.09 ng/ml

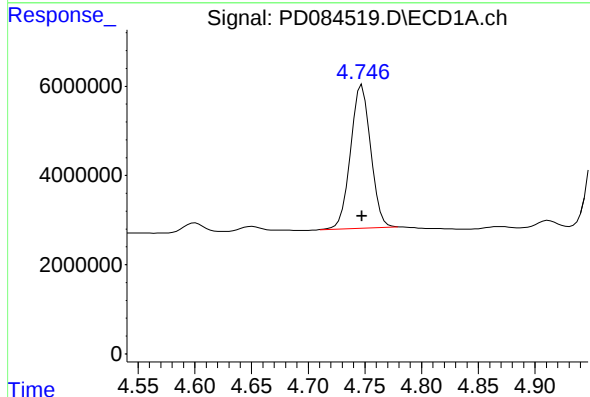


#23 Chlordane-1

R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 39713658
Conc: 763.38 ng/ml

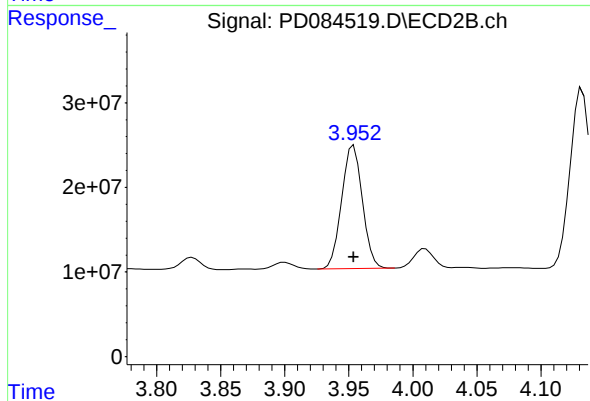

#23 Chlordane-1


R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 164090494
Conc: 742.93 ng/ml

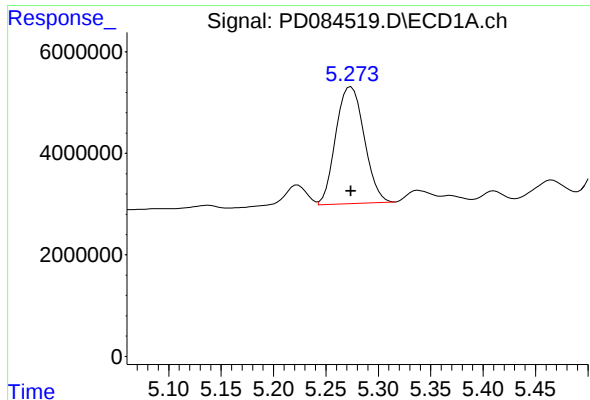

#24 Chlordane-2


R.T.: 5.274 min
Delta R.T.: 0.000 min
Response: 43420722
Conc: 751.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

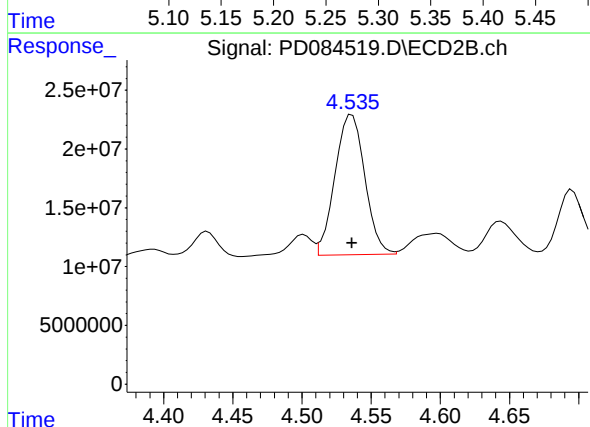


#24 Chlordane-2

R.T.: 4.536 min
Delta R.T.: 0.000 min
Response: 179102535
Conc: 742.89 ng/ml

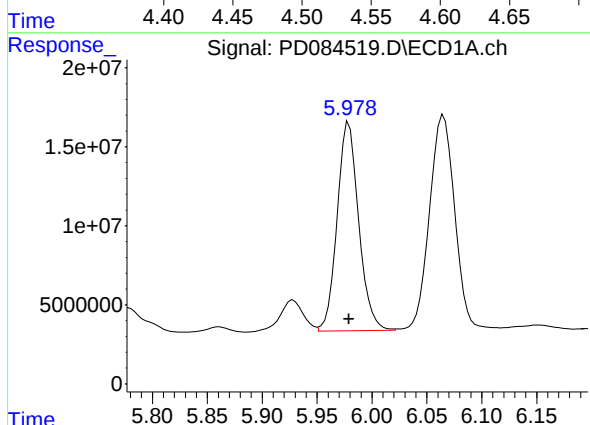


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 179742016
Conc: 748.45 ng/ml

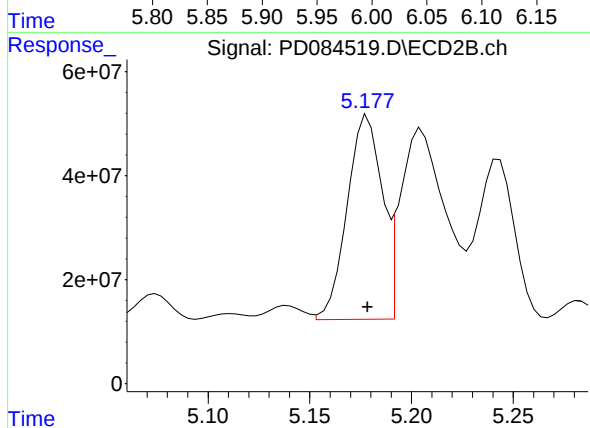

#25 Chlordane-3


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 469411754
Conc: 742.16 ng/ml

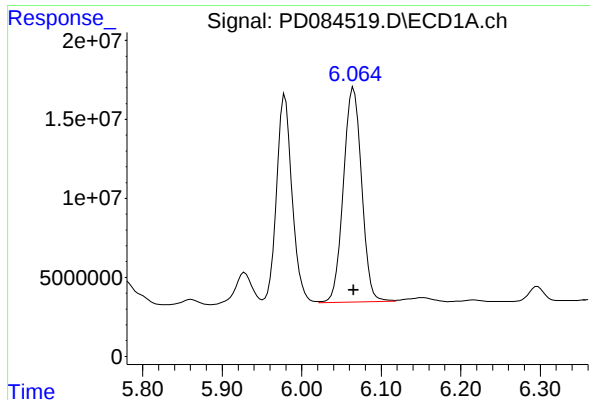

#26 Chlordane-4


R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 216021887
Conc: 745.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

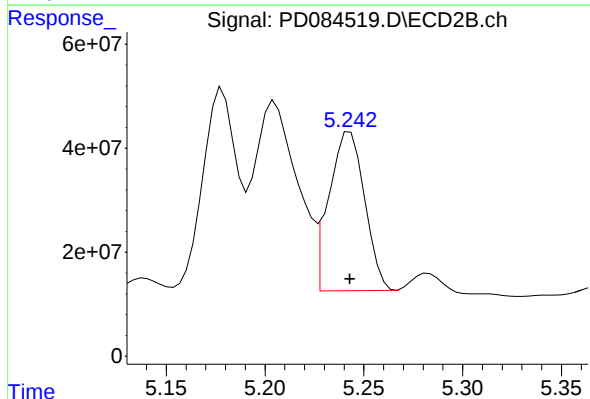


#26 Chlordane-4

R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 383838178
Conc: 740.21 ng/ml

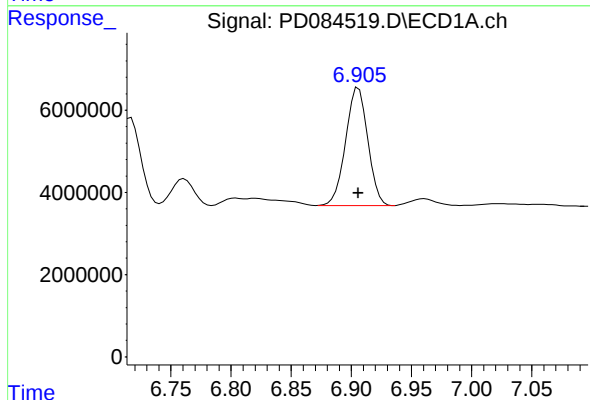


#27 Chlordane-5

R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 36874441
Conc: 731.88 ng/ml

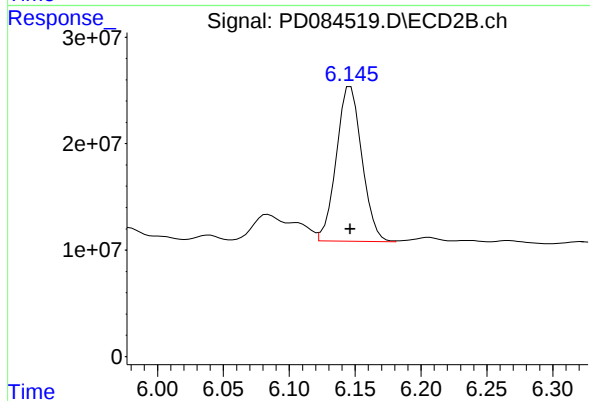

#27 Chlordane-5


R.T.: 6.147 min
Delta R.T.: 0.000 min
Response: 196073706
Conc: 742.97 ng/ml

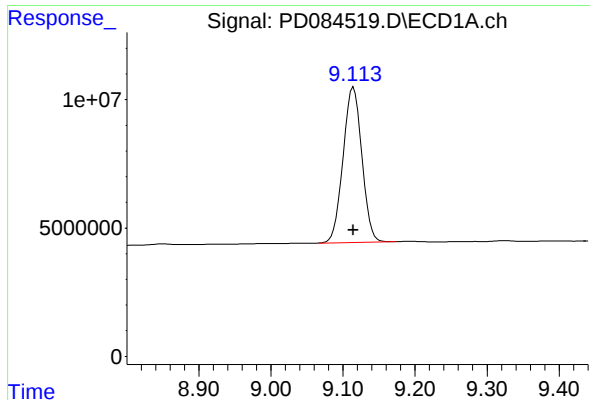

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 109253432
Conc: 74.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

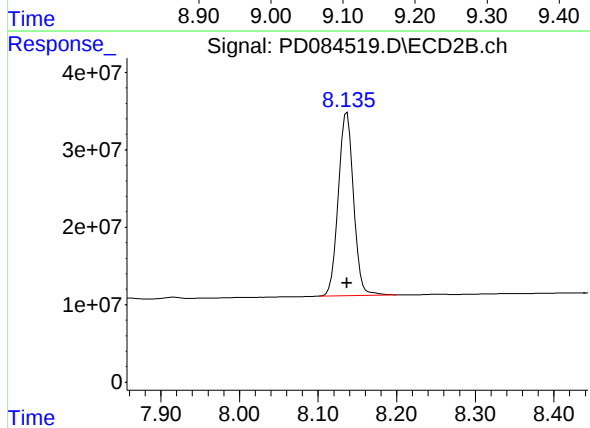

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 319140548
Conc: 74.00 ng/ml