

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081925\
 Data File : PD089985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 10:17
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 07:12:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 19 13:16:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.877	53286163	422.7E6	18.156	19.168
28)	SA Decachlor...	9.067	8.065	81944005	506.9E6	18.986	19.580
Target Compounds							
9)	A Endosulfan I	6.071	5.242	40494969	256.6E6	8.775	9.788
10)	B gamma-Chl...	5.942	5.120	44341755	310.5E6	9.066	10.485
12)	B 4,4'-DDE	6.192	5.369	80231969	586.8E6	18.283	20.358
13)	MA Dieldrin	6.343	5.507	88241294	581.0E6	18.024	19.838
19)	B Endosulfa...	7.147	6.477	72742669	489.1E6	18.564	20.061
20)	A Methoxychlor	7.491	6.748	175.6E6	1102.9E6	87.543	85.521
21)	B Endrin ke...	7.627	6.986	75544703	533.3E6	18.228	20.014



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081925\
Data File : PD089985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 10:17
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 07:12:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
Quant Title : GC Extractables
QLast Update : Tue Aug 19 13:16:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

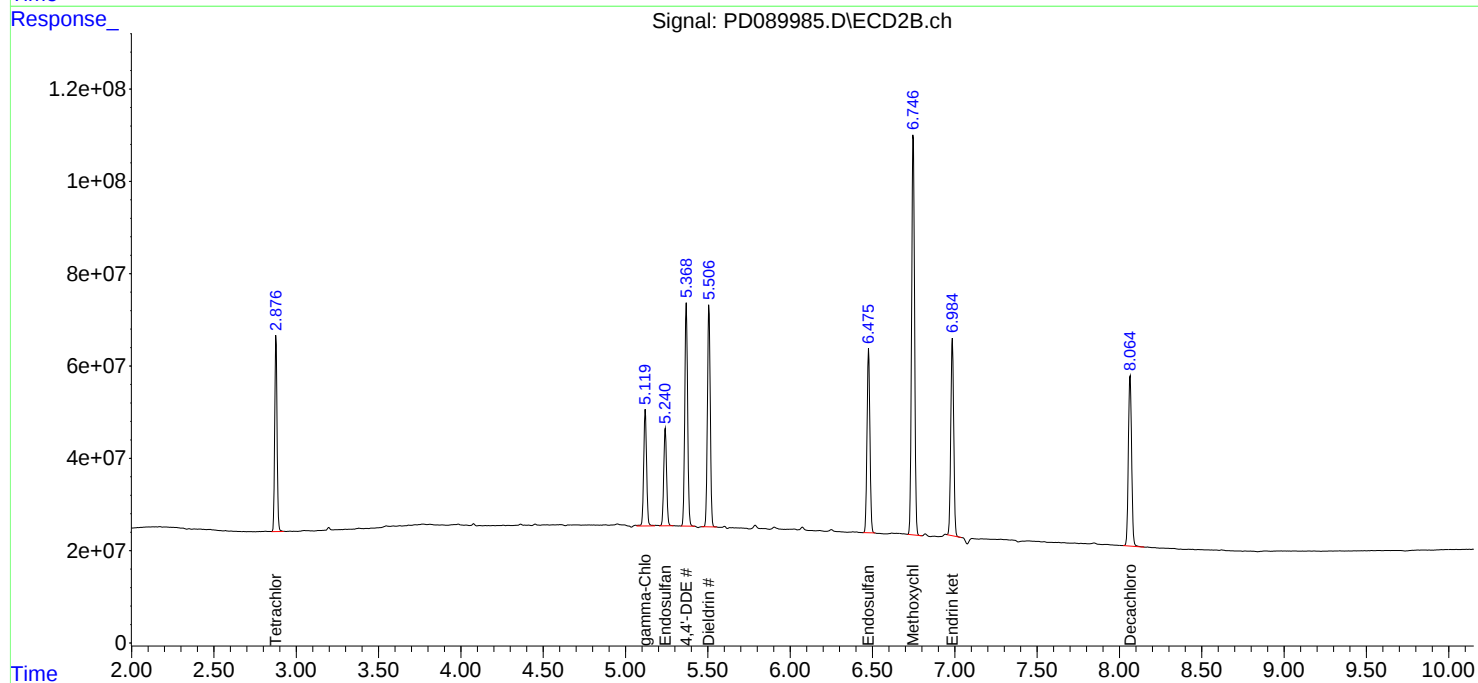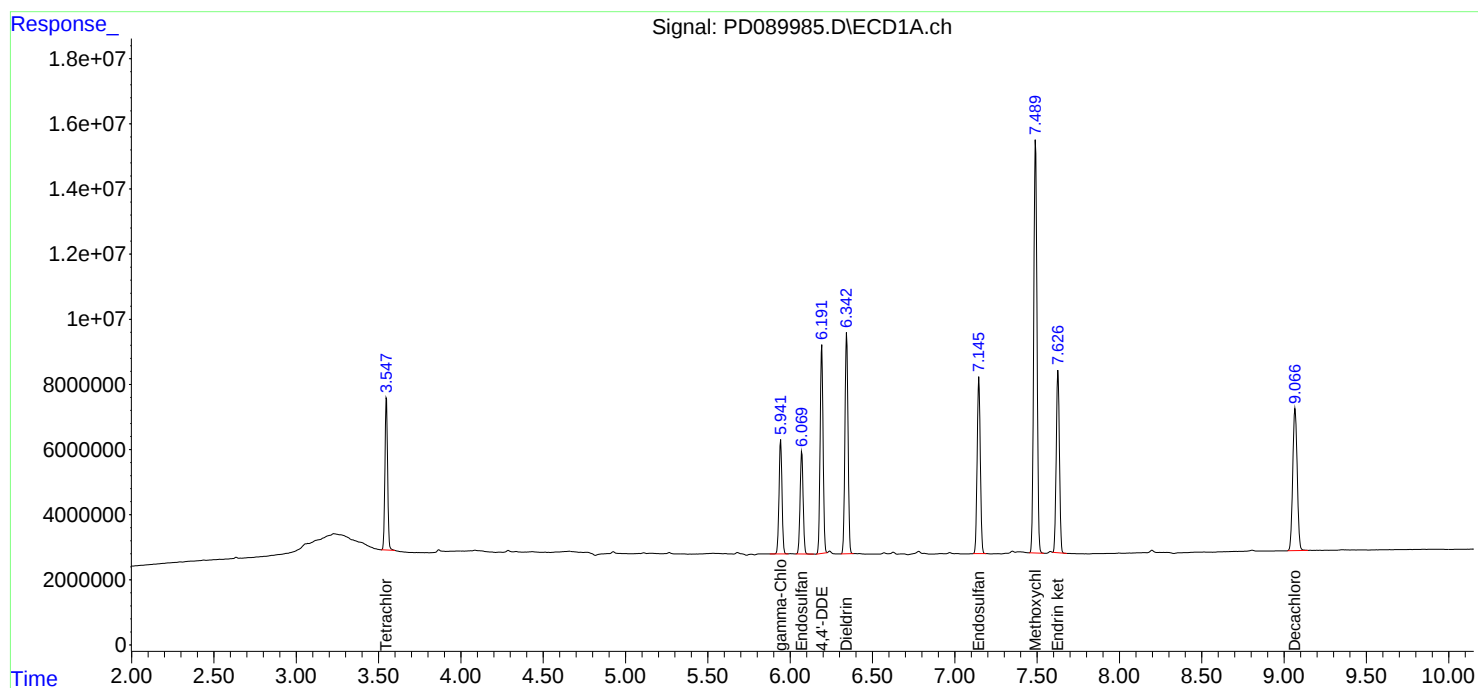


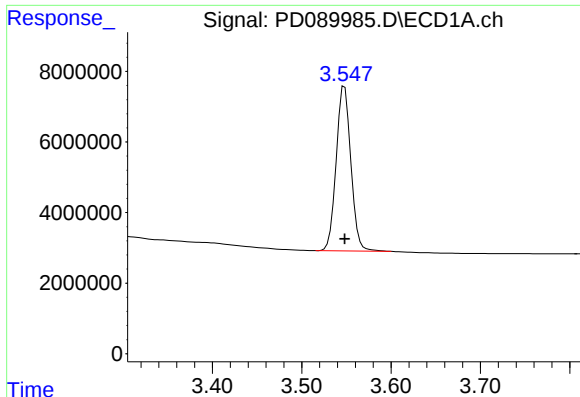

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 53286163
Conc: 18.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

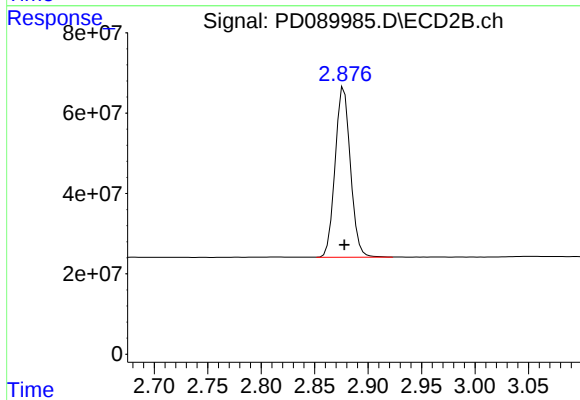


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 422674889
Conc: 19.17 ng/ml

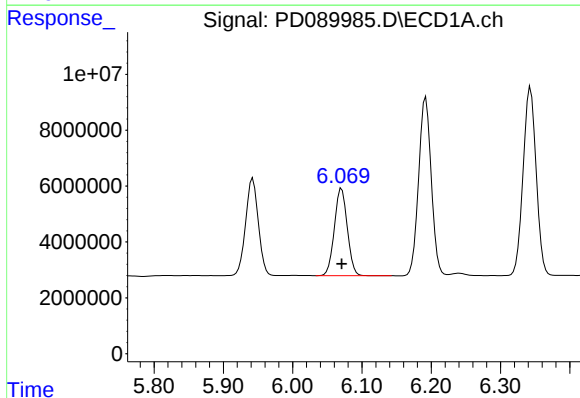


#9 Endosulfan I

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 40494969
Conc: 8.77 ng/ml

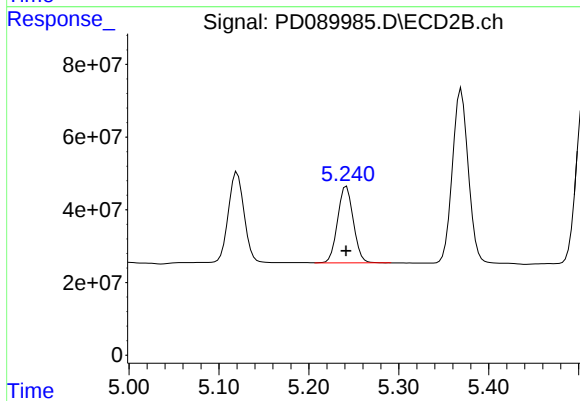

#9 Endosulfan I


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 256648709
Conc: 9.79 ng/ml

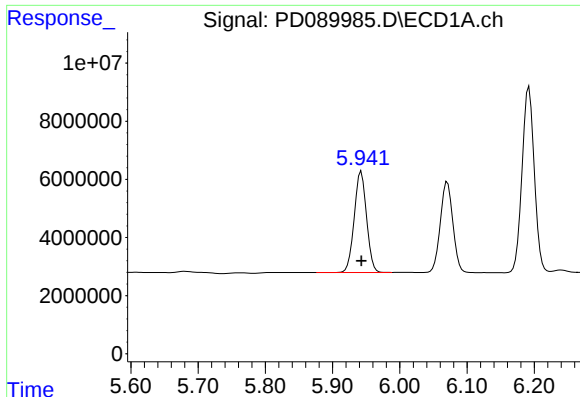

#10 gamma-Chlordane


R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 44341755
Conc: 9.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

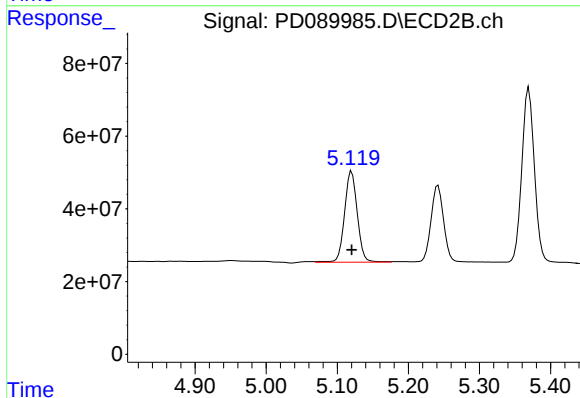


#10 gamma-Chlordane

R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 310478007
Conc: 10.49 ng/ml

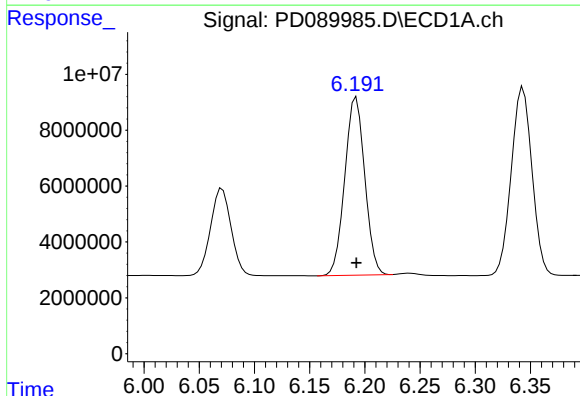


#12 4,4'-DDE

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 80231969
Conc: 18.28 ng/ml

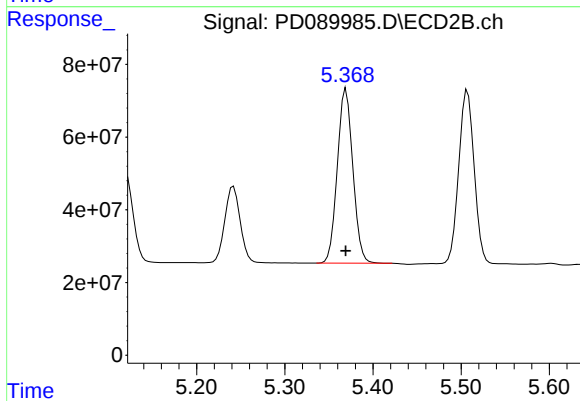

#12 4,4'-DDE


R.T.: 5.369 min
Delta R.T.: 0.000 min
Response: 586775013
Conc: 20.36 ng/ml

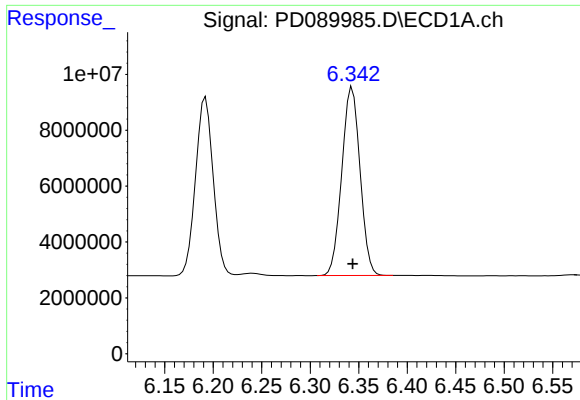

#13 Dieldrin


R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 88241294
Conc: 18.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

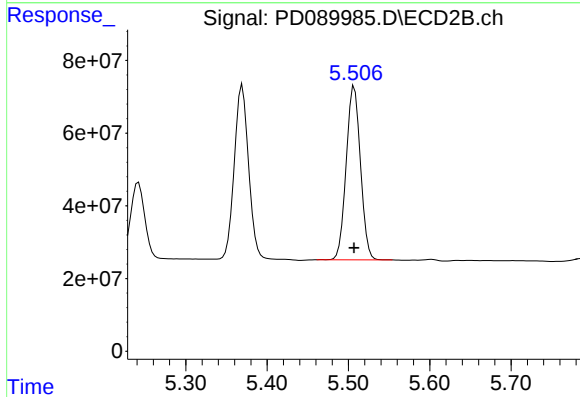


#13 Dieldrin

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 580992913
Conc: 19.84 ng/ml

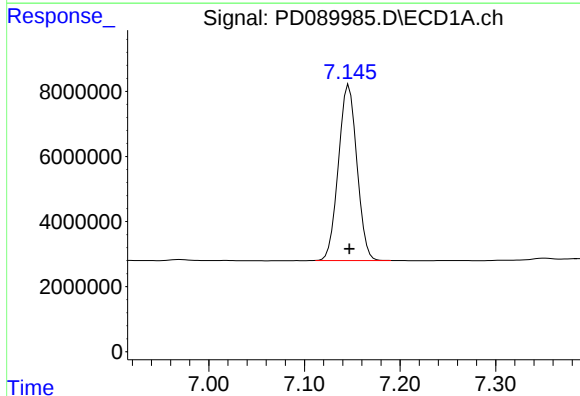


#19 Endosulfan Sulfate

R.T.: 7.147 min
Delta R.T.: 0.000 min
Response: 72742669
Conc: 18.56 ng/ml

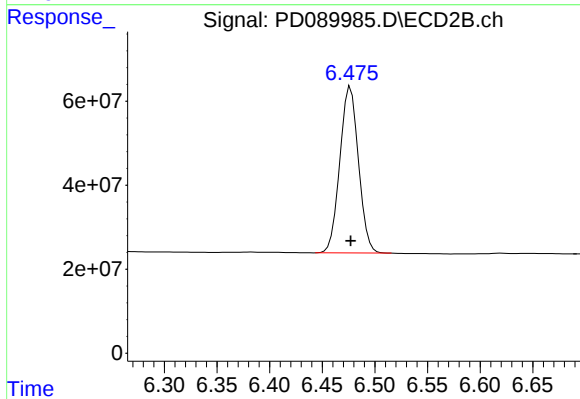

#19 Endosulfan Sulfate


R.T.: 6.477 min
Delta R.T.: 0.000 min
Response: 489088346
Conc: 20.06 ng/ml

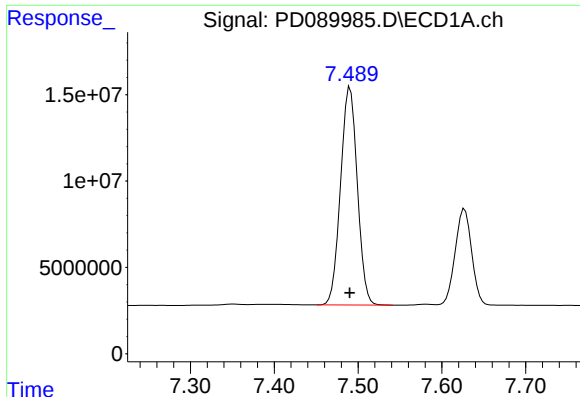

#20 Methoxychlor


R.T.: 7.491 min
Delta R.T.: 0.000 min
Response: 175577758
Conc: 87.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

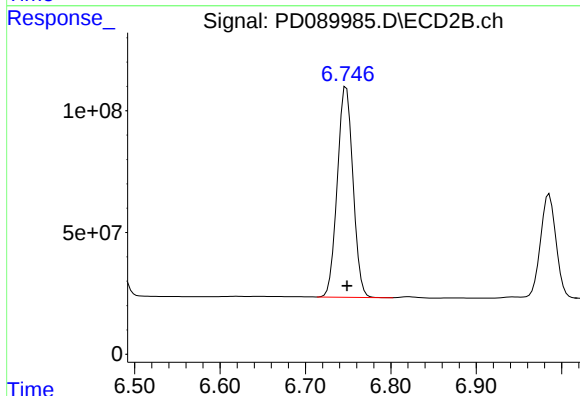


#20 Methoxychlor

R.T.: 6.748 min
Delta R.T.: -0.001 min
Response: 1102856556
Conc: 85.52 ng/ml

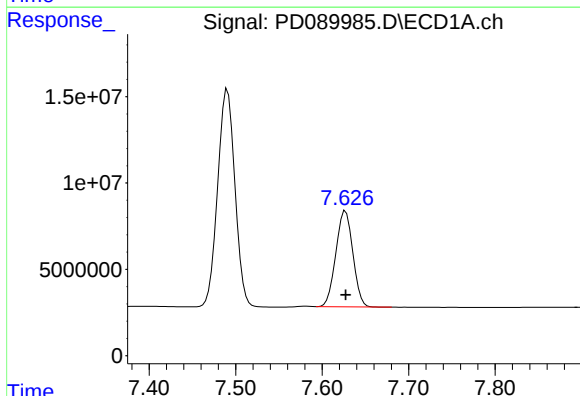


#21 Endrin ketone

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 75544703
Conc: 18.23 ng/ml

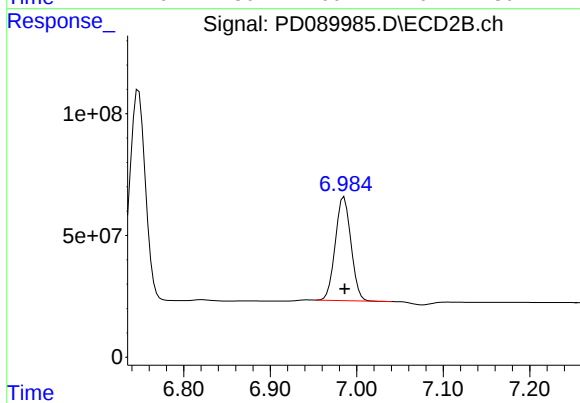

#21 Endrin ketone


R.T.: 6.986 min
Delta R.T.: 0.000 min
Response: 533270173
Conc: 20.01 ng/ml

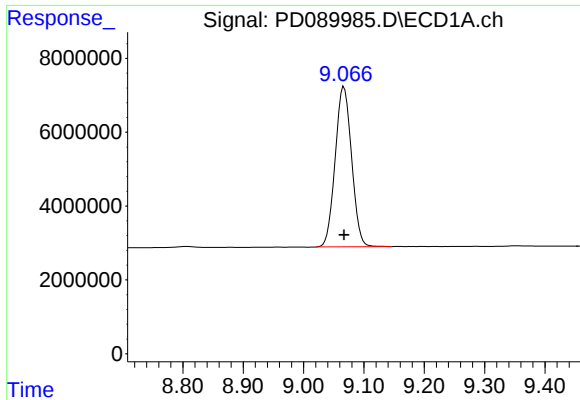

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 81944005
Conc: 18.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

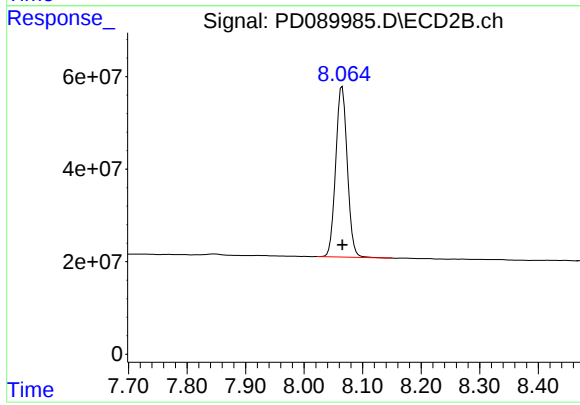

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 506853874
Conc: 19.58 ng/ml