

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081925\
 Data File : PD089988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 11:24
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 13:03:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 19 13:03:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.876	109.8E6	1057.1E6	50.000	50.000
28)	SA Decachlor...	9.068	8.064	161.9E6	1032.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.713	3.901	92125896	474.3E6	500.000	500.000
24)	Chlordane-2	5.239	4.482	93180795	493.5E6	500.000	500.000
25)	Chlordane-3	5.944	5.120	366.6E6	1460.8E6	500.000	500.000
26)	Chlordane-4	6.029	5.184	446.2E6	1262.6E6	500.000	500.000
27)	Chlordane-5	6.868	6.084	75389263	588.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081925\
Data File : PD089988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 11:24
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 13:03:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081825.M
Quant Title : GC Extractables
QLast Update : Tue Aug 19 13:03:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

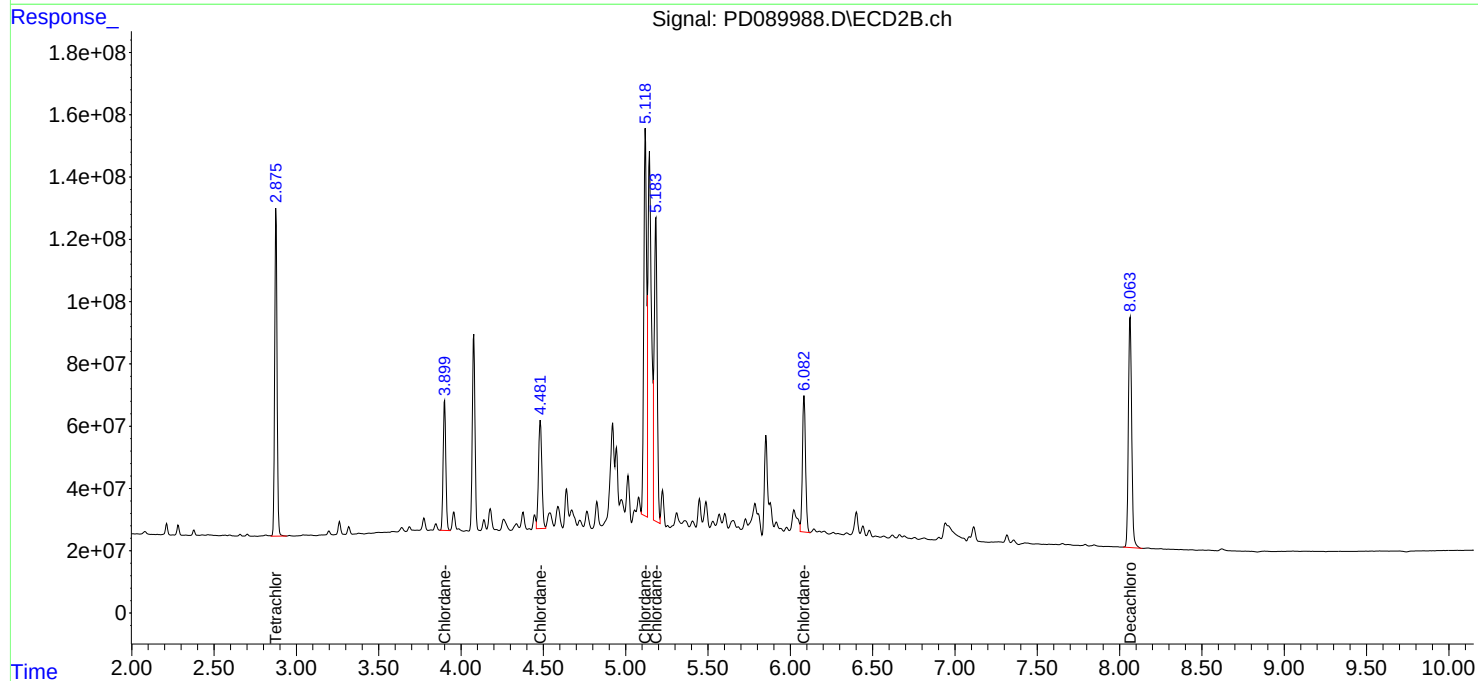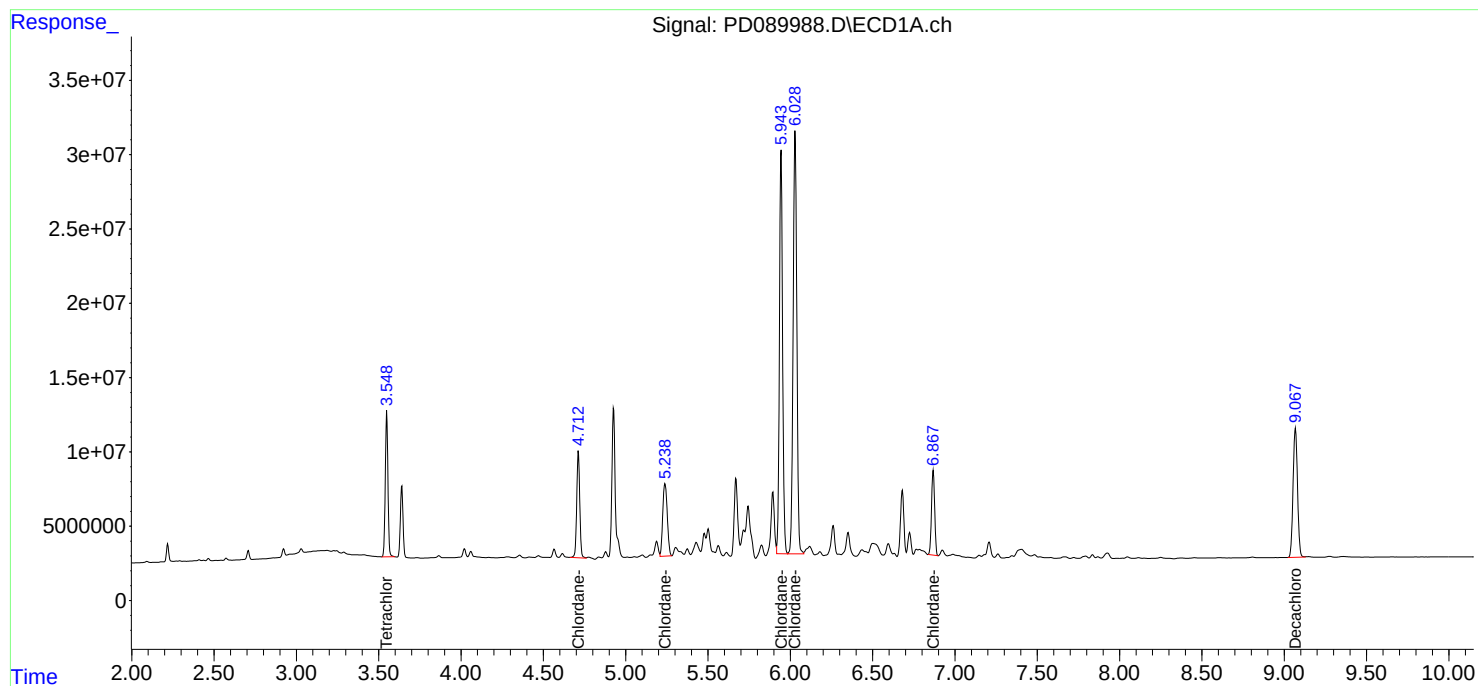


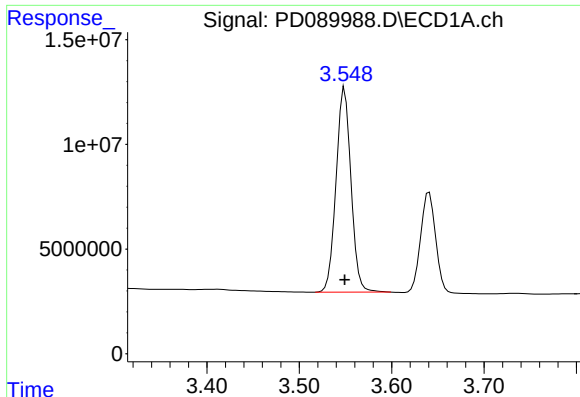

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 109813767
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

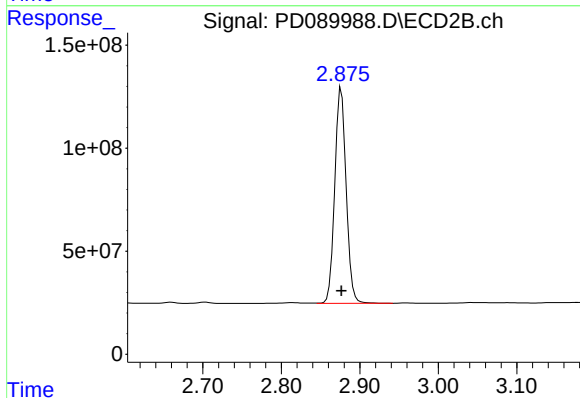


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 1057096075
Conc: 50.00 ng/ml

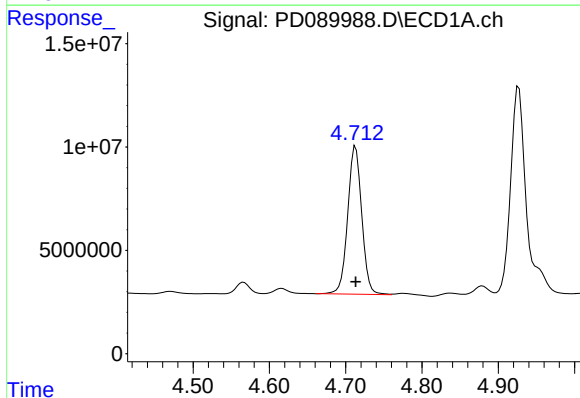


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 92125896
Conc: 500.00 ng/ml

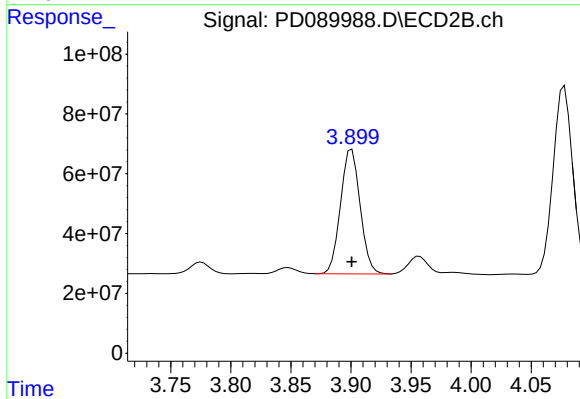

#23 Chlordane-1


R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 474266214
Conc: 500.00 ng/ml

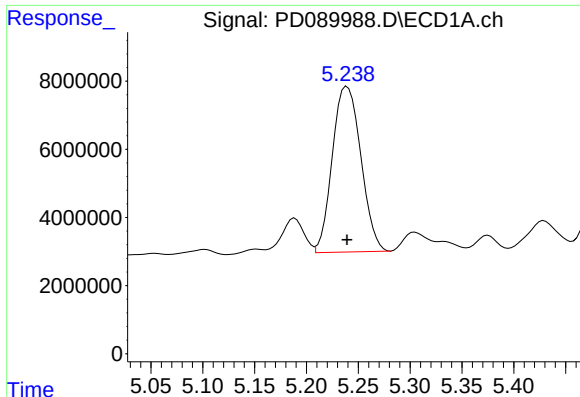

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 93180795
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

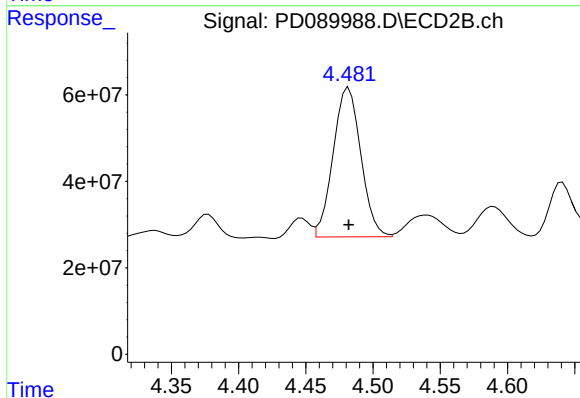


#24 Chlordane-2

R.T.: 4.482 min
Delta R.T.: 0.000 min
Response: 493523178
Conc: 500.00 ng/ml

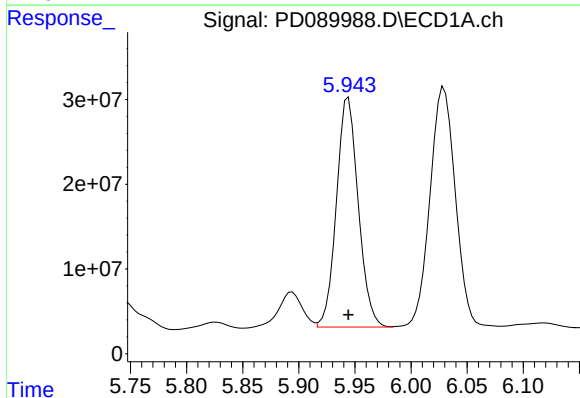


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 366649042
Conc: 500.00 ng/ml

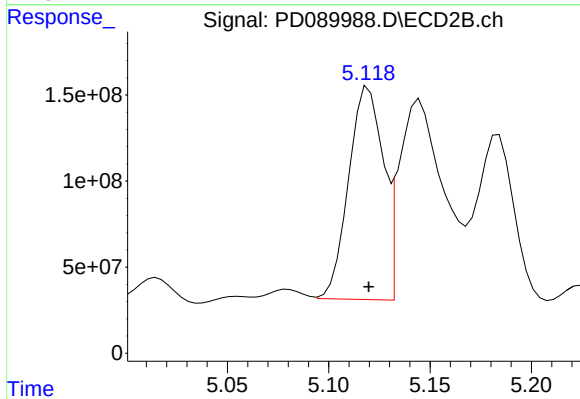

#25 Chlordane-3


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 1460789048
Conc: 500.00 ng/ml

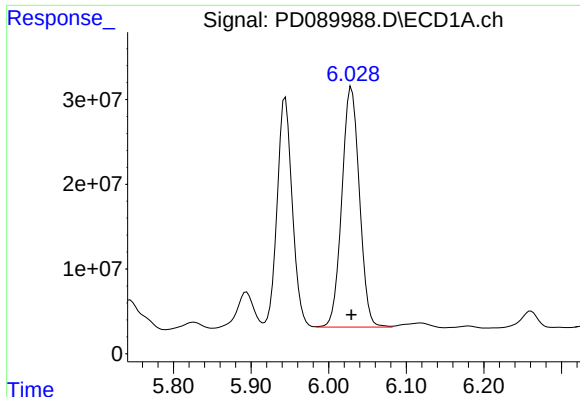

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 446160270
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

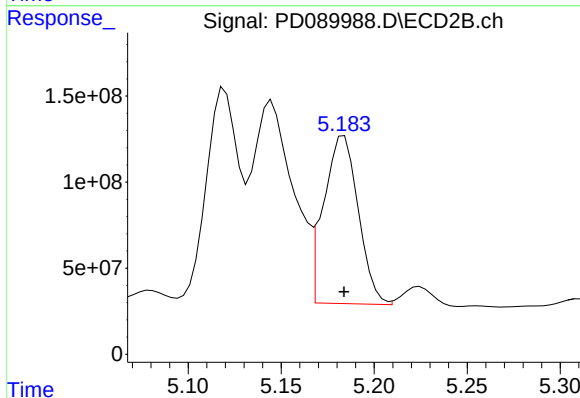


#26 Chlordane-4

R.T.: 5.184 min
Delta R.T.: 0.000 min
Response: 1262600245
Conc: 500.00 ng/ml

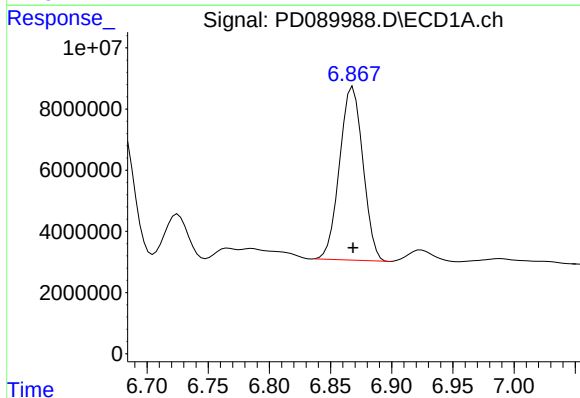


#27 Chlordane-5

R.T.: 6.868 min
Delta R.T.: 0.000 min
Response: 75389263
Conc: 500.00 ng/ml

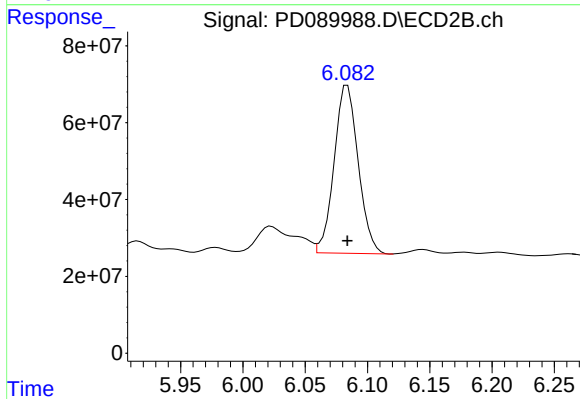

#27 Chlordane-5


R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 588291533
Conc: 500.00 ng/ml

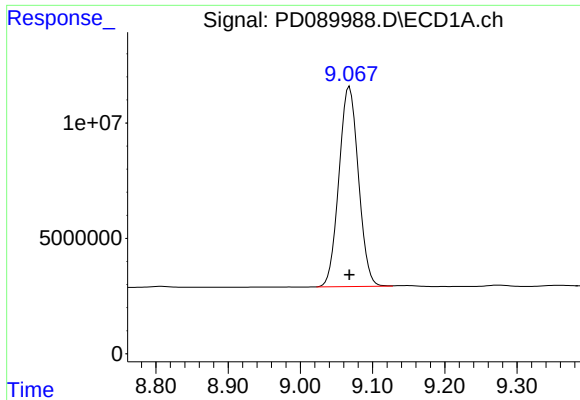

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.000 min
Response: 161936087
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

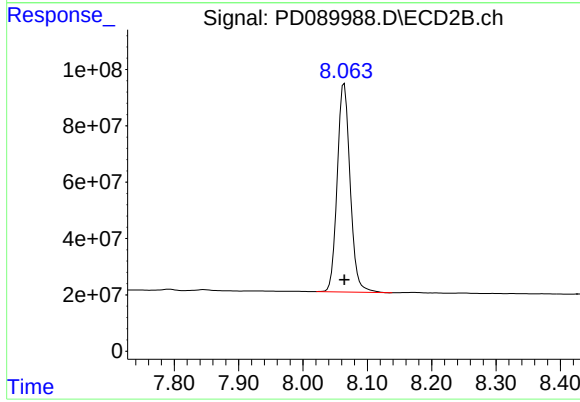

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 1032683856
Conc: 50.00 ng/ml