

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082019\
 Data File : PD054326.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 8:55
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:22:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 16 08:45:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	14263643	20020929	23.727	23.717
28)	SA Decachlor...	8.006	9.023	12218794	17128478	19.053	19.725
Target Compounds							
18)	B Endrin al...	6.274f	0.000	128359	0	0.206	N.D. #
20)	A Methoxychlor	6.752f	0.000	419703	0	1.963	N.D. #
22)	Mirex	0.000	8.180f	0	164758	N.D.	0.182 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082019\
Data File : PD054326.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2019 8:55
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:22:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
Quant Title : GC Extractables
QLast Update : Fri Aug 16 08:45:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

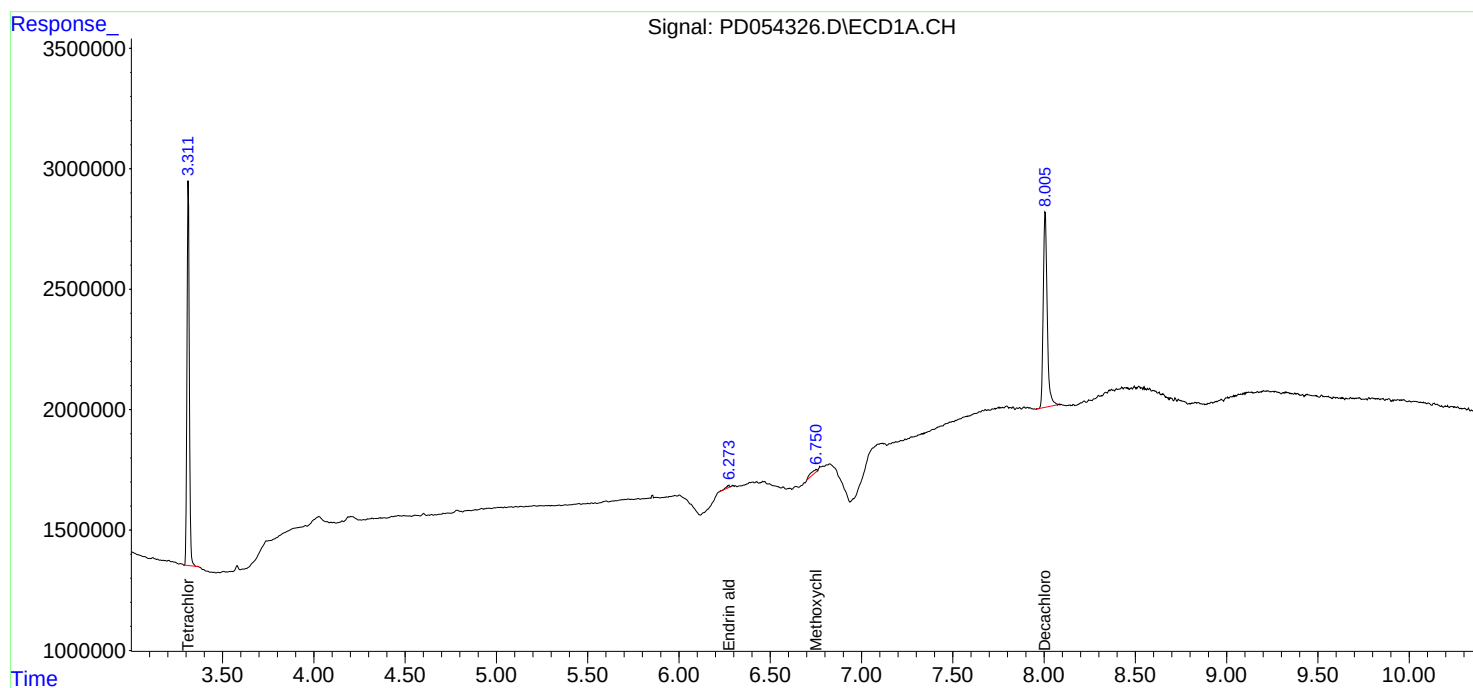


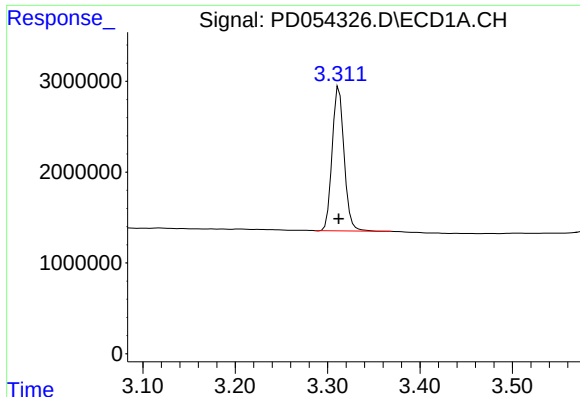

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 14263643
Conc: 23.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

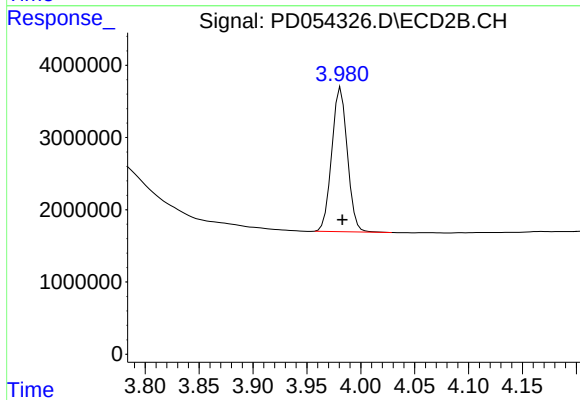


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.001 min
Response: 20020929
Conc: 23.72 ng/ml

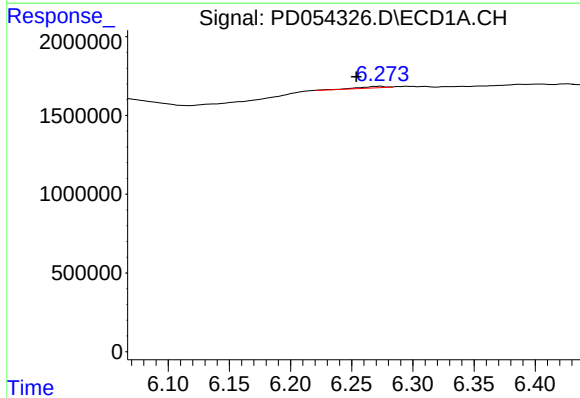


#18 Endrin aldehyde

R.T.: 6.274 min
Delta R.T.: 0.020 min
Response: 128359
Conc: 0.21 ng/ml

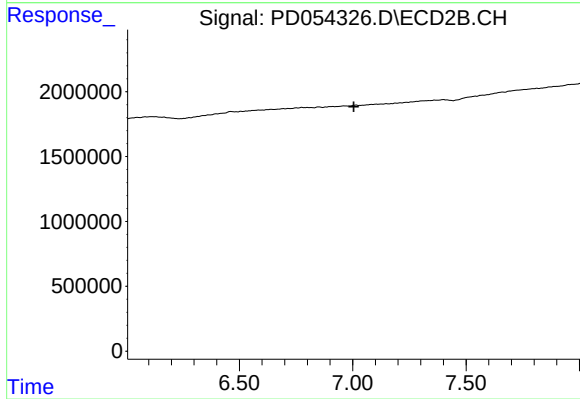

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.005 min
Response: 0
Conc: N.D.

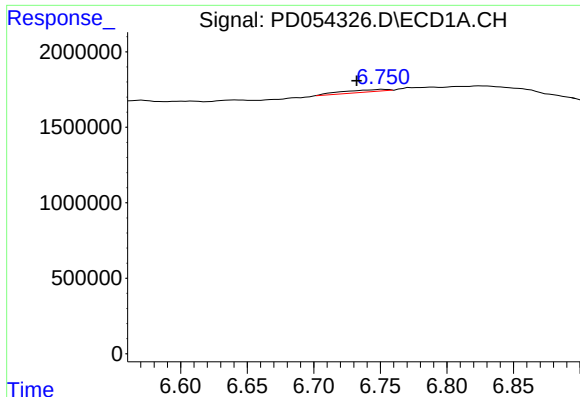

#20 Methoxychlor


R.T.: 6.752 min
Delta R.T.: 0.020 min
Response: 419703
Conc: 1.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

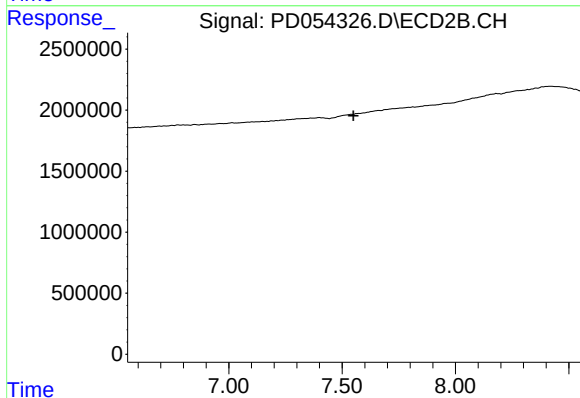


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.551 min
Response: 0
Conc: N.D.

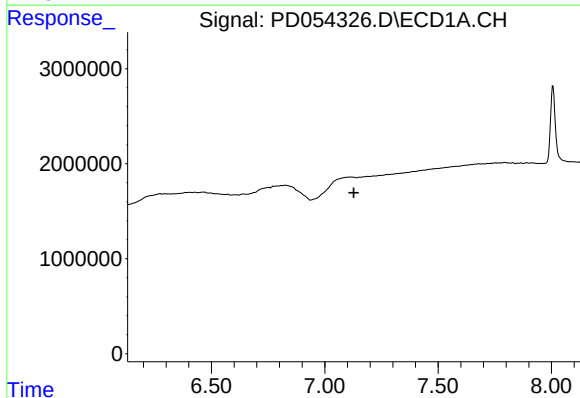


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.128 min
Response: 0
Conc: N.D.

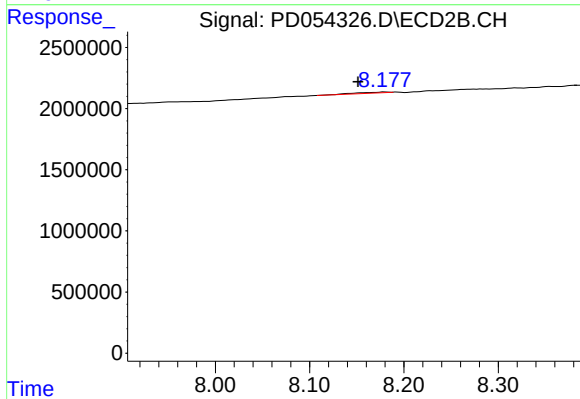

#22 Mirex


R.T.: 8.180 min
Delta R.T.: 0.029 min
Response: 164758
Conc: 0.18 ng/ml

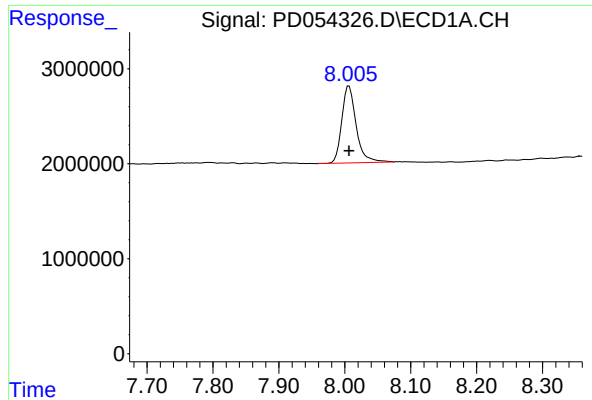

#28 Decachlorobiphenyl

R.T.: 8.006 min
Delta R.T.: 0.000 min
Response: 12218794
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

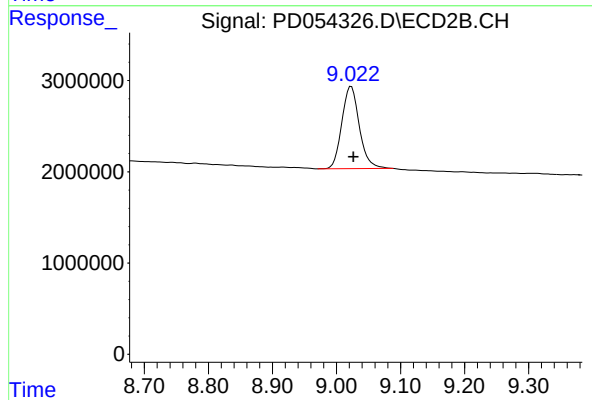

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: -0.003 min
Response: 17128478
Conc: 19.73 ng/ml