

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082019\
 Data File : PD054352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 15:04
 Operator : SG\AJ
 Sample : K4388-36
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 T6-E1-E2-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:28:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 16 08:45:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	14675100	19837231	24.412	23.500
28)	SA Decachlor...	8.005	9.022	14298583	19544409	22.296	22.507

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082019\
Data File : PD054352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2019 15:04
Operator : SG\AJ
Sample : K4388-36
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
T6-E1-E2-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:28:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
Quant Title : GC Extractables
QLast Update : Fri Aug 16 08:45:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

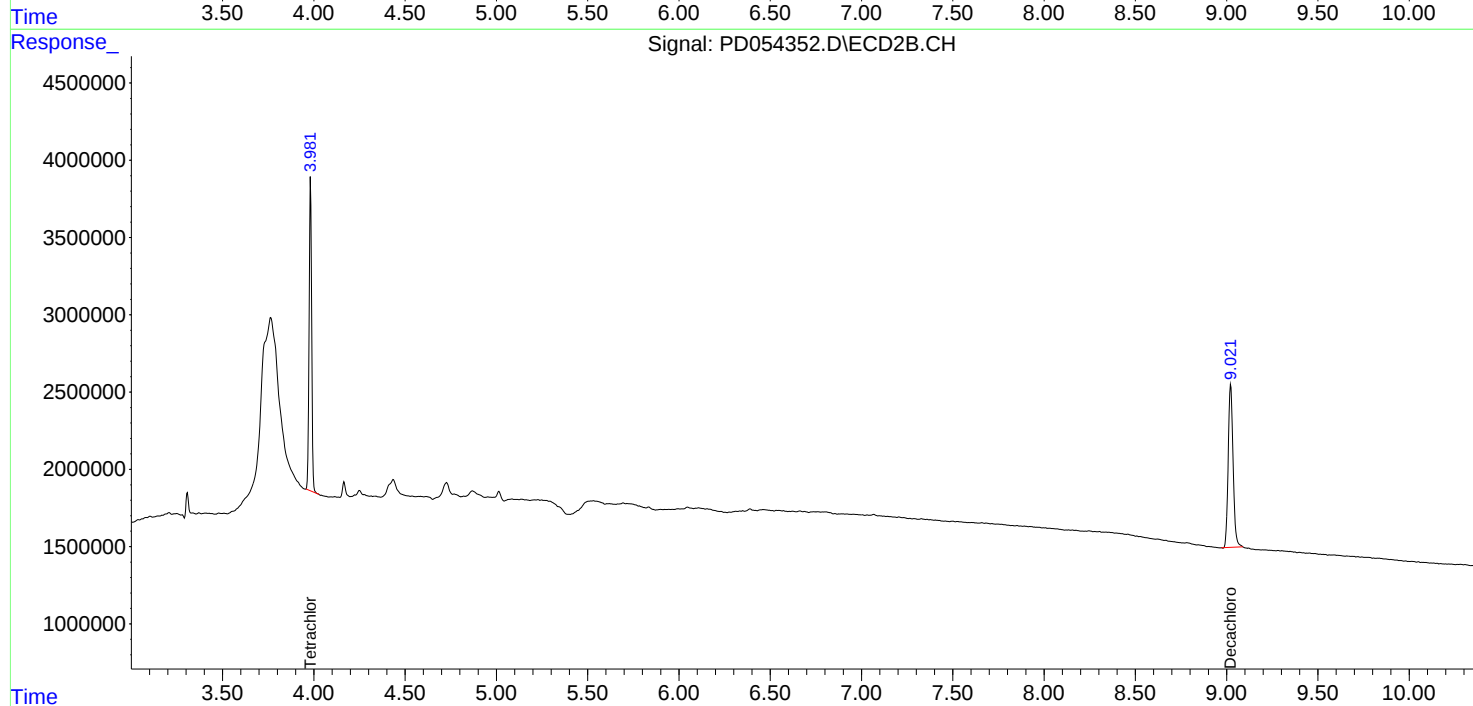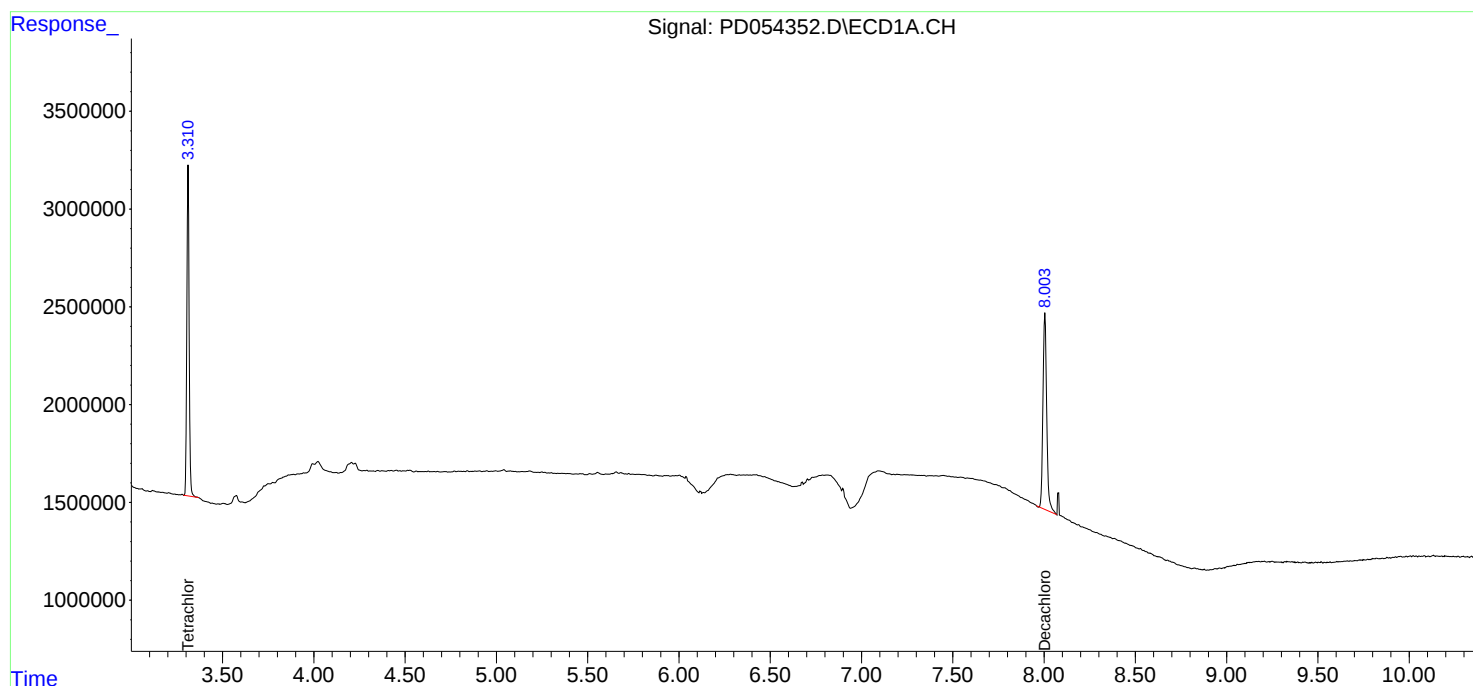


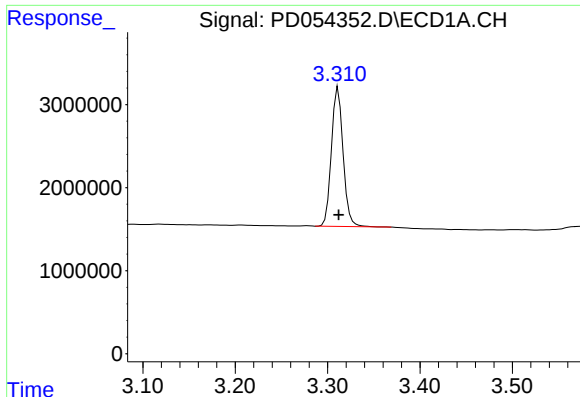

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 14675100
Conc: 24.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
T6-E1-E2-(0-2)

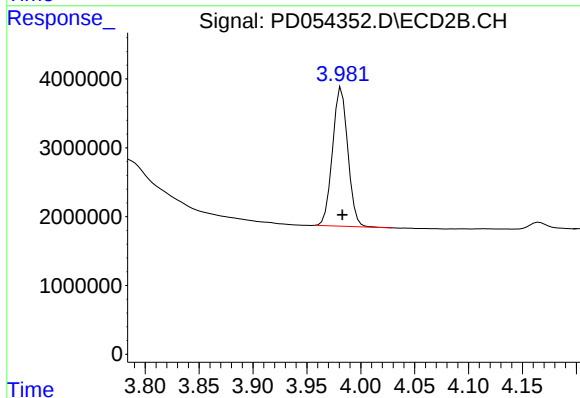


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 19837231
Conc: 23.50 ng/ml

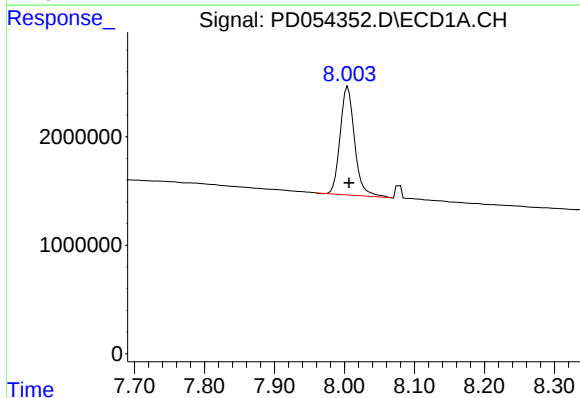

#28 Decachlorobiphenyl

R.T.: 8.005 min
Delta R.T.: -0.002 min
Response: 14298583
Conc: 22.30 ng/ml

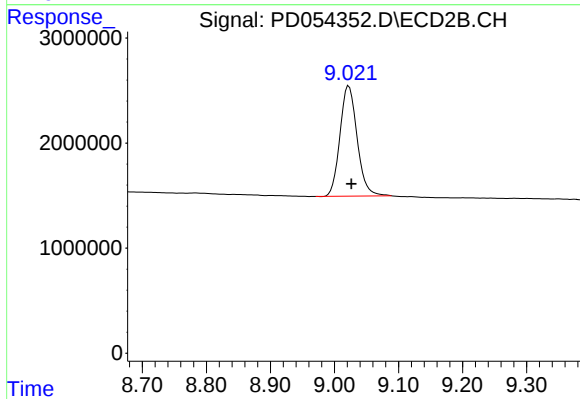

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.004 min
Response: 19544409
Conc: 22.51 ng/ml