

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 19:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:31:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	0.000	5.200	0	7672433	N.D. 0.765 #
7) B	delta-BHC	0.000	5.092	0	6849924	N.D. 0.705 #
8) B	Heptachlo...	0.000	5.887	0	35948879	N.D. 4.819 #
15) B	Endosulfa...	0.000	6.940	0	940549	N.D. 0.160 #
17) MA	4,4'-DDT	0.000	7.145	0	1339340	N.D. 0.223 #
21) B	Endrin ke...	0.000	7.762	0	1313646	N.D. 0.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 19:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:31:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

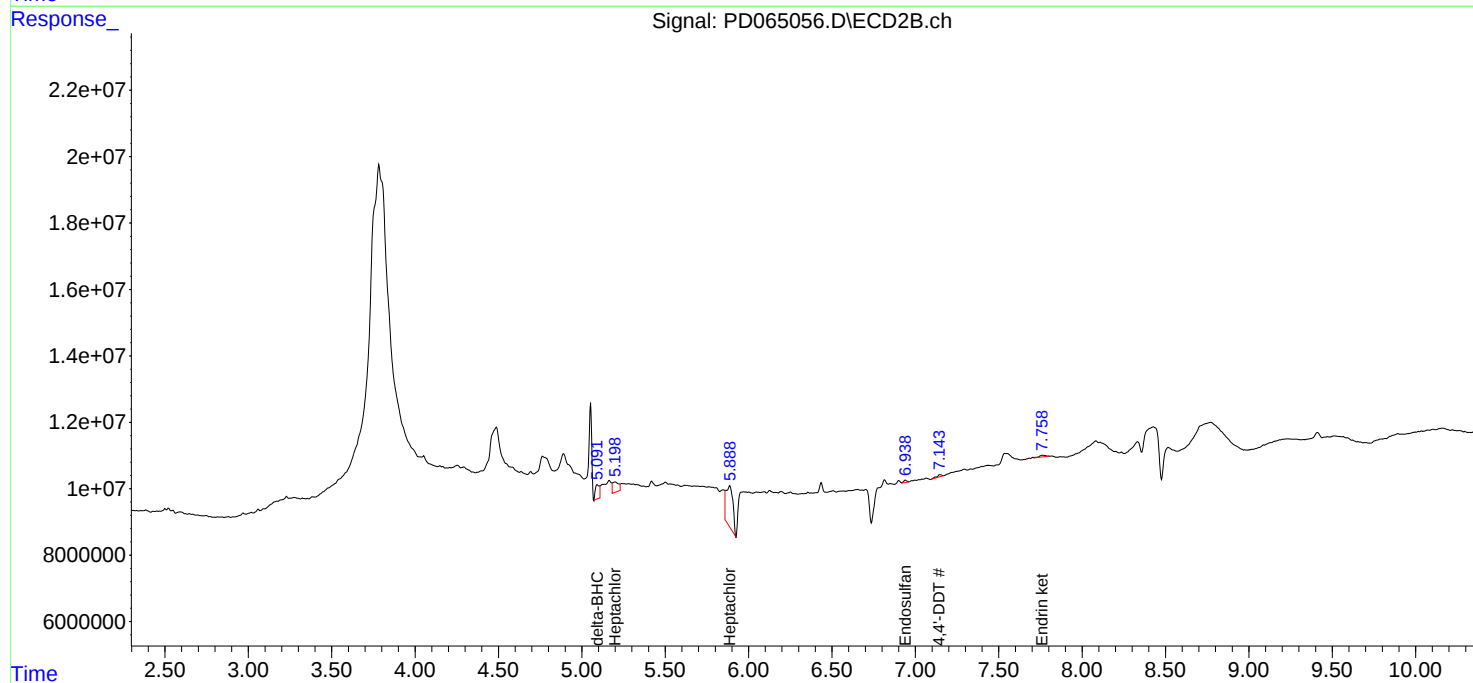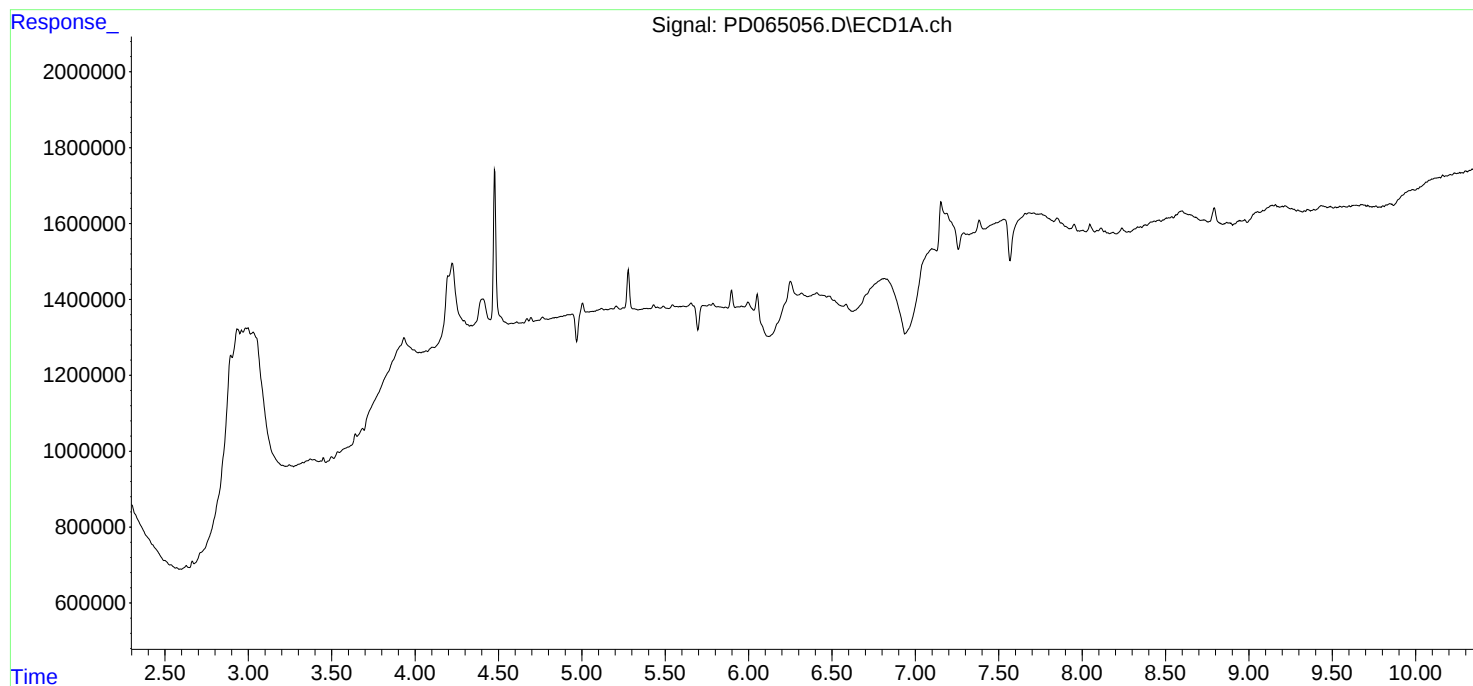


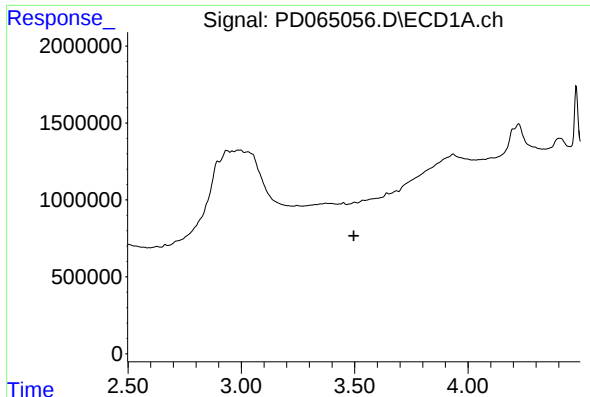

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

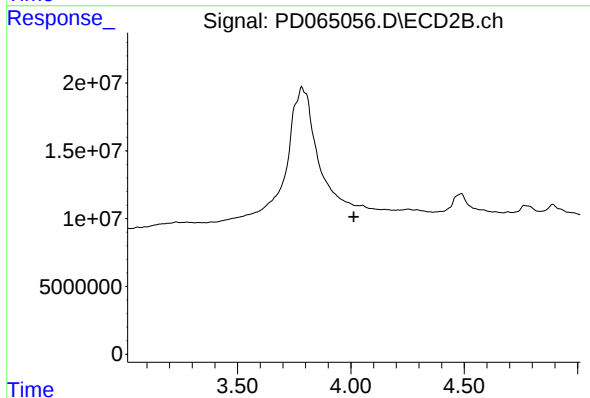


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.013 min
Response: 0
Conc: N.D.

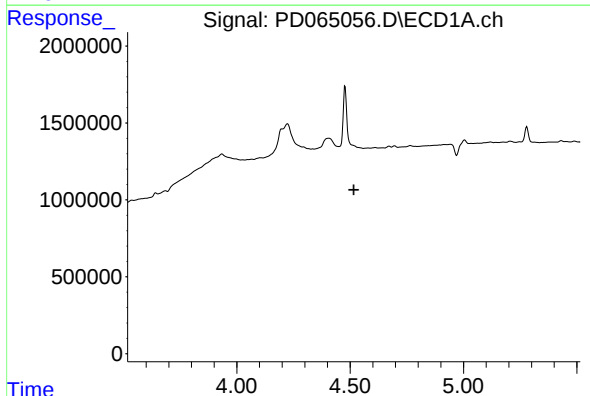


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.517 min
Response: 0
Conc: N.D.

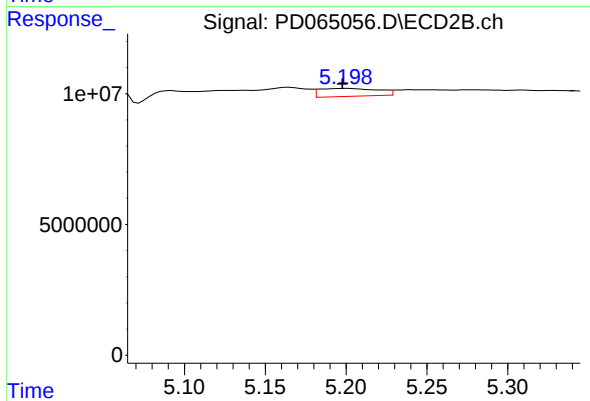

#4 Heptachlor


R.T.: 5.200 min
Delta R.T.: 0.002 min
Response: 7672433
Conc: 0.77 ng/ml

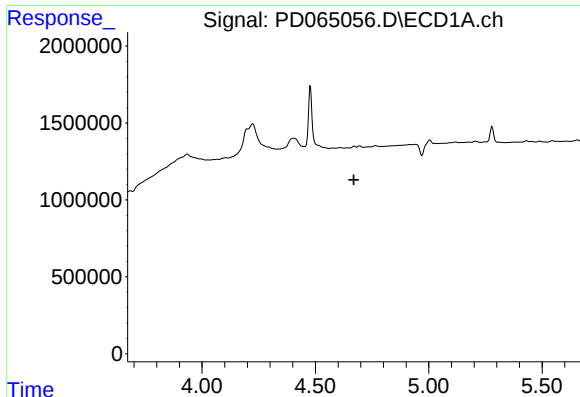

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

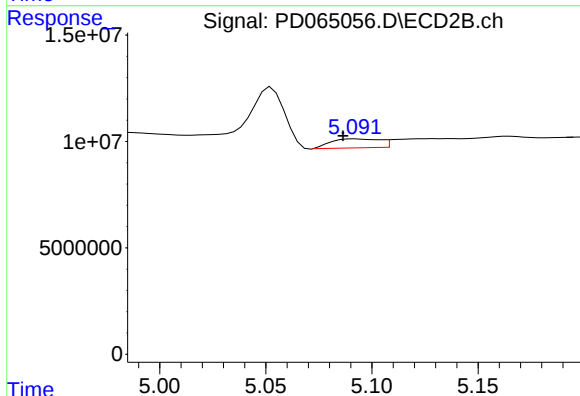


#7 delta-BHC

R.T.: 5.092 min
Delta R.T.: 0.006 min
Response: 6849924
Conc: 0.71 ng/ml

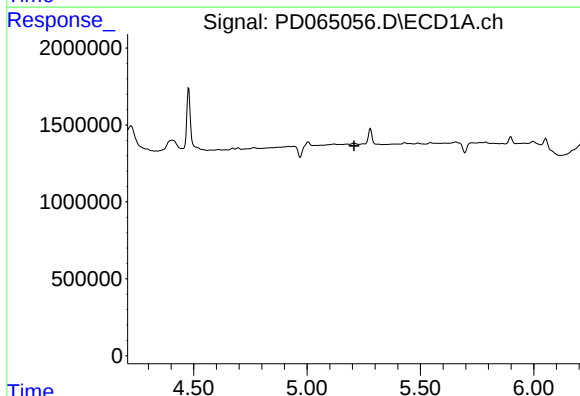


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

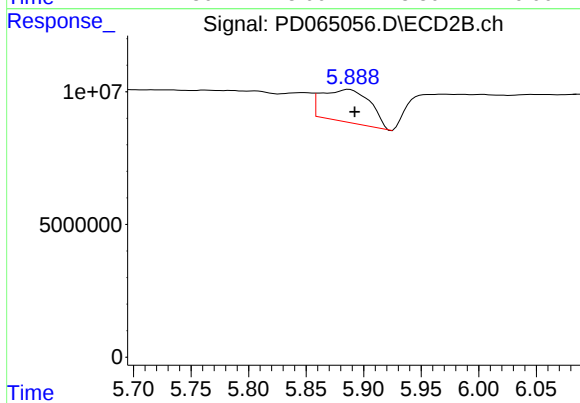

#8 Heptachlor epoxide


R.T.: 5.887 min
Delta R.T.: -0.005 min
Response: 35948879
Conc: 4.82 ng/ml

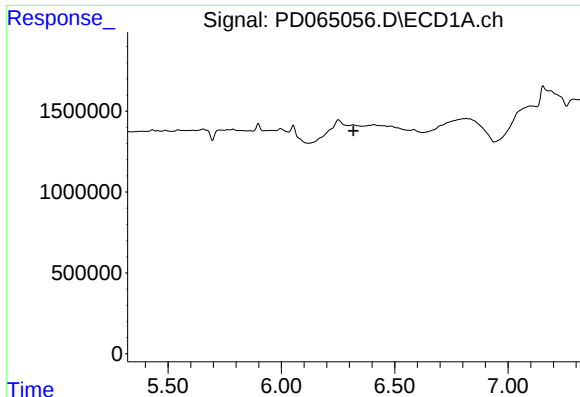

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

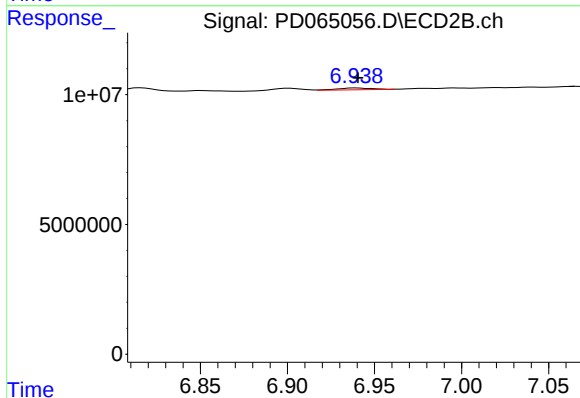


#15 Endosulfan II

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 940549
Conc: 0.16 ng/ml

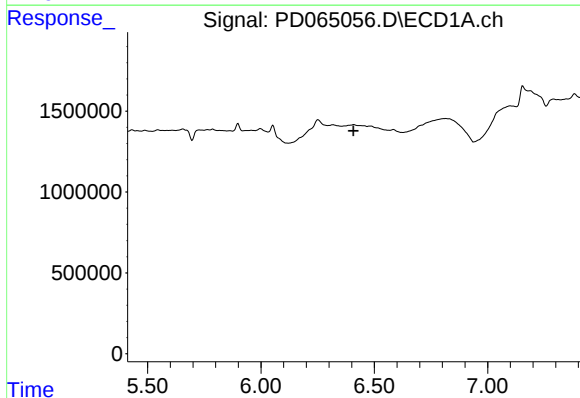


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

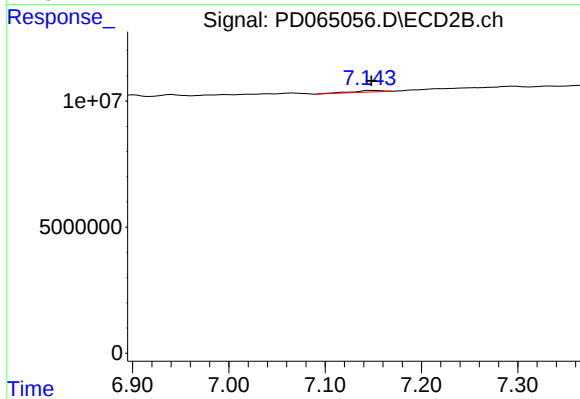

#17 4,4'-DDT


R.T.: 7.145 min
Delta R.T.: -0.003 min
Response: 1339340
Conc: 0.22 ng/ml

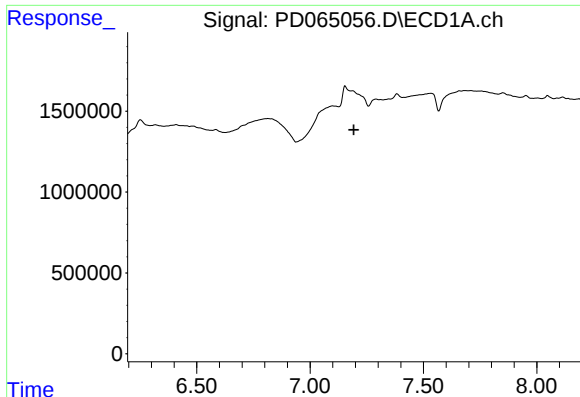

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

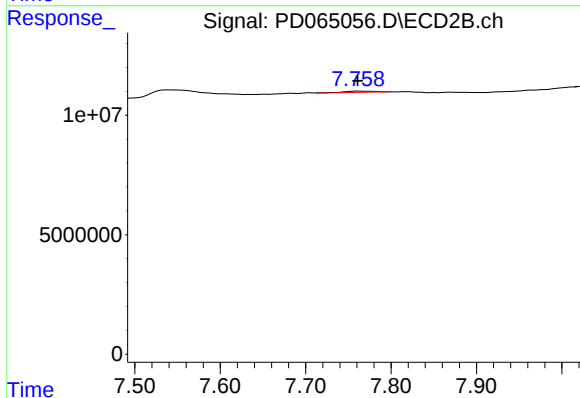


#21 Endrin ketone

R.T.: 7.762 min
Delta R.T.: 0.000 min
Response: 1313646
Conc: 0.20 ng/ml

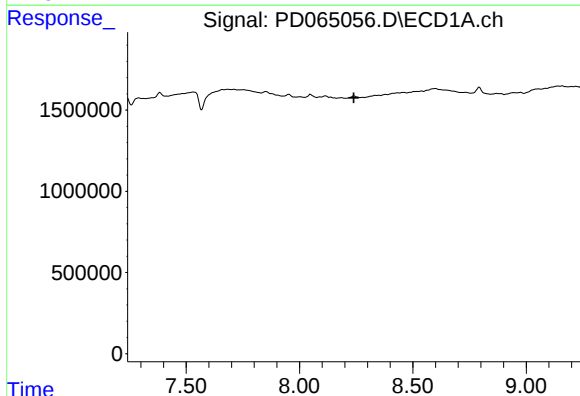

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.240 min
Response: 0
Conc: N.D.

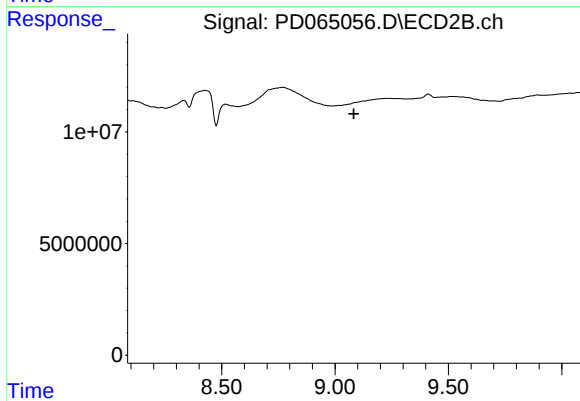

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.