

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 19:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:31:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20943523	164.6E6	20.375	20.775
28)	SA Decachlor...	8.241	9.084	23250467	96842859	20.520	20.463
Target Compounds							
4)	MA Heptachlor	0.000	5.202	0	1945703	N.D.	0.194 #
7)	B delta-BHC	0.000	5.116f	0	6270746	N.D.	0.646 #
15)	B Endosulfa...	0.000	6.950	0	2453534	N.D.	0.418 #
17)	MA 4,4'-DDT	0.000	7.157	0	364454	N.D.	0.061 #
23)	Chlordane-1	4.394f	0.000	2025594	0	53.485	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 19:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:31:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

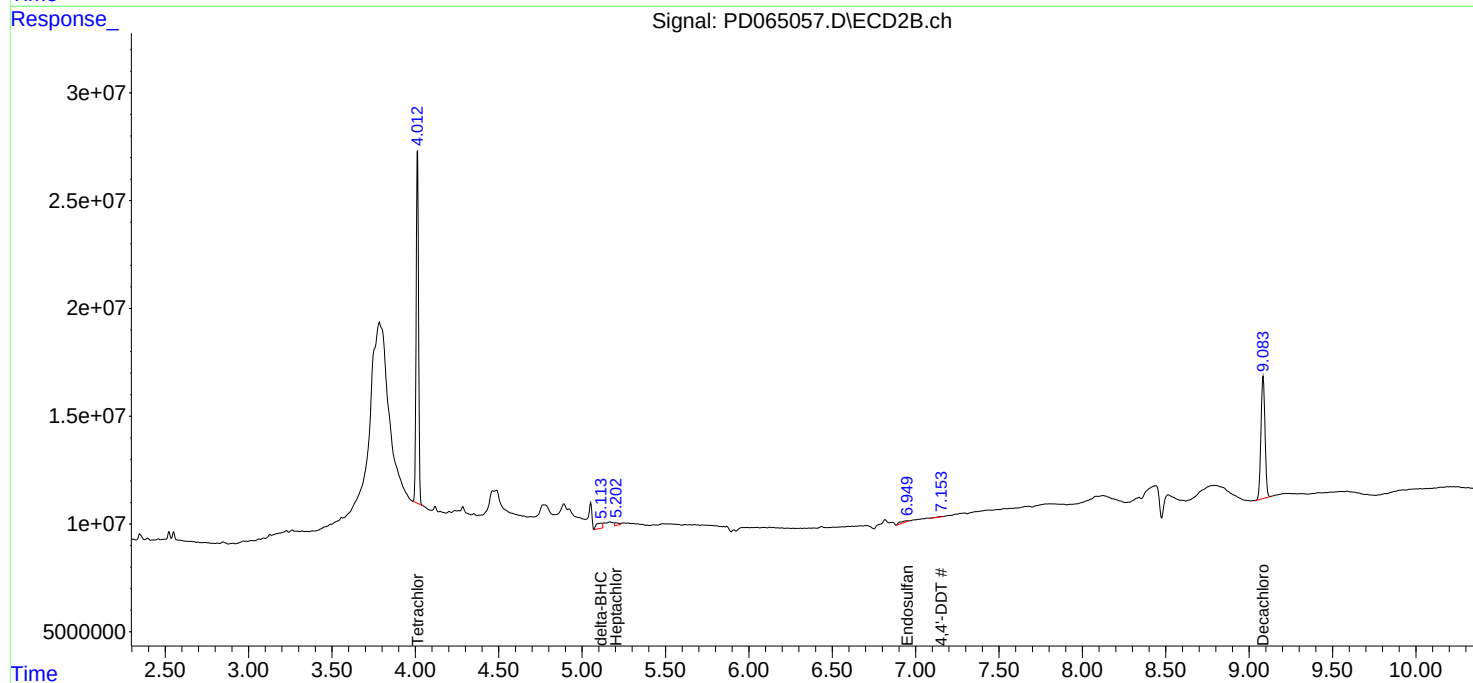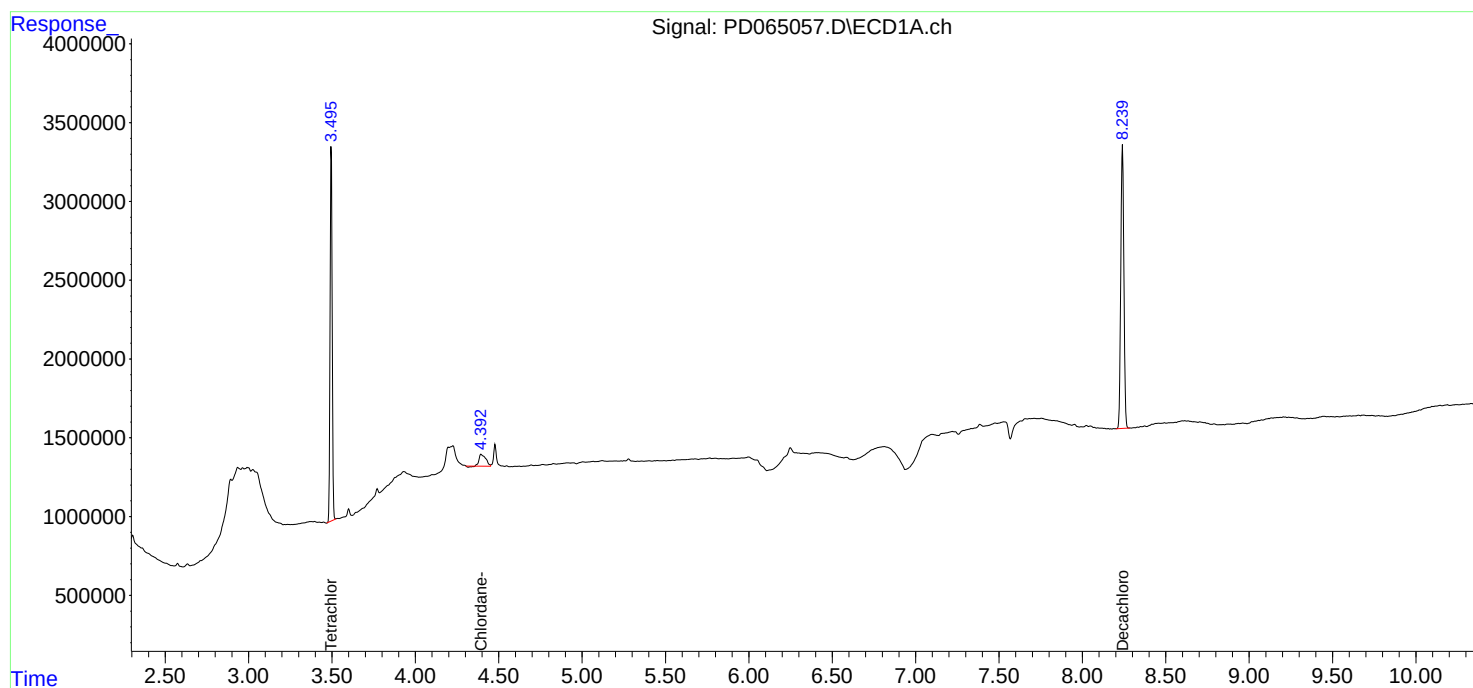


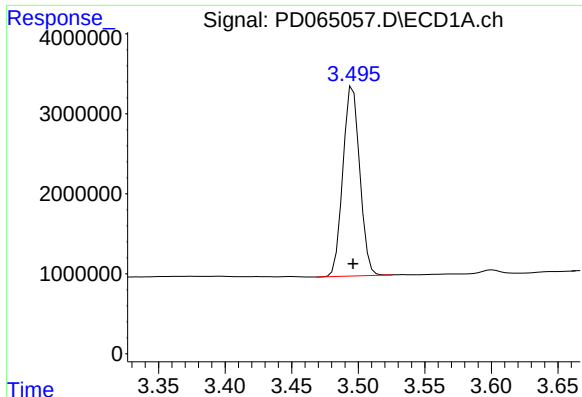

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 20943523
Conc: 20.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

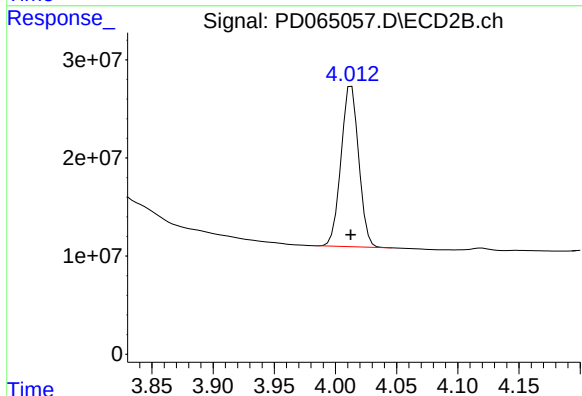


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 164551723
Conc: 20.77 ng/ml

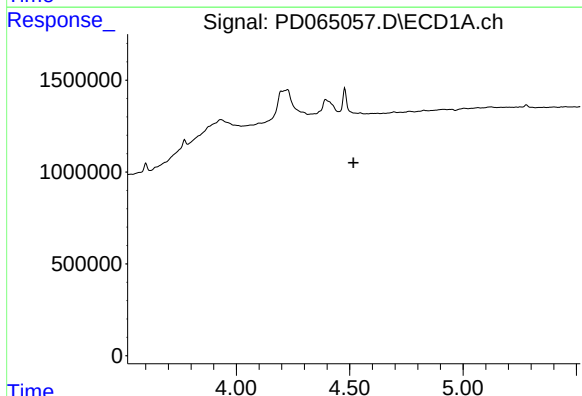


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.517 min
Response: 0
Conc: N.D.

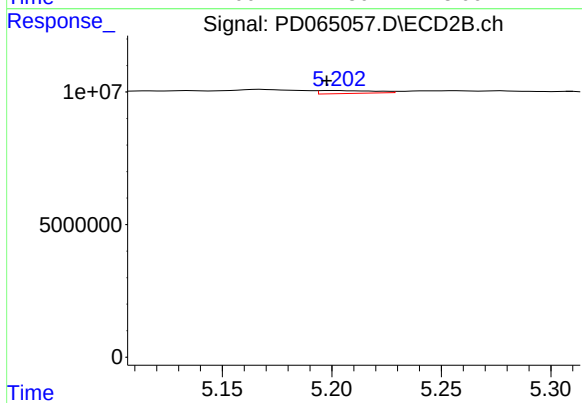

#4 Heptachlor


R.T.: 5.202 min
Delta R.T.: 0.005 min
Response: 1945703
Conc: 0.19 ng/ml

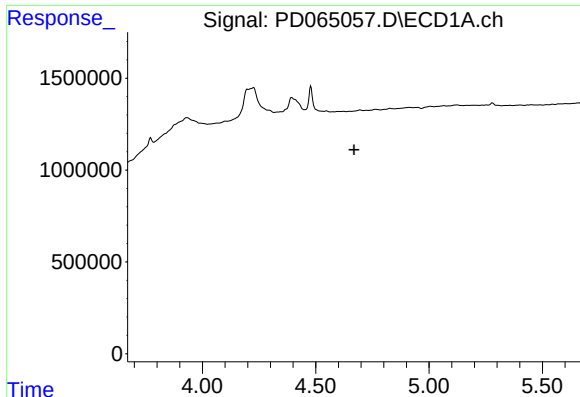

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

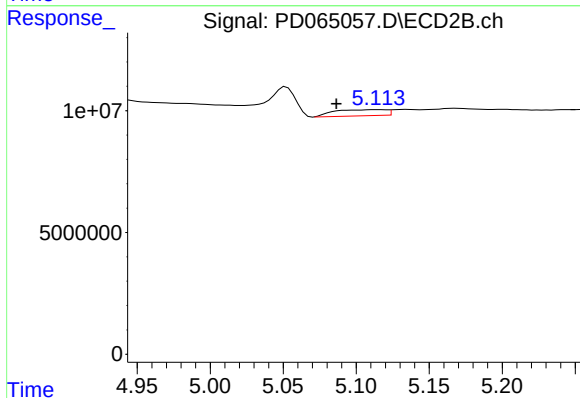


#7 delta-BHC

R.T.: 5.116 min
Delta R.T.: 0.029 min
Response: 6270746
Conc: 0.65 ng/ml

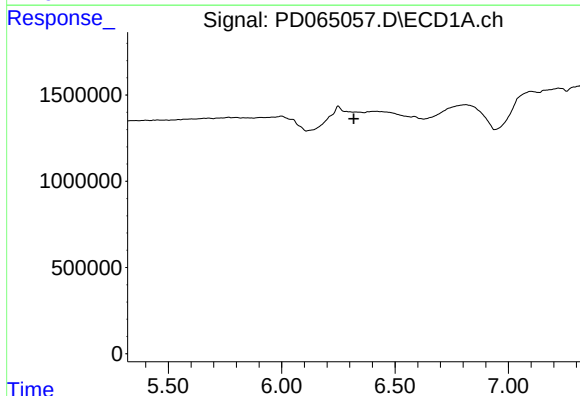


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

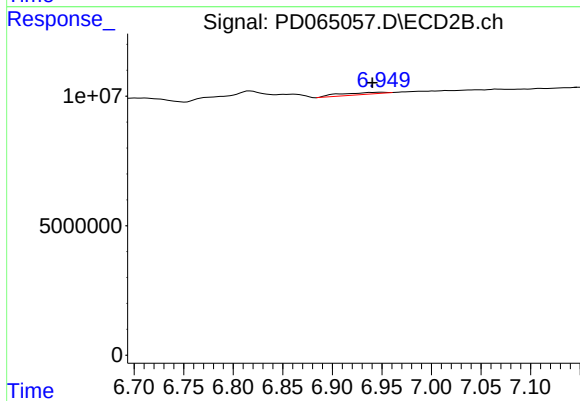

#15 Endosulfan II


R.T.: 6.950 min
Delta R.T.: 0.010 min
Response: 2453534
Conc: 0.42 ng/ml

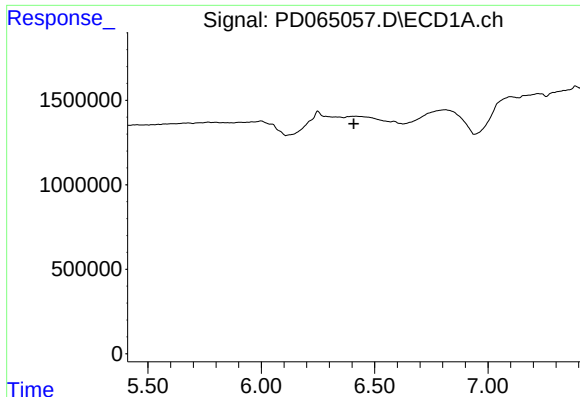

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

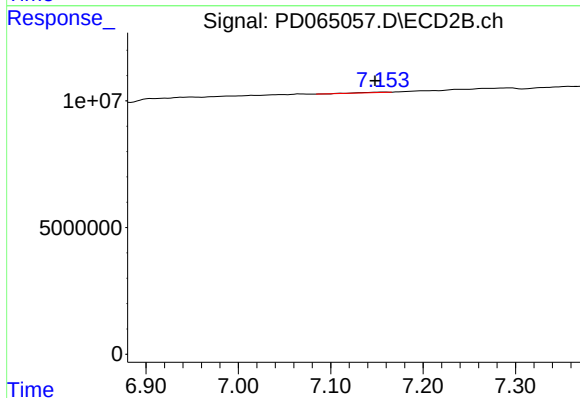


#17 4,4'-DDT

R.T.: 7.157 min
Delta R.T.: 0.009 min
Response: 364454
Conc: 0.06 ng/ml

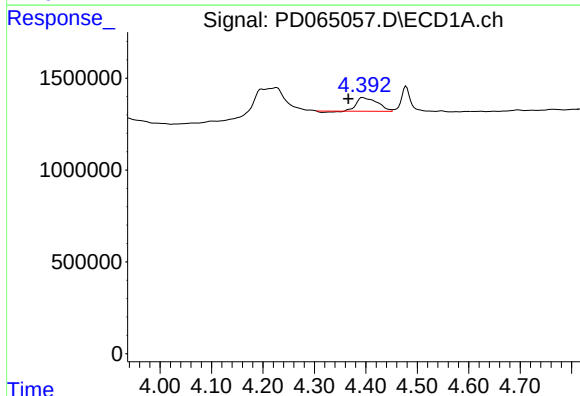


#23 Chlordane-1

R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 2025594
Conc: 53.49 ng/ml

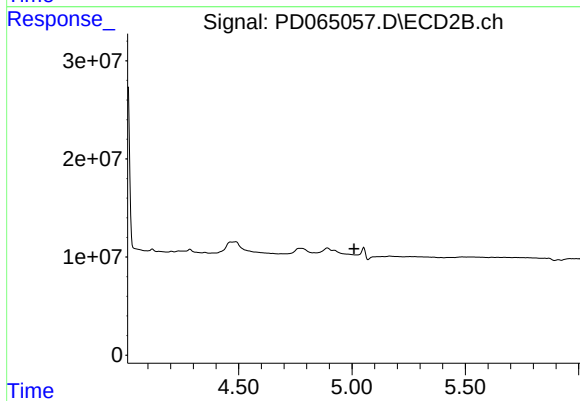

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

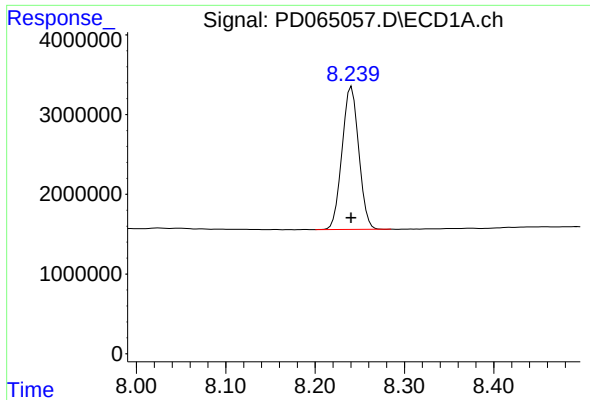

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 23250467
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

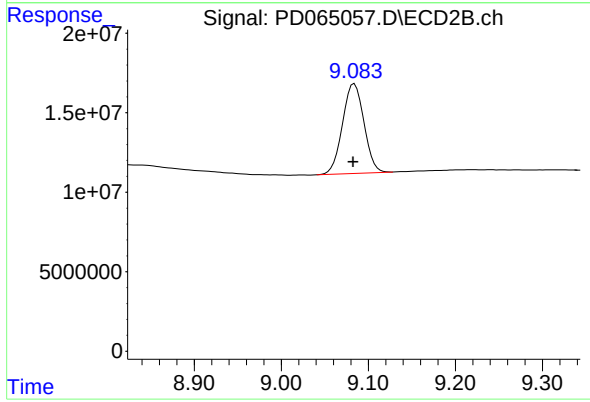

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.001 min
Response: 96842859
Conc: 20.46 ng/ml