

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 21:25
 Operator : AR\AJ
 Sample : PCHLORICC0750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:41:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 01:41:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	87566275	573.8E6	72.948	72.658
28)	SA Decachlor...	8.241	9.085	79052195	339.9E6	70.040	71.550
Target Compounds							
23)	Chlordane-1	4.366	5.009	25757021	228.0E6	708.356	727.067
24)	Chlordane-2	4.866	5.478	29496279	211.2E6	699.048	716.410
25)	Chlordane-3	5.433	6.126	75241557	717.4E6	714.242	727.924
26)	Chlordane-4	5.491	6.199	62484999	829.7E6	710.677	725.915
27)	Chlordane-5	6.328	7.009	31060604	169.6E6	721.061	728.604



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 21:25
Operator : AR\AJ
Sample : PCHLORICC0750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:41:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 01:41:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

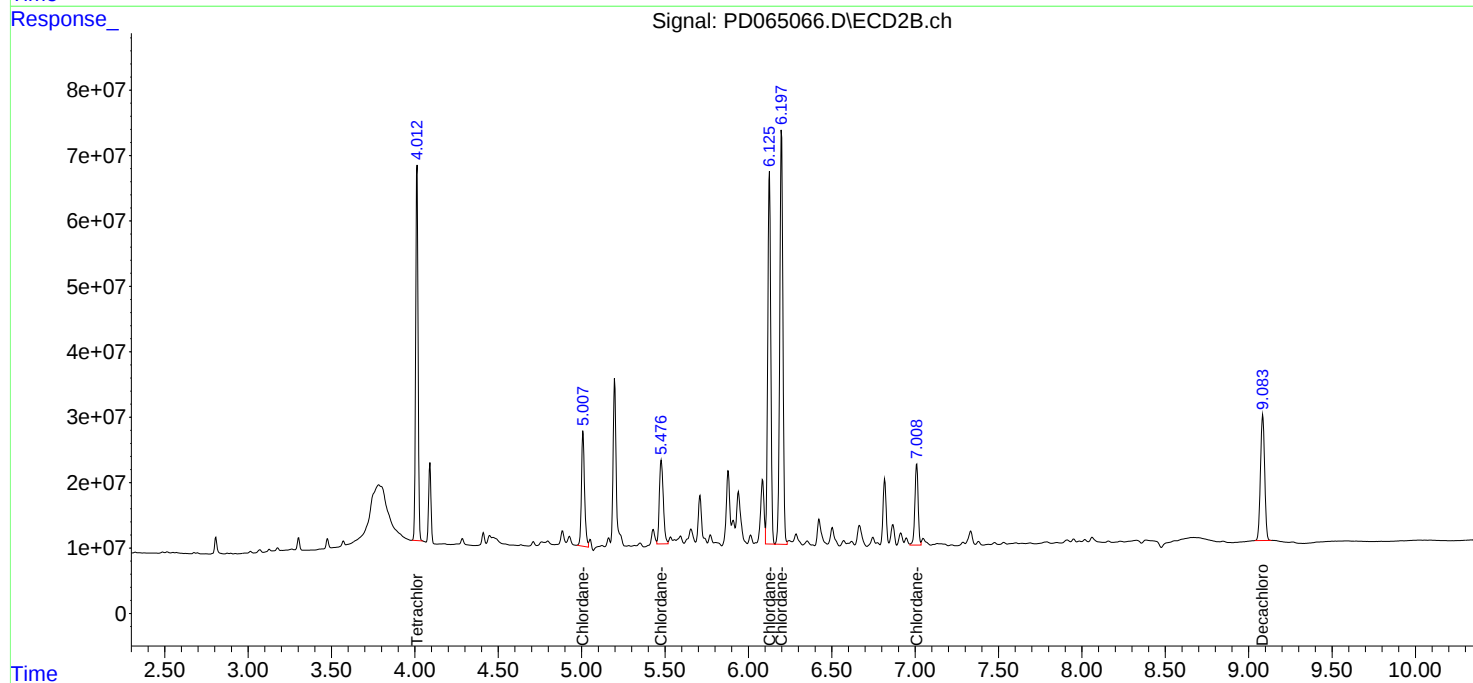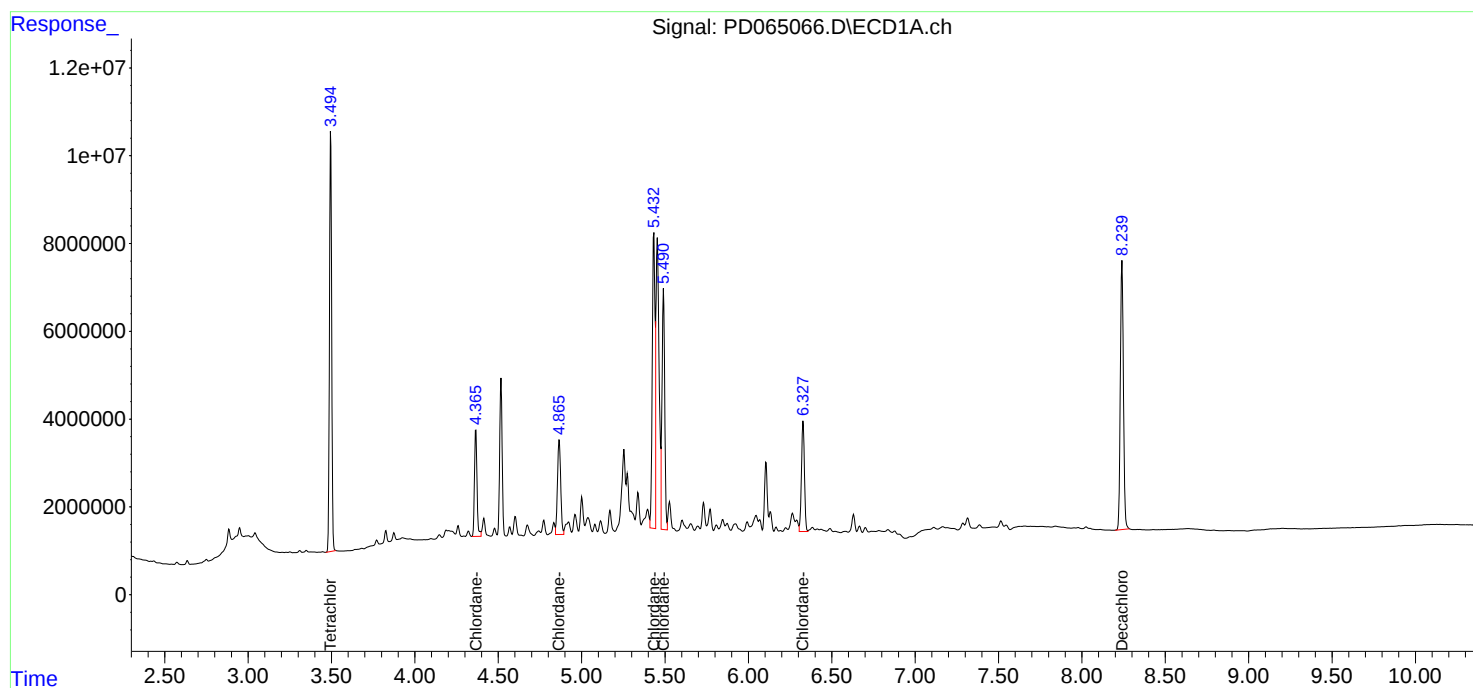


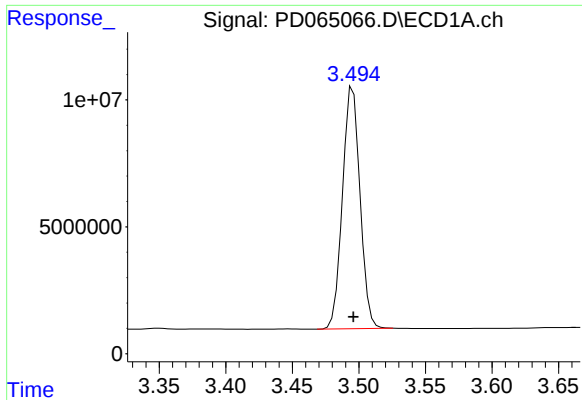

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 87566275
Conc: 72.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

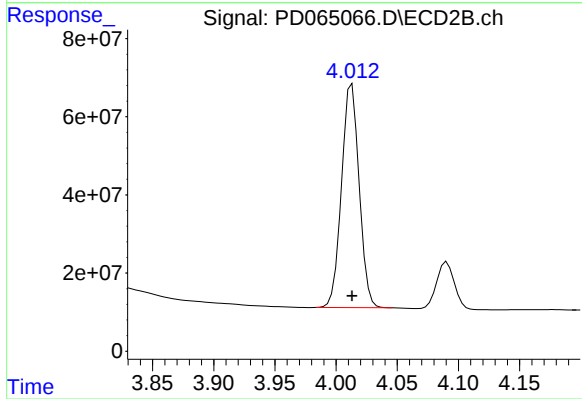


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 573796362
Conc: 72.66 ng/ml

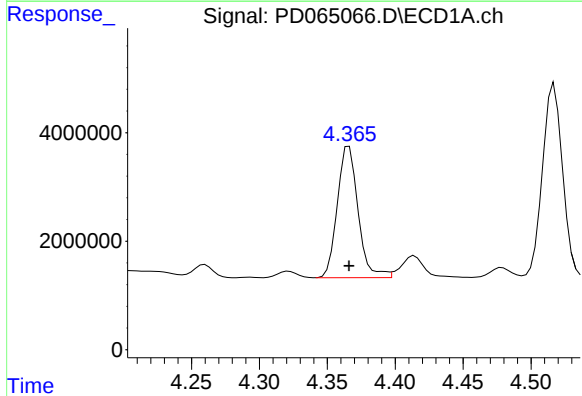


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 25757021
Conc: 708.36 ng/ml

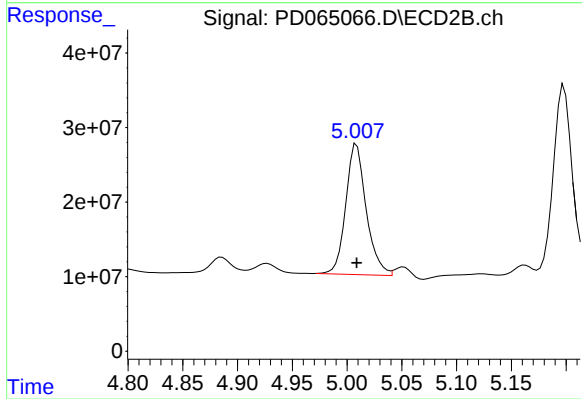

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 227971595
Conc: 727.07 ng/ml

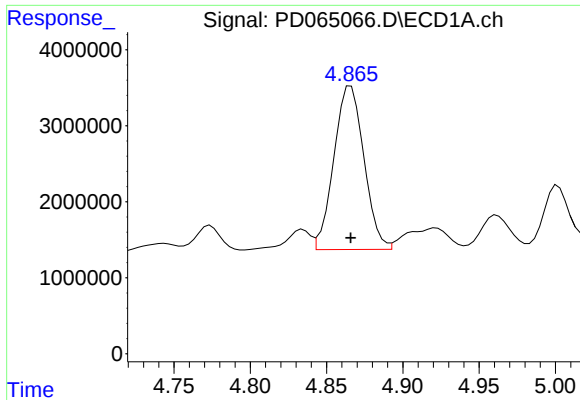

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 29496279
Conc: 699.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

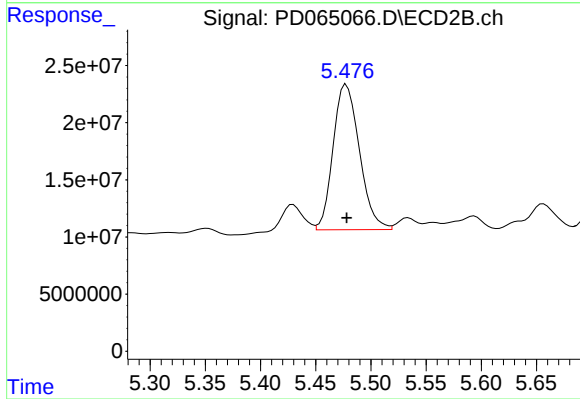


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 211176344
Conc: 716.41 ng/ml

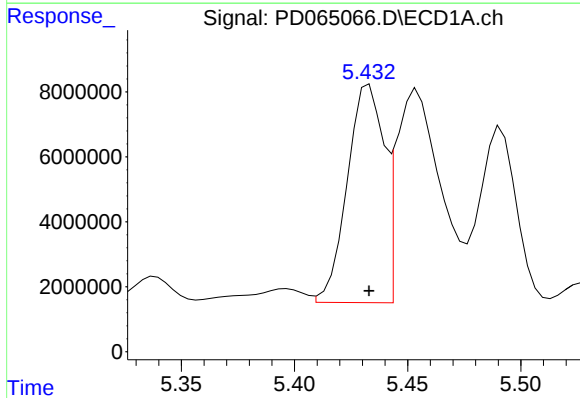


#25 Chlordane-3

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 75241557
Conc: 714.24 ng/ml

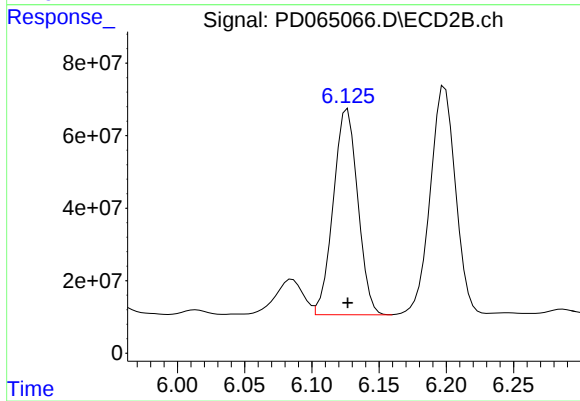

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 717384923
Conc: 727.92 ng/ml

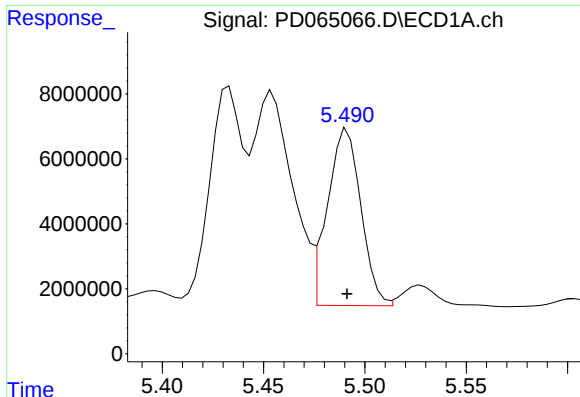

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 62484999
Conc: 710.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

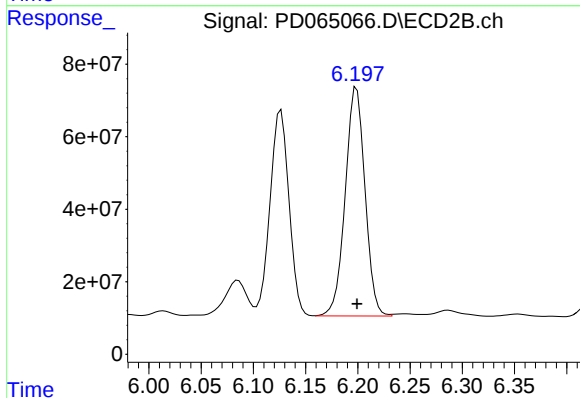


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 829651679
Conc: 725.91 ng/ml

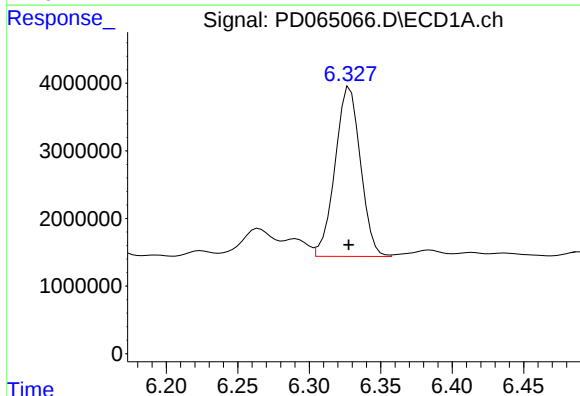


#27 Chlordane-5

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 31060604
Conc: 721.06 ng/ml

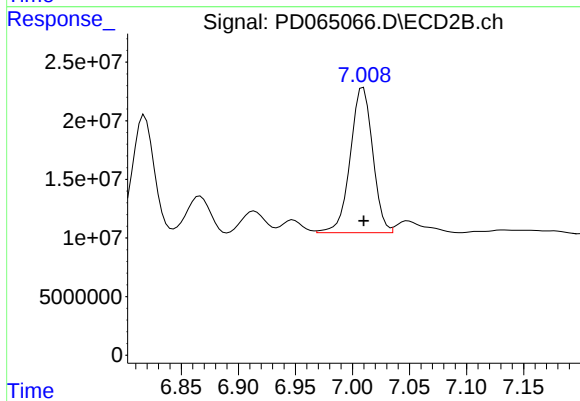

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 169586319
Conc: 728.60 ng/ml

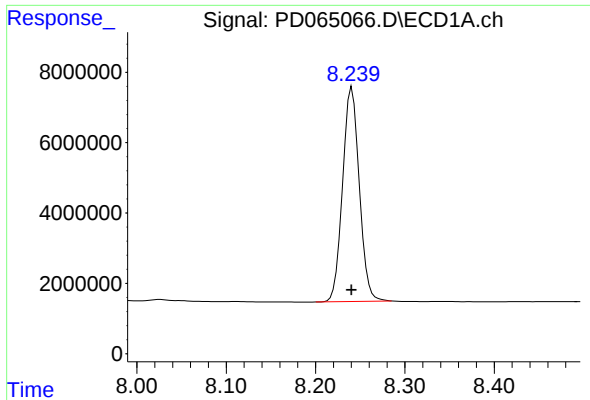

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 79052195
Conc: 70.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

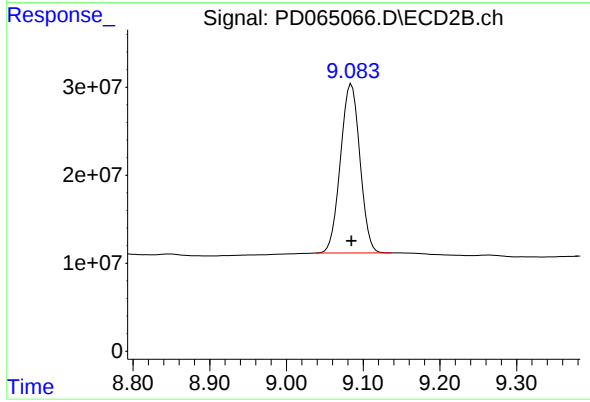

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 339866046
Conc: 71.55 ng/ml