

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 21:52
 Operator : AR\AJ
 Sample : PCHLORICC0250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:42:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 01:41:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	31239270	208.5E6	26.024	26.400
28)	SA Decachlor...	8.240	9.084	30707573	128.1E6	27.207	26.975
Target Compounds							
23)	Chlordane-1	4.366	5.009	9591949	75896295	263.793	242.055
24)	Chlordane-2	4.866	5.479	11755183	82454511	278.592	279.725
25)	Chlordane-3	5.433	6.126	27970038	259.4E6	265.510	263.230
26)	Chlordane-4	5.491	6.199	23571749	303.5E6	268.095	265.561
27)	Chlordane-5	6.328	7.010	11696306	59789428	271.526	256.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 21:52
Operator : AR\AJ
Sample : PCHLORICC0250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:42:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 01:41:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

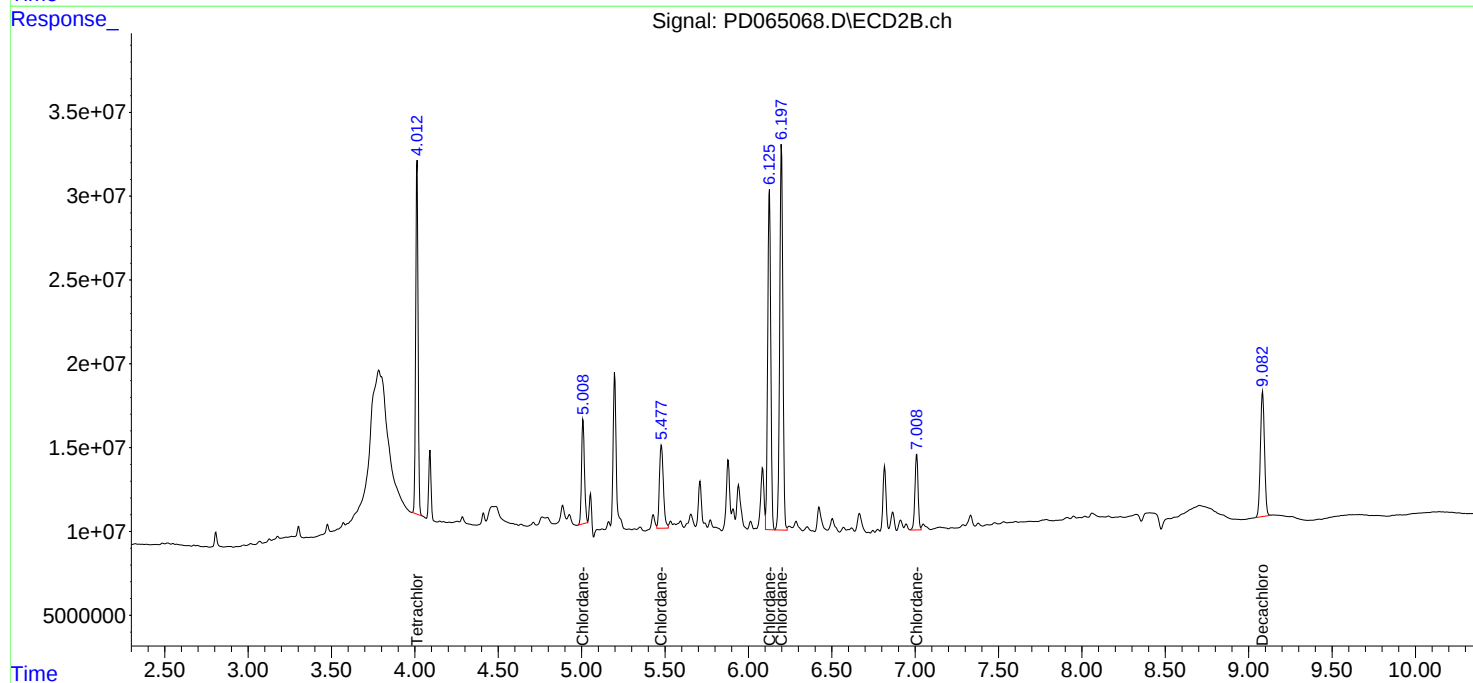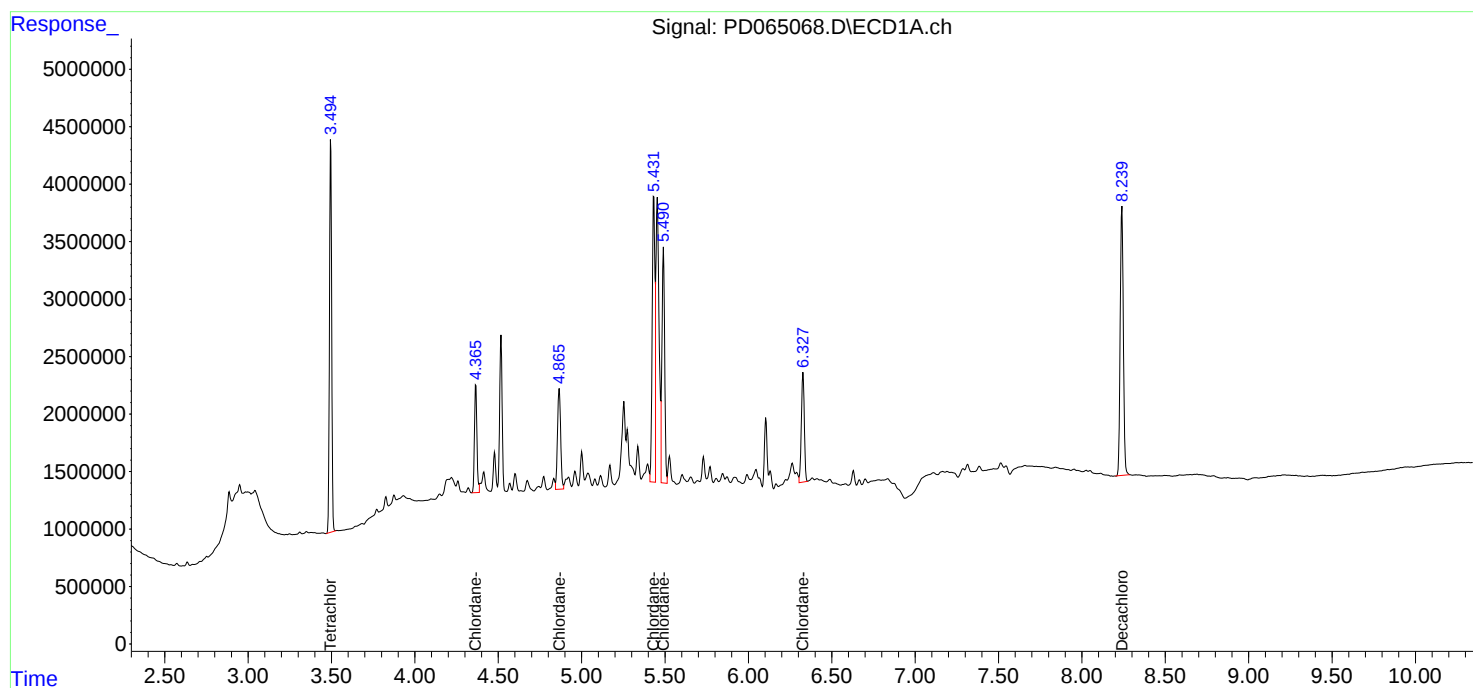


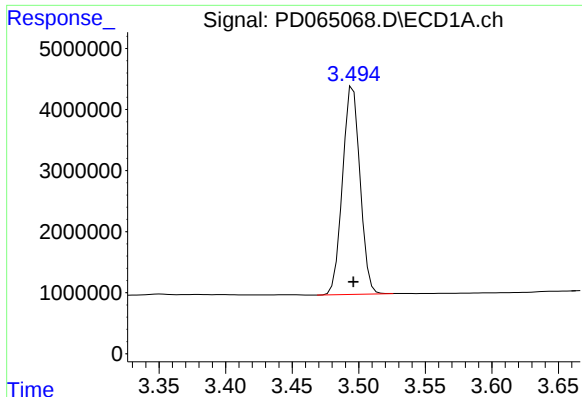

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 31239270
Conc: 26.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

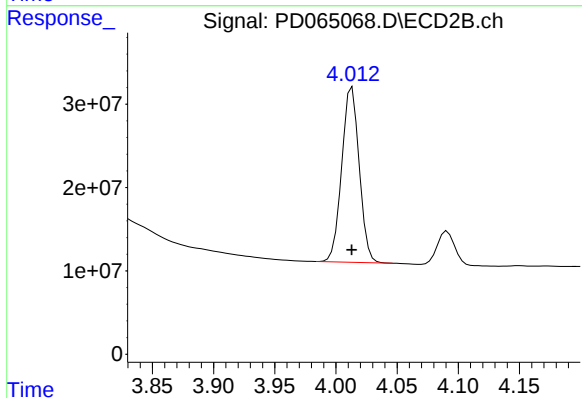


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 208482412
Conc: 26.40 ng/ml

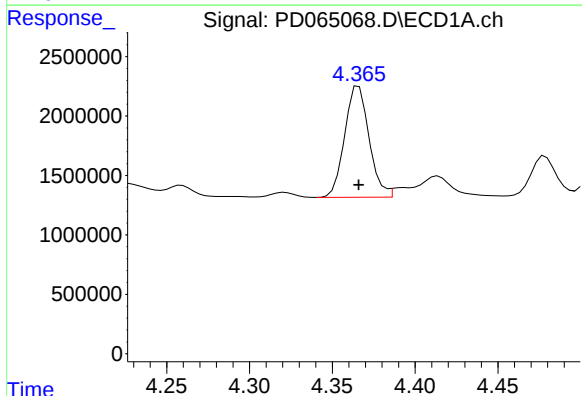


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 9591949
Conc: 263.79 ng/ml

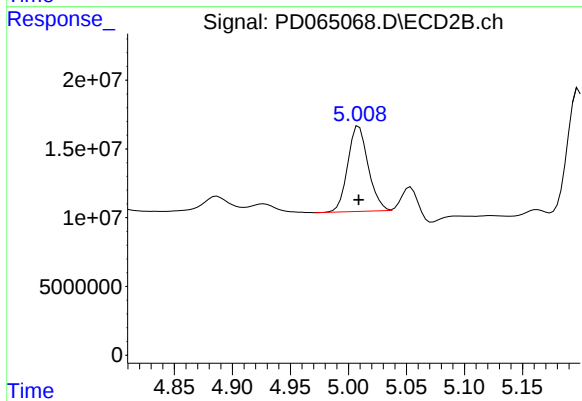

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 75896295
Conc: 242.06 ng/ml

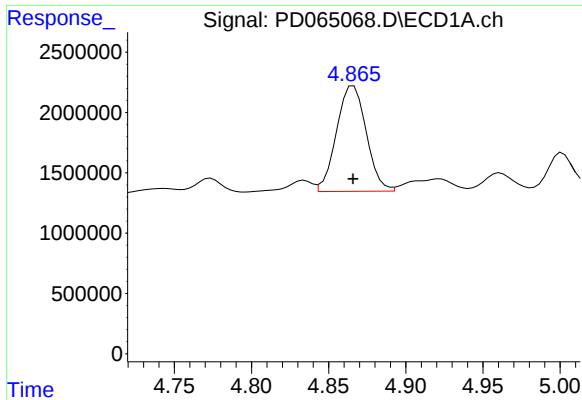

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 11755183
Conc: 278.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

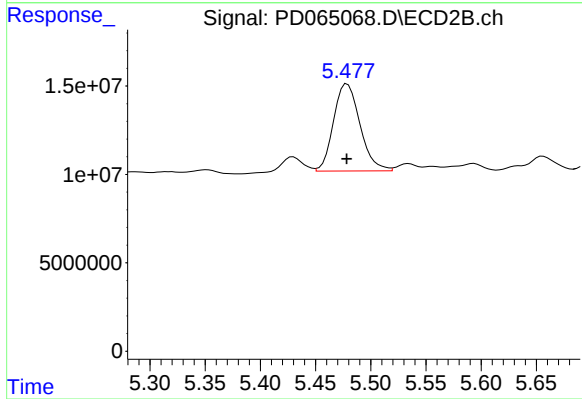


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 82454511
Conc: 279.72 ng/ml

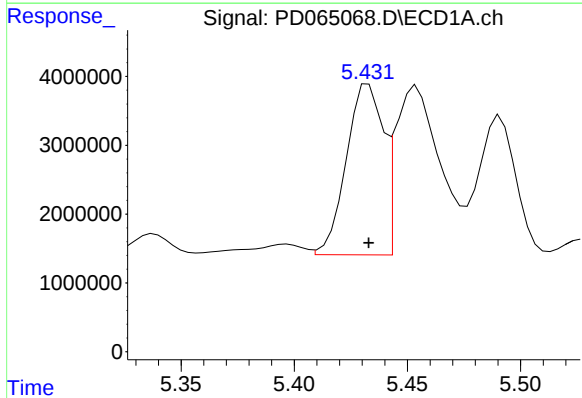


#25 Chlordane-3

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 27970038
Conc: 265.51 ng/ml

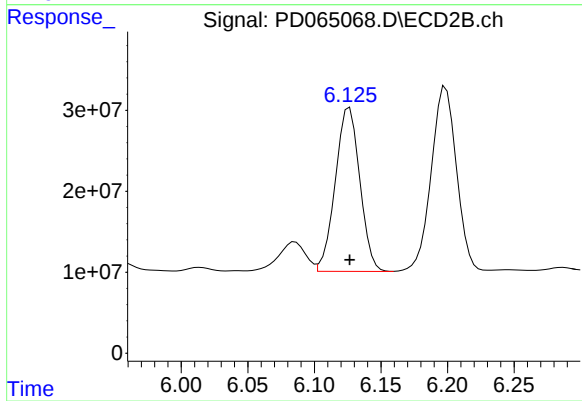

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 259418612
Conc: 263.23 ng/ml

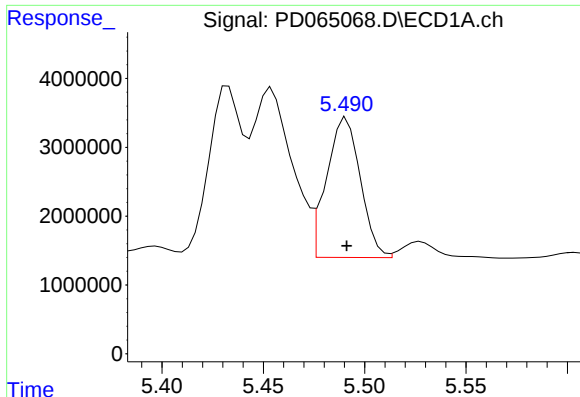

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 23571749
Conc: 268.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

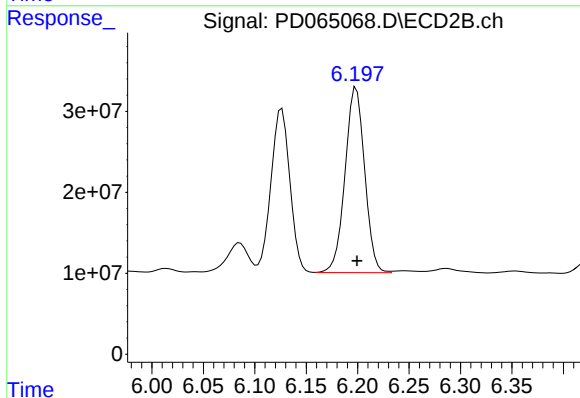


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 303510966
Conc: 265.56 ng/ml

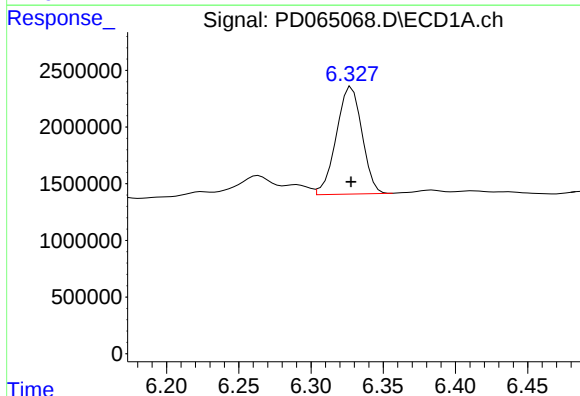


#27 Chlordane-5

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 11696306
Conc: 271.53 ng/ml

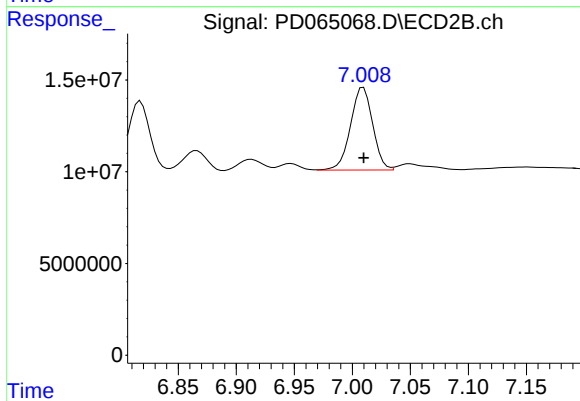

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 59789428
Conc: 256.88 ng/ml

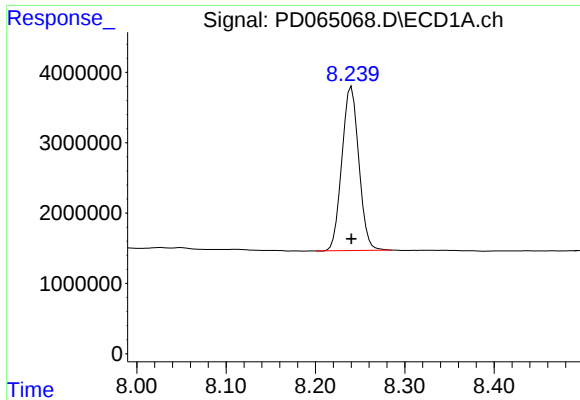

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 30707573
Conc: 27.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

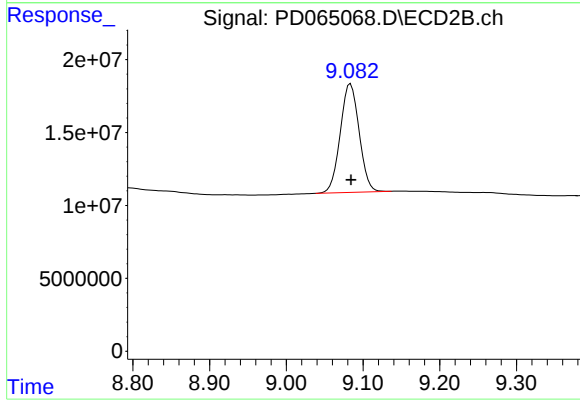

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 128132806
Conc: 26.97 ng/ml