

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 23:42
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD082021CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 02:22:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:01:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	58835627	381.6E6	46.755	46.217
28)	SA Decachlor...	8.239	9.084	58678679	236.0E6	48.803	47.060
Target Compounds							
23)	Chlordane-1	4.366	5.009	17591622	148.5E6	464.502	479.475
24)	Chlordane-2	4.866	5.478	21074118	137.7E6	482.859	440.293
25)	Chlordane-3	5.433	6.126	52817132	485.5E6	478.542	469.588
26)	Chlordane-4	5.491	6.199	44347290	564.0E6	483.066	469.100
27)	Chlordane-5	6.327	7.009	21545424	115.9E6	478.907	488.886



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 23:42
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD082021CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 02:22:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:01:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

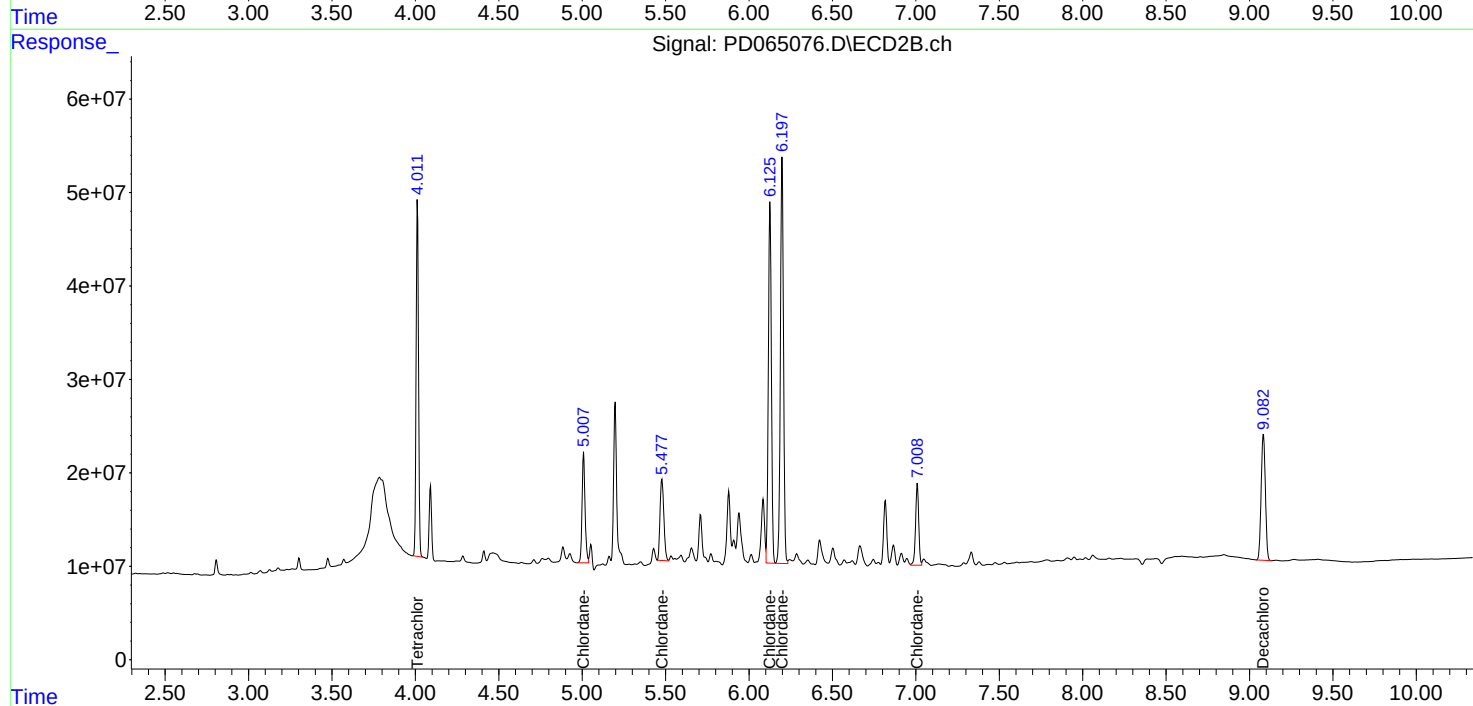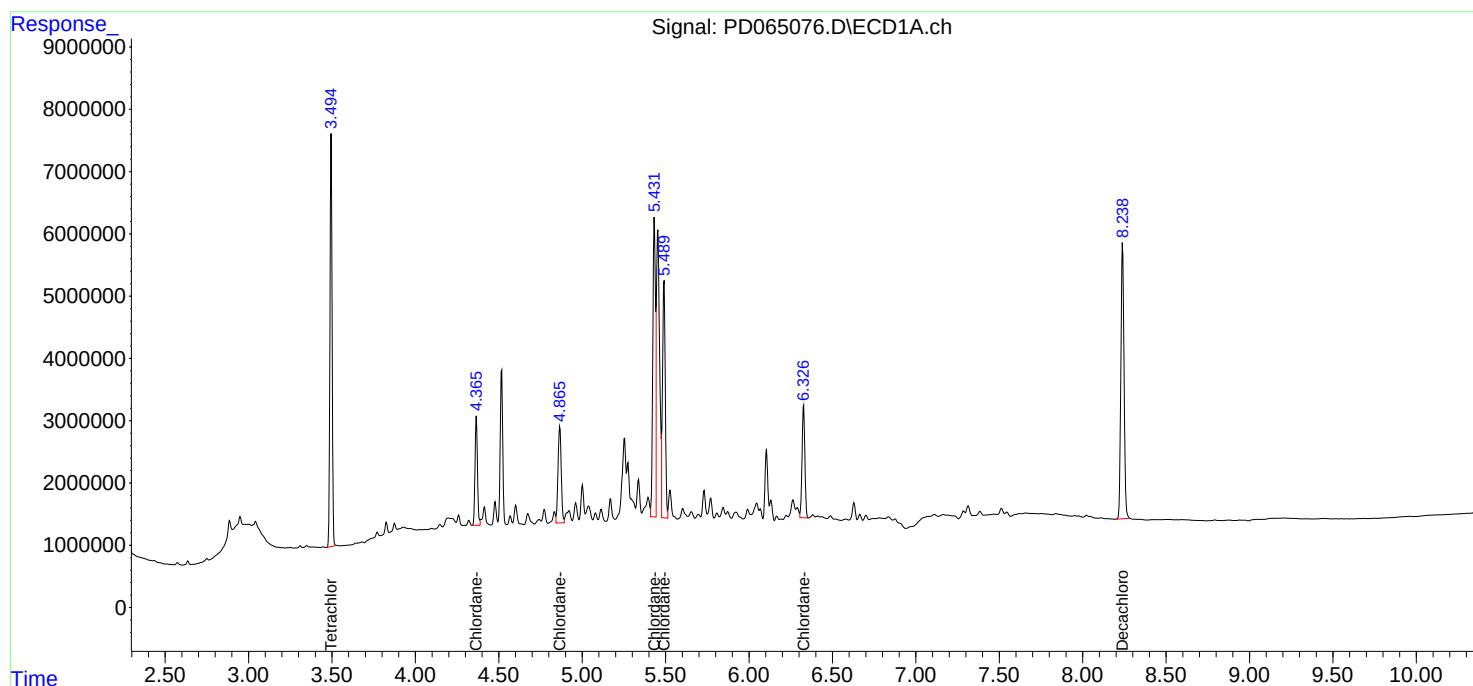


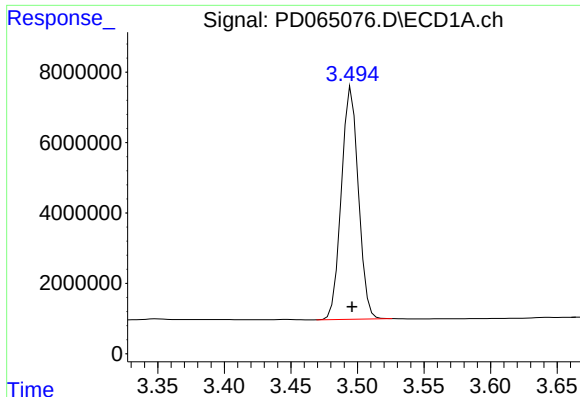

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 58835627
Conc: 46.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD082021CHLOR

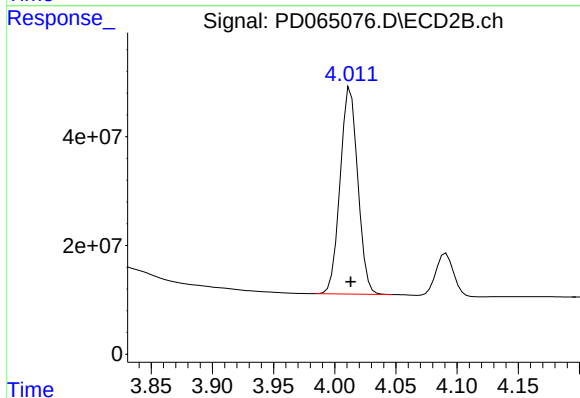


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 381593481
Conc: 46.22 ng/ml

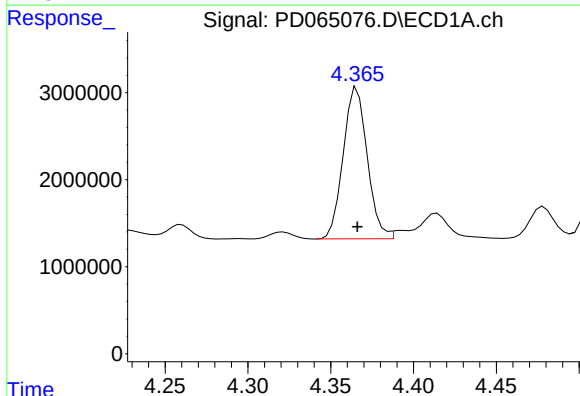


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 17591622
Conc: 464.50 ng/ml

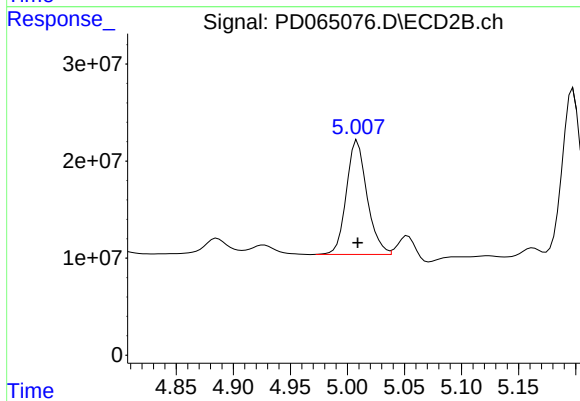

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 148505499
Conc: 479.47 ng/ml

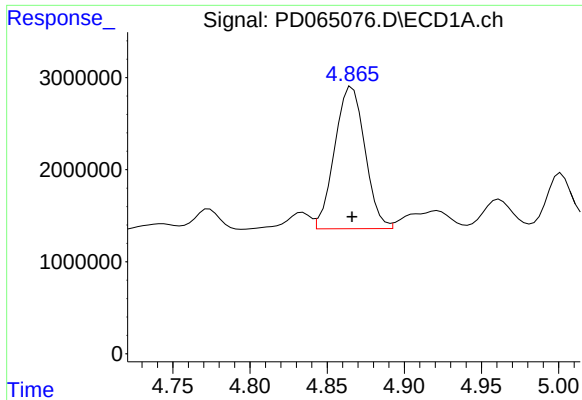

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 21074118
Conc: 482.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD082021CHLOR

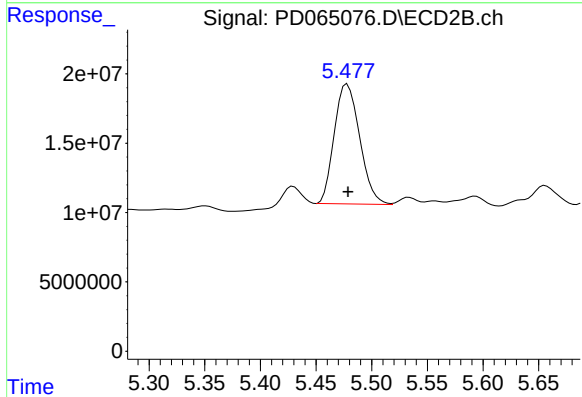


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 137734232
Conc: 440.29 ng/ml

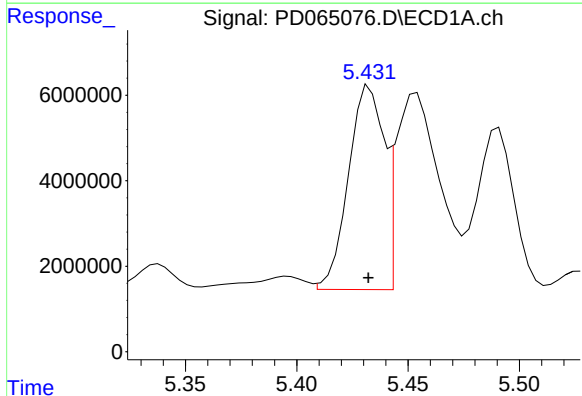


#25 Chlordane-3

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 52817132
Conc: 478.54 ng/ml

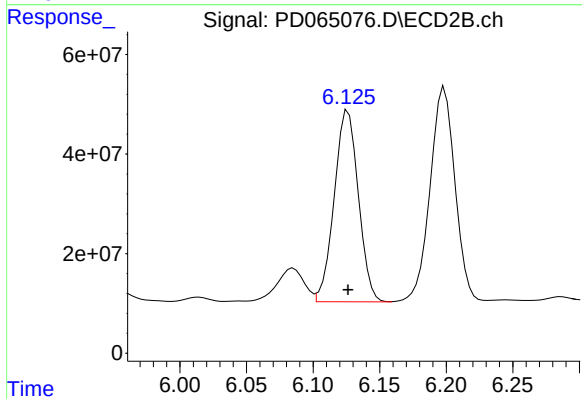

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 485485149
Conc: 469.59 ng/ml

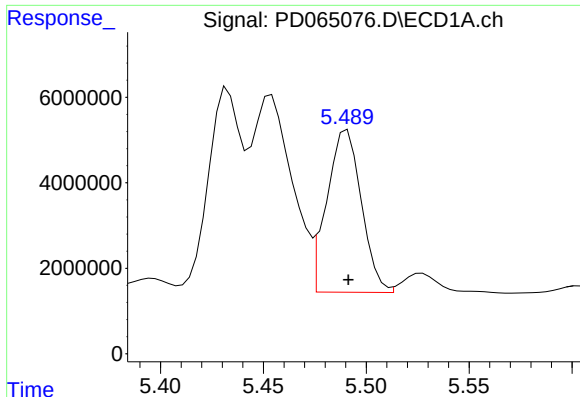

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 44347290
Conc: 483.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD082021CHLOR

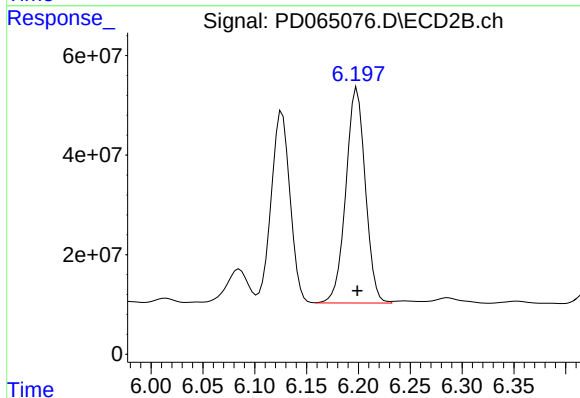


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 564008723
Conc: 469.10 ng/ml

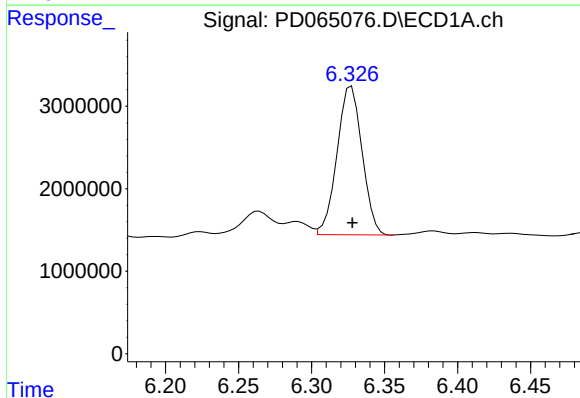


#27 Chlordane-5

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 21545424
Conc: 478.91 ng/ml

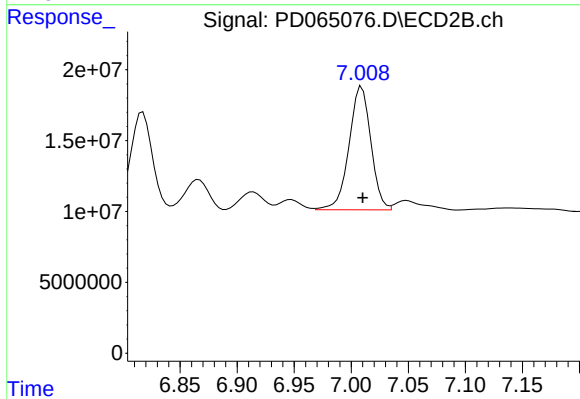

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 115917887
Conc: 488.89 ng/ml

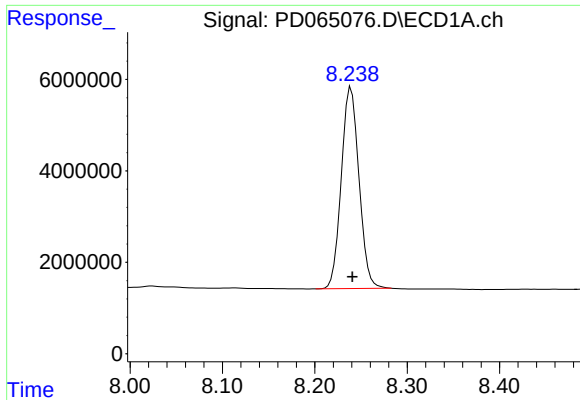

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: -0.001 min
Response: 58678679
Conc: 48.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD082021CHLOR

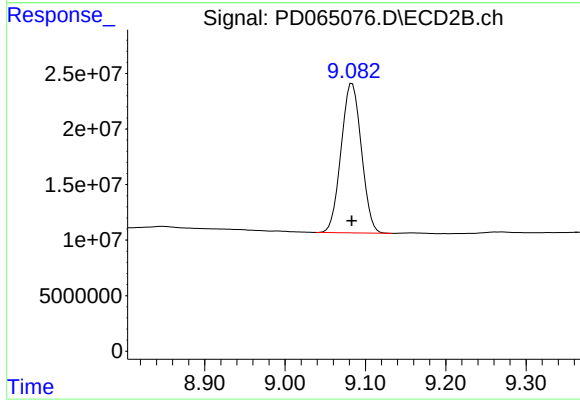

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 236034532
Conc: 47.06 ng/ml