

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 00:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 00:16:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.013	21362207	164.8E6	20.782	20.809
28)	SA Decachlor...	8.240	9.083	24449045	100.7E6	21.578	21.274
Target Compounds							
7)	B delta-BHC	0.000	5.096	0	2935655	N.D.	0.302 #
15)	B Endosulfa...	0.000	6.914f	0	760782	N.D.	0.130 #
21)	B Endrin ke...	0.000	7.790f	0	1823972	N.D.	0.281 #
23)	Chlordane-1	4.394f	0.000	2095461	0	55.330	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 00:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 00:16:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

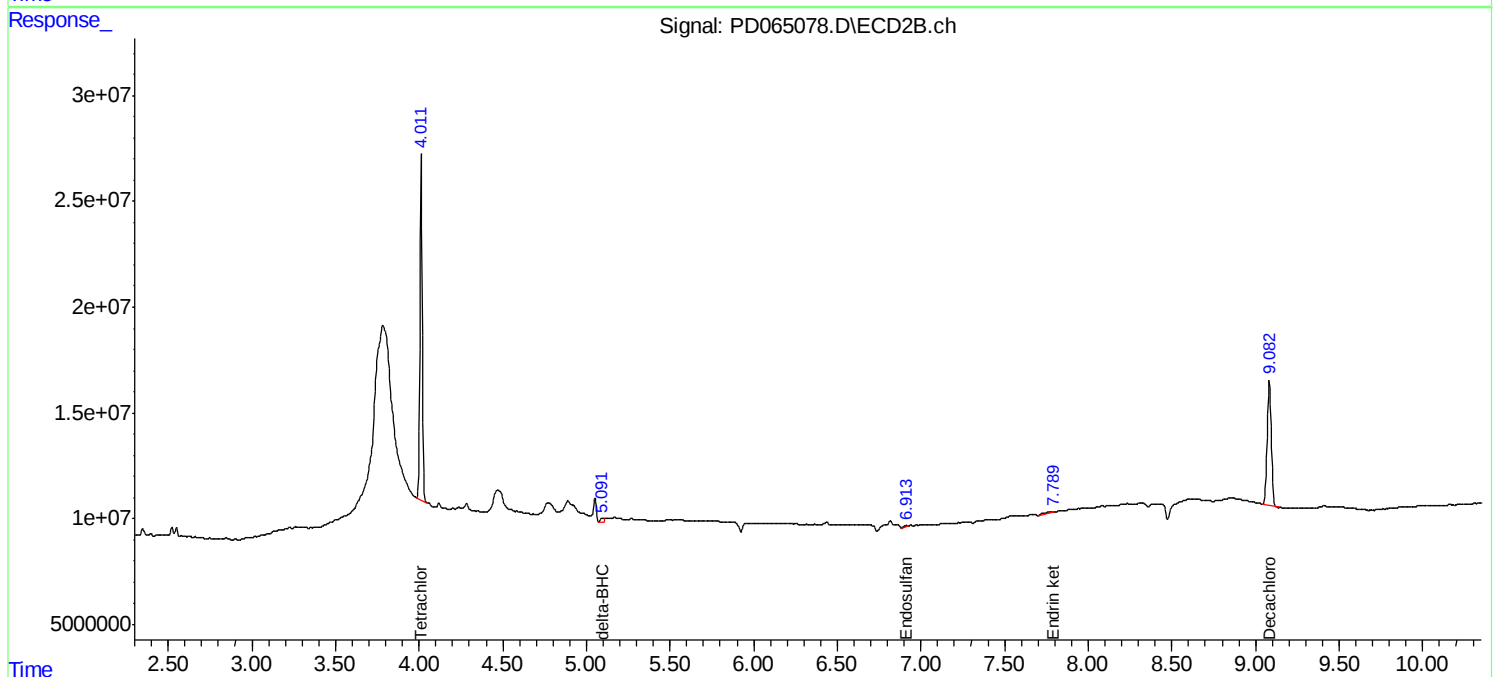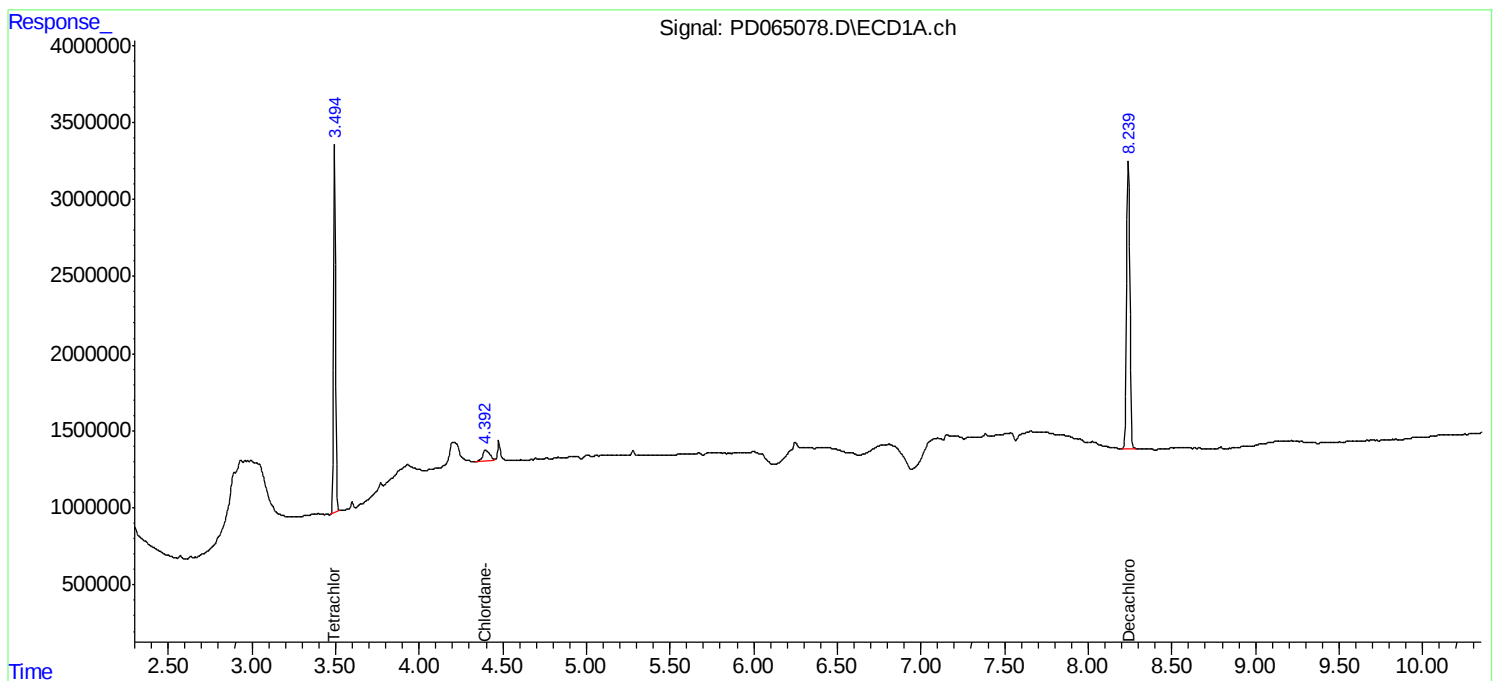


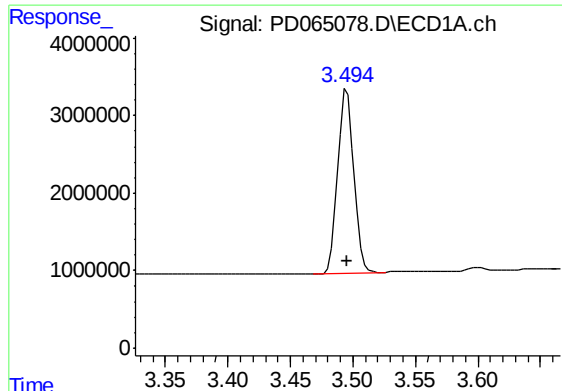

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 21362207
Conc: 20.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

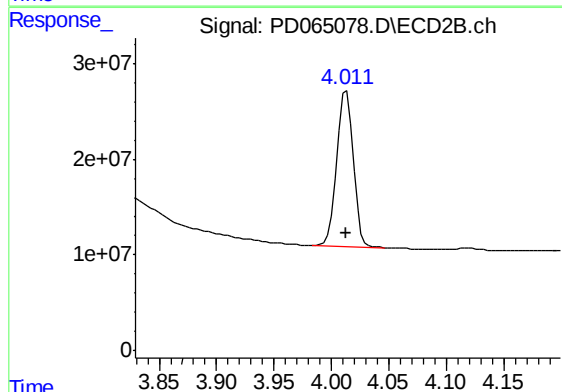


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 164825649
Conc: 20.81 ng/ml

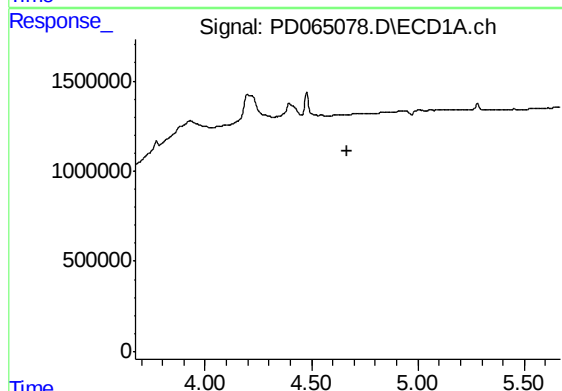


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.670 min
Response: 0
Conc: N.D.

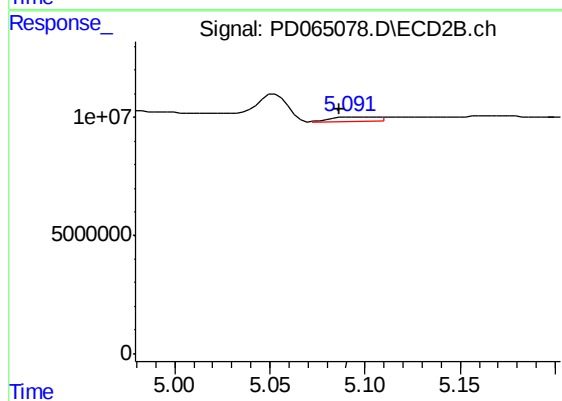

#7 delta-BHC


R.T.: 5.096 min
Delta R.T.: 0.010 min
Response: 2935655
Conc: 0.30 ng/ml

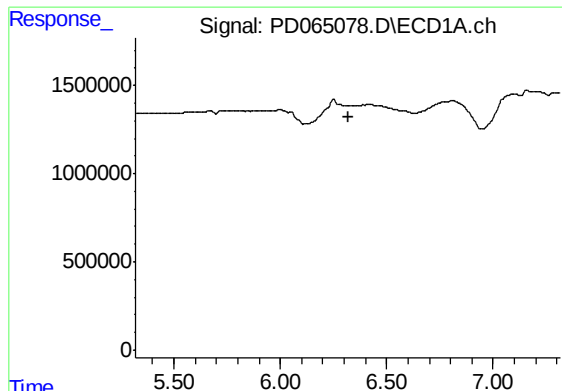

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

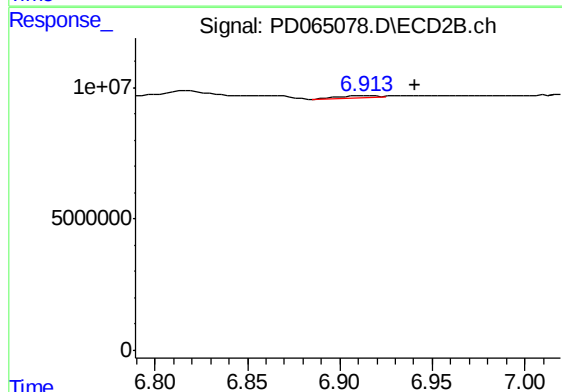


#15 Endosulfan II

R.T.: 6.914 min
Delta R.T.: -0.026 min
Response: 760782
Conc: 0.13 ng/ml

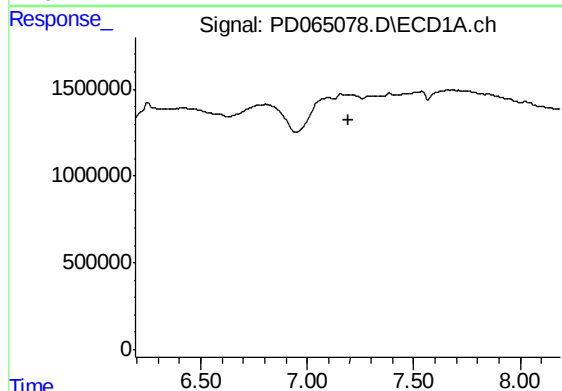


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

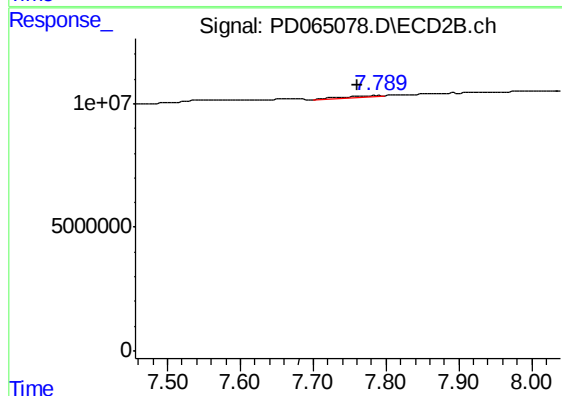

#21 Endrin ketone


R.T.: 7.790 min
Delta R.T.: 0.029 min
Response: 1823972
Conc: 0.28 ng/ml

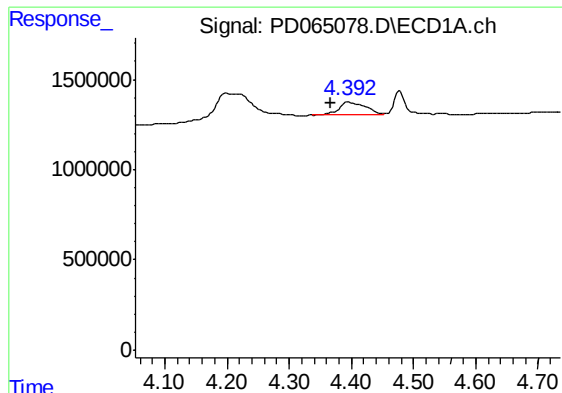

#23 Chlordane-1


R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 2095461
Conc: 55.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

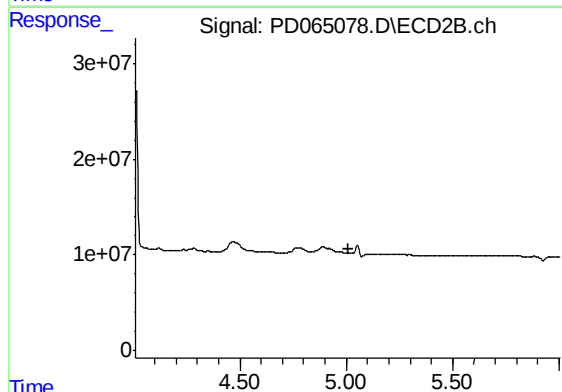


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

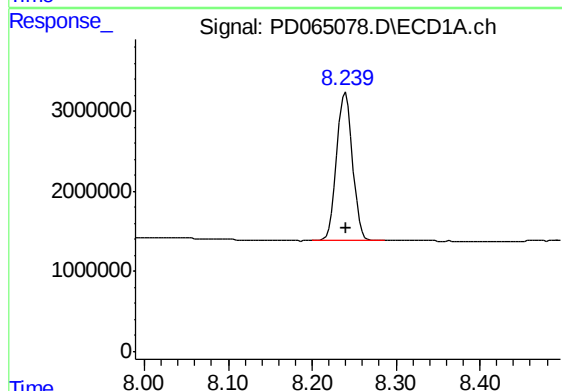

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 24449045
Conc: 21.58 ng/ml

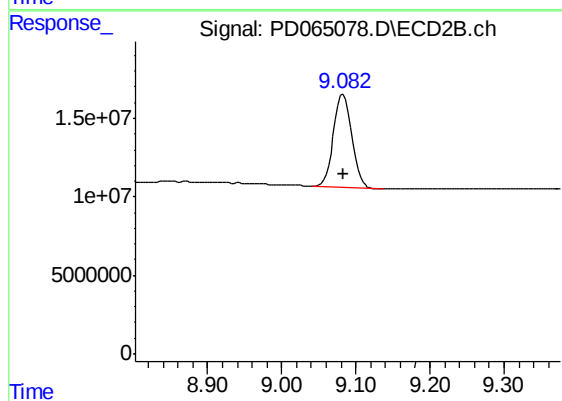

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 100681924
Conc: 21.27 ng/ml