

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 01:19
 Operator : AR\AJ
 Sample : PB137673BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB137673BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 00:17:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	19971651	156.4E6	19.430	19.749
28)	SA Decachlor...	8.240	9.083	24941817	95954983	22.013	20.276
Target Compounds							
10)	B gamma-Chl...	0.000	6.124	0	2399389	N.D.	0.314 #
23)	Chlordane-1	4.394f	0.000	1833061	0	48.401	N.D. #
25)	Chlordane-3	0.000	6.124	0	2399389	N.D.	2.321 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 01:19
Operator : AR\AJ
Sample : PB137673BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB137673BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 00:17:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

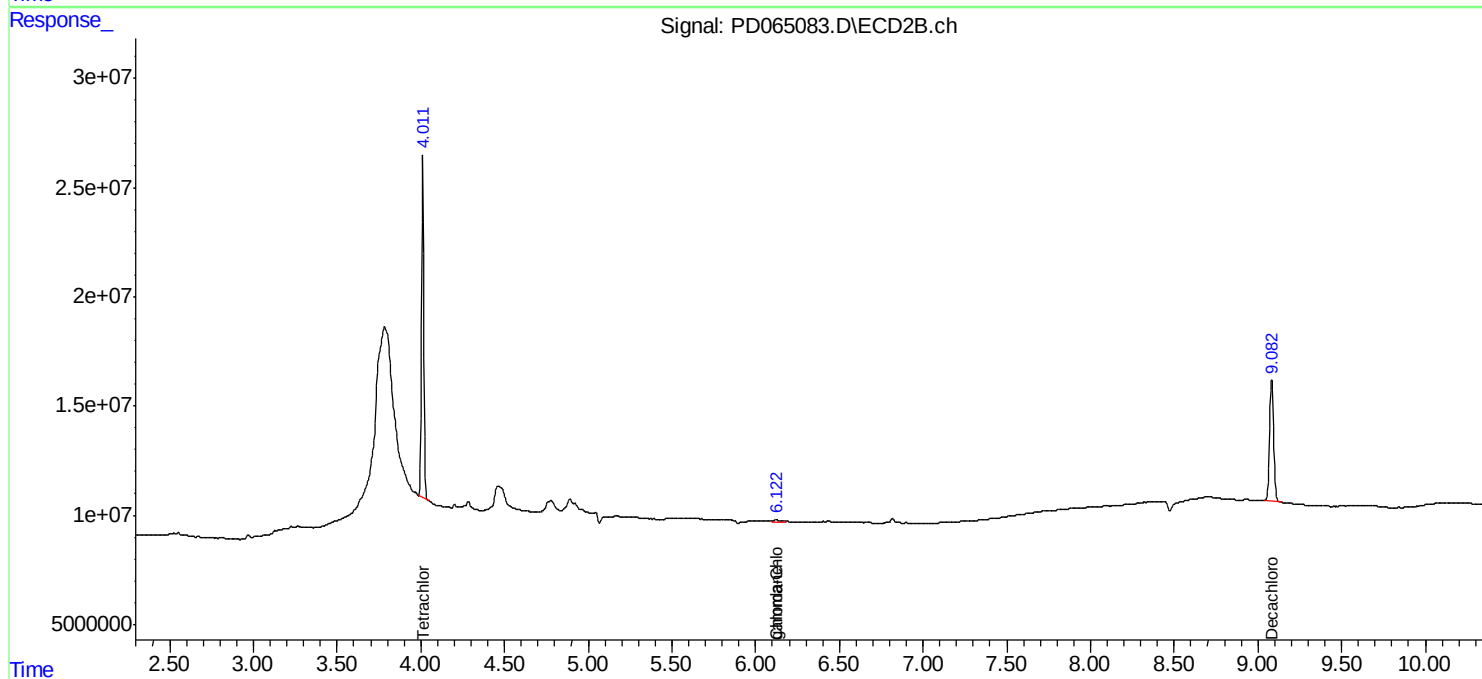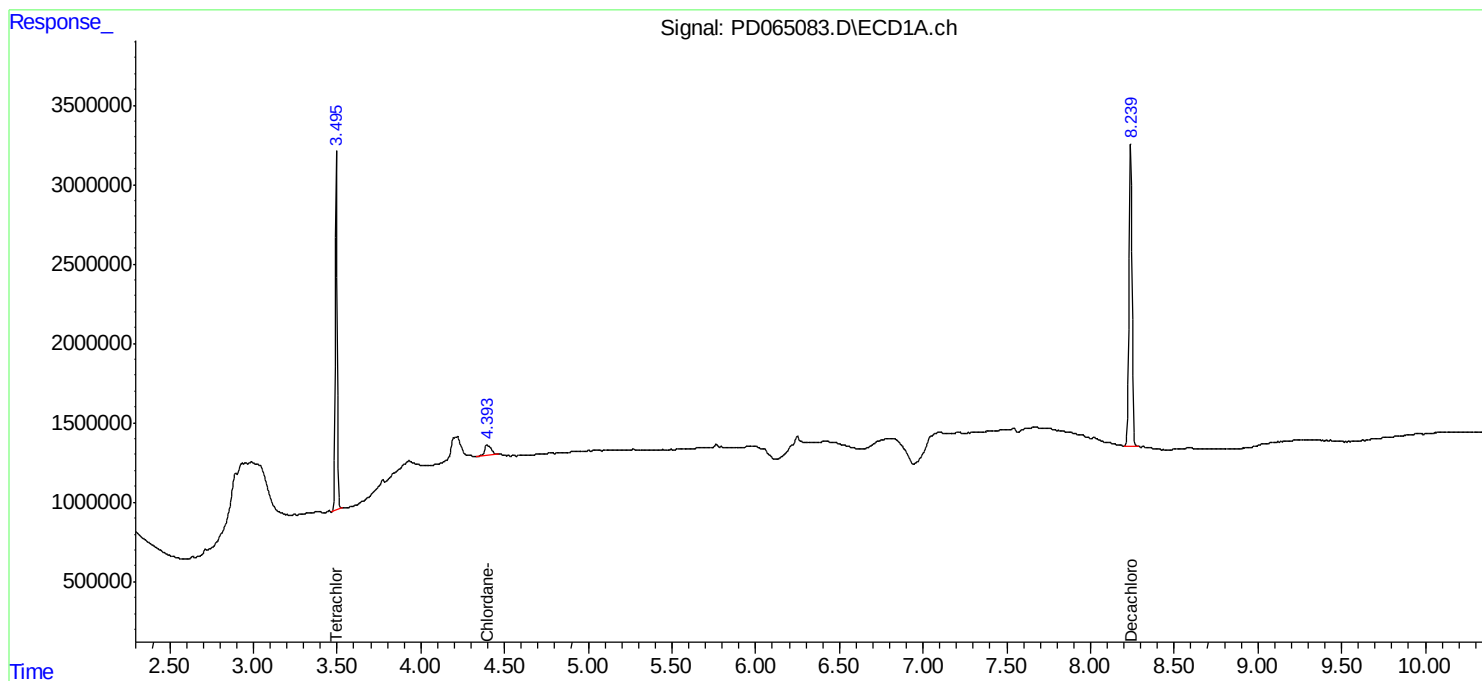


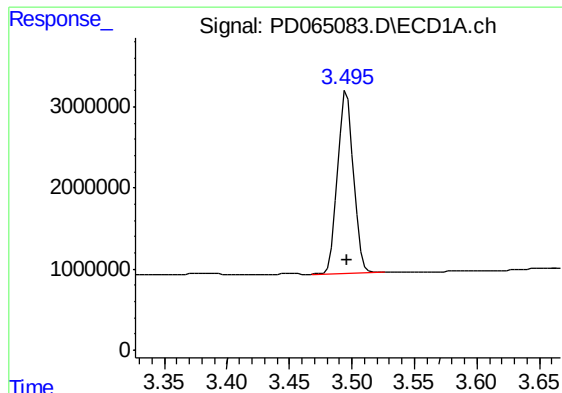

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 19971651
Conc: 19.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB137673BL

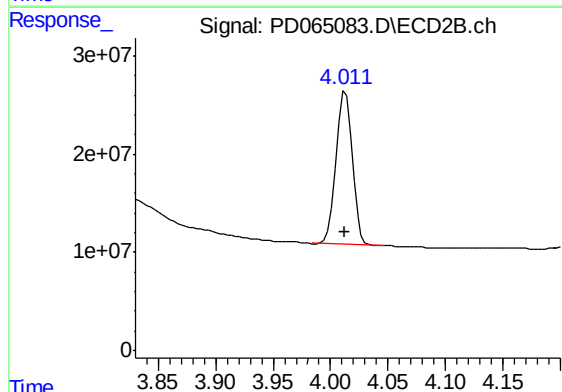


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 156422351
Conc: 19.75 ng/ml

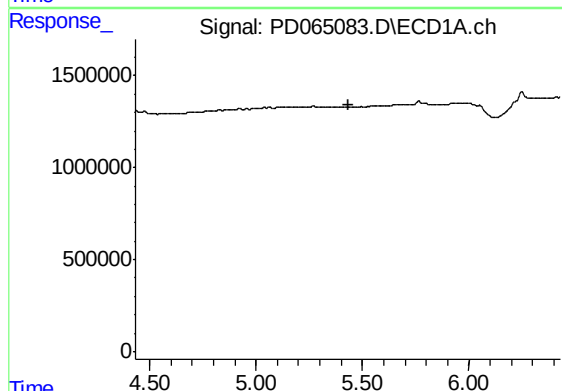


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.432 min
Response: 0
Conc: N.D.

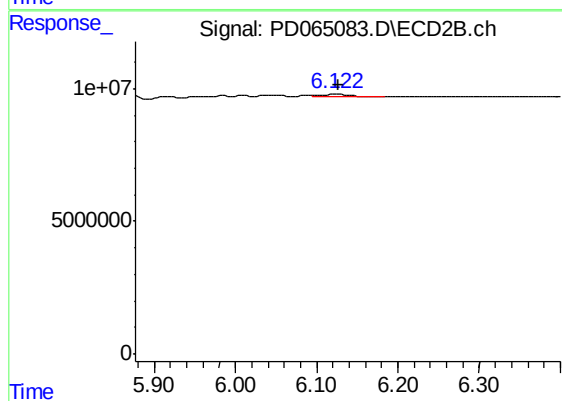

#10 gamma-Chlordane


R.T.: 6.124 min
Delta R.T.: -0.003 min
Response: 2399389
Conc: 0.31 ng/ml

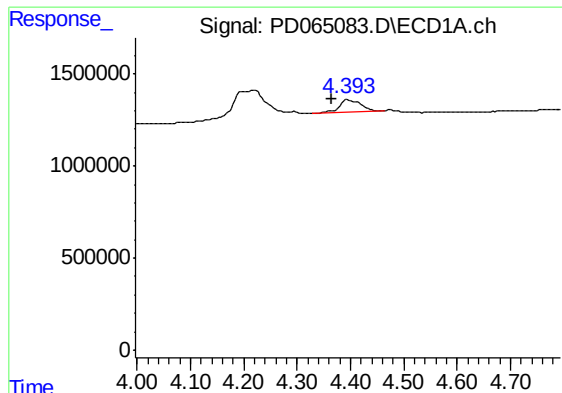

#23 Chlordane-1


R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 1833061
Conc: 48.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB137673BL

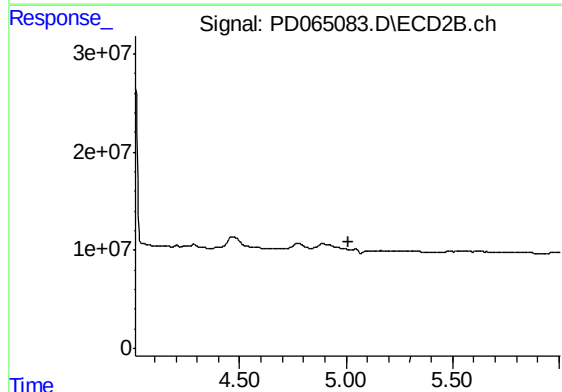


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

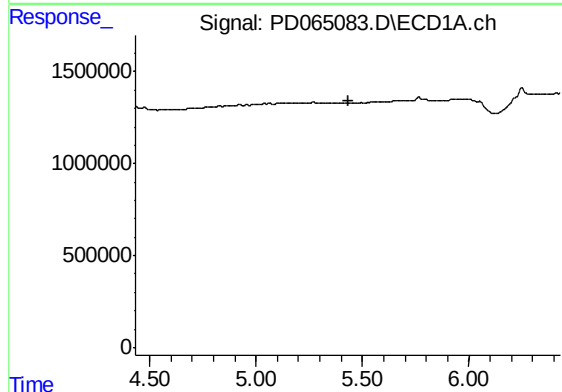


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.432 min
Response: 0
Conc: N.D.

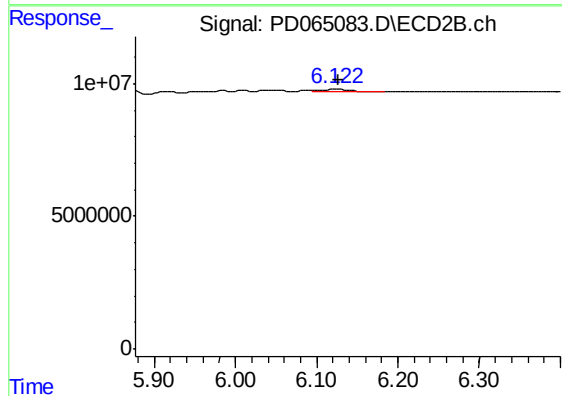

#25 Chlordane-3


R.T.: 6.124 min
Delta R.T.: -0.003 min
Response: 2399389
Conc: 2.32 ng/ml

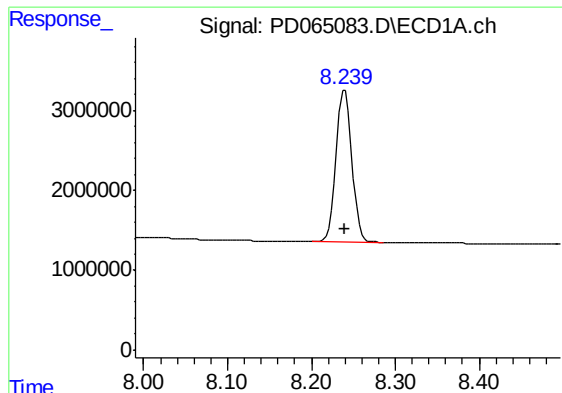

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 24941817
Conc: 22.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB137673BL

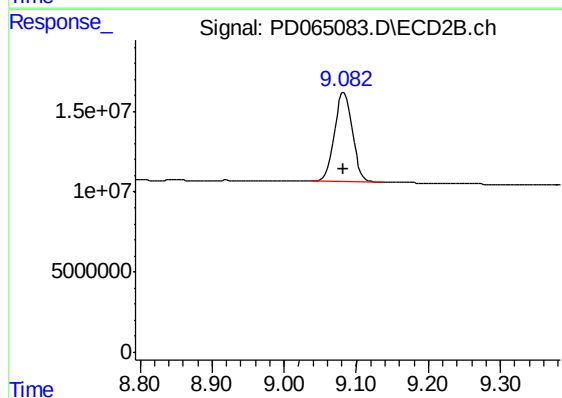

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 95954983
Conc: 20.28 ng/ml