

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 10:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 00:19:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.012	21519010	165.7E6	20.935	20.918
28)	SA Decachlor...	8.240	9.084	26666967	104.1E6	23.536	21.987
Target Compounds							
2)	A alpha-BHC	0.000	4.435f	0 13620939	N.D.	1.172	#
7)	B delta-BHC	0.000	5.097	0 1822384	N.D.	0.188	#
8)	B Heptachlo...	0.000	5.887	0 20657652	N.D.	2.769	#
10)	B gamma-Chl...	0.000	6.127	0 2924098	N.D.	0.382	#
23)	Chlordane-1	4.392f	0.000	3680495	0 97.182	N.D.	#
25)	Chlordane-3	0.000	6.127	0 2924098	N.D.	2.828	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 10:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 00:19:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

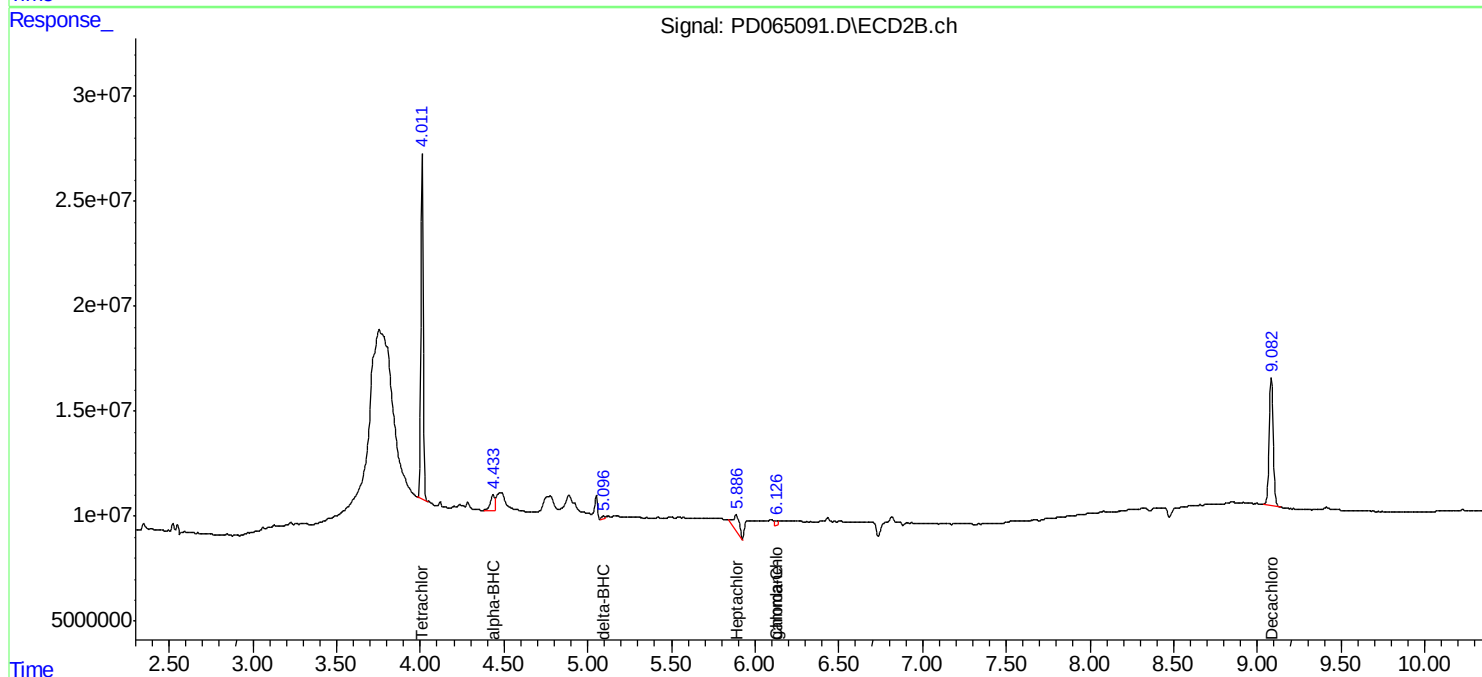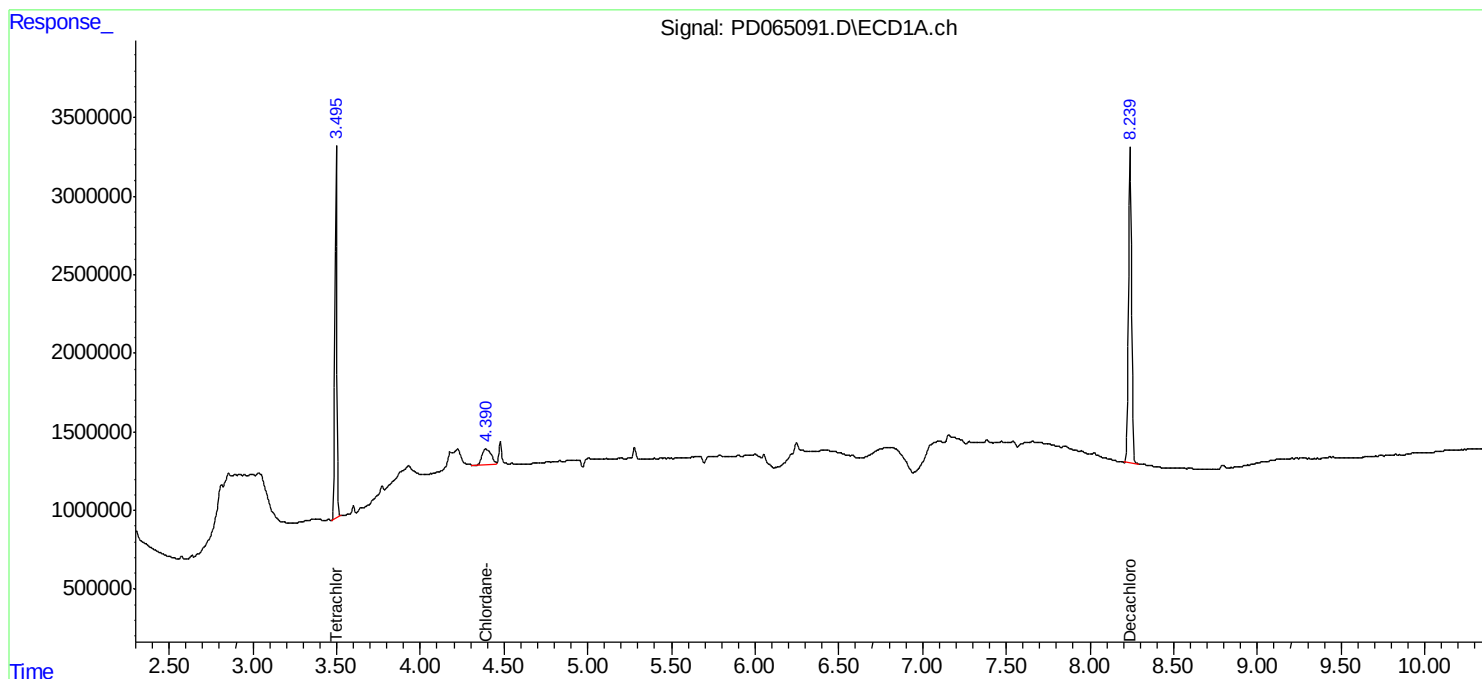


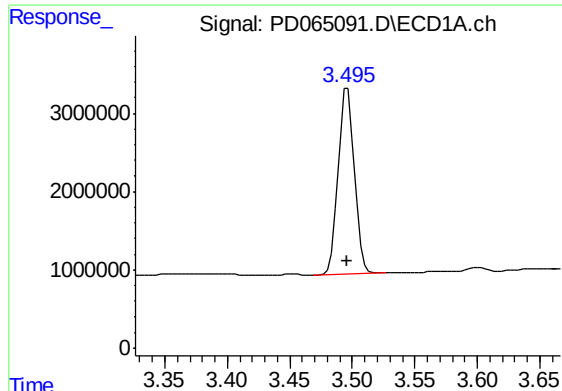

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 21519010
Conc: 20.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

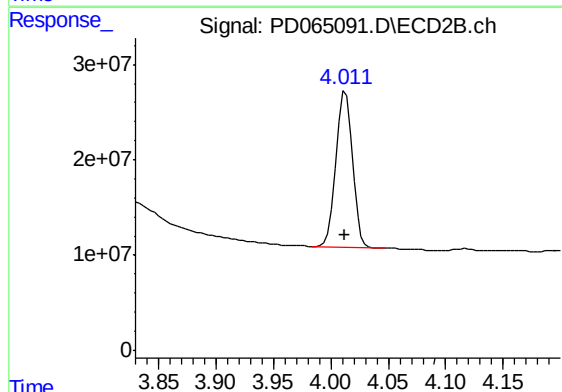


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 165683387
Conc: 20.92 ng/ml

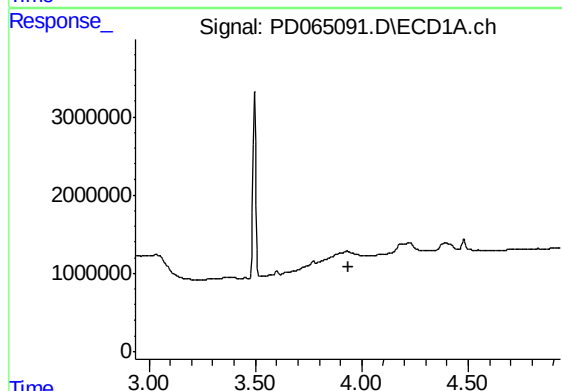


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

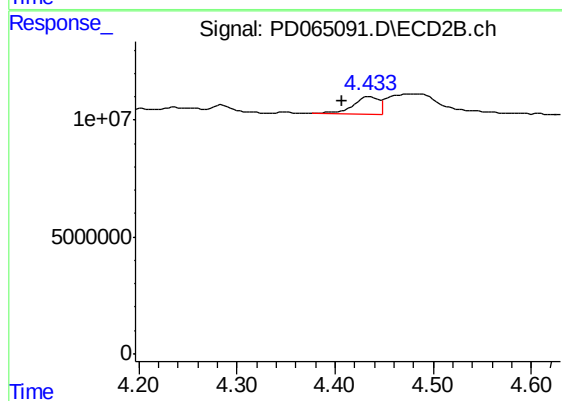

#2 alpha-BHC


R.T.: 4.435 min
Delta R.T.: 0.027 min
Response: 13620939
Conc: 1.17 ng/ml

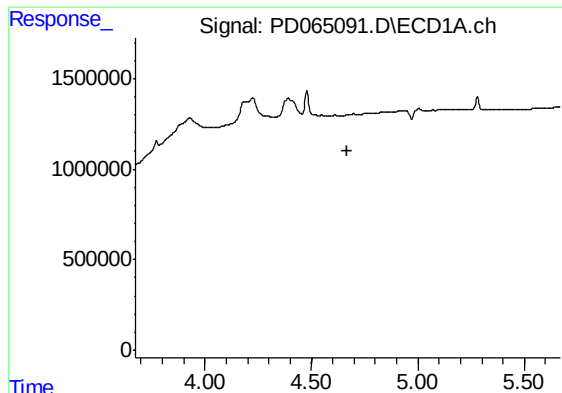

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

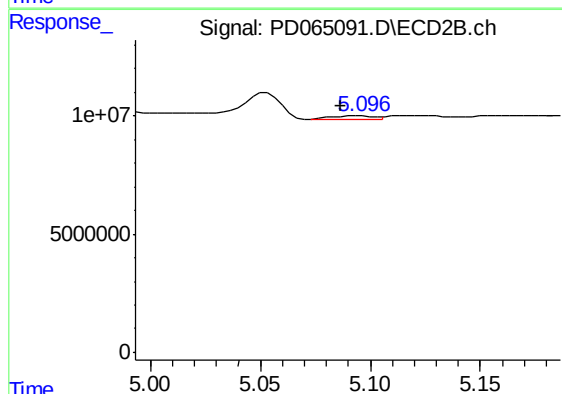


#7 delta-BHC

R.T.: 5.097 min
Delta R.T.: 0.010 min
Response: 1822384
Conc: 0.19 ng/ml

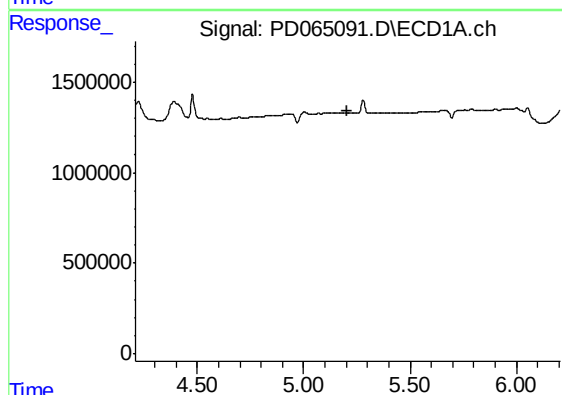


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.207 min
Response: 0
Conc: N.D.

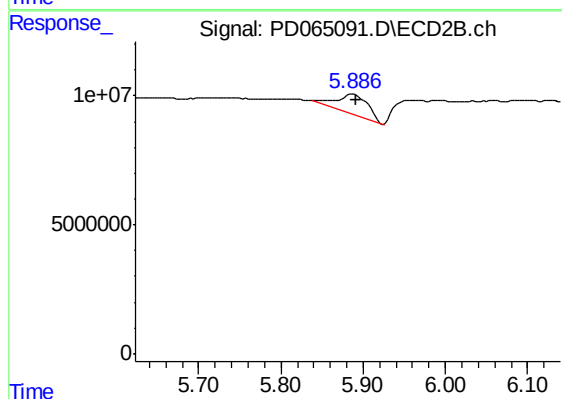

#8 Heptachlor epoxide


R.T.: 5.887 min
Delta R.T.: -0.005 min
Response: 20657652
Conc: 2.77 ng/ml

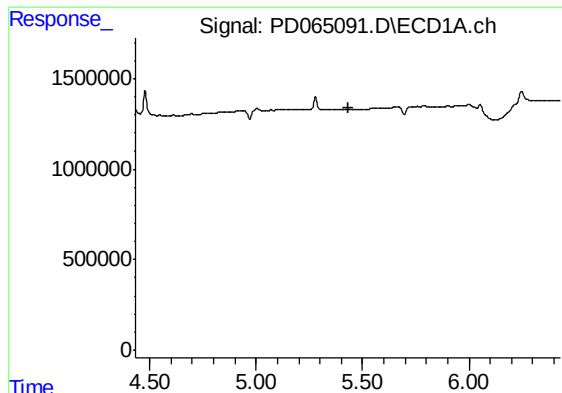

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

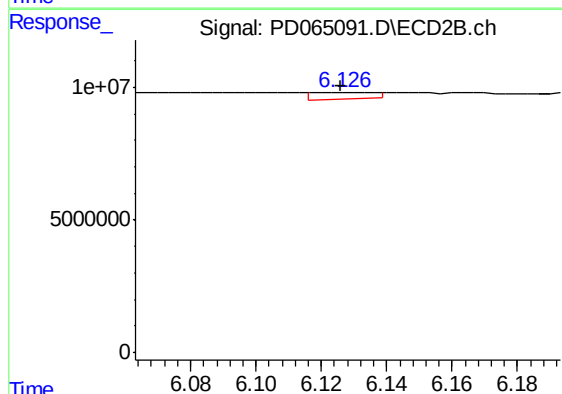


#10 gamma-Chlordane

R.T.: 6.127 min
Delta R.T.: 0.001 min
Response: 2924098
Conc: 0.38 ng/ml

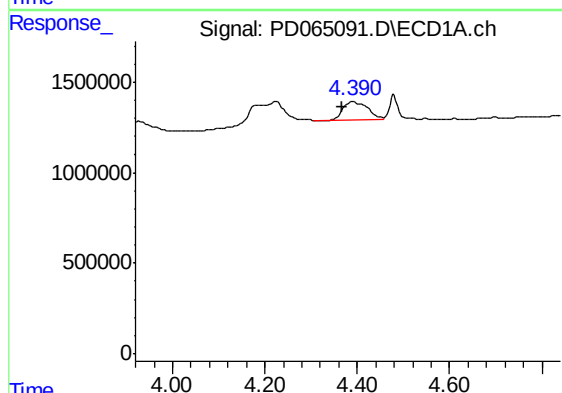


#23 Chlordane-1

R.T.: 4.392 min
Delta R.T.: 0.025 min
Response: 3680495
Conc: 97.18 ng/ml

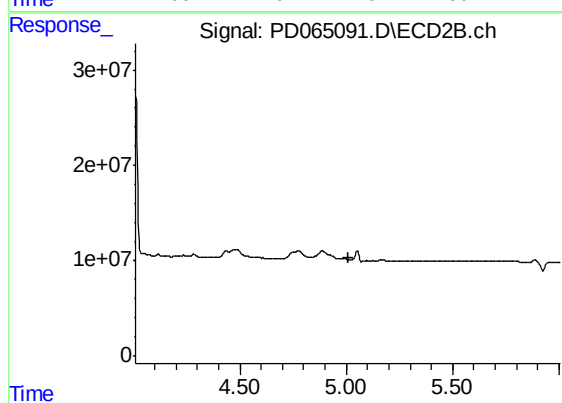

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

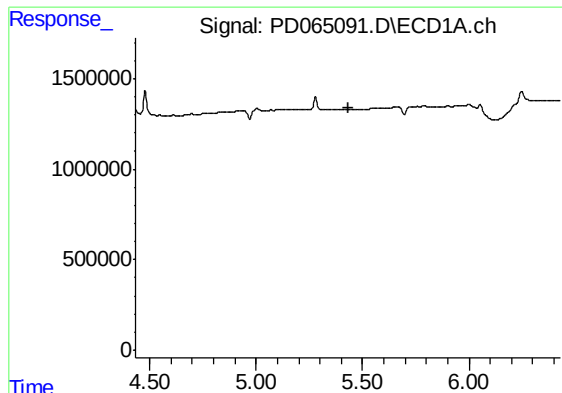

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

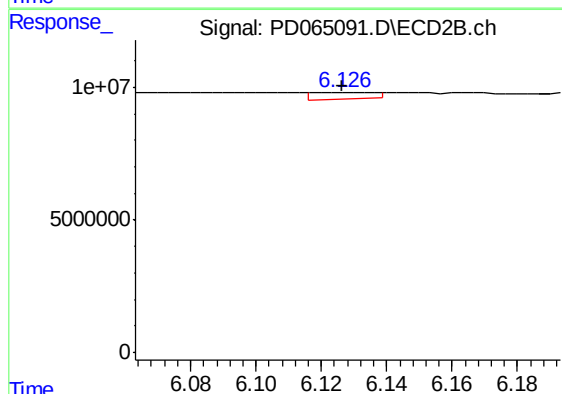


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: 0.001 min
Response: 2924098
Conc: 2.83 ng/ml

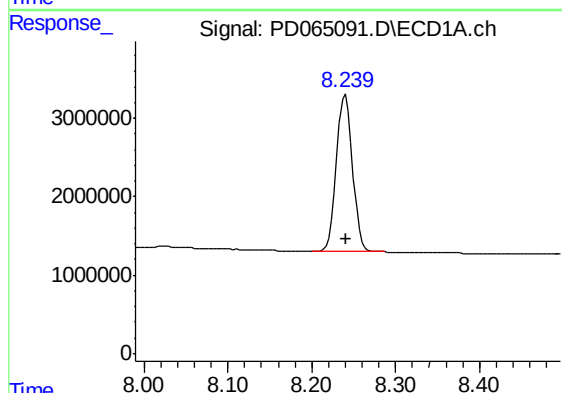

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 26666967
Conc: 23.54 ng/ml

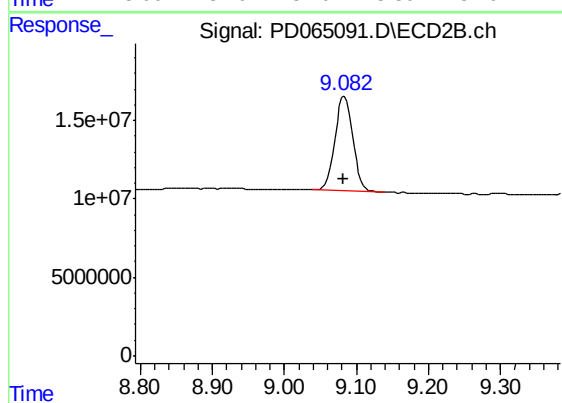

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 104054695
Conc: 21.99 ng/ml