

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 22:20
 Operator : AR\AJ
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 02:52:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:52:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.013	99411150	760.4E6	102.193	100.579
7) SA Decachlor...	8.241	9.085	107.7E6	460.0E6	93.190	98.875
Target Compounds						
2) Toxaphene-1	5.749	6.406	8077829	34961723	925.765	973.403
3) Toxaphene-2	5.910	6.599	8449428	57591369	928.613	945.407
4) Toxaphene-3	6.352	7.182	18794144	100.9E6	923.790	986.797
5) Toxaphene-4	6.597	7.269	20423037	101.5E6	929.493	988.348
6) Toxaphene-5	7.084	7.687	23377304	79574204	931.096	988.631

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 22:20
Operator : AR\AJ
Sample : PTOXICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 02:52:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:52:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

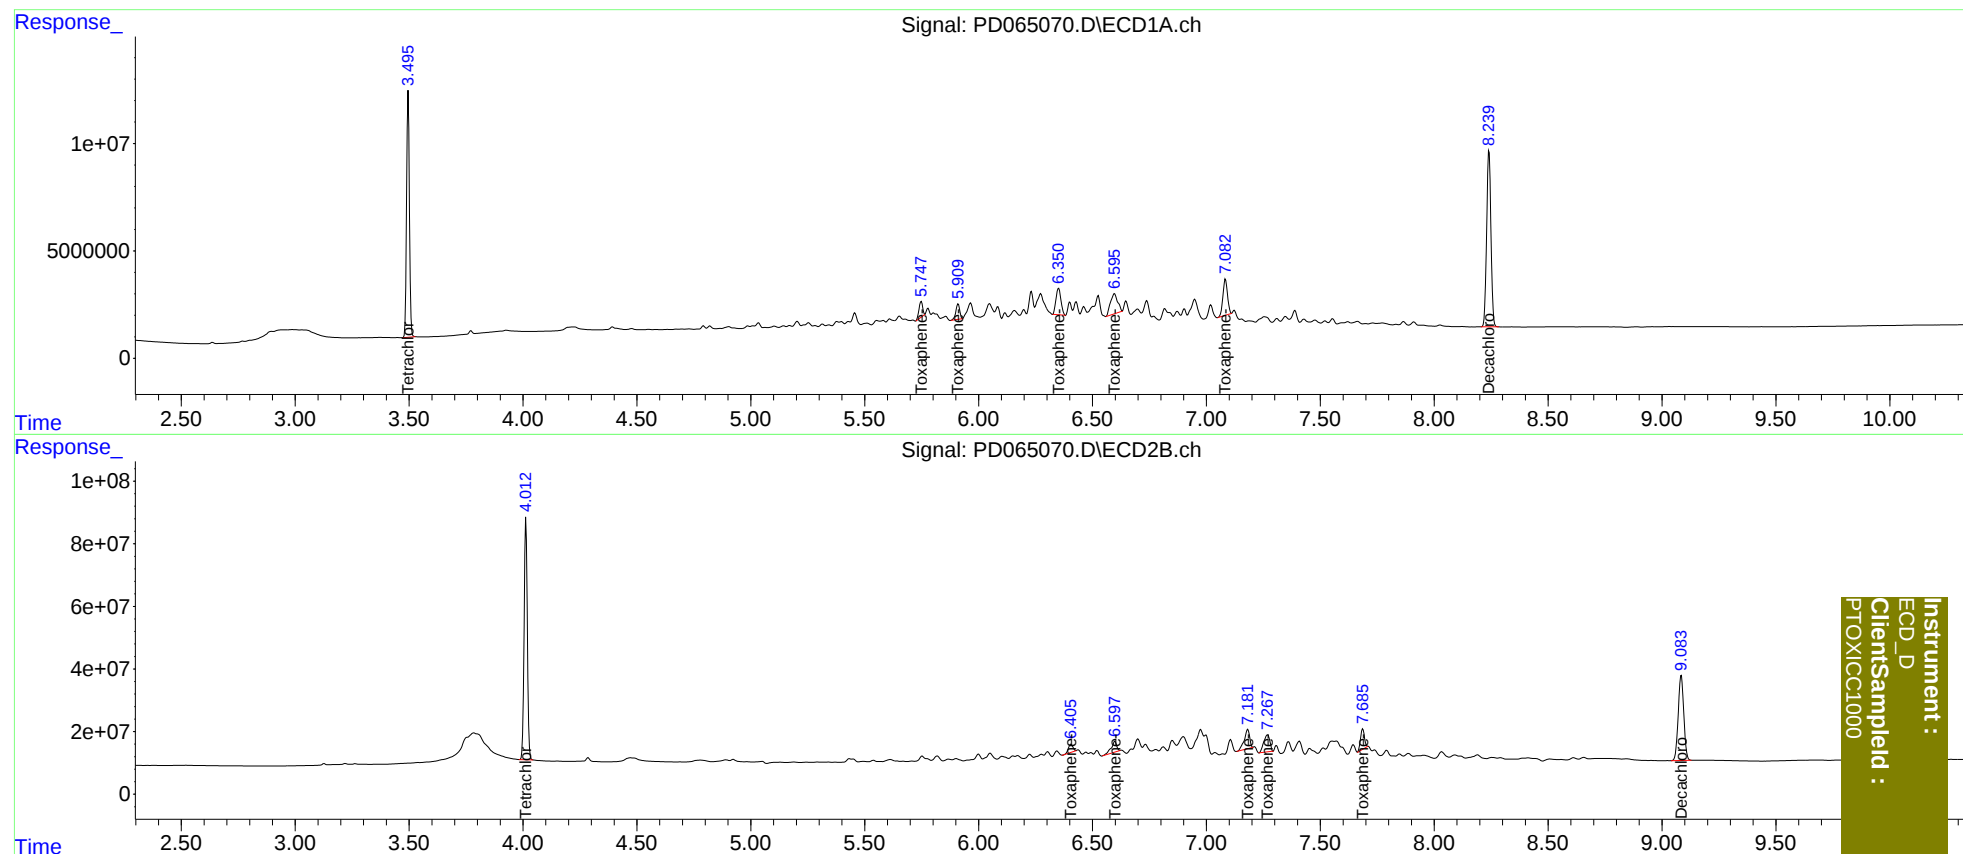

Instrument :
ECD_D
ClientSample :
PTOXICC1000